

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 13:42
 Operator : AR\AJ
 Sample : 04607-11MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBJQ2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2023
 Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:25:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	47430734	31790235	19.316	19.243
27)	SA Decachlor...	9.079	7.894	62185176	35574445	19.237	19.216
Target Compounds							
2)	A alpha-BHC	3.996	3.258	220.0E6	142.9E6	53.059	56.062
3)	MA gamma-BHC...	4.329	3.588	204.3E6	123.5E6	51.490	51.712
4)	MA Heptachlor	4.920	3.926	206.1E6	126.8E6	49.601	51.030
5)	MB Aldrin	5.262	4.206	203.3E6	123.6E6	49.998	50.376
6)	B beta-BHC	4.527	3.885	82067822	52586581	47.445	48.305
7)	B delta-BHC	4.776	4.114	163.9E6	101.3E6	41.112	41.206
8)	B Heptachlo...	5.690	4.708	185.8E6	117.8E6	50.148	51.024
9)	A Endosulfan I	6.076	5.078	168.5E6	107.8E6	50.551m	52.426
10)	B trans-Chl...	5.947	4.958	180.0E6	113.5E6	49.917	50.956
11)	B cis-Chlor...	6.026	5.022	175.1E6	115.7E6	47.187	50.371
12)	B 4,4'-DDE	6.199	5.210	371.6E6	224.0E6	103.853	104.093
13)	MA Dieldrin	6.353	5.342	397.5E6	247.5E6	106.847	104.773
14)	MA Endrin	6.583	5.618	325.3E6	228.4E6	108.202	109.176
15)	B Endosulfa...	6.803	5.913	336.6E6	216.8E6	107.627	106.779
16)	A 4,4'-DDD	6.717	5.766	283.8E6	159.6E6	109.644	101.294
17)	MA 4,4'-DDT	7.032	6.017	314.0E6	191.9E6	121.568	117.987
18)	B Endrin al...	6.934	6.093	245.1E6	157.5E6	100.855	101.583
19)	B Endosulfa...	7.169	6.315	288.2E6	193.0E6	100.930	103.716
20)	A Methoxychlor	7.509	6.591	824.1E6	494.0E6	558.476	556.966
21)	B Endrin ke...	7.656	6.821	347.6E6	235.7E6	109.314	109.712

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 13:42
Operator : AR\AJ
Sample : 04607-11MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:25:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

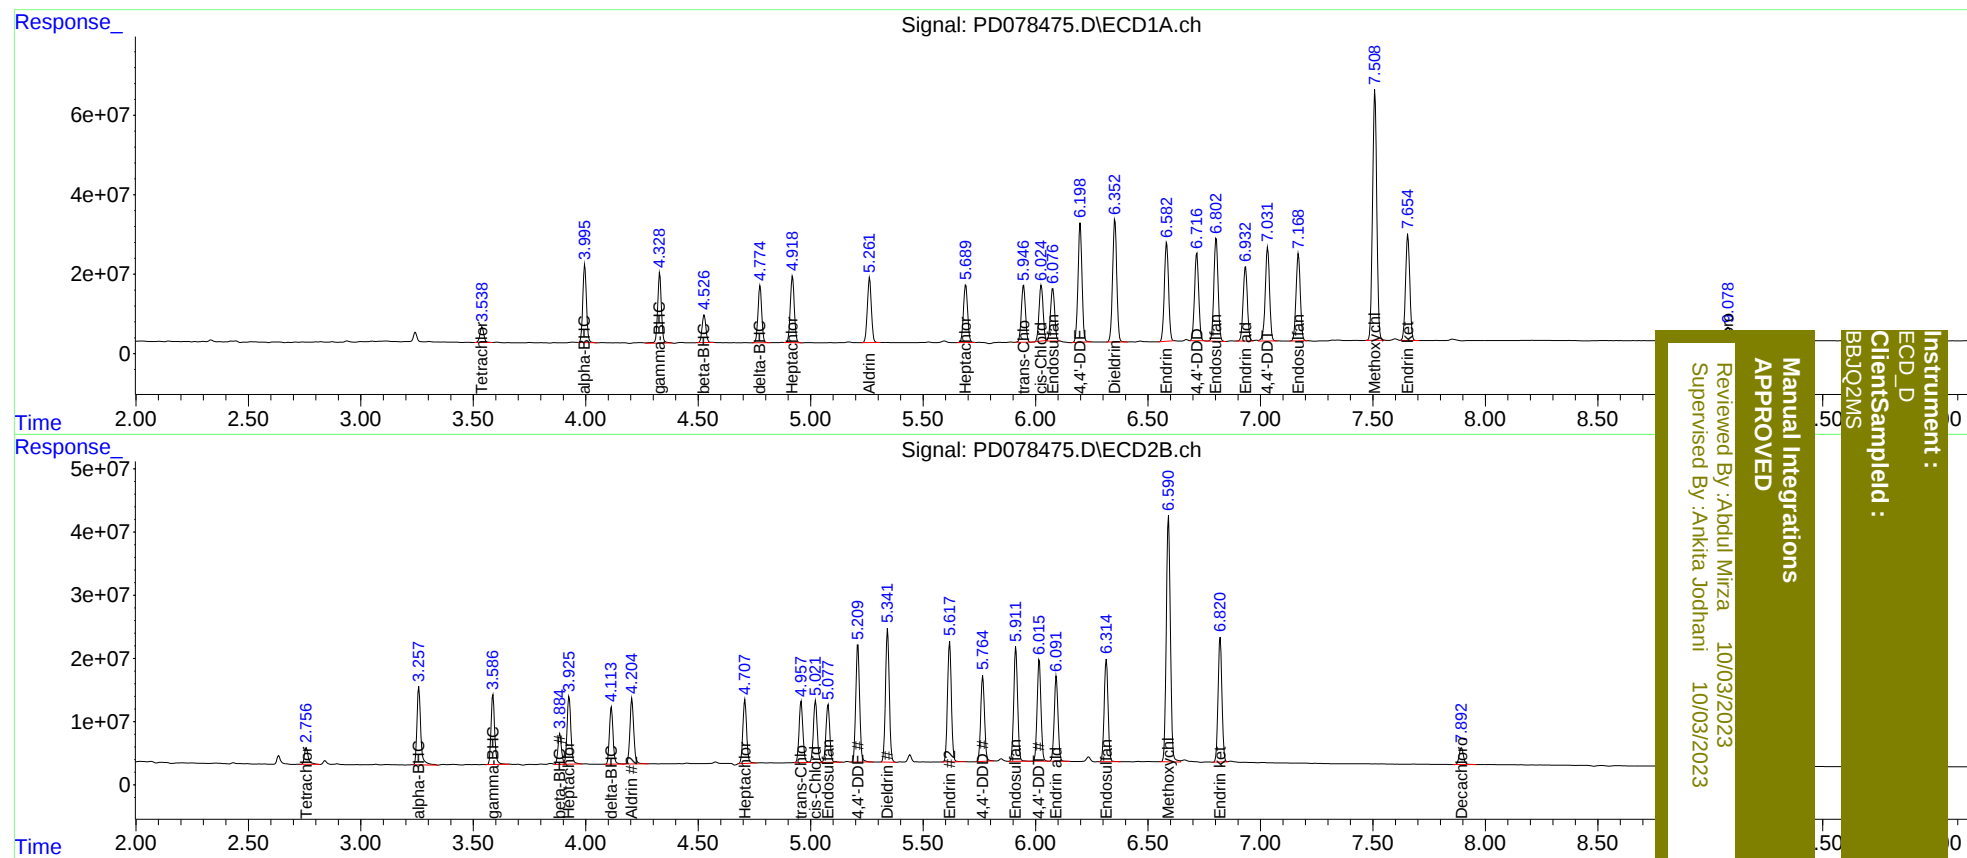

Instrument :
ECD_D
ClientSampled :
BBJQZMS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 10/03/2023
Supervised By: Ankita Jodhani 10/03/2023