

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 13:55
 Operator : AR\AJ
 Sample : 04607-12MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBJQ2MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2023
 Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:26:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.758	47305601	31447097	19.265	19.035
27)	SA Decachlor...	9.080	7.894	61087008	35128456	18.897	18.975
Target Compounds							
2)	A alpha-BHC	3.996	3.259	220.3E6	142.2E6	53.134	55.782
3)	MA gamma-BHC...	4.330	3.588	203.8E6	123.3E6	51.380	51.616
4)	MA Heptachlor	4.920	3.927	206.8E6	126.8E6	49.772	51.017
5)	MB Aldrin	5.263	4.206	204.3E6	123.7E6	50.261	50.422
6)	B beta-BHC	4.527	3.885	82229305	52857802	47.539	48.555
7)	B delta-BHC	4.776	4.114	165.6E6	101.2E6	41.538	41.149
8)	B Heptachlo...	5.690	4.708	186.7E6	117.5E6	50.386	50.894
9)	A Endosulfan I	6.076	5.078	169.0E6	108.4E6	50.694m	52.716
10)	B trans-Chl...	5.948	4.958	181.0E6	113.8E6	50.205	51.068
11)	B cis-Chlor...	6.027	5.023	176.0E6	115.8E6	47.431	50.408
12)	B 4,4'-DDE	6.199	5.211	372.7E6	224.2E6	104.150	104.166
13)	MA Dieldrin	6.354	5.343	398.3E6	247.4E6	107.056	104.727
14)	MA Endrin	6.583	5.619	328.6E6	227.5E6	109.326	108.748
15)	B Endosulfa...	6.804	5.913	337.1E6	216.6E6	107.786	106.697
16)	A 4,4'-DDD	6.718	5.766	285.7E6	161.6E6	110.390	102.569
17)	MA 4,4'-DDT	7.032	6.016	315.4E6	191.5E6	122.093	117.706
18)	B Endrin al...	6.934	6.092	246.4E6	158.0E6	101.421	101.937
19)	B Endosulfa...	7.169	6.315	291.1E6	193.2E6	101.933	103.773
20)	A Methoxychlor	7.509	6.592	831.6E6	493.4E6	563.567	556.259
21)	B Endrin ke...	7.656	6.821	352.4E6	236.2E6	110.812	109.937

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 13:55
Operator : AR\AJ
Sample : 04607-12MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:26:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

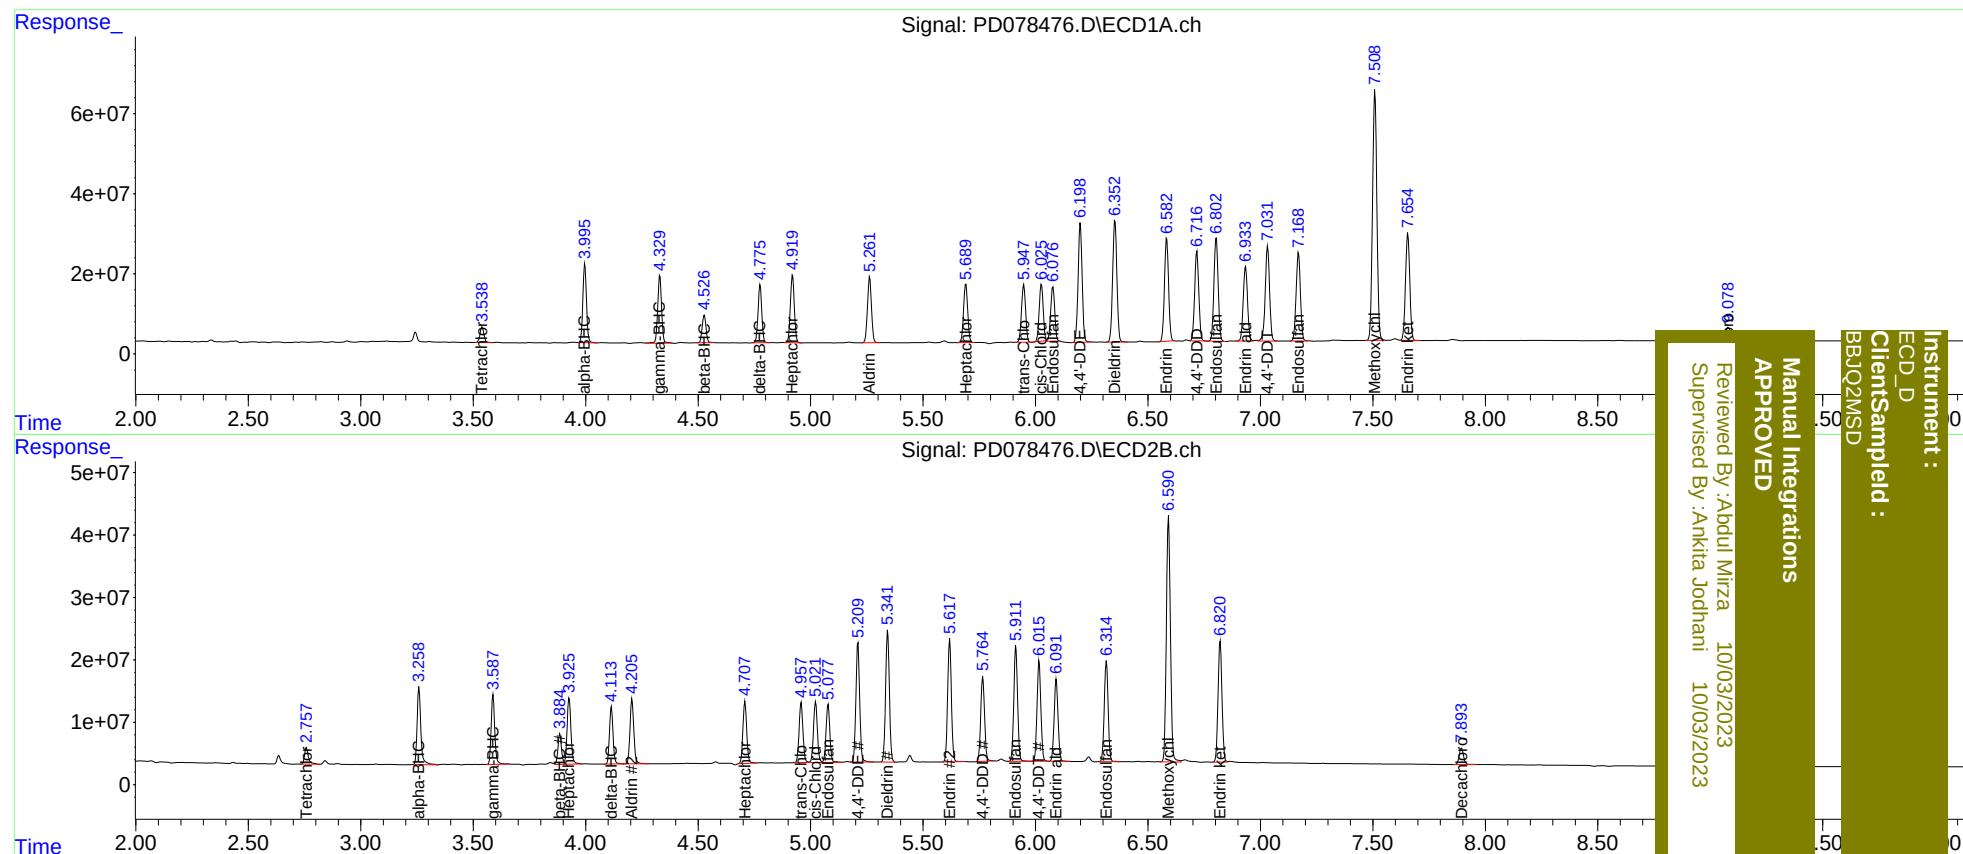

Instrument :
ECD_D
ClientSampled :
BBJQ2MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023