

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 17:15
 Operator : AR\AJ
 Sample : PB155923BS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS923

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2023
 Supervised By :Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 21:40:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.758	48305842	31573709	19.673	19.112
27)	SA Decachlor...	9.077	7.893	112.4E6	64207684	34.756	34.683
Target Compounds							
2)	A alpha-BHC	3.995	3.258	19272033	11834993	4.648	4.642
3)	MA gamma-BHC...	4.328	3.587	19398398	11025767	4.890	4.617
4)	MA Heptachlor	4.919	3.926	21504014	12708997	5.176	5.114
5)	MB Aldrin	5.261	4.205	21613069	14443818	5.316	5.888
6)	B beta-BHC	4.526	3.885	9251077	5483598	5.348	5.037
7)	B delta-BHC	4.773	4.114	14017138	6627748	3.517	2.696
8)	B Heptachlo...	5.688	4.707	20548708	11790310	5.547	5.109
9)	A Endosulfan I	6.074	5.077	17934766	10796637	5.380m	5.248
10)	B trans-Chl...	5.946	4.957	19182443	11679054	5.319	5.242
11)	B cis-Chlor...	6.025	5.021	18972770	12050915	5.114	5.247
12)	B 4,4'-DDE	6.198	5.210	37800592	23719829	10.564	11.021
13)	MA Dieldrin	6.351	5.342	38864071	23579041	10.446	9.982
14)	MA Endrin	6.582	5.617	31740001	22165494	10.559	10.595
15)	B Endosulfa...	6.802	5.912	35161725	21467256	11.243	10.574
16)	A 4,4'-DDD	6.716	5.764	27572650	16763666	10.654	10.638
17)	MA 4,4'-DDT	7.031	6.015	26993436	15466328	10.451	9.507
18)	B Endrin al...	6.933	6.092	26617682	16528074	10.954	10.661
19)	B Endosulfa...	7.168	6.314	28523508	17677068	9.988	9.497
20)	A Methoxychlor	7.508	6.591	82439745	49677295	55.866	56.005
21)	B Endrin ke...	7.655	6.821	35461326	22751826	11.152	10.591

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 17:15
Operator : AR\AJ
Sample : PB155923BS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 21:40:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

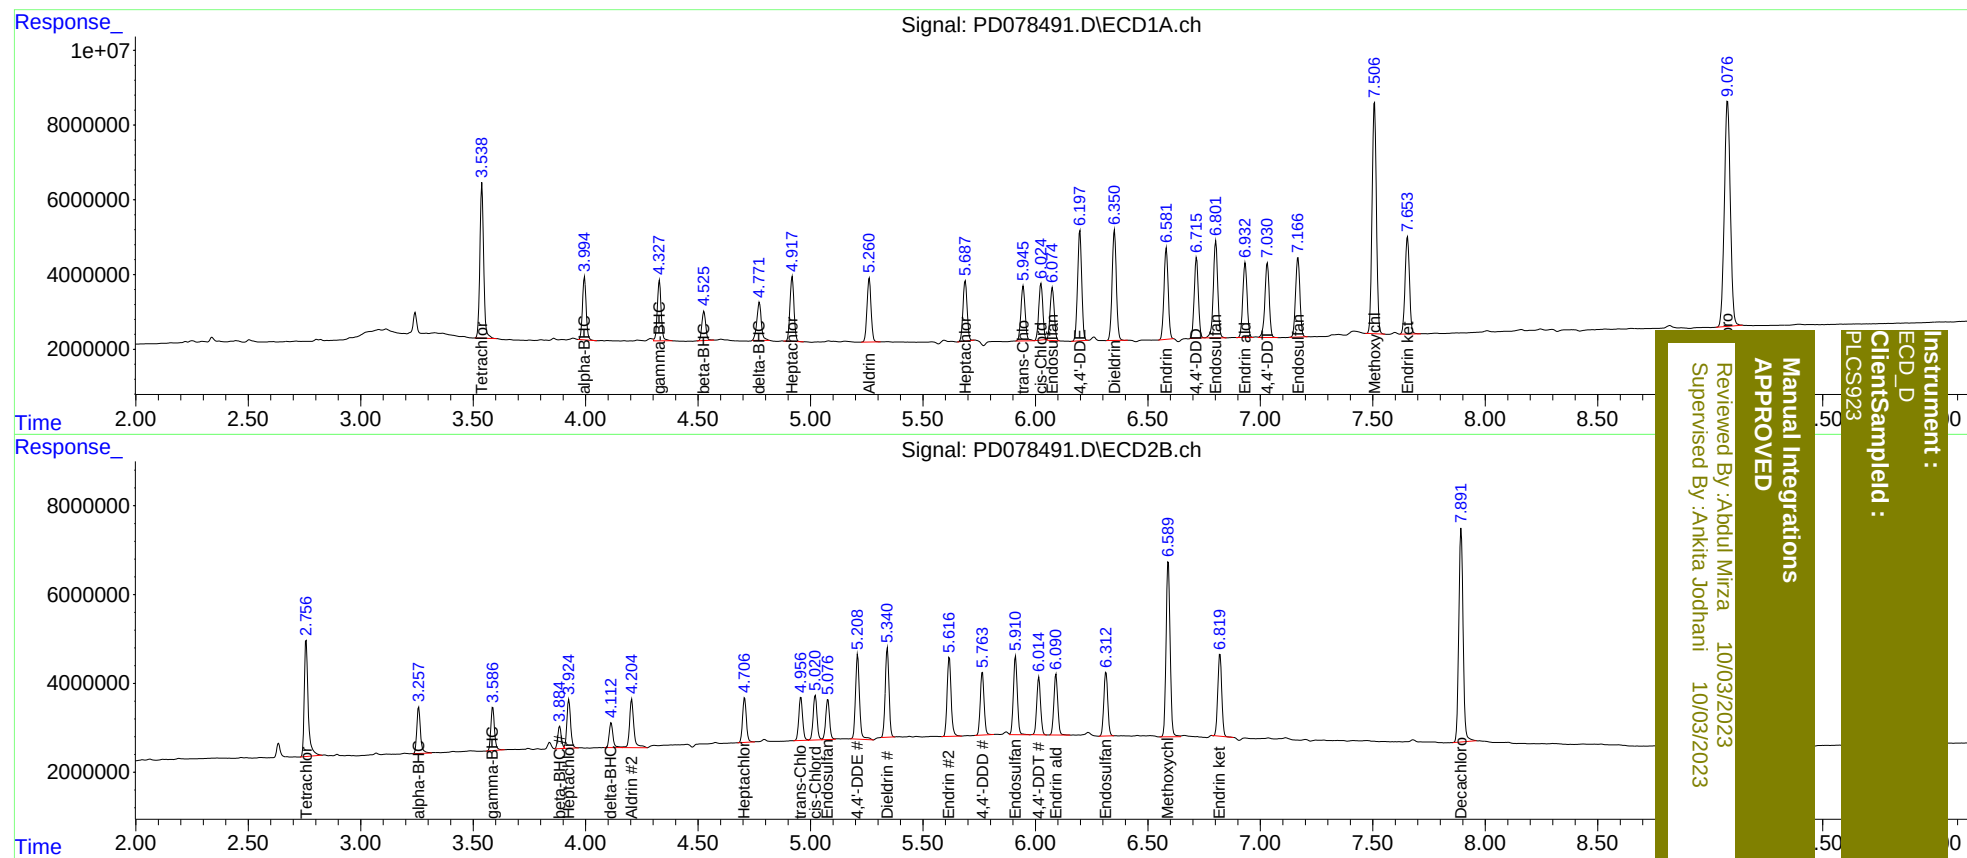

Instrument :
ECD_D
ClientSampled :
PLCS923

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/03/2023
Supervised By: Ankita Jodhani 10/03/2023