

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
 Data File : PD078505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 20:22
 Operator : AR\AJ
 Sample : 04527-13
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYY6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/03/2023
 Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 22:46:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 28 13:47:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.758	26452881	22021141	10.773	13.330
27)	SA Decachlor...	9.076	7.893	45942648	25158073	14.212	13.589
Target Compounds							
5)	MB Aldrin	5.256	4.216	10590580	6403452	2.605	2.610
12)	B 4,4'-DDE	6.197	5.208	17490091	11794262	4.888	5.480m
19)	B Endosulfa...	7.161	6.333	7468474	5984846	2.615	3.215

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092923\
Data File : PD078505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 20:22
Operator : AR\AJ
Sample : 04527-13
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 22:46:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092823CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 28 13:47:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

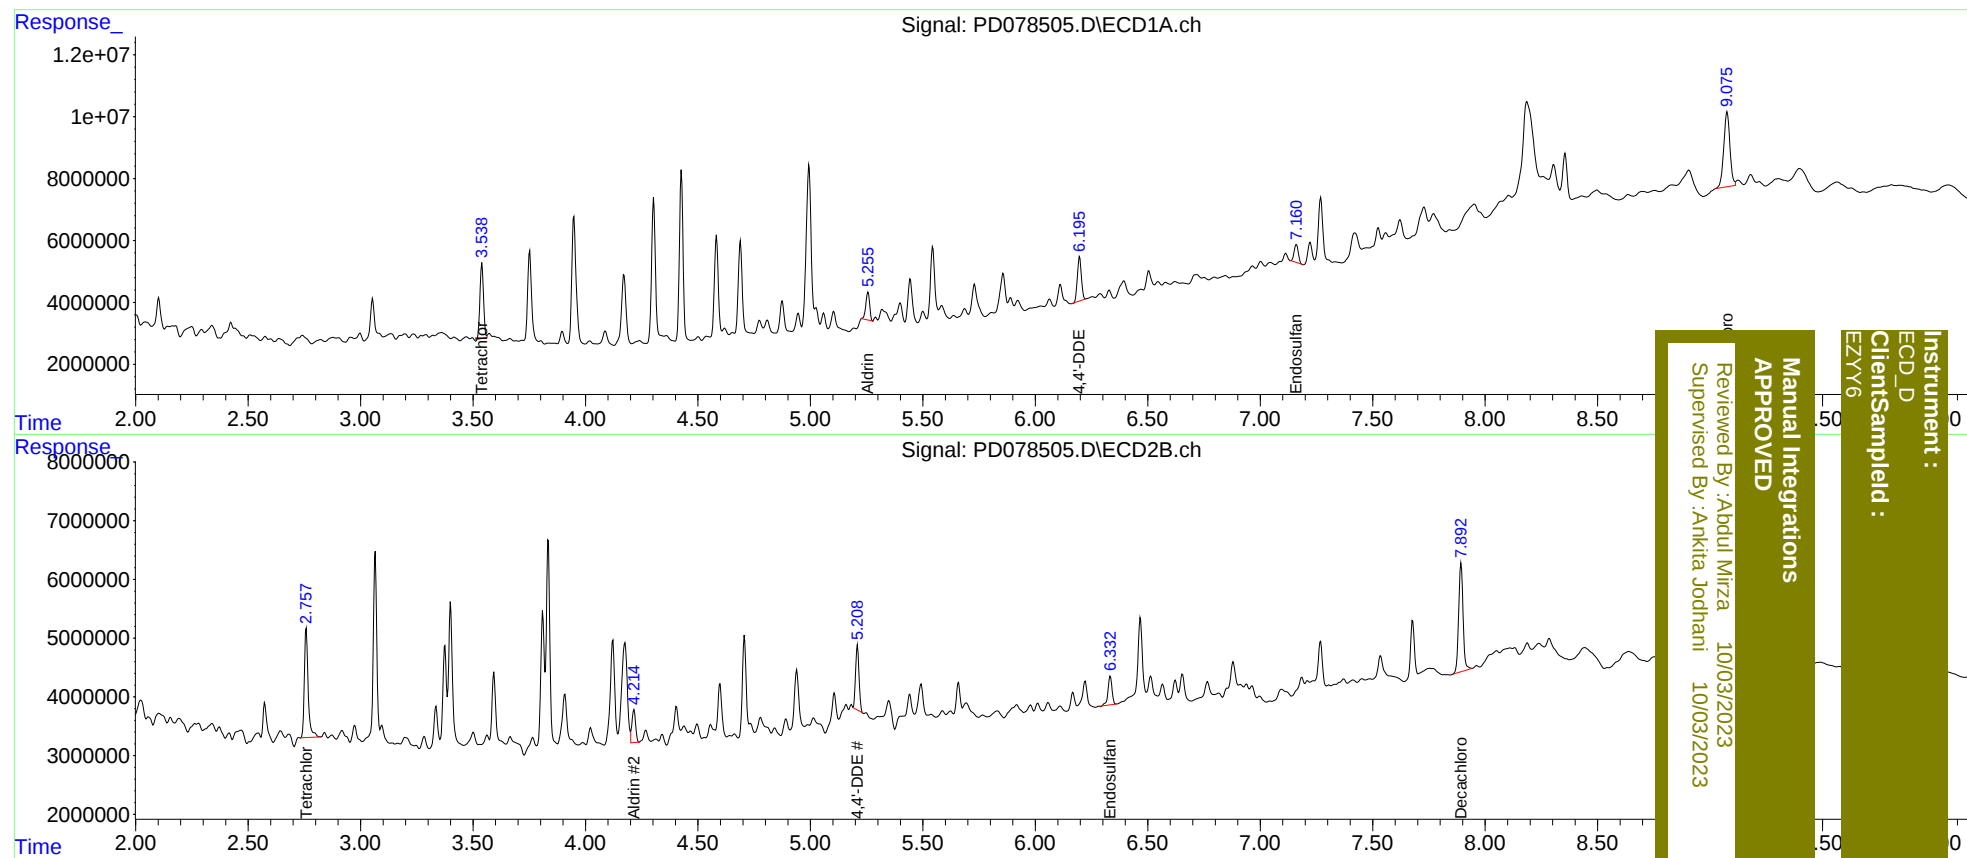

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/03/2023
Supervised By: Ankita Jodhani 10/03/2023

Instrument :
ECD_D
ClientSampled :
EZY6