

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092925\
 Data File : PD090442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 22:25
 Operator : AR\AJ
 Sample : Q3208-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-ESM-COMP-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/30/2025
 Supervised By : mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 02:35:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:52:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.874	45910491	389.0E6	14.124m	14.170m
28) SA Decachlor...	9.063	8.061	62607535	409.8E6	12.976	12.643

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD092925\
Data File : PD090442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 22:25
Operator : AR\AJ
Sample : Q3208-06
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SU-ESM-COMP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/30/2025
Supervised By : mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 02:35:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:52:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

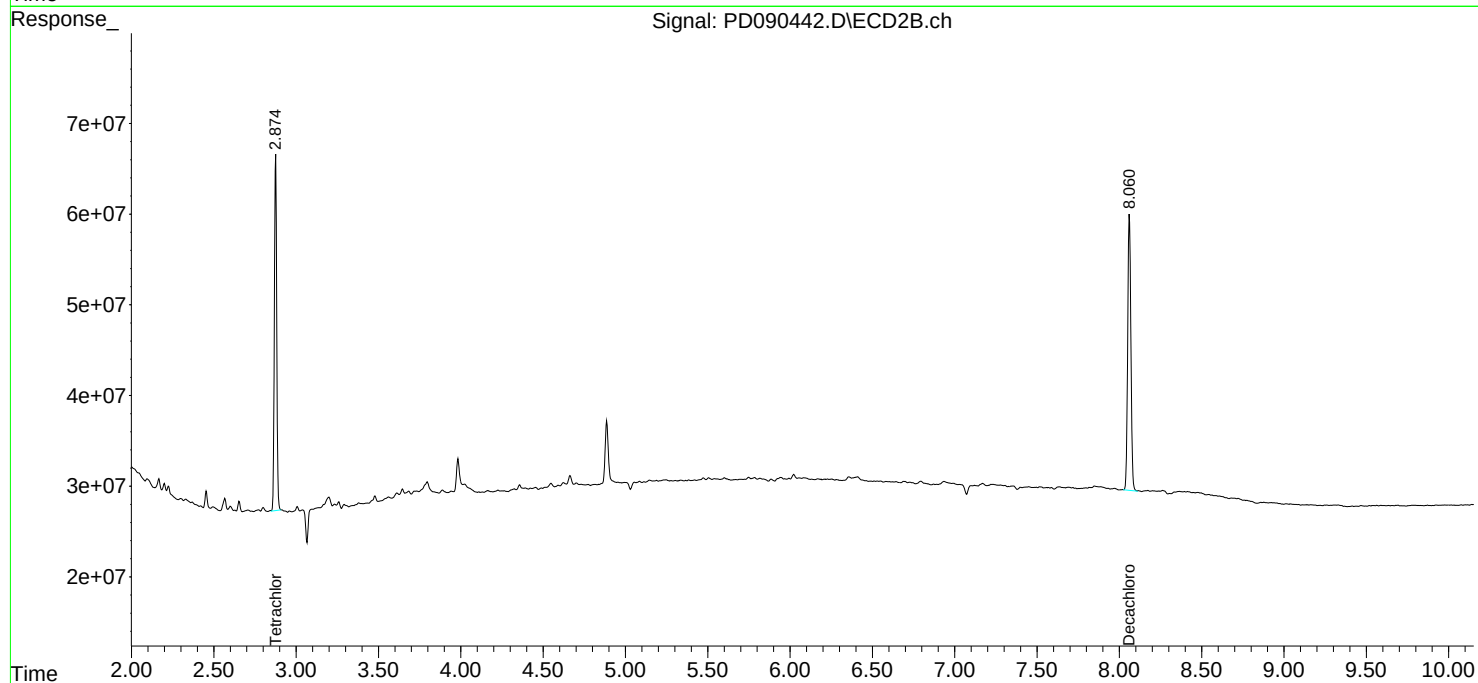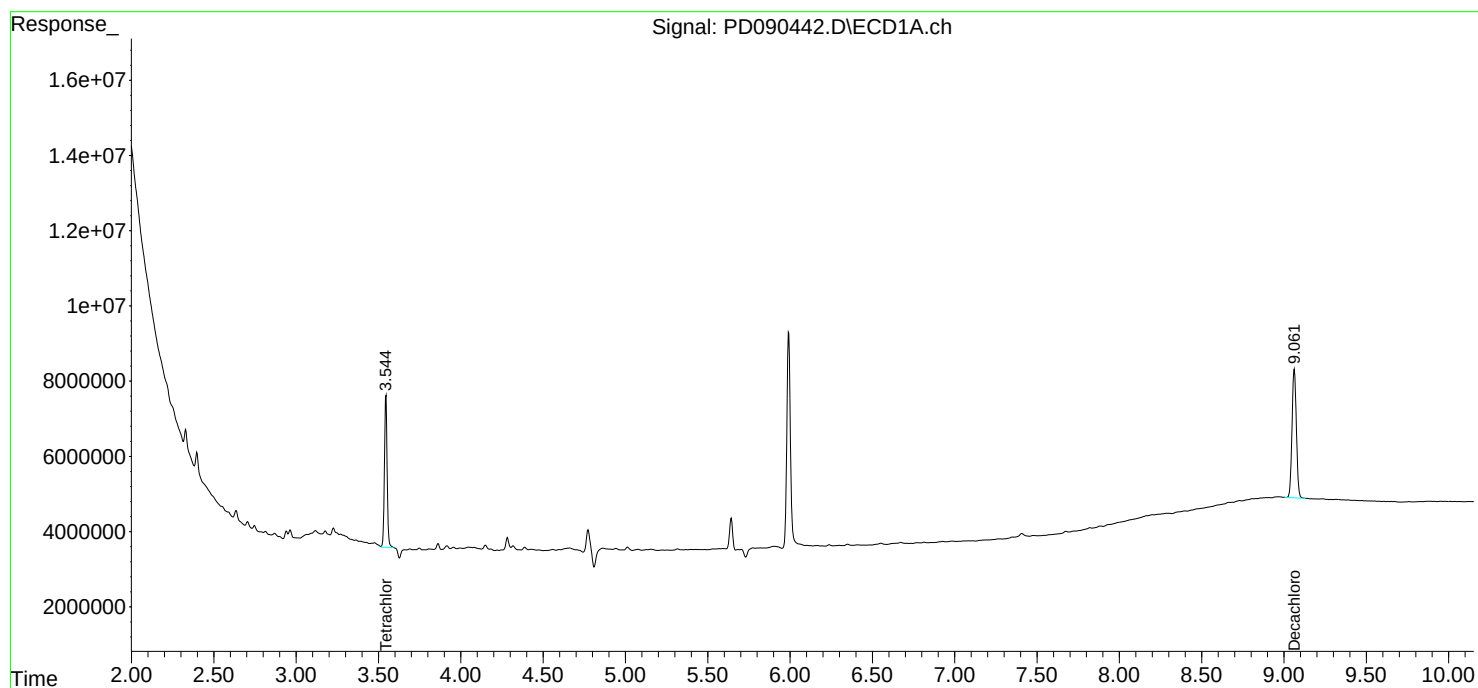

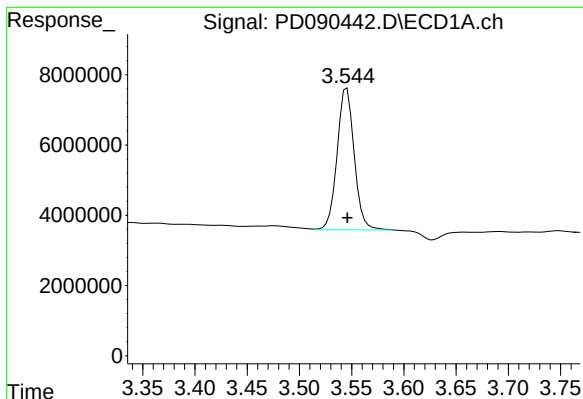


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.002 min
Response: 45910491
Conc: 14.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-ESM-COMP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

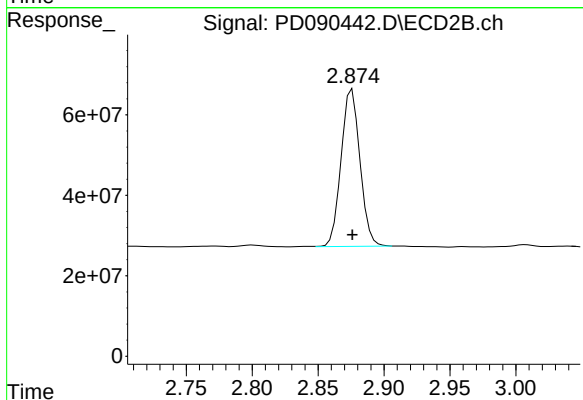


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: -0.001 min
Response: 388969186
Conc: 14.17 ng/ml m

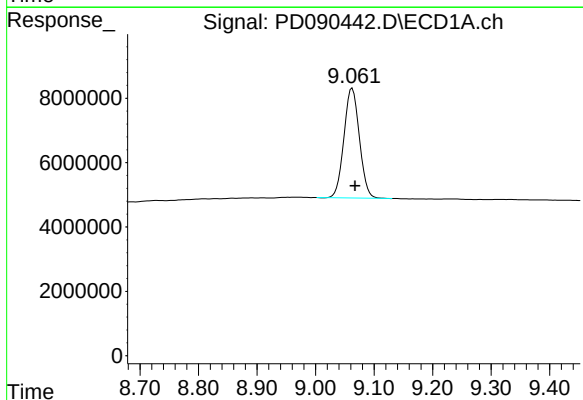

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: -0.005 min
Response: 62607535
Conc: 12.98 ng/ml

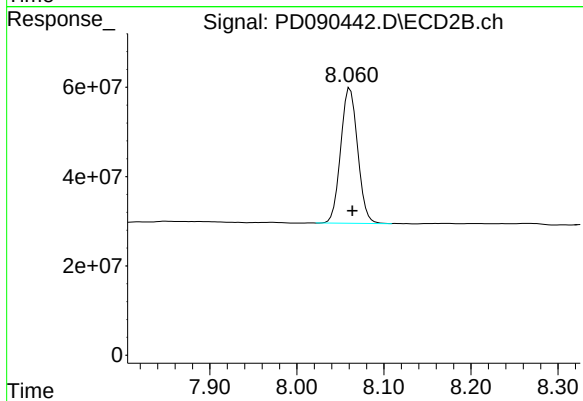

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: -0.003 min
Response: 409804971
Conc: 12.64 ng/ml