

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 09:00
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 07:50:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.961	17096080	24955363	21.805	21.801
28)	SA Decachlor...	7.970	8.995	29420161	42377607	34.104	34.792
Target Compounds							
9)	A Endosulfan I	0.000	6.162f	0	4007449	N.D.	2.932 #
19)	B Endosulfa...	6.432	0.000	2802012	0	3.461	N.D. #
26)	Chlordane-4	0.000	6.162f	0	4007449	N.D.	16.724 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 09:00
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 07:50:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

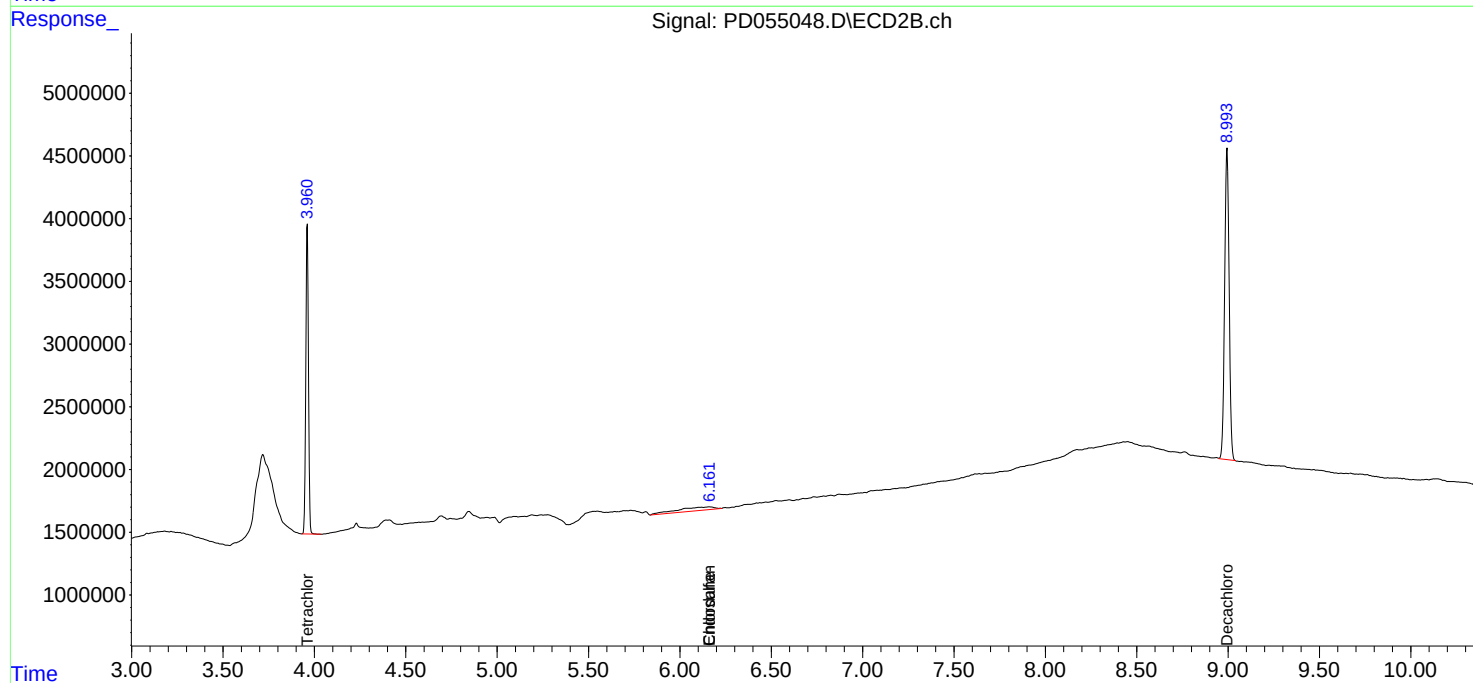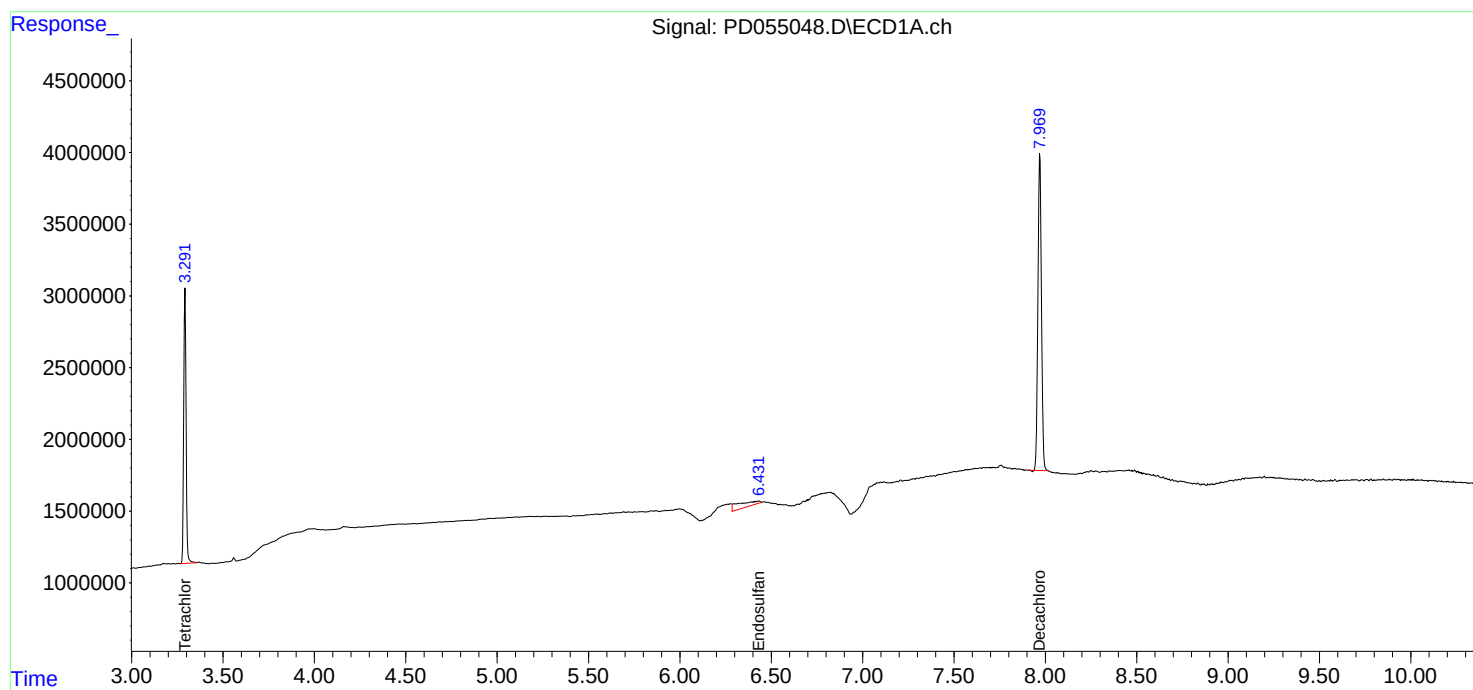

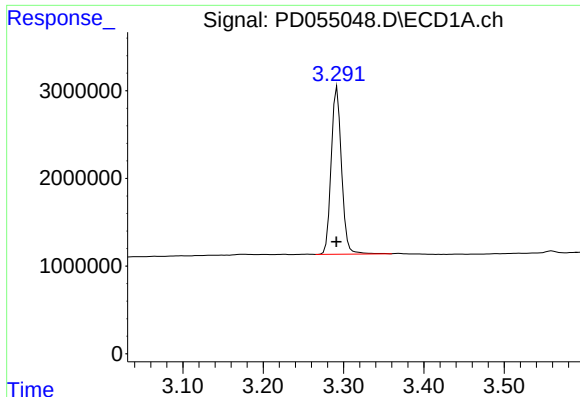


#1 Tetrachloro-m-xylene

R.T.: 3.292 min
Delta R.T.: 0.001 min
Response: 17096080
Conc: 21.81 ng/ml

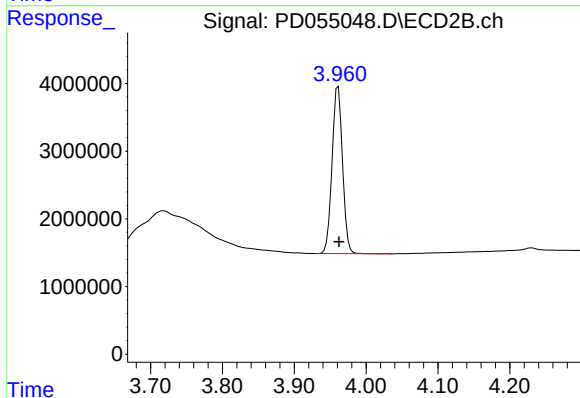


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 24955363
Conc: 21.80 ng/ml

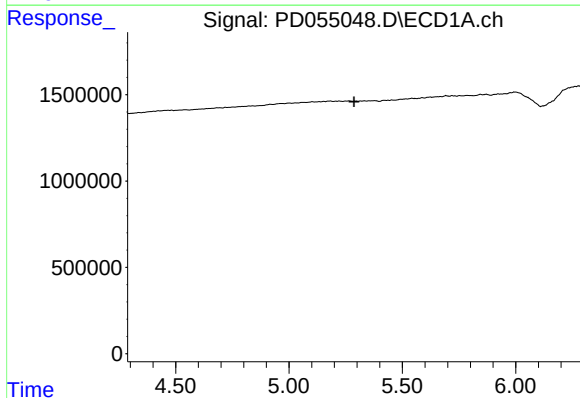


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.287 min
Response: 0
Conc: N.D.

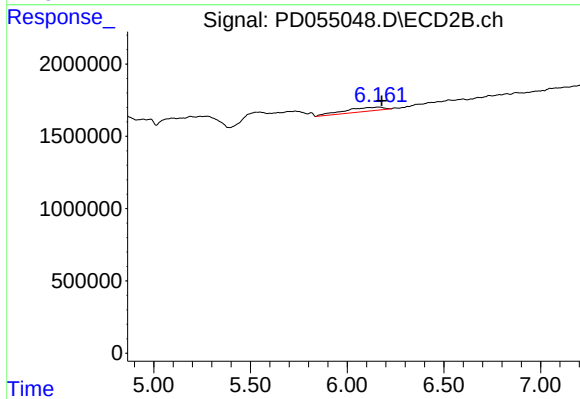


#9 Endosulfan I

R.T.: 6.162 min
Delta R.T.: -0.018 min
Response: 4007449
Conc: 2.93 ng/ml

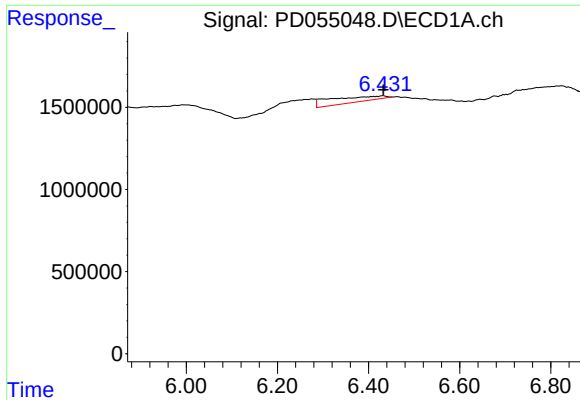


#19 Endosulfan Sulfate

R.T.: 6.432 min
Delta R.T.: 0.000 min
Response: 2802012
Conc: 3.46 ng/ml

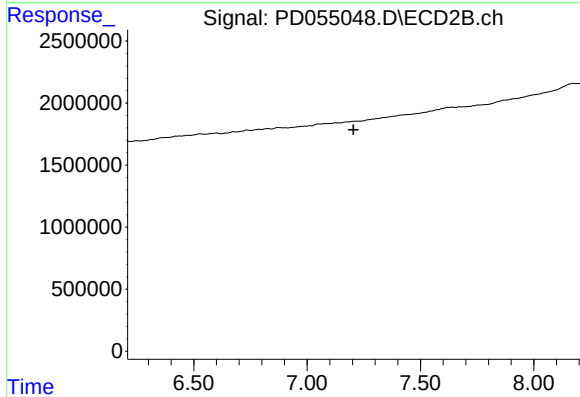


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.205 min
Response: 0
Conc: N.D.

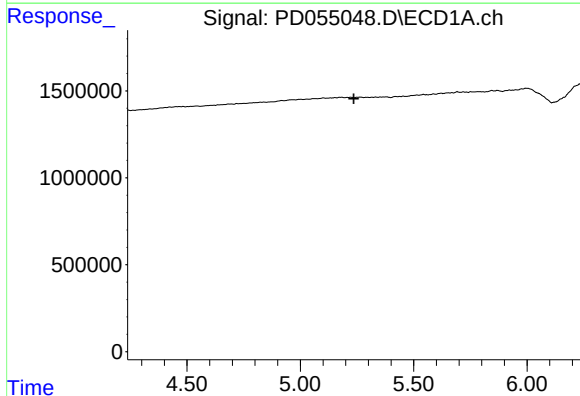


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.236 min
Response: 0
Conc: N.D.

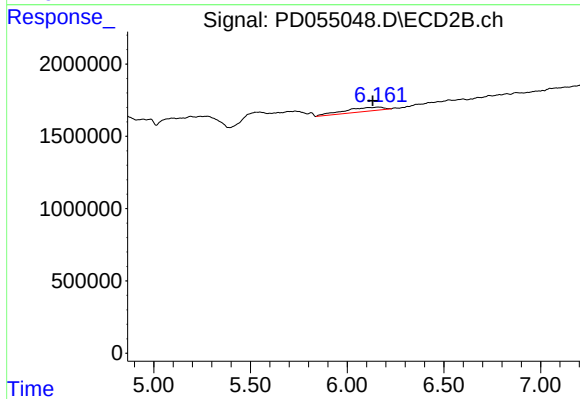


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.030 min
Response: 4007449
Conc: 16.72 ng/ml

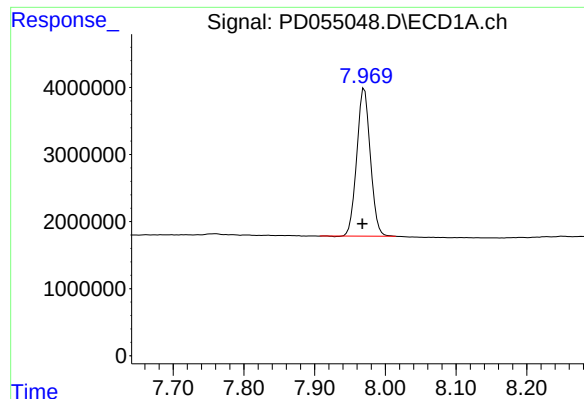

#28 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: 0.003 min
Response: 29420161
Conc: 34.10 ng/ml

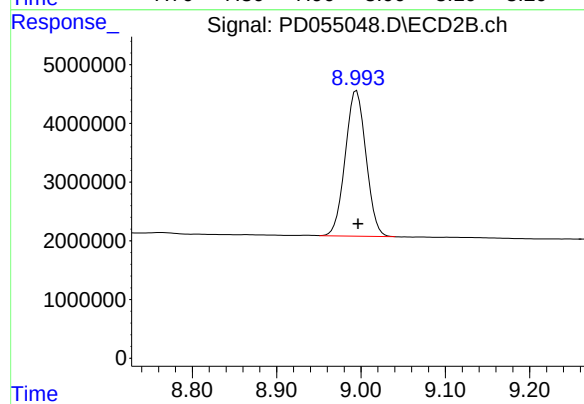

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.002 min
Response: 42377607
Conc: 34.79 ng/ml