

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 20:03
 Operator : SG\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 05:48:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 05:46:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	85292897	111.3E6	101.944	100.258
28)	SA Decachlor...	7.969	8.995	80998691	109.8E6	95.300	95.294
Target Compounds							
23)	Chlordane-1	4.133	4.950	25313893	42788280	1038.003	992.231
24)	Chlordane-2	4.624	5.415	29424387	47036405	964.644	1002.651
25)	Chlordane-3	5.179	6.058	91673557	197.7E6	1003.515	1024.948
26)	Chlordane-4	5.235	6.132	80676867	235.5E6	1007.913	1022.083
27)	Chlordane-5	6.059	6.932	28805283	41960813	974.667	996.773



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 20:03
Operator : SG\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 05:48:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 05:46:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

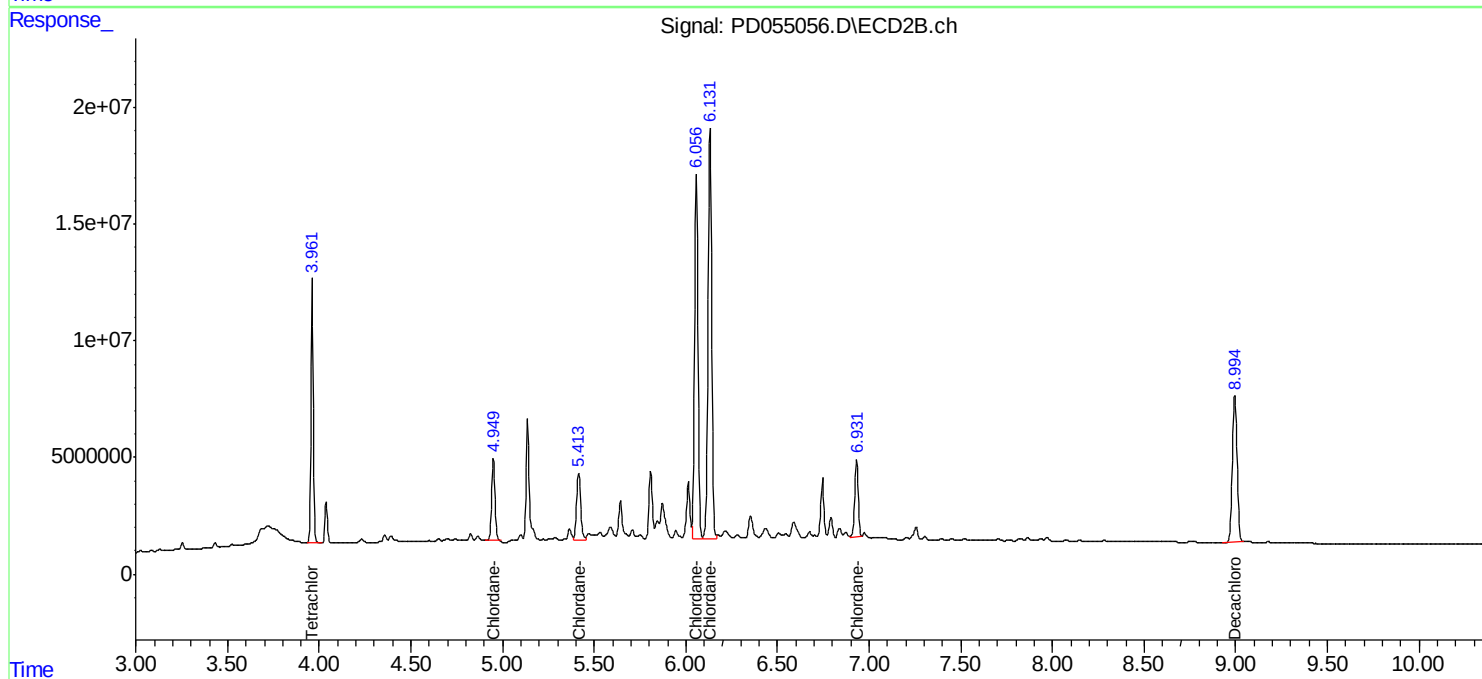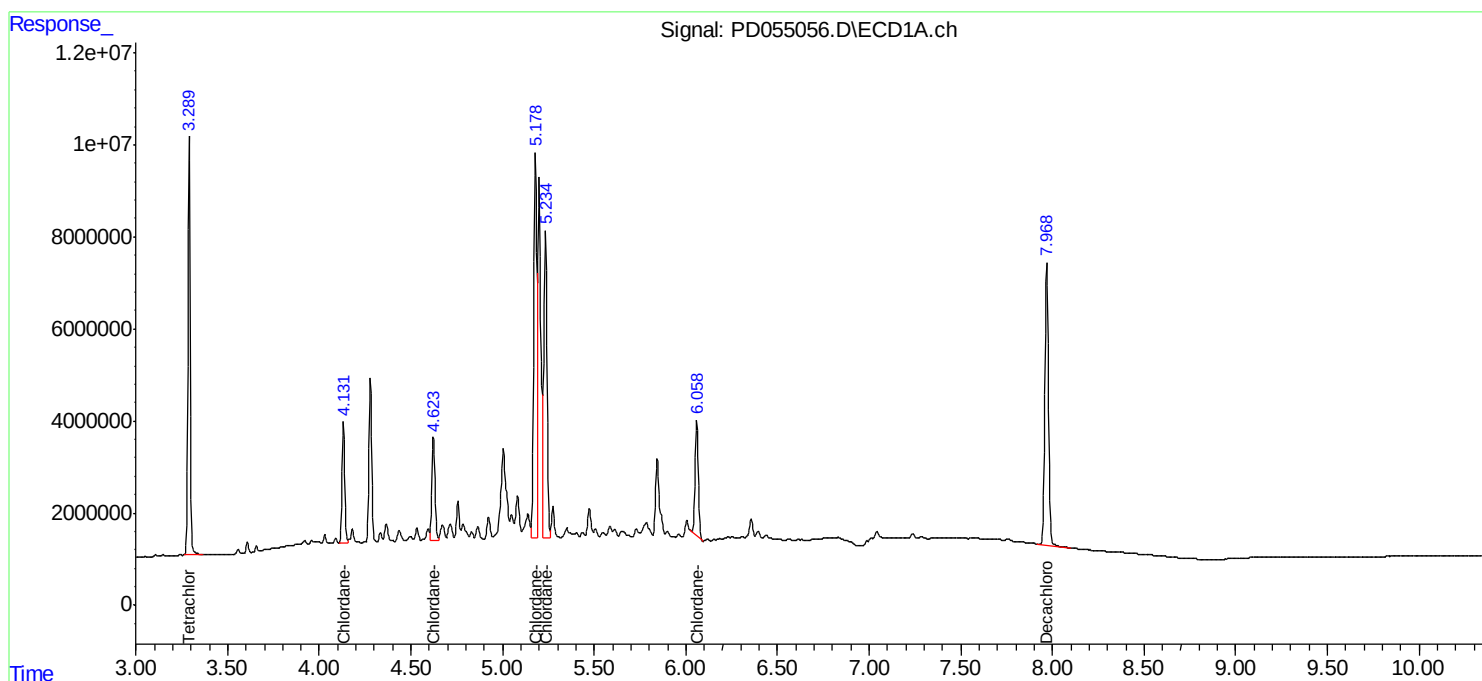


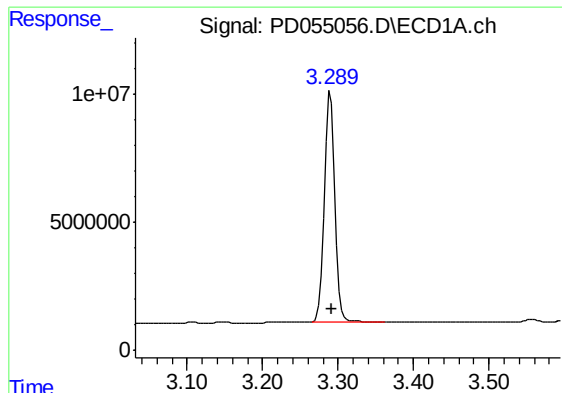

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 85292897
Conc: 101.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

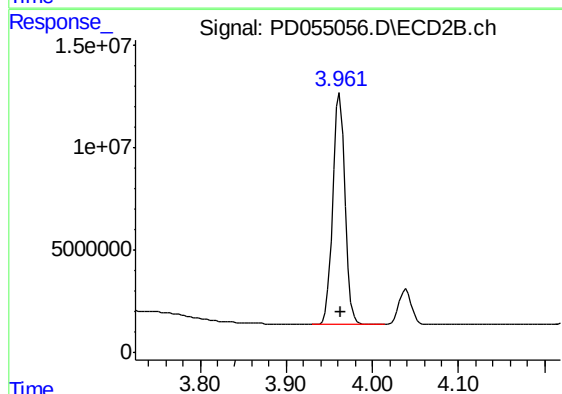


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 111272908
Conc: 100.26 ng/ml

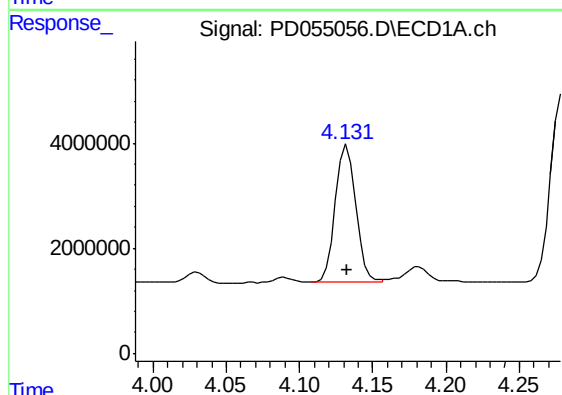


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 25313893
Conc: 1038.00 ng/ml

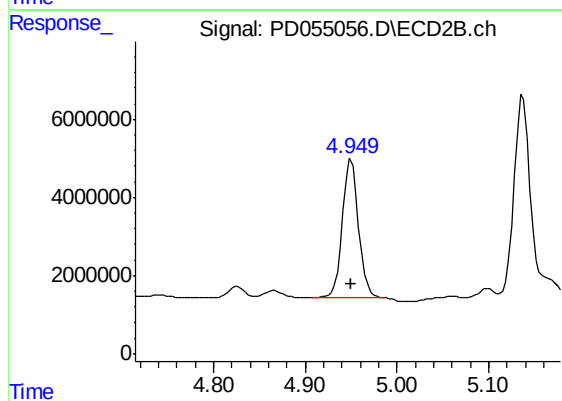

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 42788280
Conc: 992.23 ng/ml

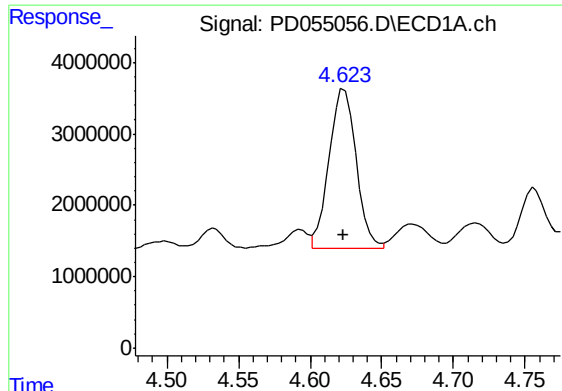

#24 Chlordane-2


R.T.: 4.624 min
Delta R.T.: 0.000 min
Response: 29424387
Conc: 964.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

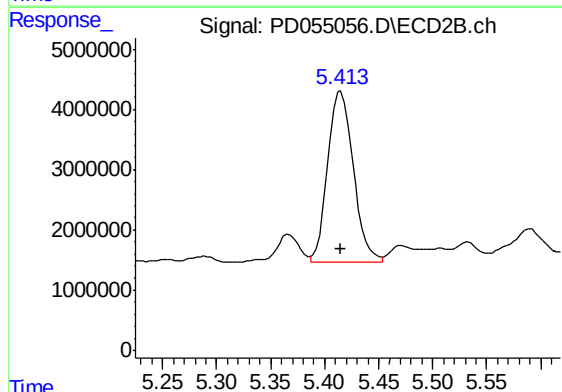


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 47036405
Conc: 1002.65 ng/ml

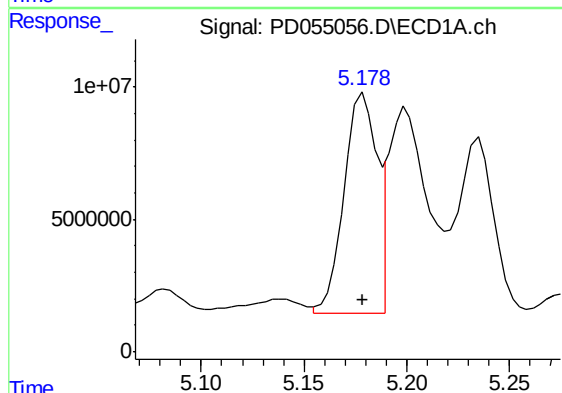


#25 Chlordane-3

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 91673557
Conc: 1003.51 ng/ml

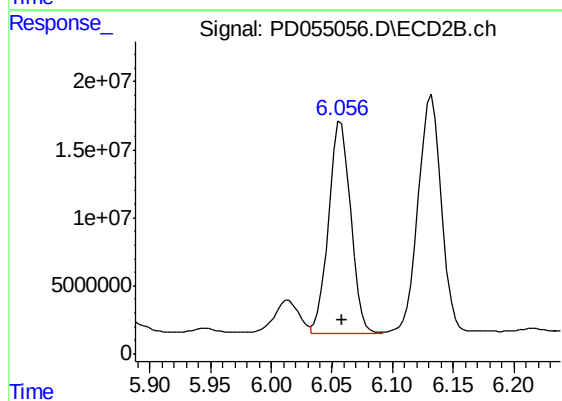

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 197688673
Conc: 1024.95 ng/ml

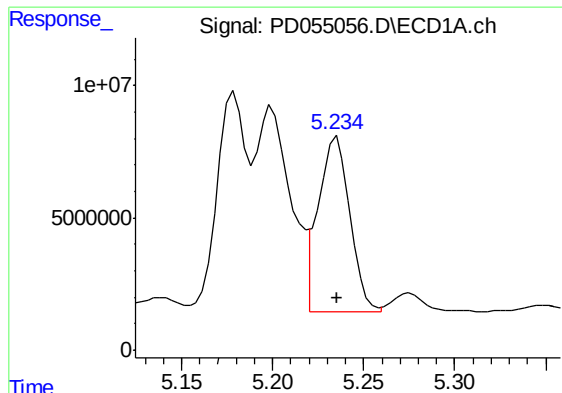

#26 Chlordane-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 80676867
Conc: 1007.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

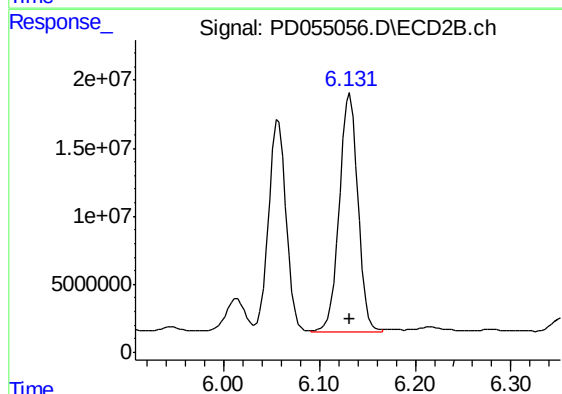


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 235520216
Conc: 1022.08 ng/ml

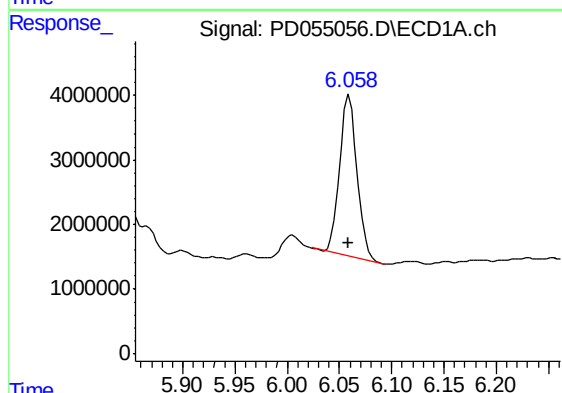


#27 Chlordane-5

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 28805283
Conc: 974.67 ng/ml

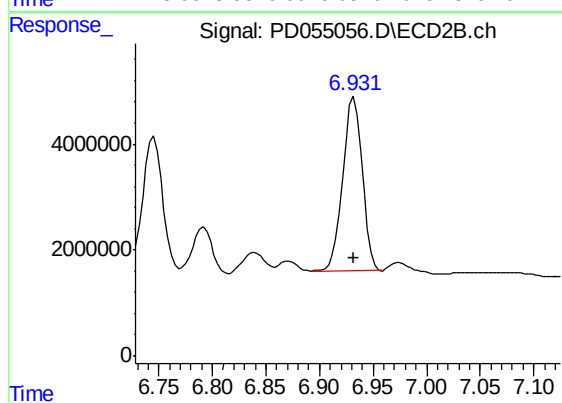

#27 Chlordane-5


R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 41960813
Conc: 996.77 ng/ml

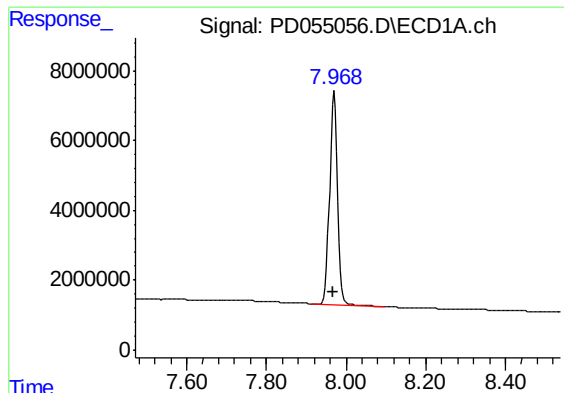

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 80998691
Conc: 95.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

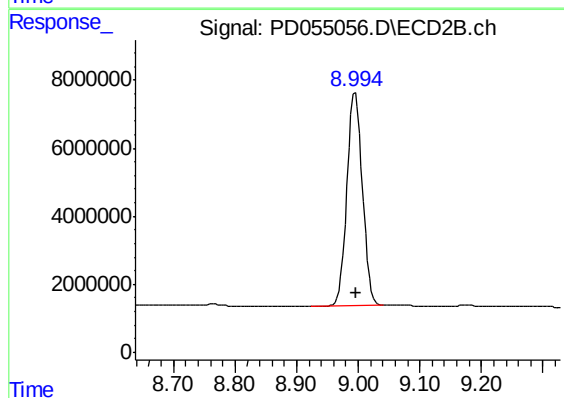

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.002 min
Response: 109761372
Conc: 95.29 ng/ml