

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 20:17
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 05:48:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 05:46:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	61919700	81561800	74.008	73.488
28)	SA Decachlor...	7.969	8.997	60408200	81907745	71.074	71.112
Target Compounds							
23)	Chlordane-1	4.133	4.950	18445109	31584813	756.347	732.430
24)	Chlordane-2	4.624	5.415	21944790	34526239	719.434	735.978
25)	Chlordane-3	5.179	6.058	67155754	143.5E6	735.128	744.027
26)	Chlordane-4	5.235	6.132	58290028	172.0E6	728.229	746.641
27)	Chlordane-5	6.059	6.933	21215891	30557560	717.870	725.890



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 20:17
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 05:48:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 05:46:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

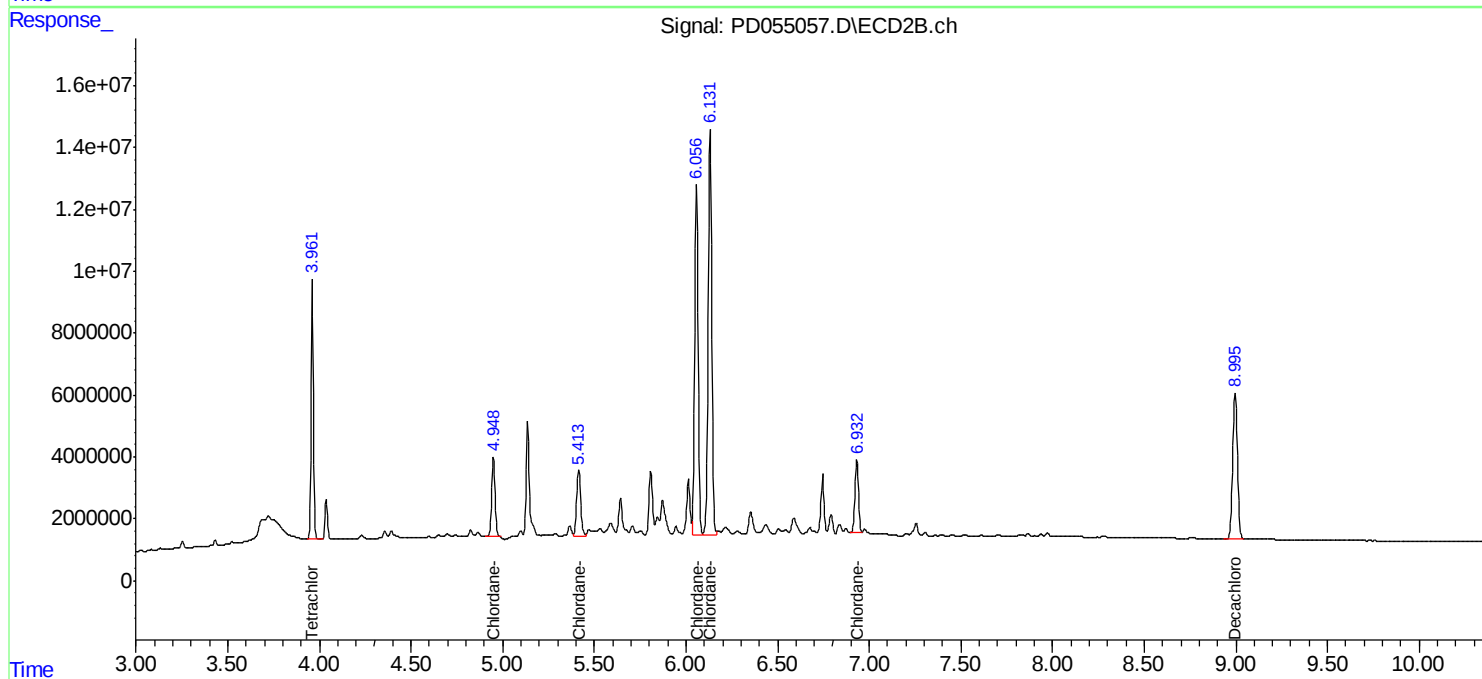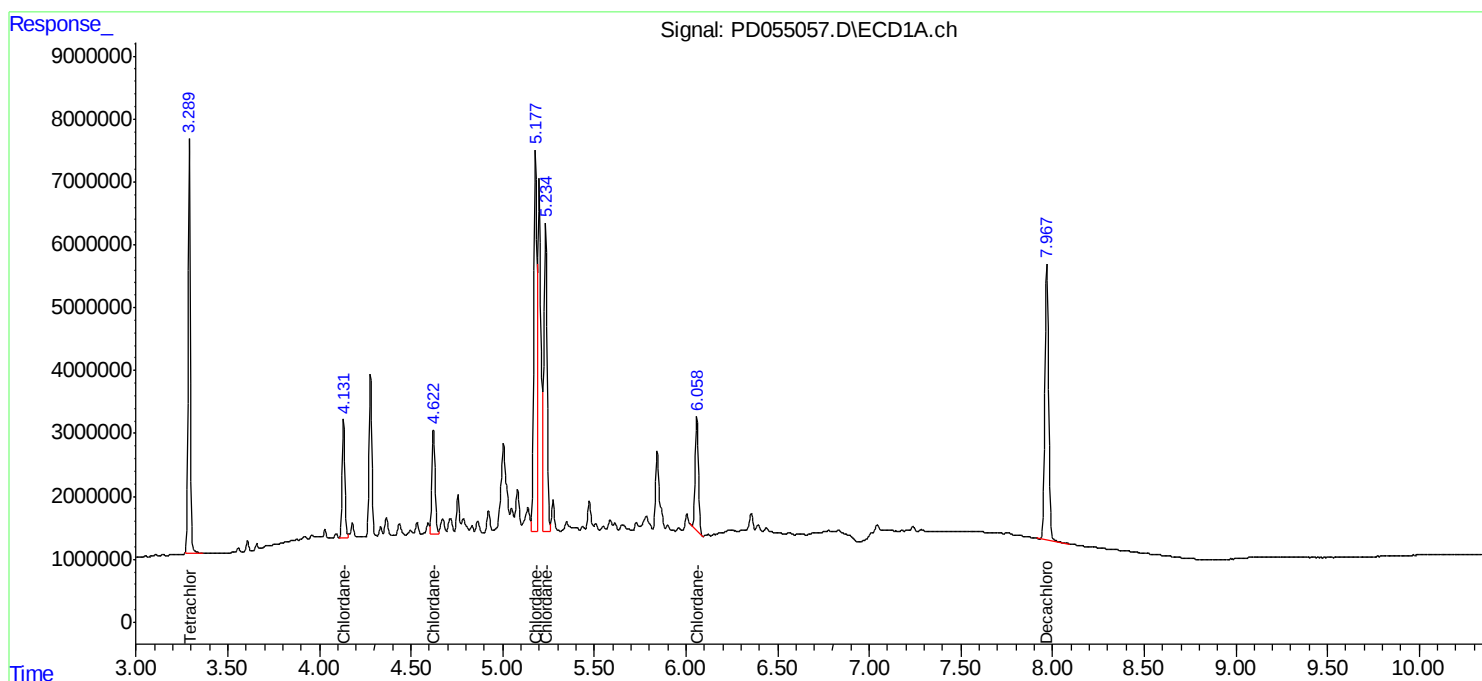


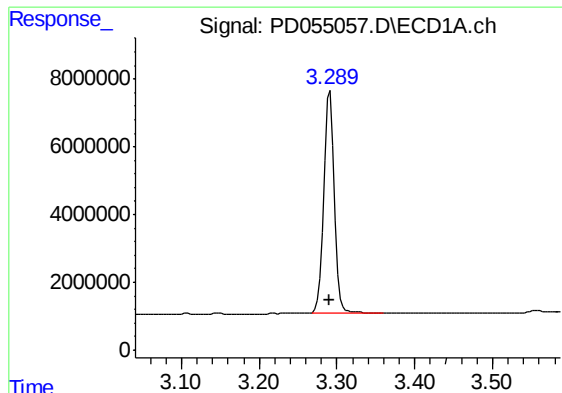

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 61919700
Conc: 74.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

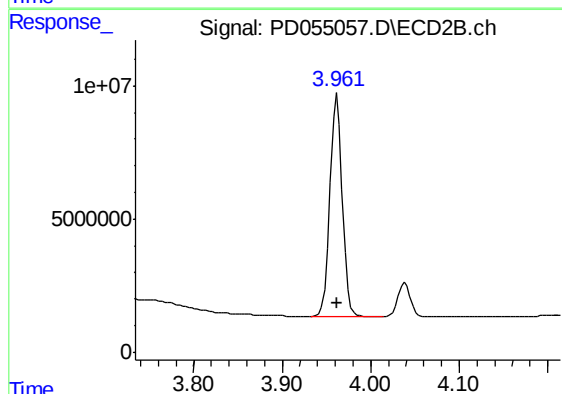


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 81561800
Conc: 73.49 ng/ml

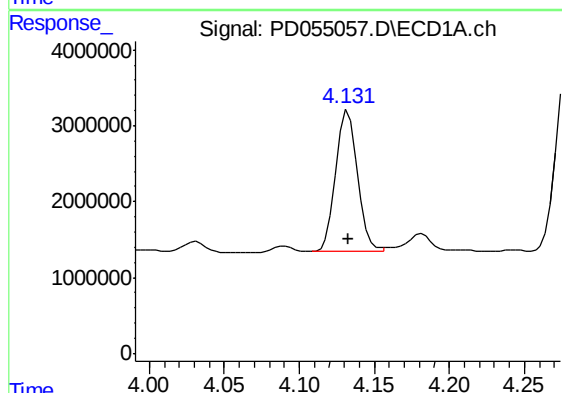


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 18445109
Conc: 756.35 ng/ml

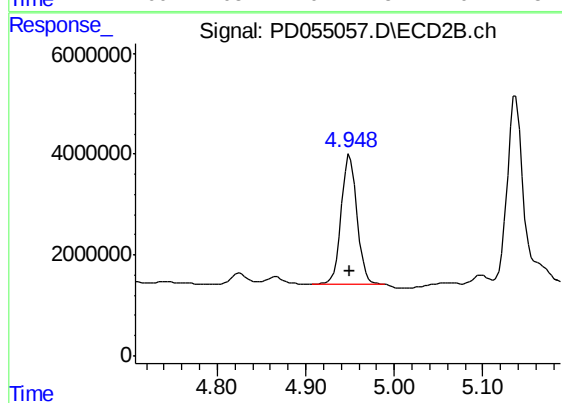

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 31584813
Conc: 732.43 ng/ml

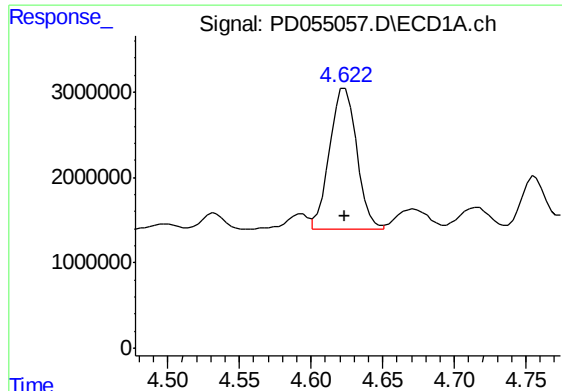

#24 Chlordane-2


R.T.: 4.624 min
Delta R.T.: 0.000 min
Response: 21944790
Conc: 719.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

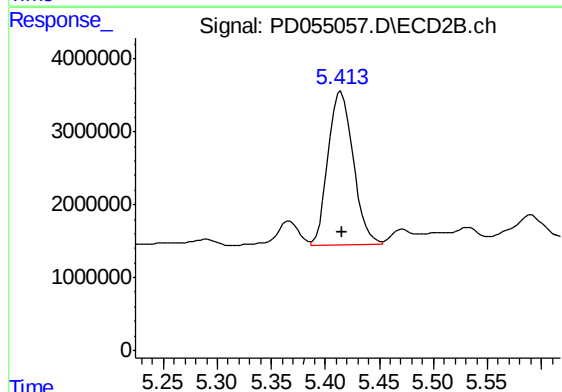


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 34526239
Conc: 735.98 ng/ml

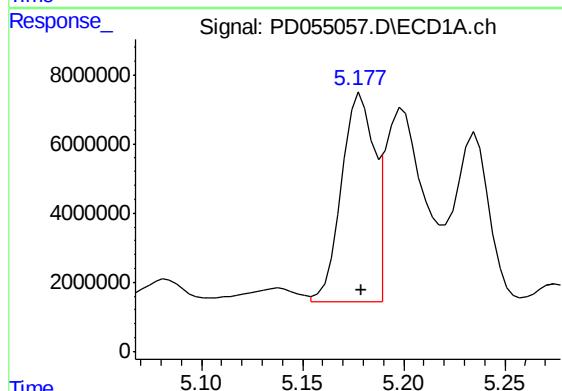


#25 Chlordane-3

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 67155754
Conc: 735.13 ng/ml

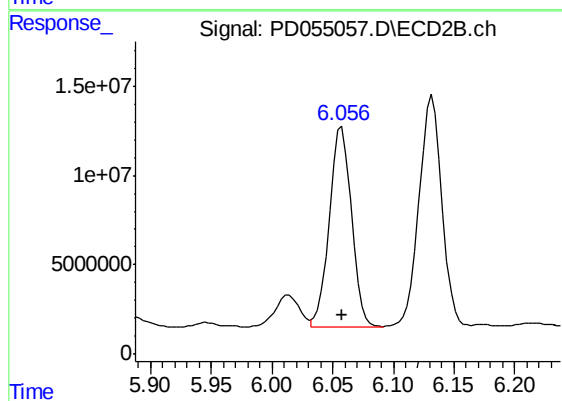

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 143505585
Conc: 744.03 ng/ml

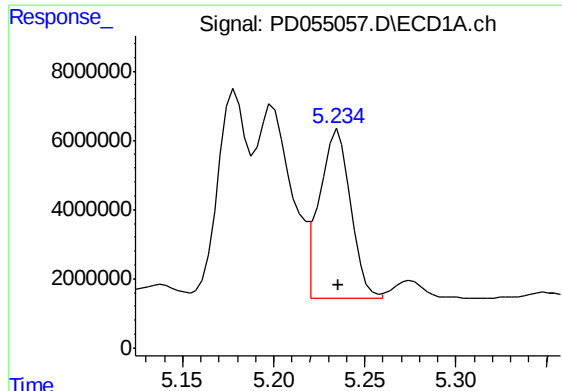

#26 Chlordane-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 58290028
Conc: 728.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

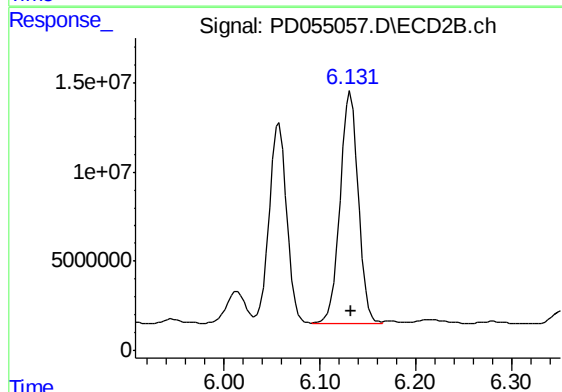


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 172049552
Conc: 746.64 ng/ml

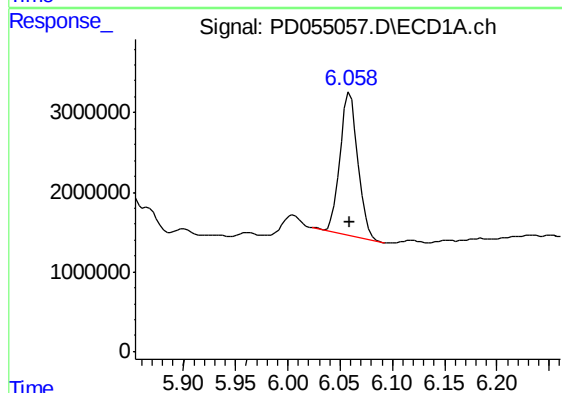


#27 Chlordane-5

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 21215891
Conc: 717.87 ng/ml

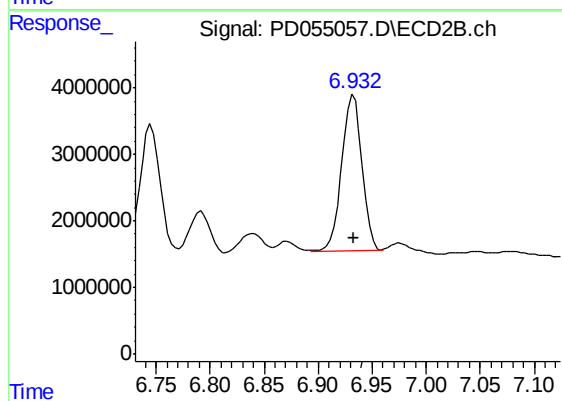

#27 Chlordane-5


R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 30557560
Conc: 725.89 ng/ml

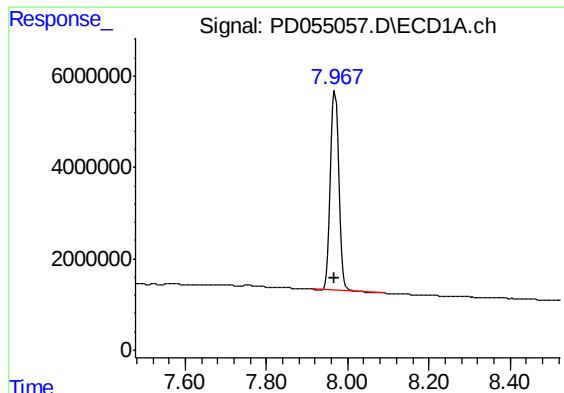

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 60408200
Conc: 71.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

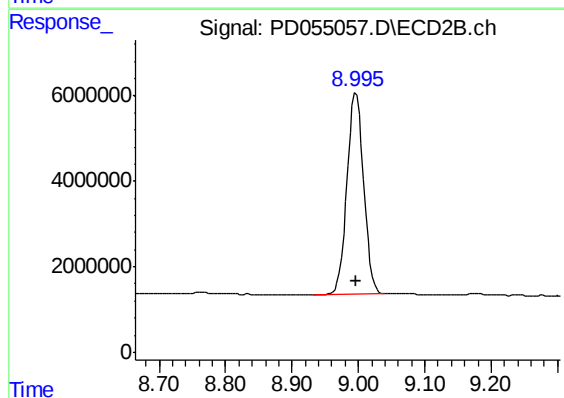

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 81907745
Conc: 71.11 ng/ml