

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 20:31
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 05:48:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 05:46:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.963	41833073	55493081	50.000	50.000
28)	SA Decachlor...	7.969	8.997	42496690	57590646	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.133	4.950	12193557	21561662	500.000	500.000
24)	Chlordane-2	4.623	5.415	15251425	23456023	500.000	500.000
25)	Chlordane-3	5.179	6.058	45676237	96438434	500.000	500.000
26)	Chlordane-4	5.236	6.132	40021758	115.2E6	500.000	500.000
27)	Chlordane-5	6.059	6.932	14776980	21048340	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 20:31
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 05:48:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 05:46:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

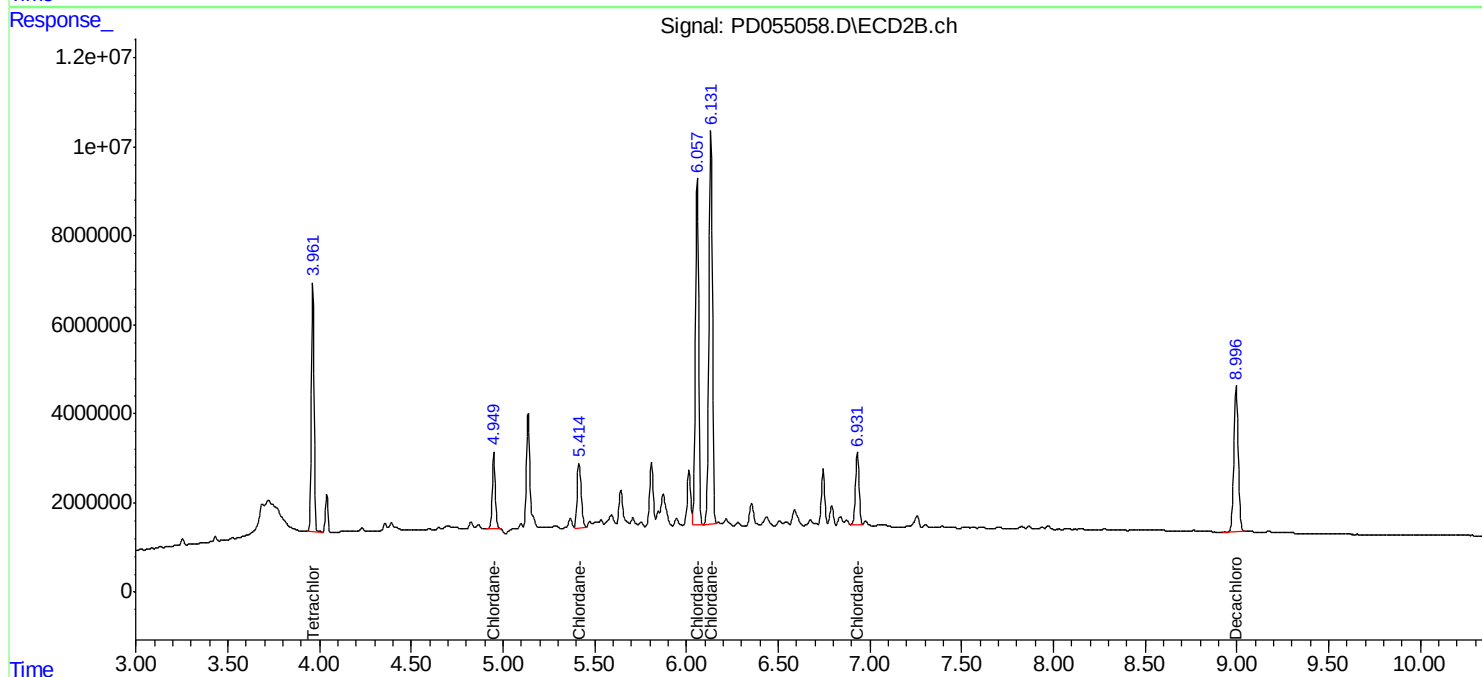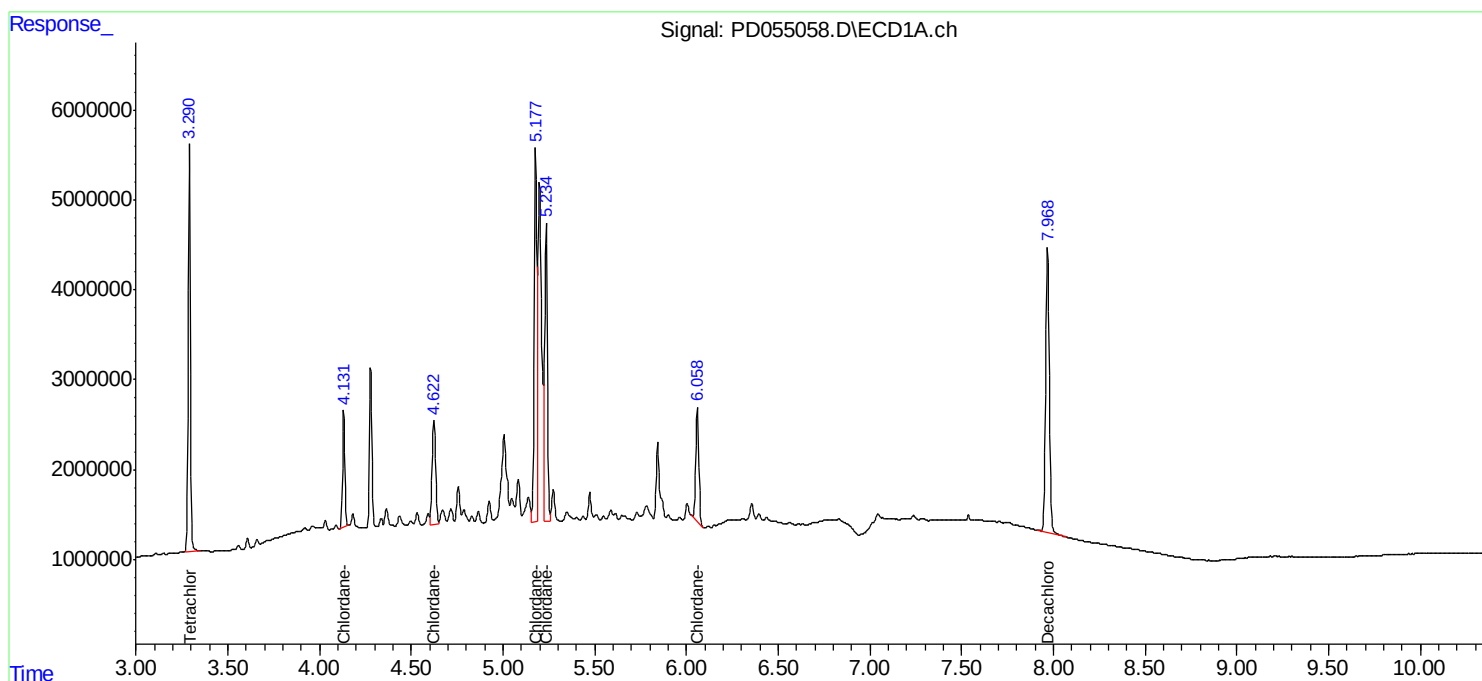


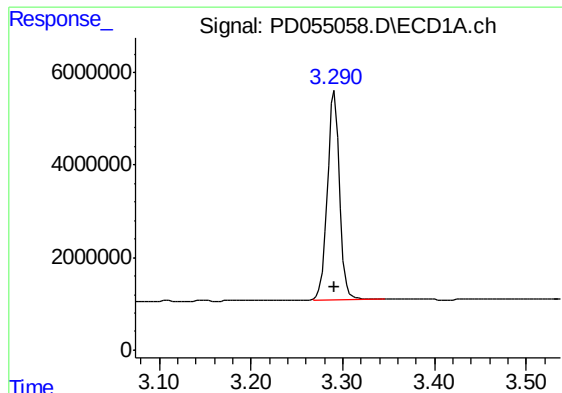

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 41833073
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

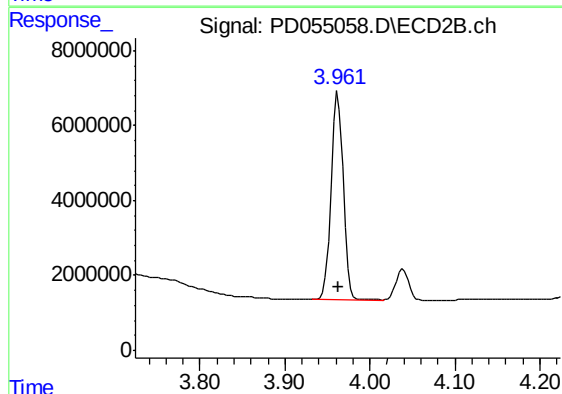


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 55493081
Conc: 50.00 ng/ml

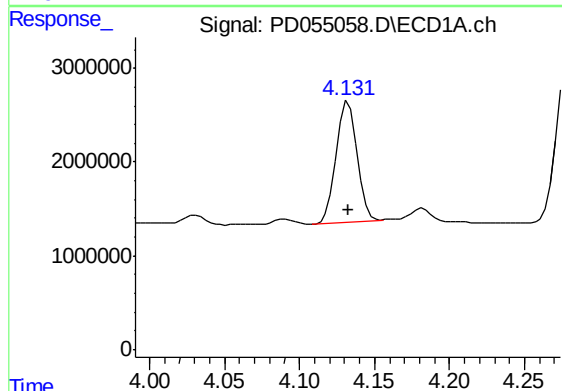


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 12193557
Conc: 500.00 ng/ml

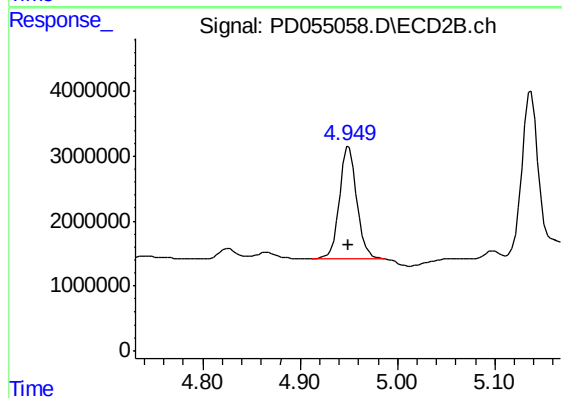

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 21561662
Conc: 500.00 ng/ml

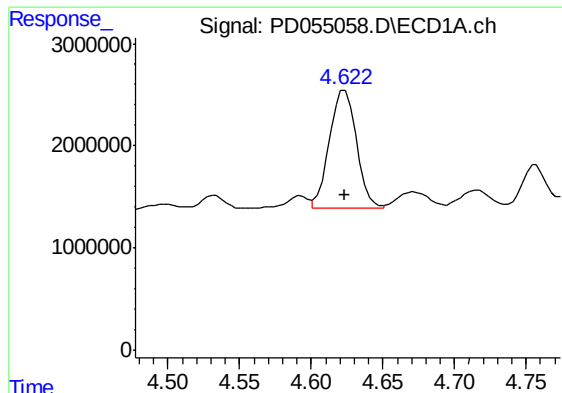

#24 Chlordane-2


R.T.: 4.623 min
Delta R.T.: 0.000 min
Response: 15251425
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

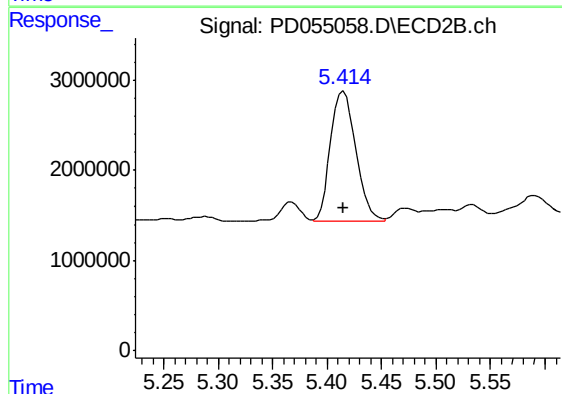


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 23456023
Conc: 500.00 ng/ml

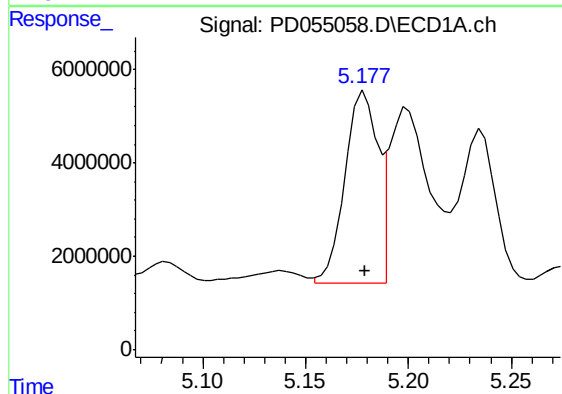


#25 Chlordane-3

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 45676237
Conc: 500.00 ng/ml

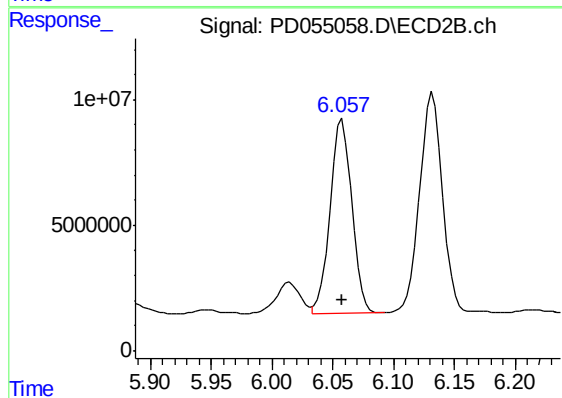

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 96438434
Conc: 500.00 ng/ml

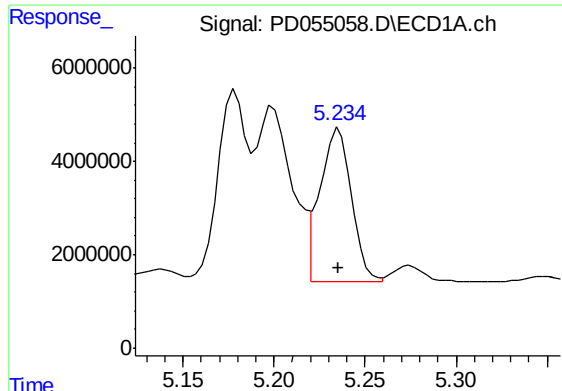

#26 Chlordane-4


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 40021758
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

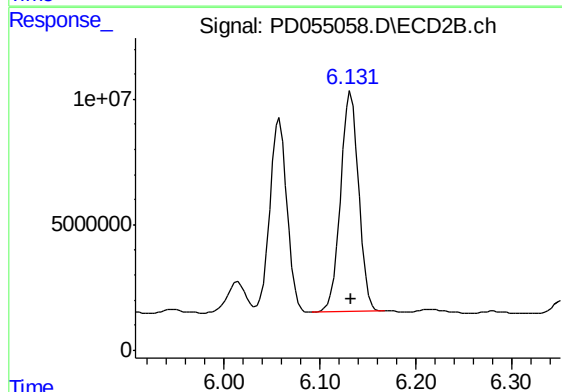


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 115215783
Conc: 500.00 ng/ml

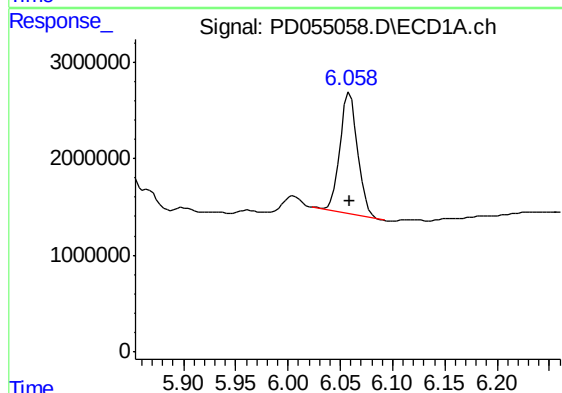


#27 Chlordane-5

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 14776980
Conc: 500.00 ng/ml

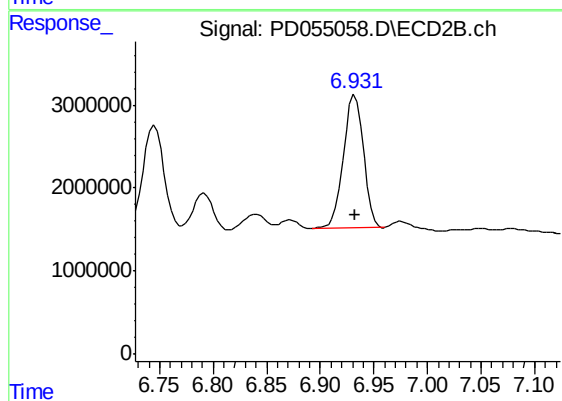

#27 Chlordane-5


R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 21048340
Conc: 500.00 ng/ml

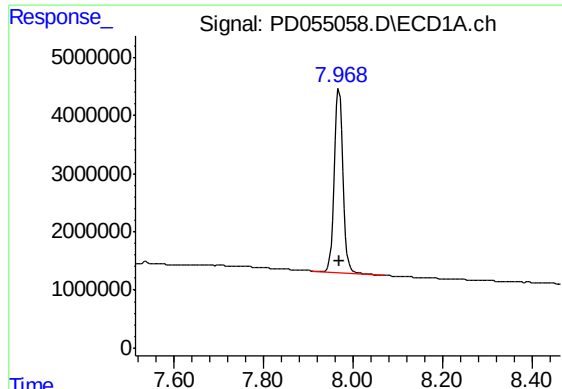

#28 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 42496690
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

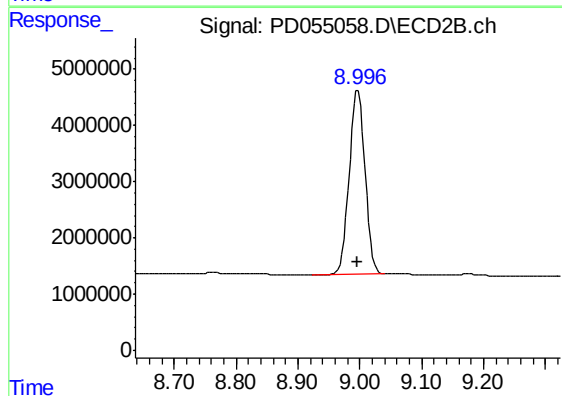

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 57590646
Conc: 50.00 ng/ml