

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 20:46
 Operator : SG\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 06:02:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 05:46:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	20826379	28025335	24.892	25.251
28)	SA Decachlor...	7.968	8.996	21687486	30469341	25.517	26.453
Target Compounds							
23)	Chlordane-1	4.133	4.950	6515975	11075188	267.189	256.826
24)	Chlordane-2	4.623	5.415	7900888	12306842	259.021	262.339
25)	Chlordane-3	5.179	6.058	22720833	48340915	248.716	250.631
26)	Chlordane-4	5.235	6.133	19918773	58979607	248.849	255.953
27)	Chlordane-5	6.059	6.932	7232331	10525445	244.716	250.030



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 20:46
Operator : SG\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 06:02:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 05:46:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

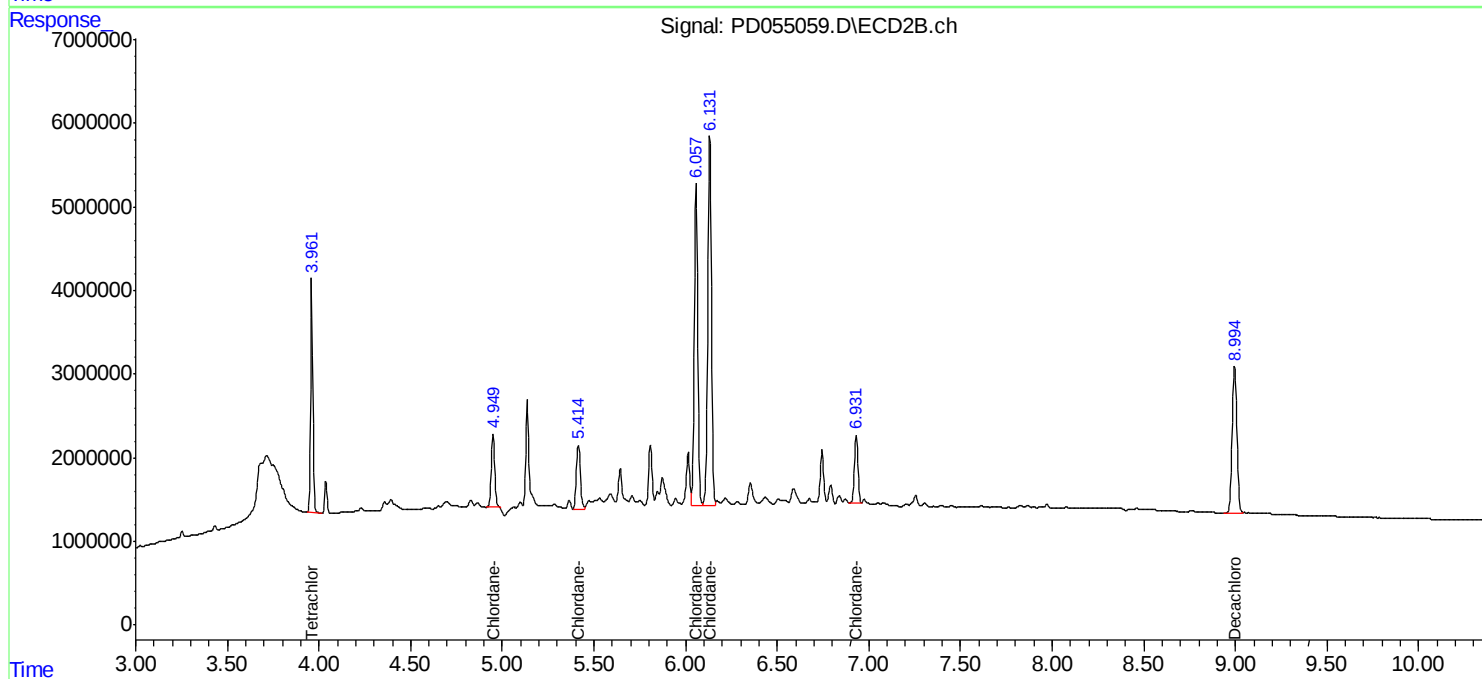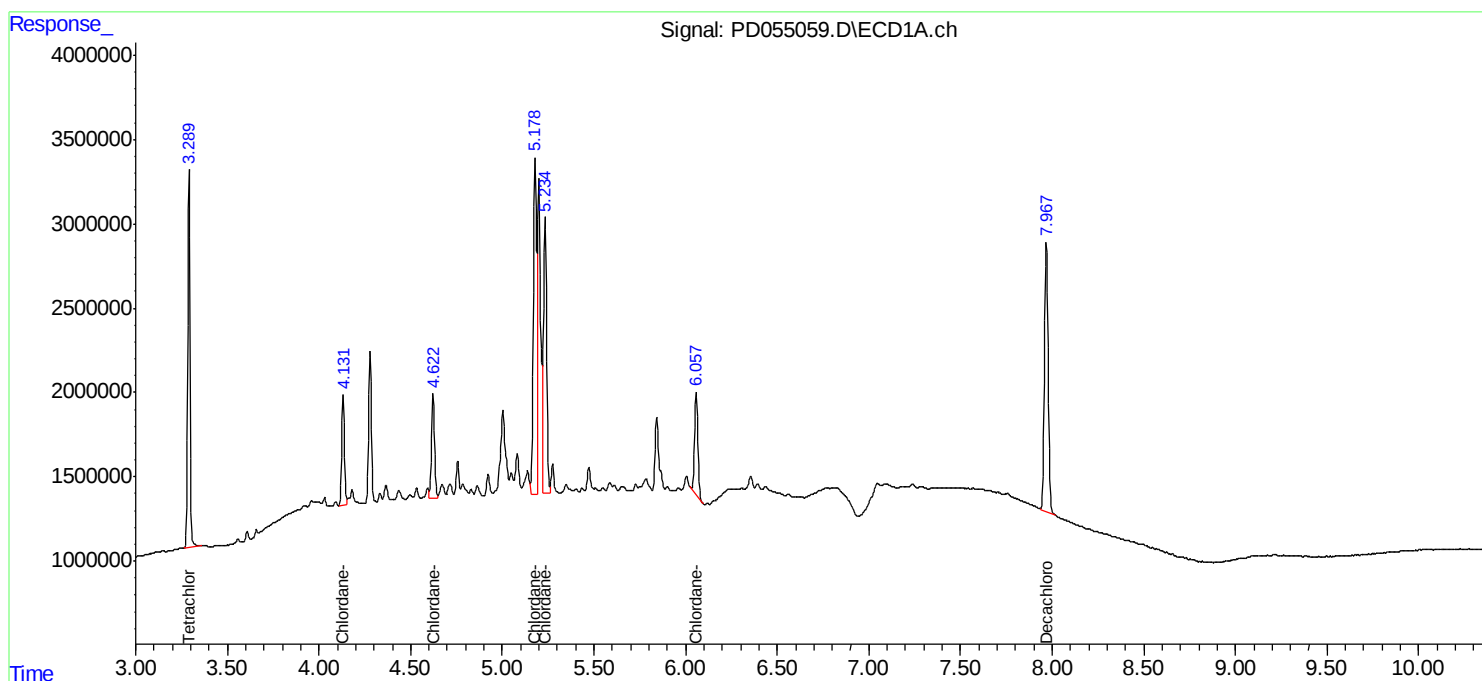


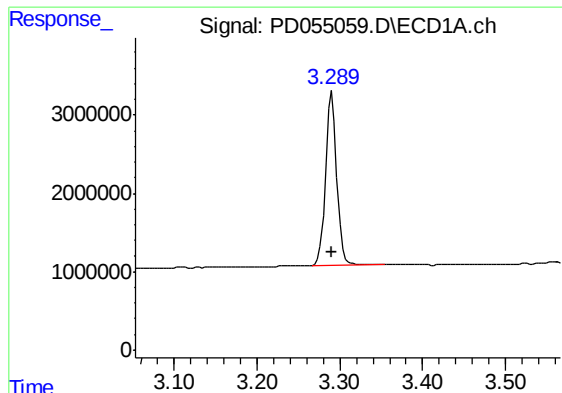

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 20826379
Conc: 24.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

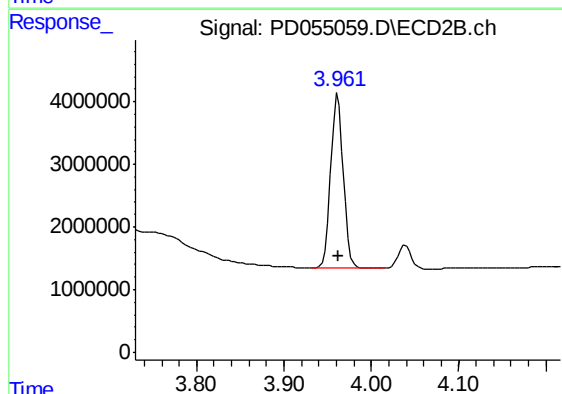


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 28025335
Conc: 25.25 ng/ml

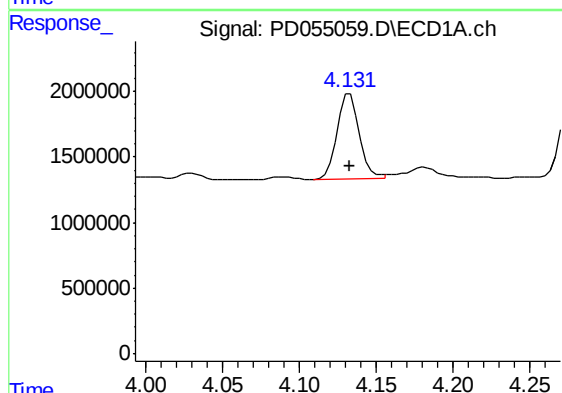


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 6515975
Conc: 267.19 ng/ml

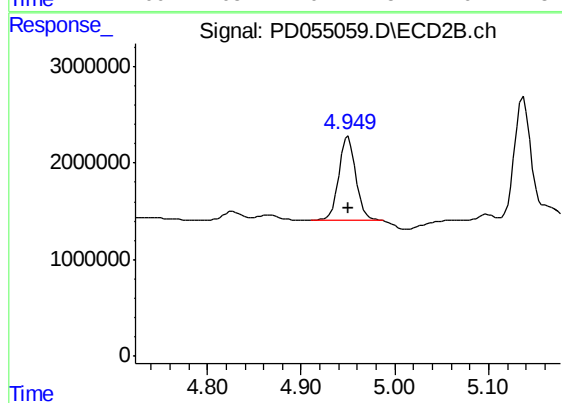

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 11075188
Conc: 256.83 ng/ml

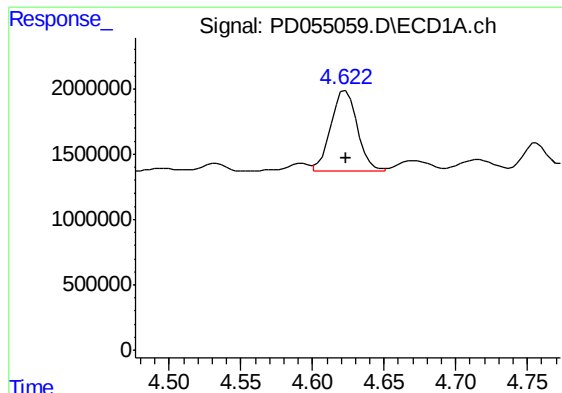

#24 Chlordane-2


R.T.: 4.623 min
Delta R.T.: 0.000 min
Response: 7900888
Conc: 259.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

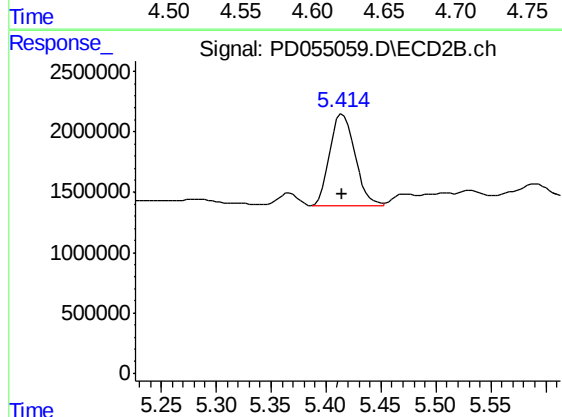


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 12306842
Conc: 262.34 ng/ml

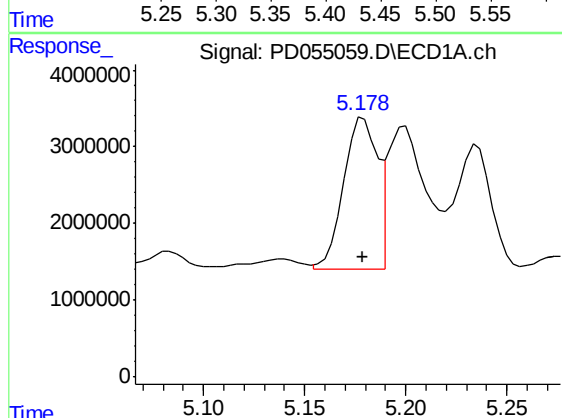


#25 Chlordane-3

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 22720833
Conc: 248.72 ng/ml

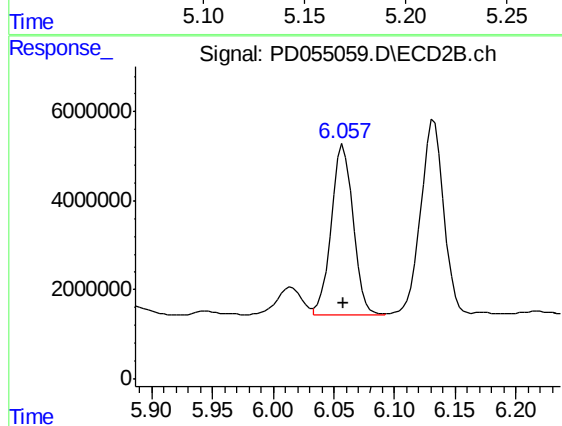

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 48340915
Conc: 250.63 ng/ml

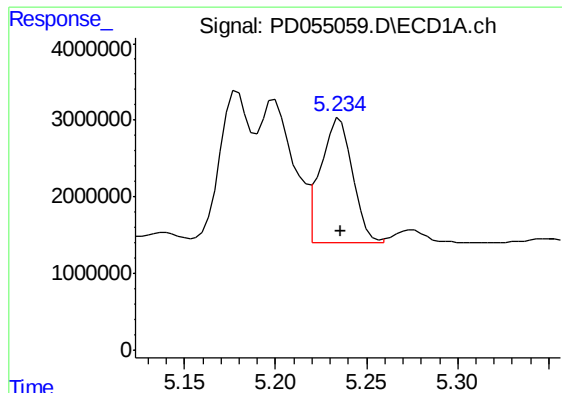

#26 Chlordane-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 19918773
Conc: 248.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

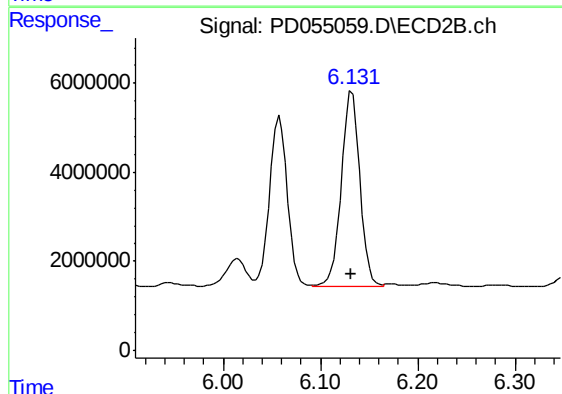


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 58979607
Conc: 255.95 ng/ml

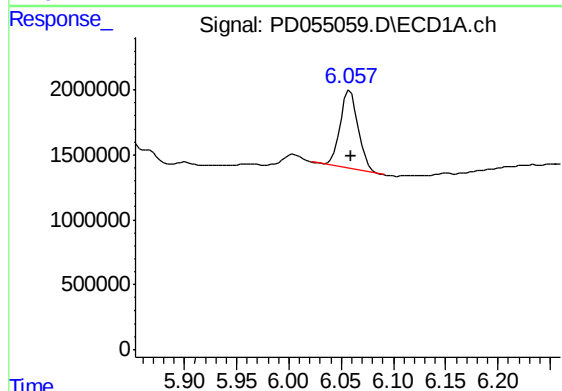


#27 Chlordane-5

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 7232331
Conc: 244.72 ng/ml

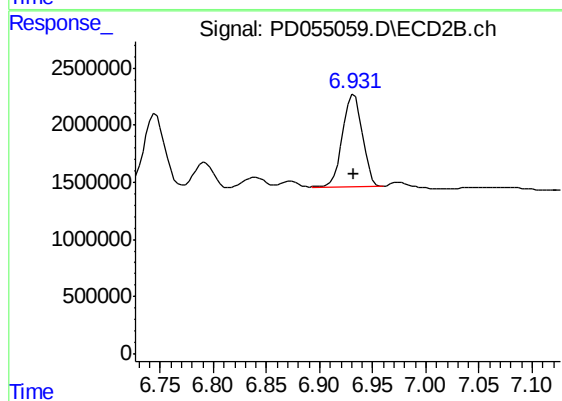

#27 Chlordane-5


R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 10525445
Conc: 250.03 ng/ml

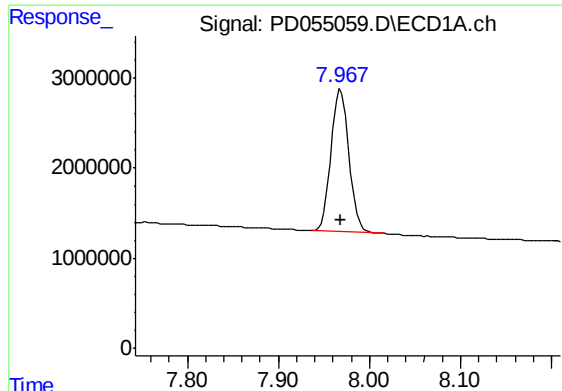

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 21687486
Conc: 25.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

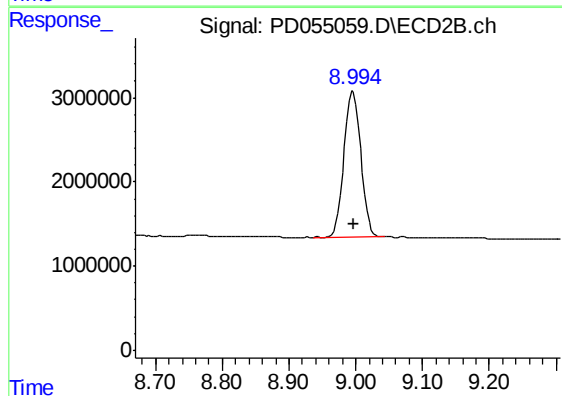

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.001 min
Response: 30469341
Conc: 26.45 ng/ml