

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
 Data File : PD055067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2019 22:41
 Operator : SG\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD093019CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 07:45:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	42658361	55843778	54.409	48.784
28)	SA Decachlor...	7.968	8.996	42630720	58402185	49.417	47.948
Target Compounds							
23)	Chlordane-1	4.133	4.950	12896669	21803748	523.016	488.217
24)	Chlordane-2	4.624	5.415	15858297	24134363	521.583	494.704
25)	Chlordane-3	5.179	6.058	46068055	100.1E6	502.728	507.104
26)	Chlordane-4	5.235	6.132	41297375	120.8E6	514.710	503.959
27)	Chlordane-5	6.059	6.932	15052000	23104959	524.683	551.627



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093019\
Data File : PD055067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2019 22:41
Operator : SG\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD093019CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 07:45:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

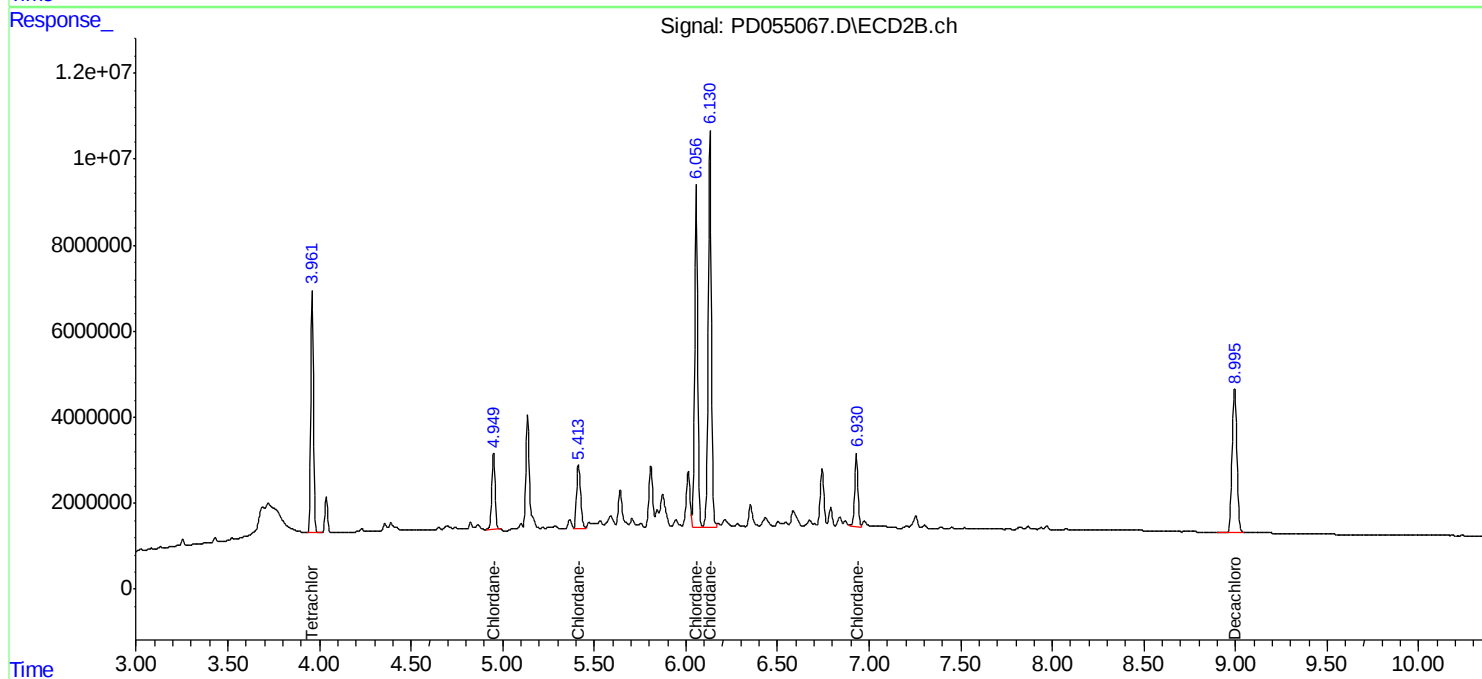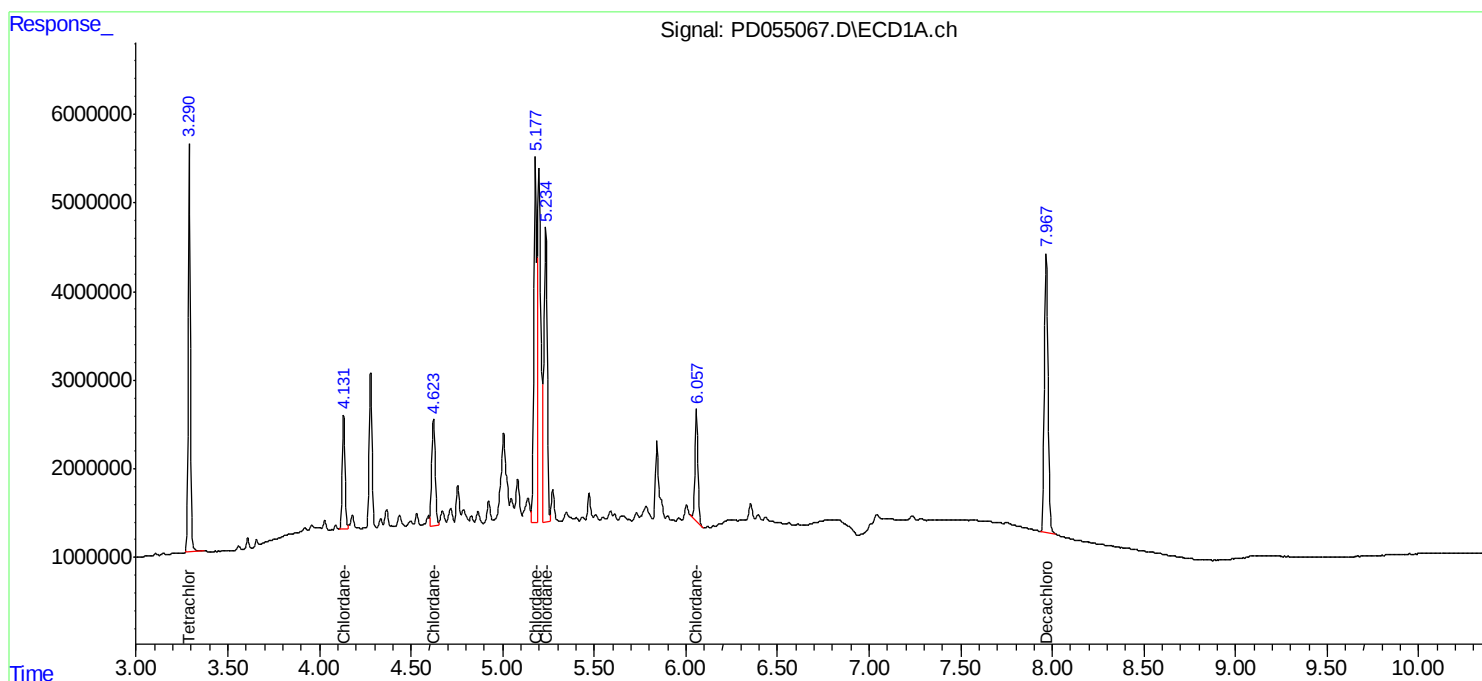


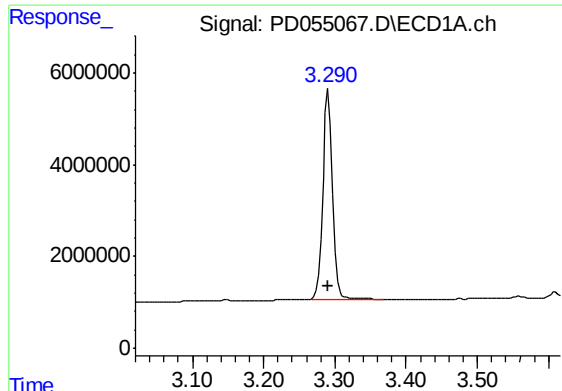

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 42658361
Conc: 54.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093019CHLOR

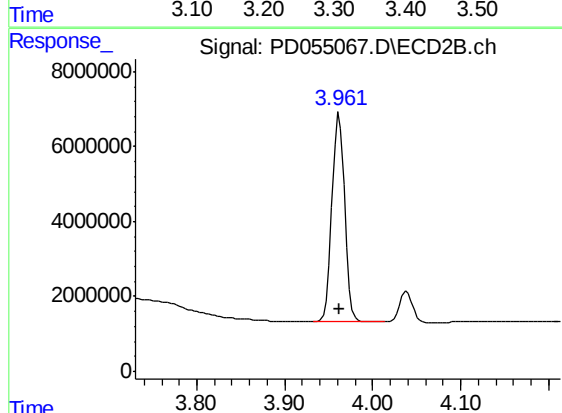


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 55843778
Conc: 48.78 ng/ml

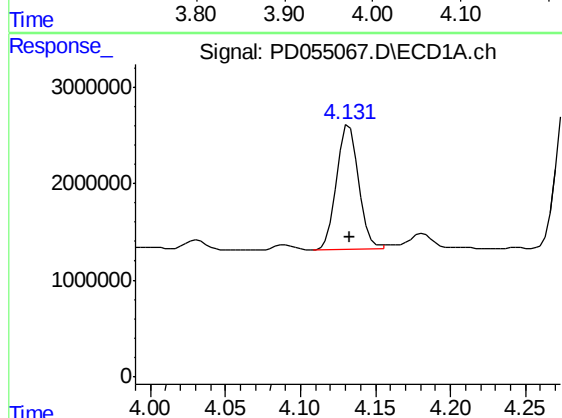


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 12896669
Conc: 523.02 ng/ml

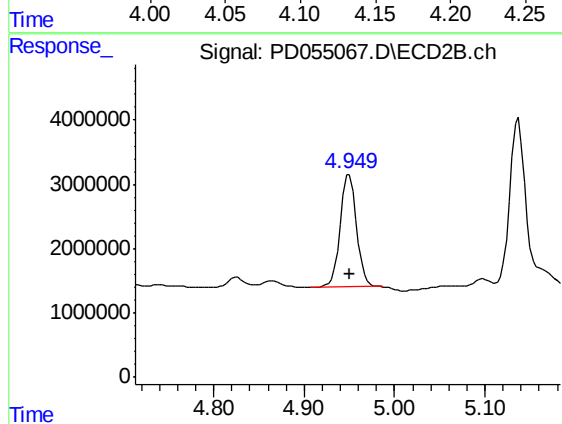

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 21803748
Conc: 488.22 ng/ml

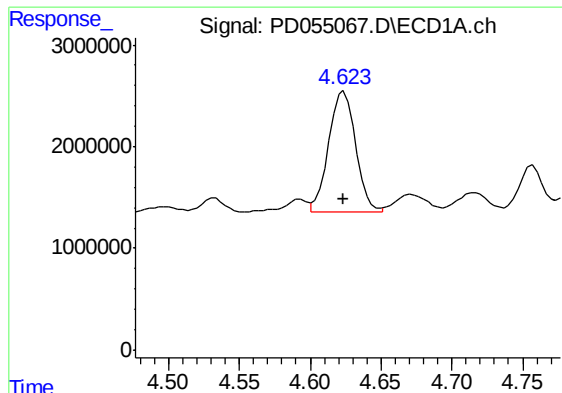

#24 Chlordane-2


R.T.: 4.624 min
Delta R.T.: 0.000 min
Response: 15858297
Conc: 521.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093019CHLOR

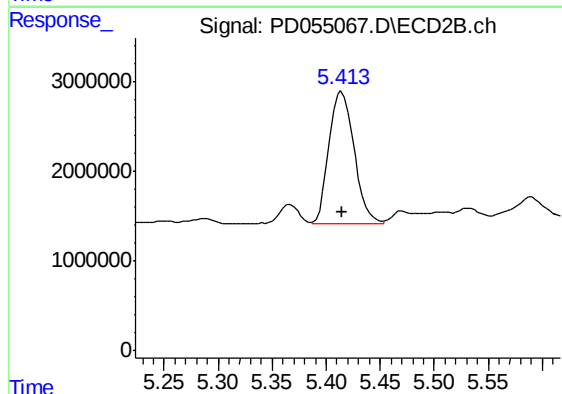


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 24134363
Conc: 494.70 ng/ml

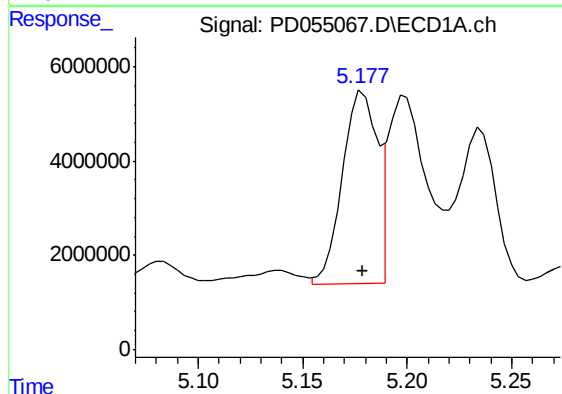


#25 Chlordane-3

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 46068055
Conc: 502.73 ng/ml

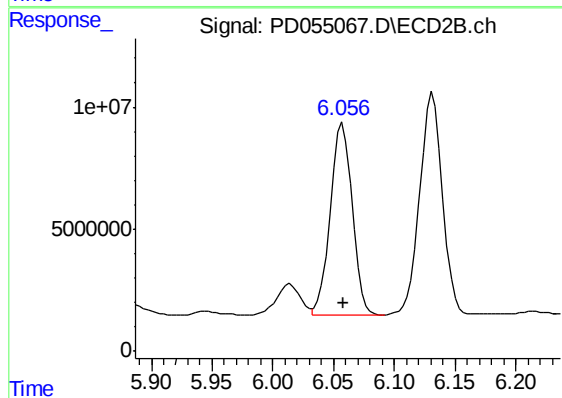

#25 Chlordane-3


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 100148187
Conc: 507.10 ng/ml

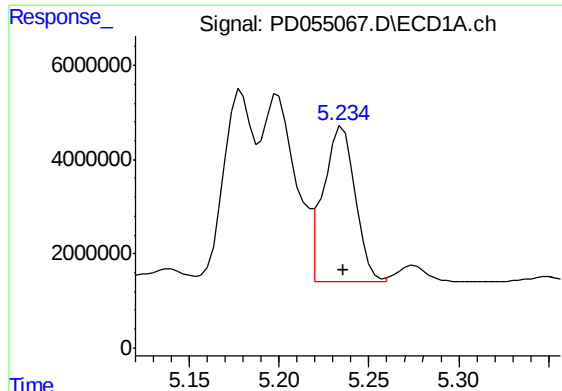

#26 Chlordane-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 41297375
Conc: 514.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093019CHLOR

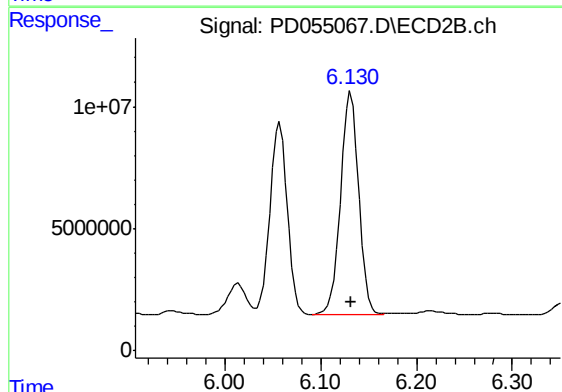


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 120762133
Conc: 503.96 ng/ml

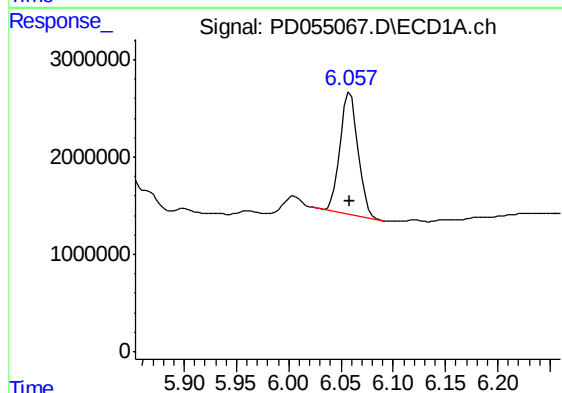


#27 Chlordane-5

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 15052000
Conc: 524.68 ng/ml

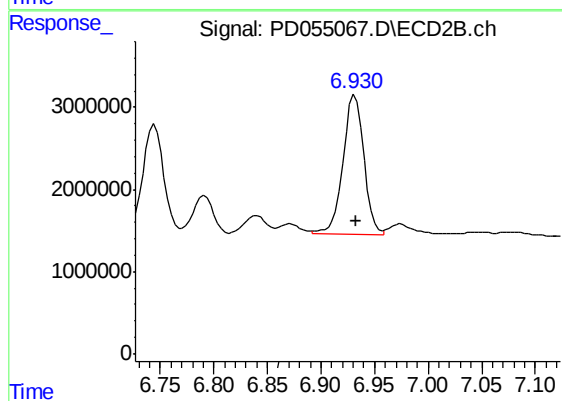

#27 Chlordane-5


R.T.: 6.932 min
Delta R.T.: 0.000 min
Response: 23104959
Conc: 551.63 ng/ml

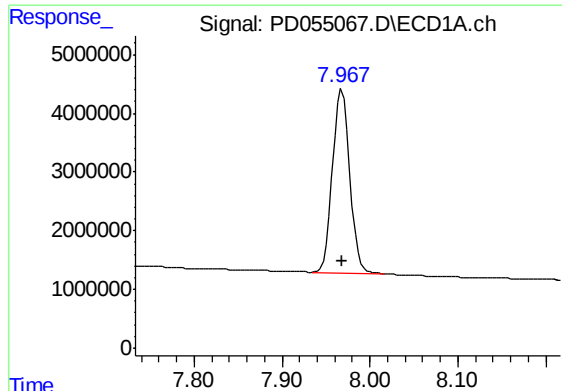

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 42630720
Conc: 49.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093019CHLOR

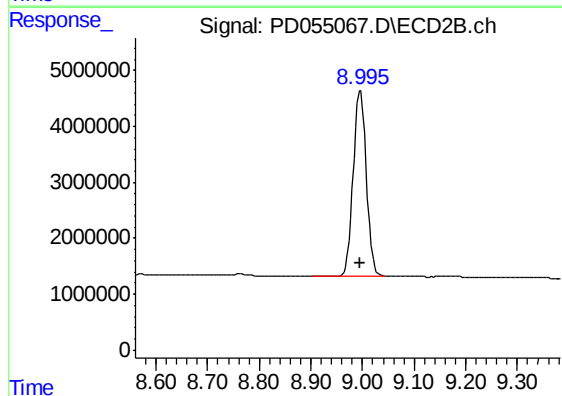

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 58402185
Conc: 47.95 ng/ml