

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
 Data File : PD059430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 20:27
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 06:21:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 30 06:19:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	53290174	75173625	37.709	38.585
27)	SA Decachlor...	8.323	9.114	72434786	105.1E6	72.020	77.967
Target Compounds							
2)	A alpha-BHC	3.955	4.417	79675181	113.1E6	38.218	39.215
3)	MA gamma-BHC...	4.242	4.703	73299312	102.2E6	37.880	39.353
4)	MA Heptachlor	4.552	5.215	73338261	98672272	38.093	39.431
9)	A Endosulfan I	5.594	6.266	55415375	75130455	37.419	39.310
13)	MA Dieldrin	5.841	6.524	119.0E6	165.9E6	76.889	79.258
14)	MA Endrin	6.100	6.743	98849539	134.2E6	77.247	79.754
16)	A 4,4'-DDD	6.225	6.861	94457797	127.3E6	77.638	80.169
17)	MA 4,4'-DDT	6.470	7.161	100.8E6	130.4E6	77.422	80.146
20)	A Methoxychlor	7.020	7.617	229.1E6	327.9E6	375.637	391.133


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 20:27
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 06:21:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 30 06:19:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

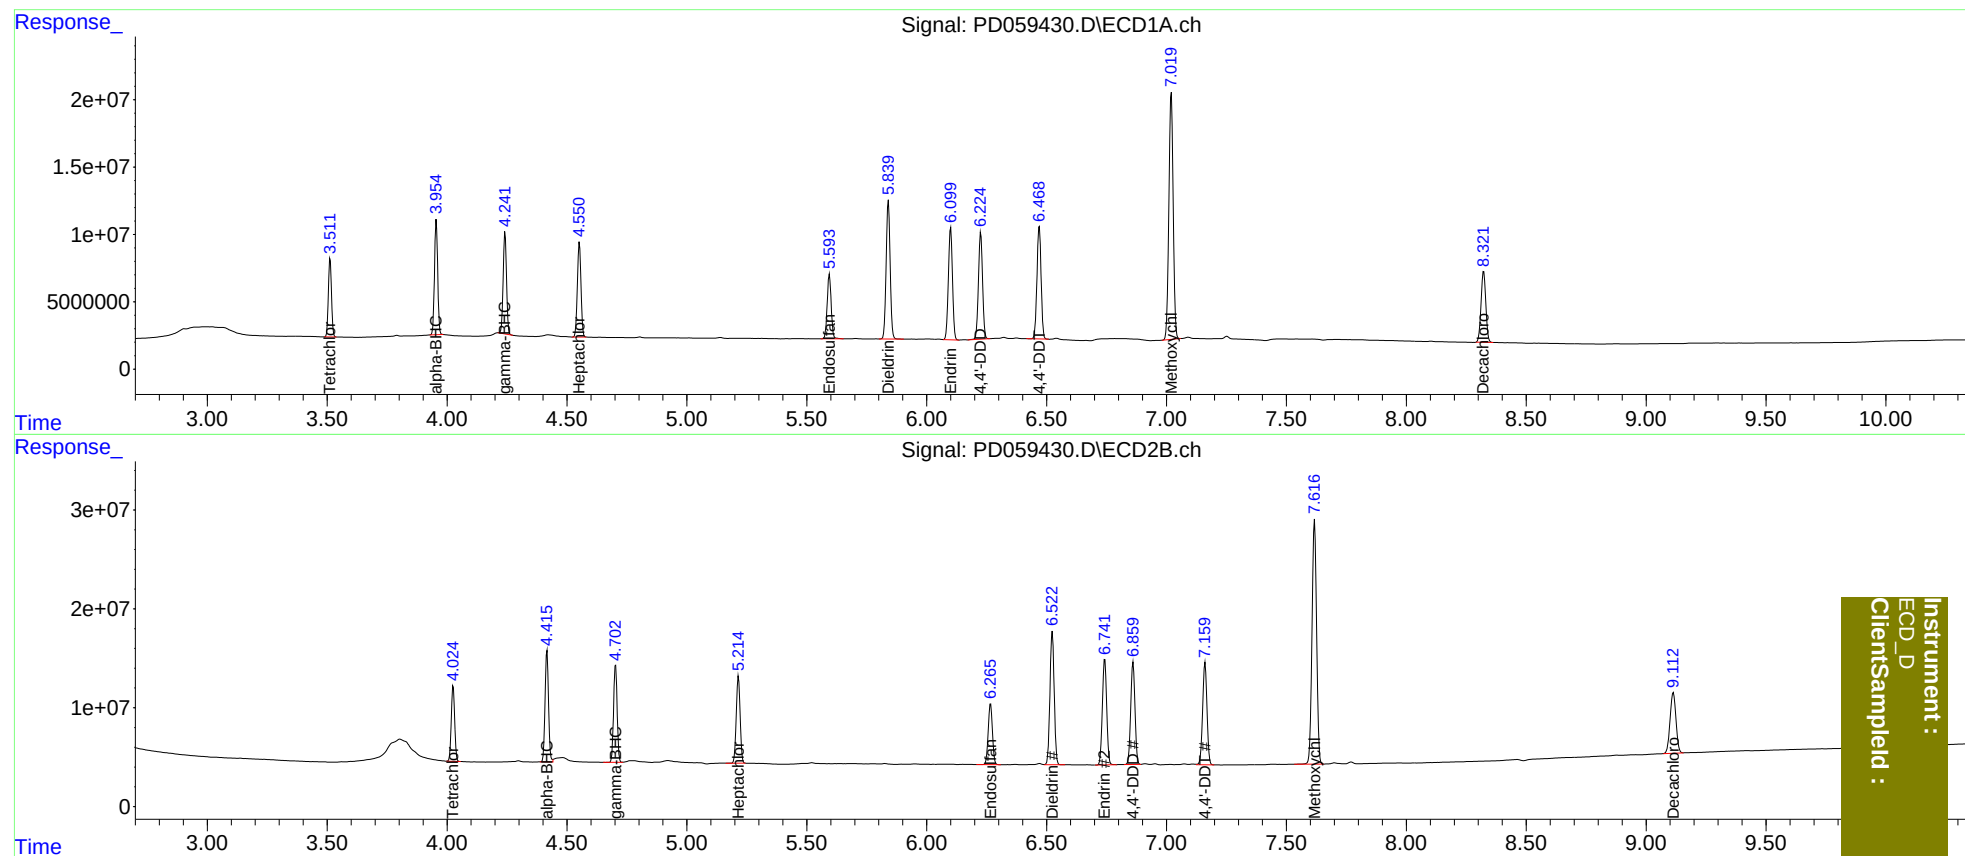


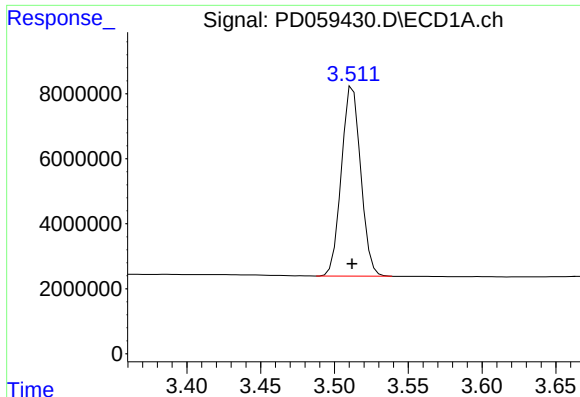

#1 Tetrachloro-m-xylene


R.T.: 3.513 min
Delta R.T.: 0.000 min
Response: 53290174
Conc: 37.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

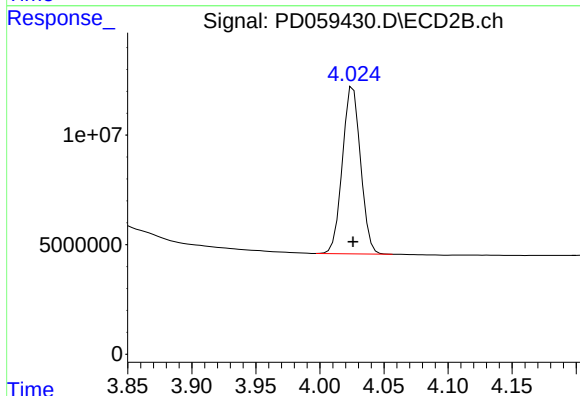


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 75173625
Conc: 38.58 ng/ml

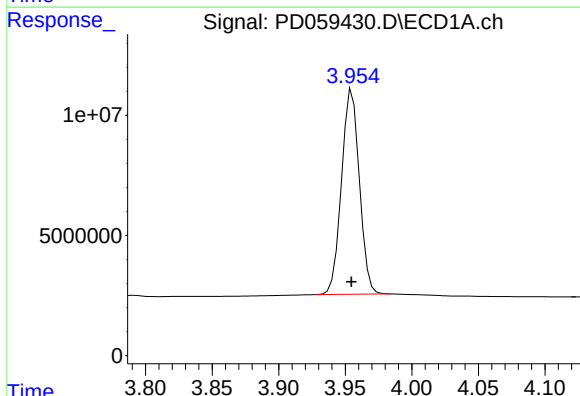


#2 alpha-BHC

R.T.: 3.955 min
Delta R.T.: 0.000 min
Response: 79675181
Conc: 38.22 ng/ml

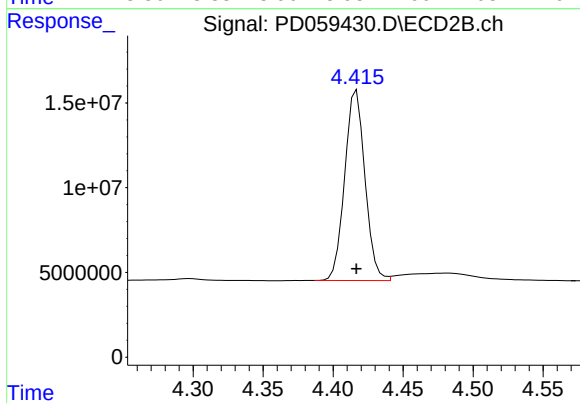

#2 alpha-BHC


R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 113067943
Conc: 39.22 ng/ml

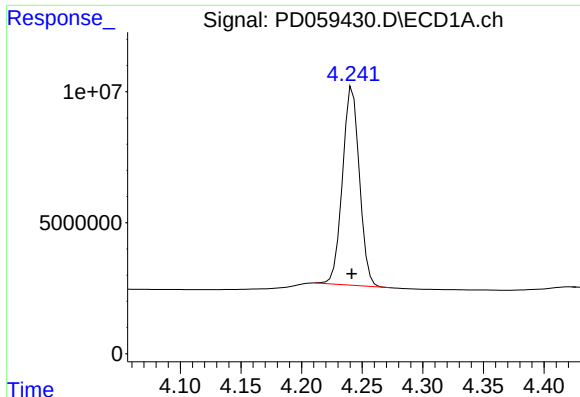

#3 gamma-BHC (Lindane)


R.T.: 4.242 min
Delta R.T.: 0.000 min
Response: 73299312
Conc: 37.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

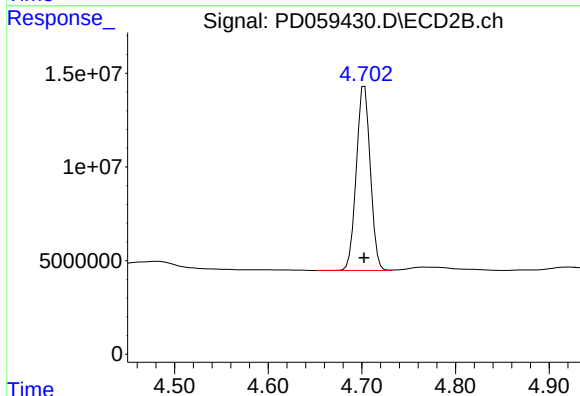


#3 gamma-BHC (Lindane)

R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 102232945
Conc: 39.35 ng/ml

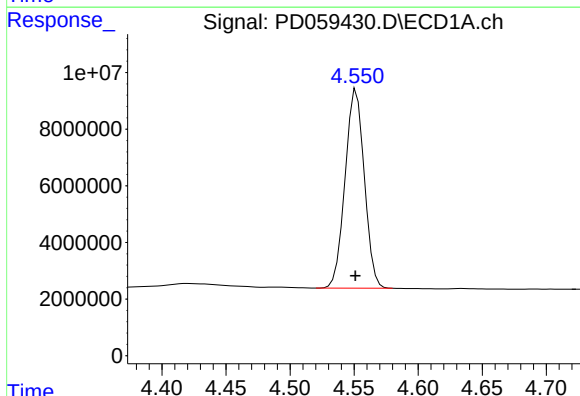


#4 Heptachlor

R.T.: 4.552 min
Delta R.T.: 0.000 min
Response: 73338261
Conc: 38.09 ng/ml

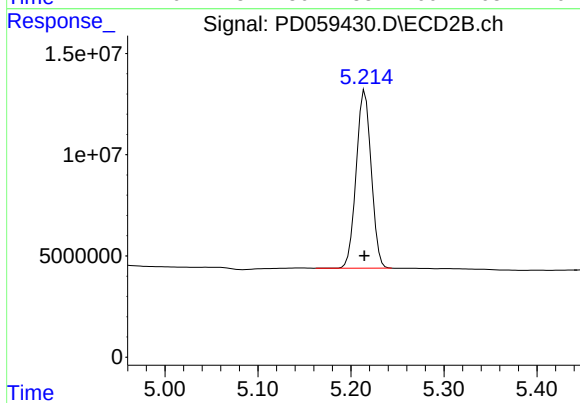

#4 Heptachlor


R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 98672272
Conc: 39.43 ng/ml

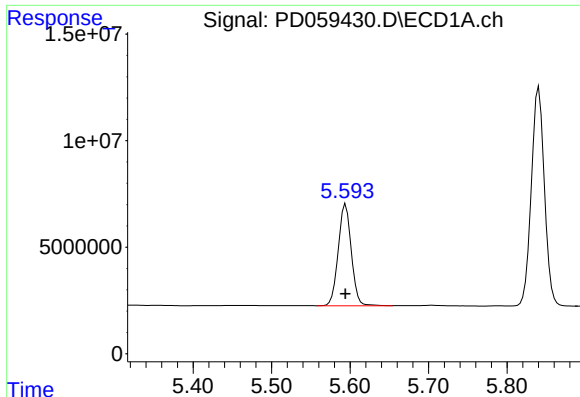

#9 Endosulfan I


R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 55415375
Conc: 37.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

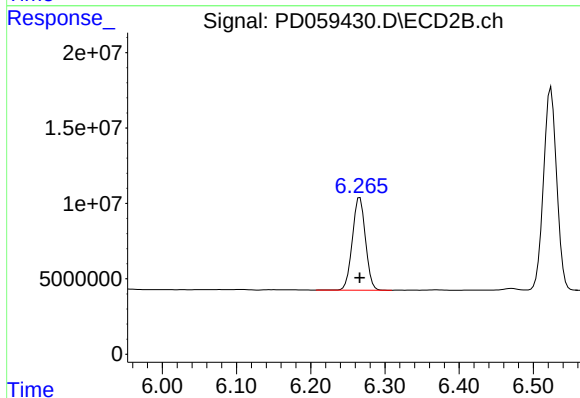


#9 Endosulfan I

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 75130455
Conc: 39.31 ng/ml

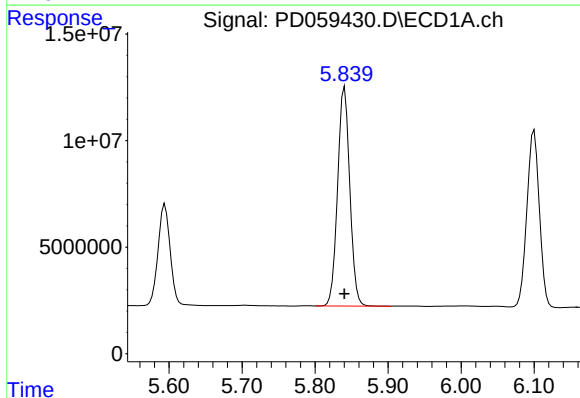


#13 Dieldrin

R.T.: 5.841 min
Delta R.T.: 0.000 min
Response: 118997445
Conc: 76.89 ng/ml

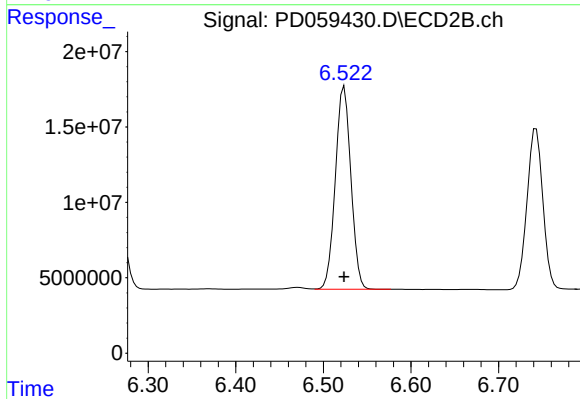

#13 Dieldrin


R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 165932750
Conc: 79.26 ng/ml

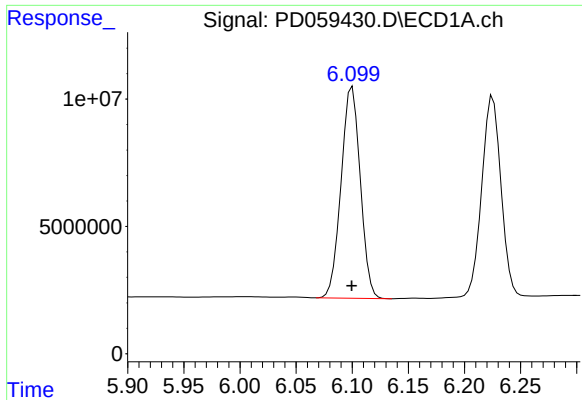

#14 Endrin


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 98849539
Conc: 77.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

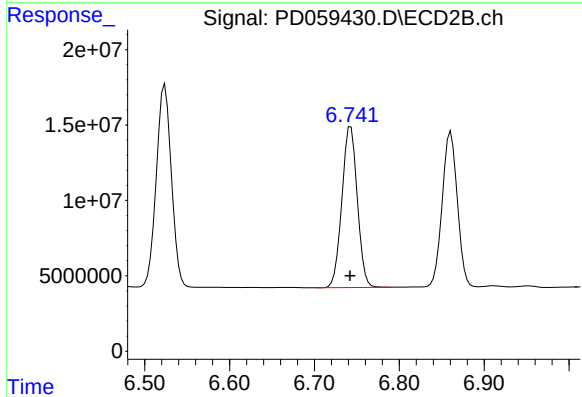


#14 Endrin

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 134201348
Conc: 79.75 ng/ml

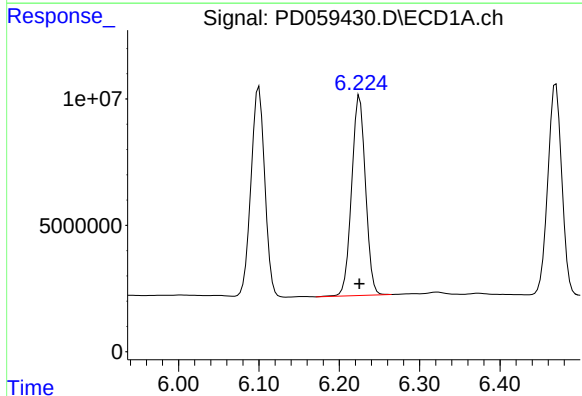


#16 4,4'-DDD

R.T.: 6.225 min
Delta R.T.: 0.000 min
Response: 94457797
Conc: 77.64 ng/ml

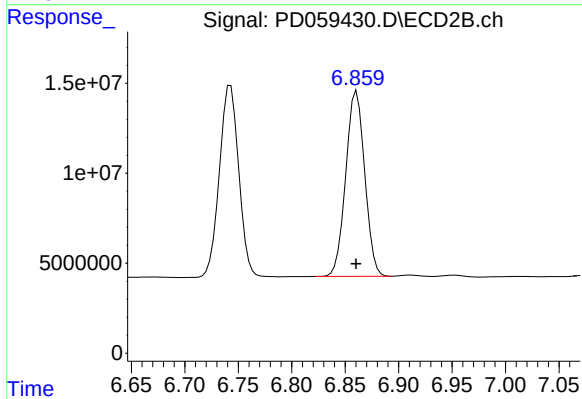

#16 4,4'-DDD


R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 127289762
Conc: 80.17 ng/ml

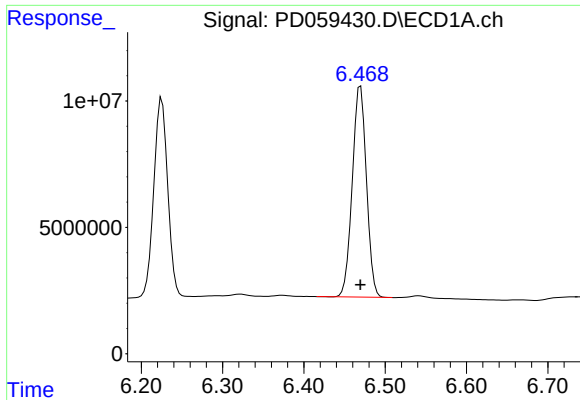

#17 4,4'-DDT


R.T.: 6.470 min
Delta R.T.: 0.000 min
Response: 100793531
Conc: 77.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

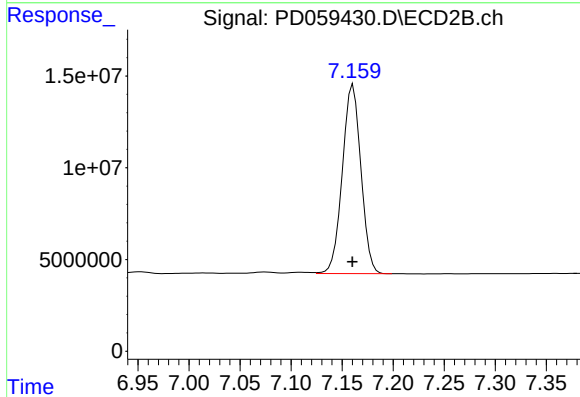


#17 4,4'-DDT

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 130433371
Conc: 80.15 ng/ml

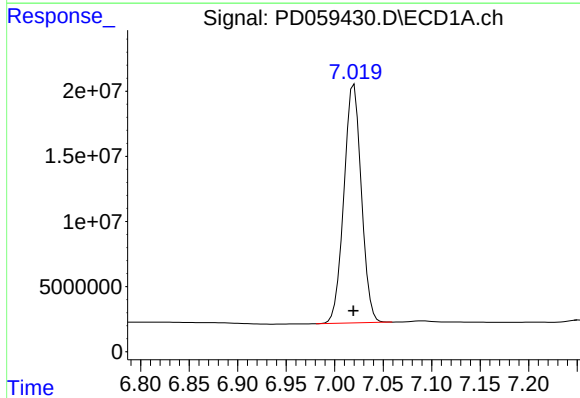


#20 Methoxychlor

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 229052353
Conc: 375.64 ng/ml

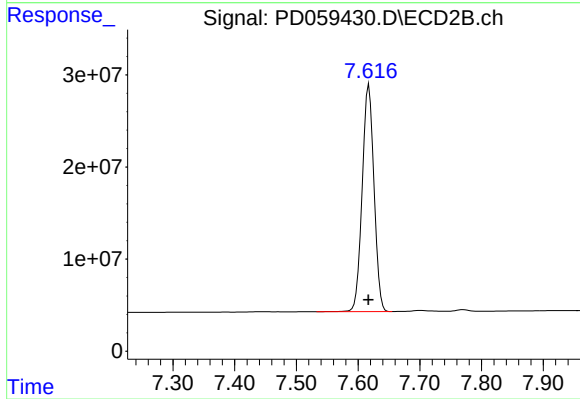

#20 Methoxychlor


R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 327856439
Conc: 391.13 ng/ml

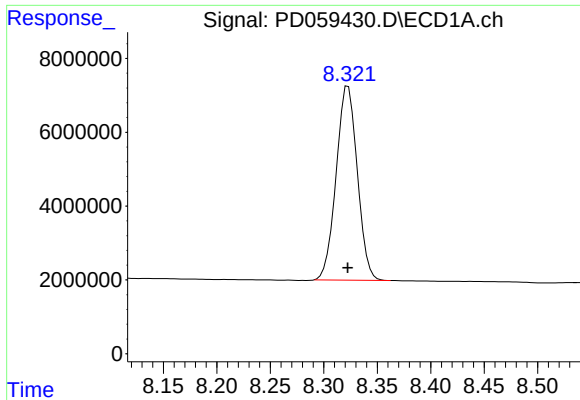

#27 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 72434786
Conc: 72.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

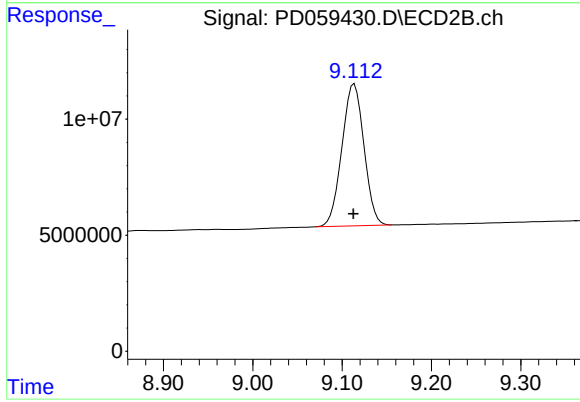

#27 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.001 min
Response: 105080351
Conc: 77.97 ng/ml