

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
 Data File : PD059430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 20:27
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 06:21:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 30 06:19:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.513	4.026	53290174	75173625	37.709	38.585
27)	SA Decachlor...	8.323	9.114	72434786	105.1E6	72.020	77.967
Target Compounds							
2)	A alpha-BHC	3.955	4.417	79675181	113.1E6	38.218	39.215
3)	MA gamma-BHC...	4.242	4.703	73299312	102.2E6	37.880	39.353
4)	MA Heptachlor	4.552	5.215	73338261	98672272	38.093	39.431
9)	A Endosulfan I	5.594	6.266	55415375	75130455	37.419	39.310
13)	MA Dieldrin	5.841	6.524	119.0E6	165.9E6	76.889	79.258
14)	MA Endrin	6.100	6.743	98849539	134.2E6	77.247	79.754
16)	A 4,4'-DDD	6.225	6.861	94457797	127.3E6	77.638	80.169
17)	MA 4,4'-DDT	6.470	7.161	100.8E6	130.4E6	77.422	80.146
20)	A Methoxychlor	7.020	7.617	229.1E6	327.9E6	375.637	391.133

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 20:27
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 06:21:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 30 06:19:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

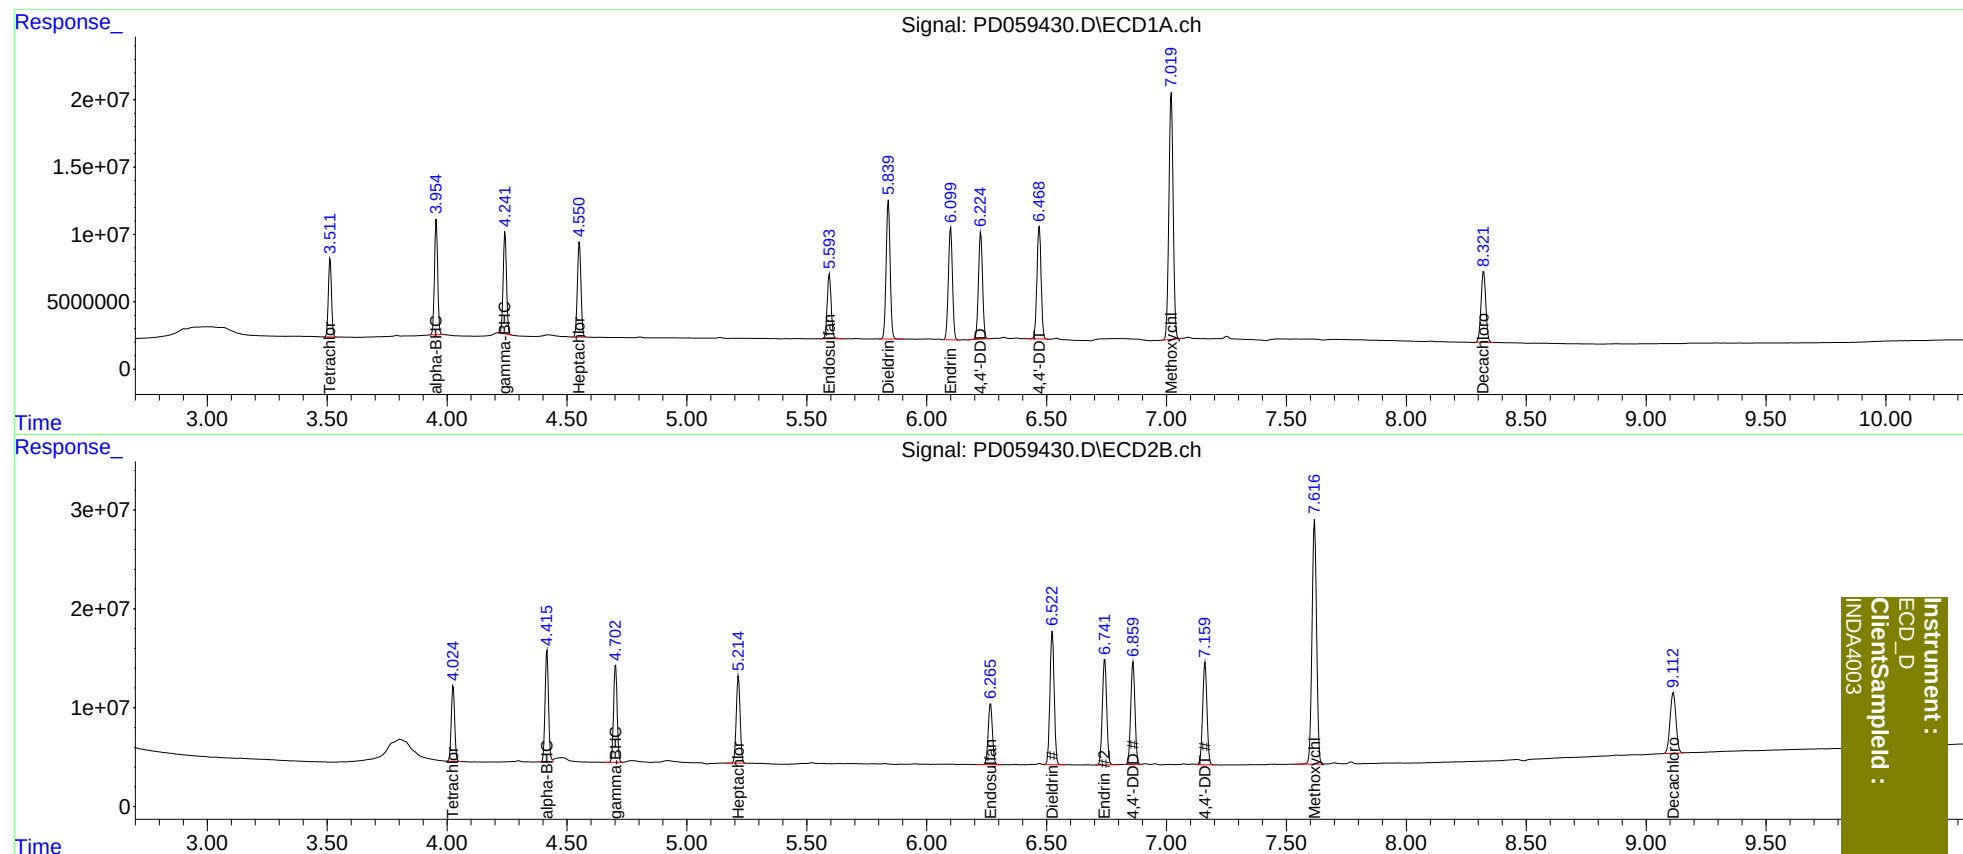

Instrument :
ECD_D
ClientSample :
INDA4003