

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
 Data File : PD059417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2020 17:22
 Operator : DD\AJ
 Sample : RESC56
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC056

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 07:28:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 30 06:37:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.512	4.025	26329866	36741725	19.109	19.313
2)	SA Decachlor...	8.322	9.112	37953912	50878790	38.110	38.225
Target Compounds							
2)	A alpha-BHC	3.955	4.417	19008305	26215469	9.264	9.149
3)	MA gamma-BHC...	4.242	4.702	17963018	23442039	9.242	9.209
4)	MA Heptachlor	4.551	5.214	17777535	22843957	9.476	9.268
5)	MB Aldrin	4.803	5.521	17325706	22393176	9.844	9.796
6)	B beta-BHC	4.492	4.869	7374667	10960130	9.701	9.840
7)	B delta-BHC	4.700	5.089	17364689	18515298	9.670	7.922
8)	B Heptachlo...	5.250	5.908	15188550	19607647	9.824	9.301
9)	A Endosulfan I	5.594	6.266	14651432	17603809	10.397	9.302
10)	B trans-Chl...	5.480	6.142	15039978	18912754	9.778	9.380
11)	B cis-Chlor...	5.539	6.215	14996785	19536194	9.812	9.617
12)	B 4,4'-DDE	5.705	6.370	28633788	37329132	19.476	18.991
13)	MA Dieldrin	5.840	6.523	28850910	37873965	18.978	18.332
14)	MA Endrin	6.100	6.742	24328480	31254287	19.365	18.862
15)	B Endosulfa...	6.373	6.949	23716239	31715541	19.463	19.074
16)	A 4,4'-DDD	6.225	6.860	23701231	28844501	19.411	18.430
17)	MA 4,4'-DDT	6.469	7.160	23808523	31299249	18.635	19.279
18)	B Endrin al...	6.542	7.074	19232680	26454750	19.626	19.290
19)	B Endosulfa...	6.758	7.296	23256310	32680250	19.942	20.004
20)	A Methoxychlor	7.020	7.617	59122625	78065049	97.941	94.611
21)	B Endrin ke...	7.253	7.769	25010863	32390590	19.915	19.645

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 17:22
Operator : DD\AJ
Sample : RESC56
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 07:28:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 30 06:37:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

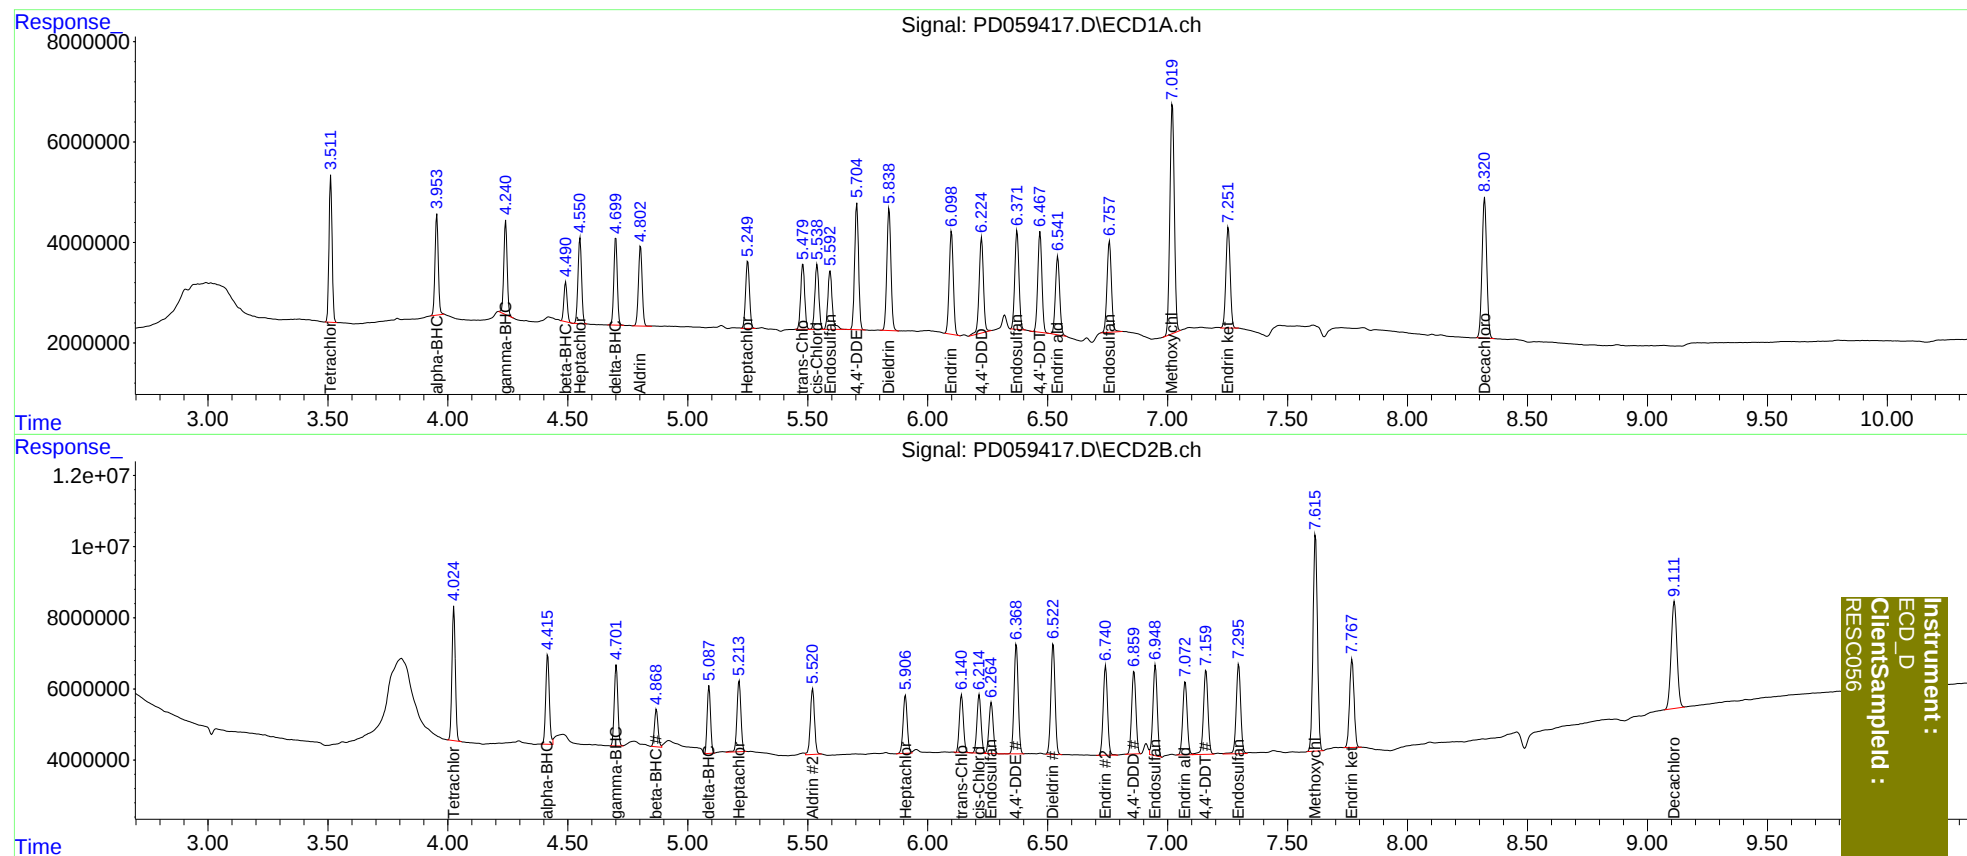

Instrument :
ECD_D
ClientSampled :
RESC056

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059417.D
Acq On : 29 Sep 2020 17:22
Operator : DD\AJ
Sample : RESC56
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC056

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Title : GC Extractables
Last Update : Wed Sep 30 06:37:17 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.512	3.955	100.00%
3.955	4.242	100.00%
4.242	4.492	100.00%
4.492	4.551	100.00%
4.551	4.700	100.00%
4.700	4.803	100.00%
4.803	5.250	100.00%
5.250	5.480	100.00%
5.480	5.539	100.00%
5.539	5.594	99.17%
5.594	5.705	100.00%
5.705	5.840	100.00%
5.840	6.100	100.00%
6.100	6.225	100.00%
6.225	6.373	100.00%
6.373	6.469	100.00%
6.469	6.542	100.00%
6.542	6.758	100.00%
6.758	7.020	100.00%
7.020	7.253	100.00%
7.253	8.322	100.00%

Signal #2


4.025	4.417	100.00%
4.417	4.702	100.00%
4.702	4.869	100.00%
4.869	5.089	100.00%
5.089	5.214	100.00%
5.214	5.521	100.00%
5.521	5.908	100.00%
5.908	6.142	100.00%
6.142	6.215	100.00%
6.215	6.266	99.15%
6.266	6.370	100.00%
6.370	6.523	100.00%
6.523	6.742	100.00%
6.742	6.860	100.00%
6.860	6.949	100.00%
6.949	7.074	100.00%
7.074	7.160	98.29%
7.160	7.296	100.00%
7.296	7.617	100.00%
7.617	7.769	100.00%
7.769	9.112	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 17:22
Operator : DD\AJ
Sample : RESC056
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC056

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 07:28:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 30 06:37:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

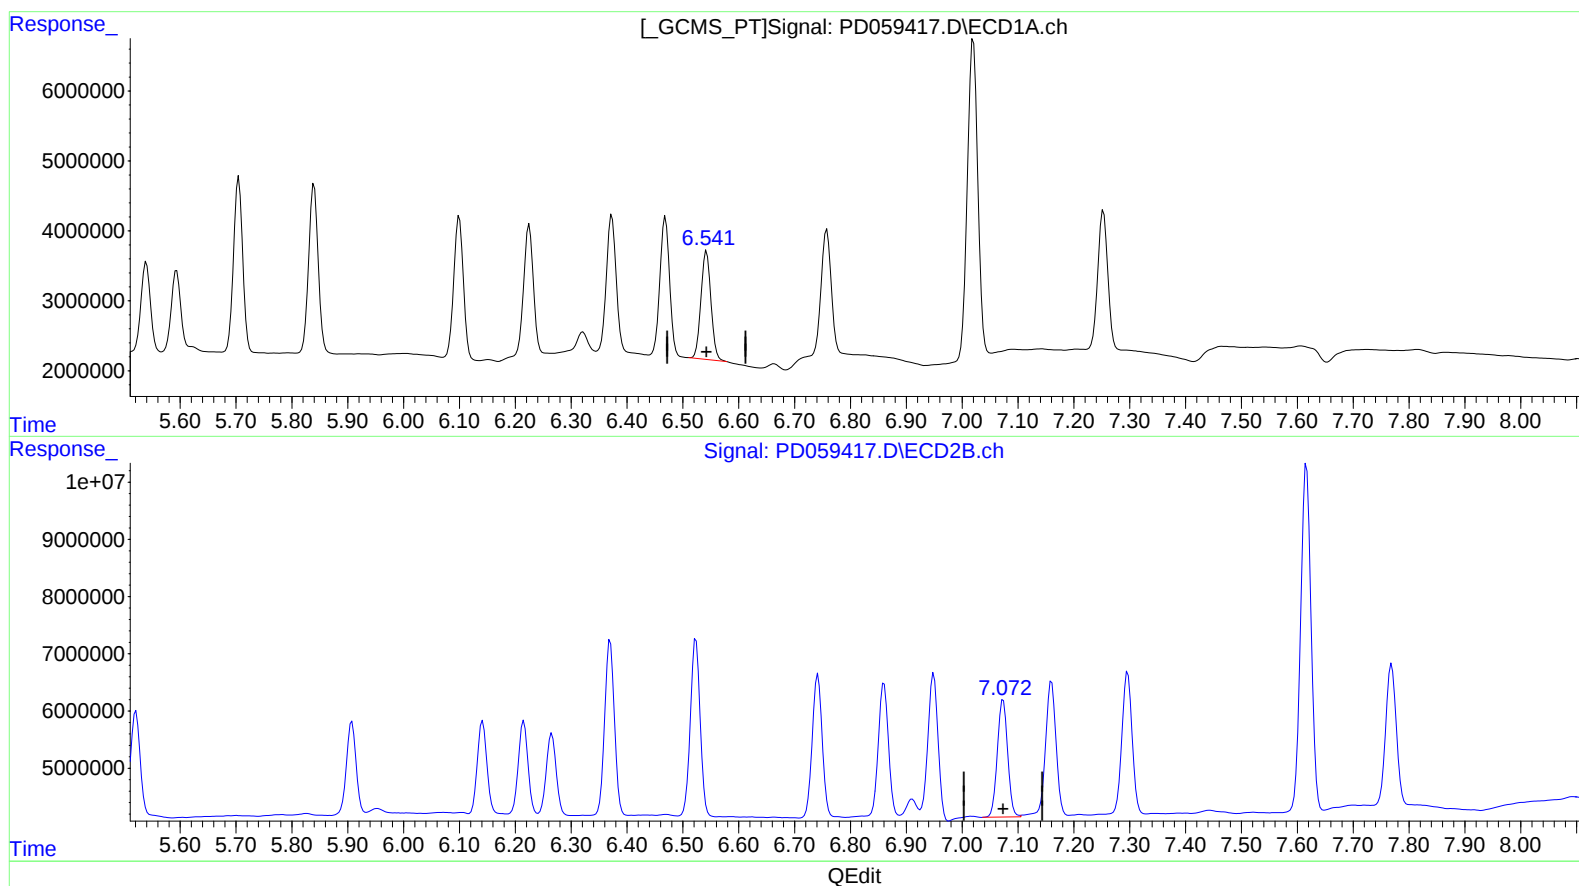

(18) Endrin aldehyde (B)

6.542min 19.626 ng/ml

response 19232680

(18) Endrin aldehyde #2 (B)

7.074min 19.290 ng/ml


response 26454750

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093020\
Data File : PD059417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2020 17:22
Operator : DD\AJ
Sample : RESC56
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC056

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 07:28:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093020CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 30 06:37:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

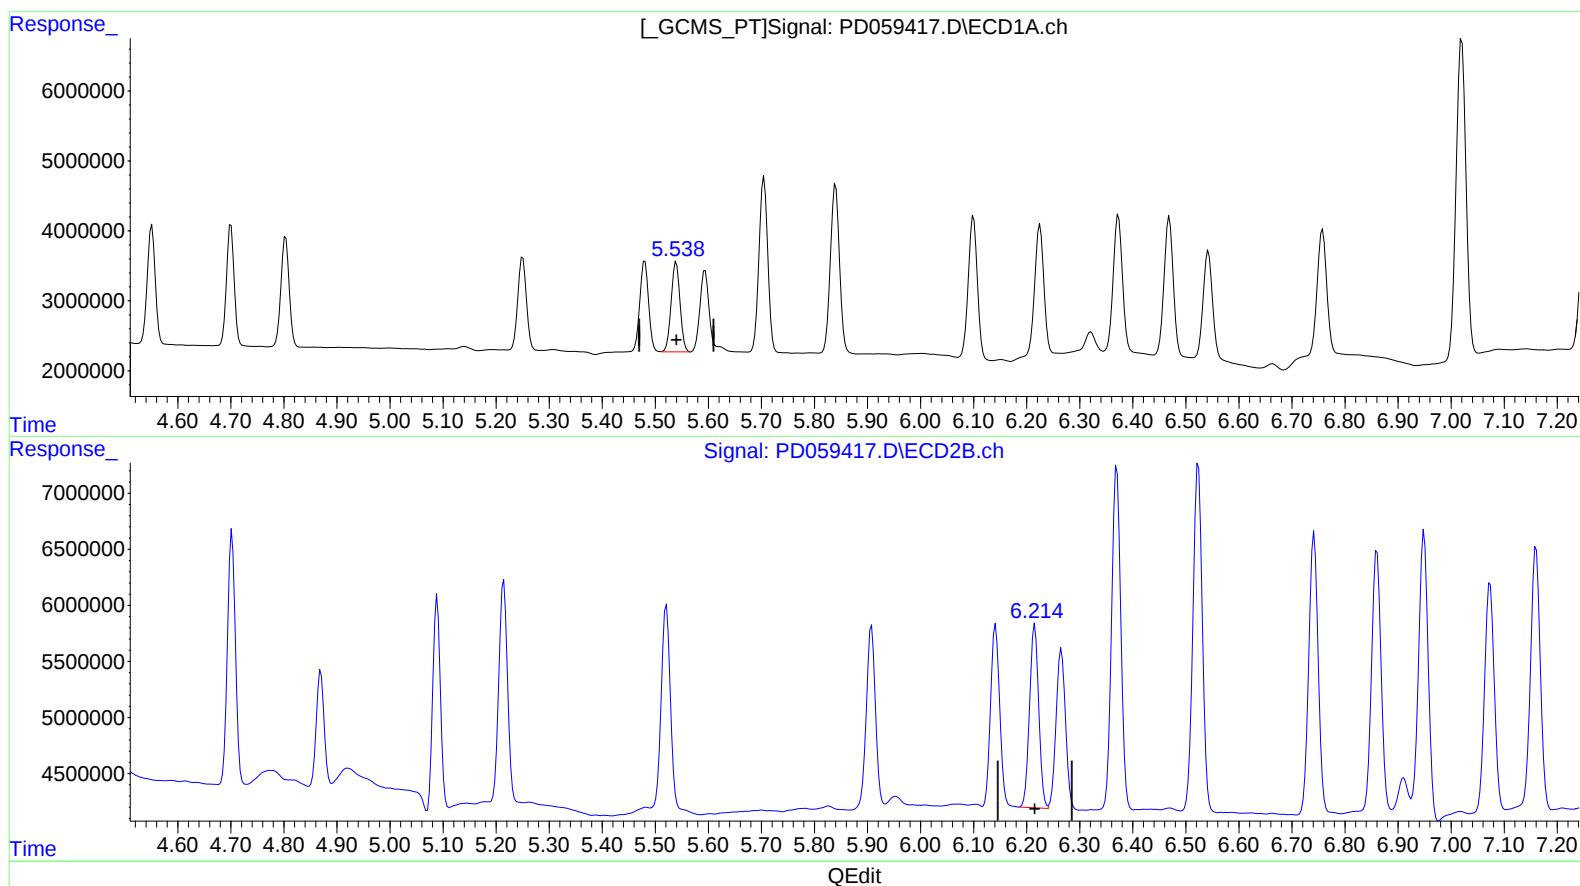

(11) cis-Chlordane (B)

5.539min 9.812 ng/ml

response 14996785

(11) cis-Chlordane #2 (B)

6.215min 9.617 ng/ml

response 19536194