

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
 Data File : PD065985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2021 10:33
 Operator : AR\AJ
 Sample : M3877-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2L6

Manual Integrations
 APPROVED

Ankita
 10/6/2021 1:30:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:05:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	4.011	12864419	59329635	14.864	8.343m#
27)	SA Decachlor...	8.234	9.083	32455341	108.2E6	21.949	25.013
Target Compounds							
10)	B trans-Chl...	5.424	6.122	853077	20710089	0.655	2.906m#
11)	B cis-Chlor...	5.488	6.196	1360977	6268107	1.046	0.897
12)	B 4,4'-DDE	5.648	6.354	666879	8311136	0.559	1.275 #
15)	B Endosulfa...	6.321	6.946	3676985	12657133	2.945	2.126m#
17)	MA 4,4'-DDT	6.401	7.147	1184266	2926694	1.021	0.541 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
Data File : PD065985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2021 10:33
Operator : AR\AJ
Sample : M3877-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:05:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

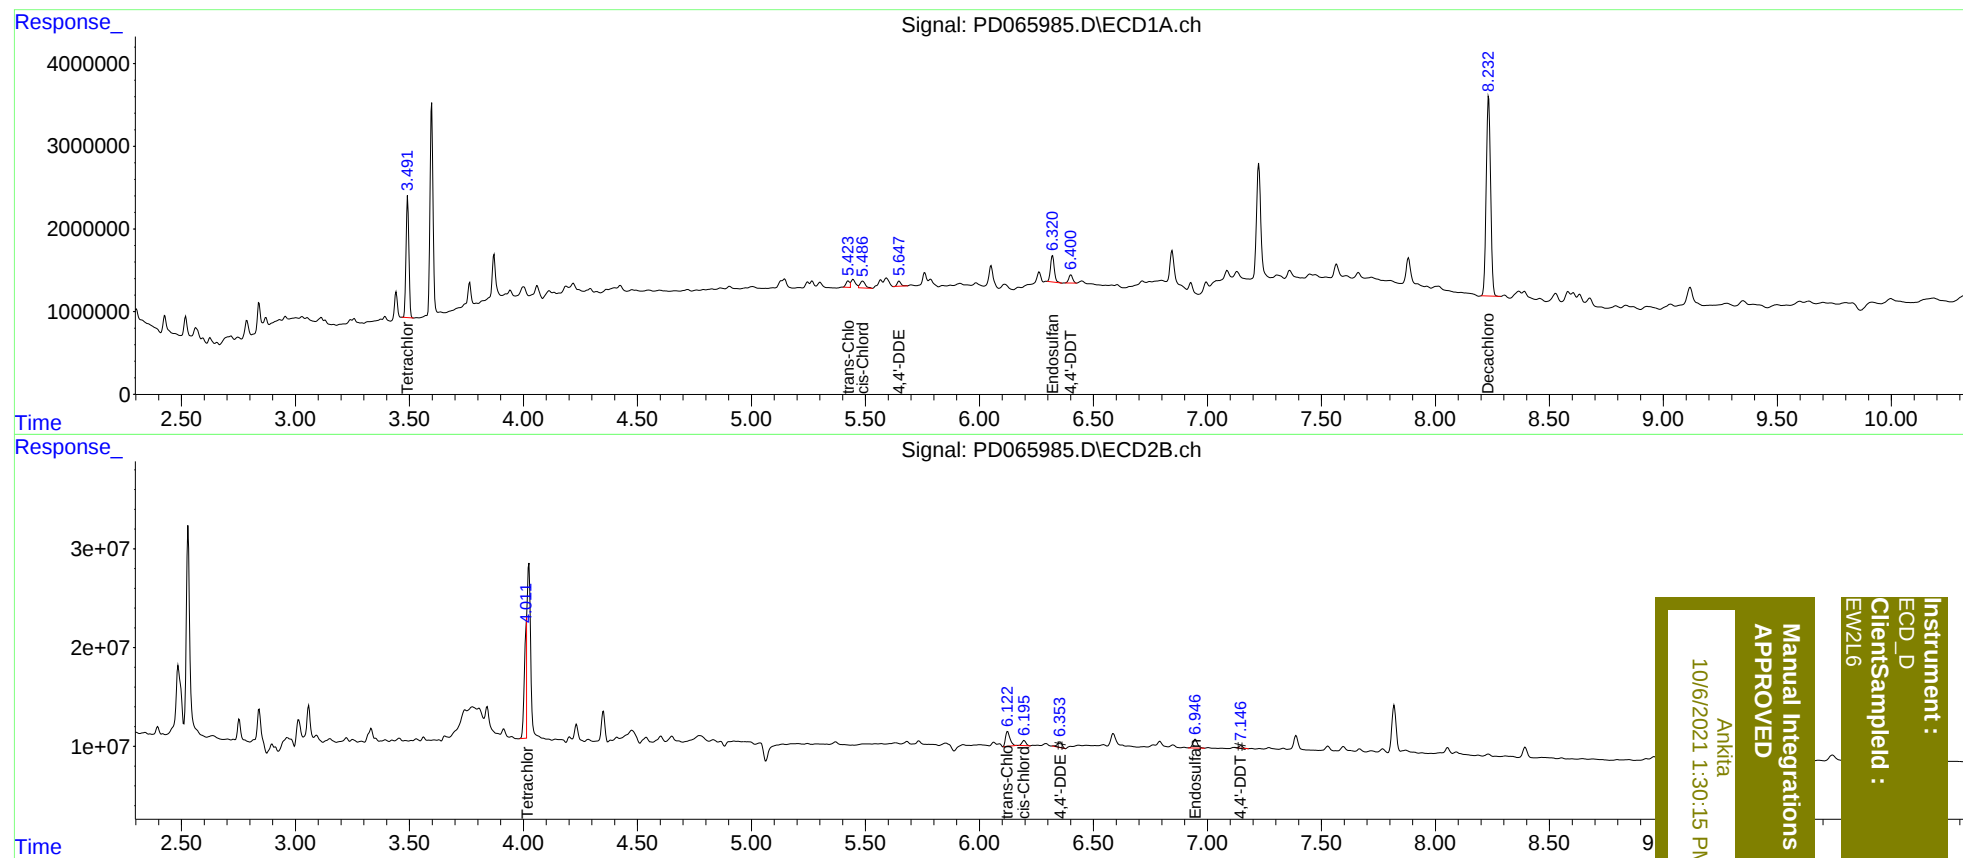

Manual Integrations
APPROVED

10/6/2021 1:30:15 PM
Ankita

Instrument :
ECD_D
Client Sampled :
EW2L6