

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
 Data File : PD065992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2021 12:10
 Operator : AR\AJ
 Sample : M3877-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2M4

Manual Integrations
 APPROVED

Ankita
 10/6/2021 1:30:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:53:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.492	4.012	14349884	101.9E6	16.580	14.329
27) SA Decachlor...	8.234	9.084	31759381	112.9E6	21.478	26.116
Target Compounds						
8) B Heptachlo...	5.201	5.878	1249244	8252531	1.004m	1.207
10) B trans-Chl...	5.427	6.123	13961294	113.3E6	10.716	15.893m#
11) B cis-Chlor...	5.485	6.197	13673724	136.8E6	10.509	19.587 #
12) B 4,4'-DDE	5.648	6.355	1941500	16739600	1.629	2.569 #
17) MA 4,4'-DDT	6.403	7.148	3926827	17398154	3.386	3.216

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
Data File : PD065992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2021 12:10
Operator : AR\AJ
Sample : M3877-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:53:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

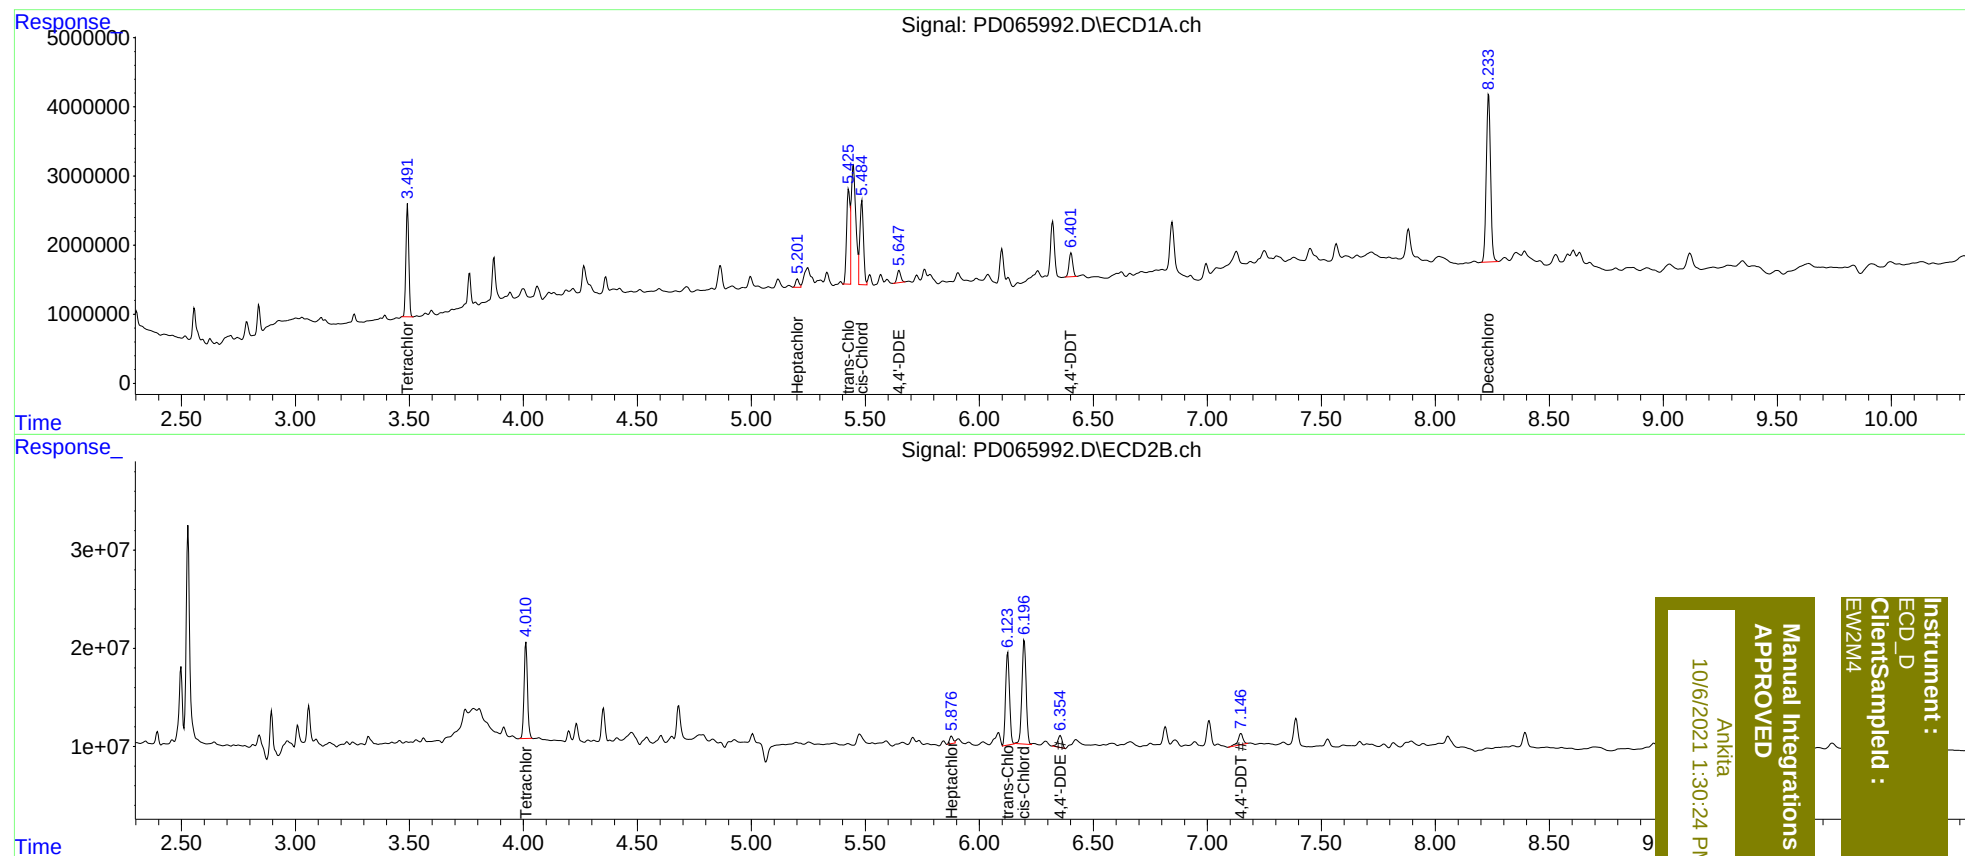

Manual Integrations
APPROVED

Ankita
10/6/2021 1:30:24 PM

Instrument :
ECD_D
ClientSampled :
EW2M4