

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
 Data File : PD065998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2021 13:32
 Operator : AR\AJ
 Sample : M3877-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2N0

Manual Integrations
 APPROVED

Ankita
 10/6/2021 1:30:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 01:58:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	4.012	15629761	107.4E6	18.059	15.101
27)	SA Decachlor...	8.233	9.082	36638488	124.9E6	24.778	28.871m
Target Compounds							
10)	B trans-Chl...	5.428	6.123	11364728	133.7E6	8.723	18.764m#
11)	B cis-Chlor...	5.485	6.197	17831180	179.4E6	13.705	25.680 #
12)	B 4,4'-DDE	5.648	6.355	21093128	118.5E6	17.696	18.189
16)	A 4,4'-DDD	6.166	6.850	2668974	22169137	2.496m	4.014m#
17)	MA 4,4'-DDT	6.403	7.146	9496329	34550755	8.188	6.386m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
Data File : PD065998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2021 13:32
Operator : AR\AJ
Sample : M3877-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 01:58:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

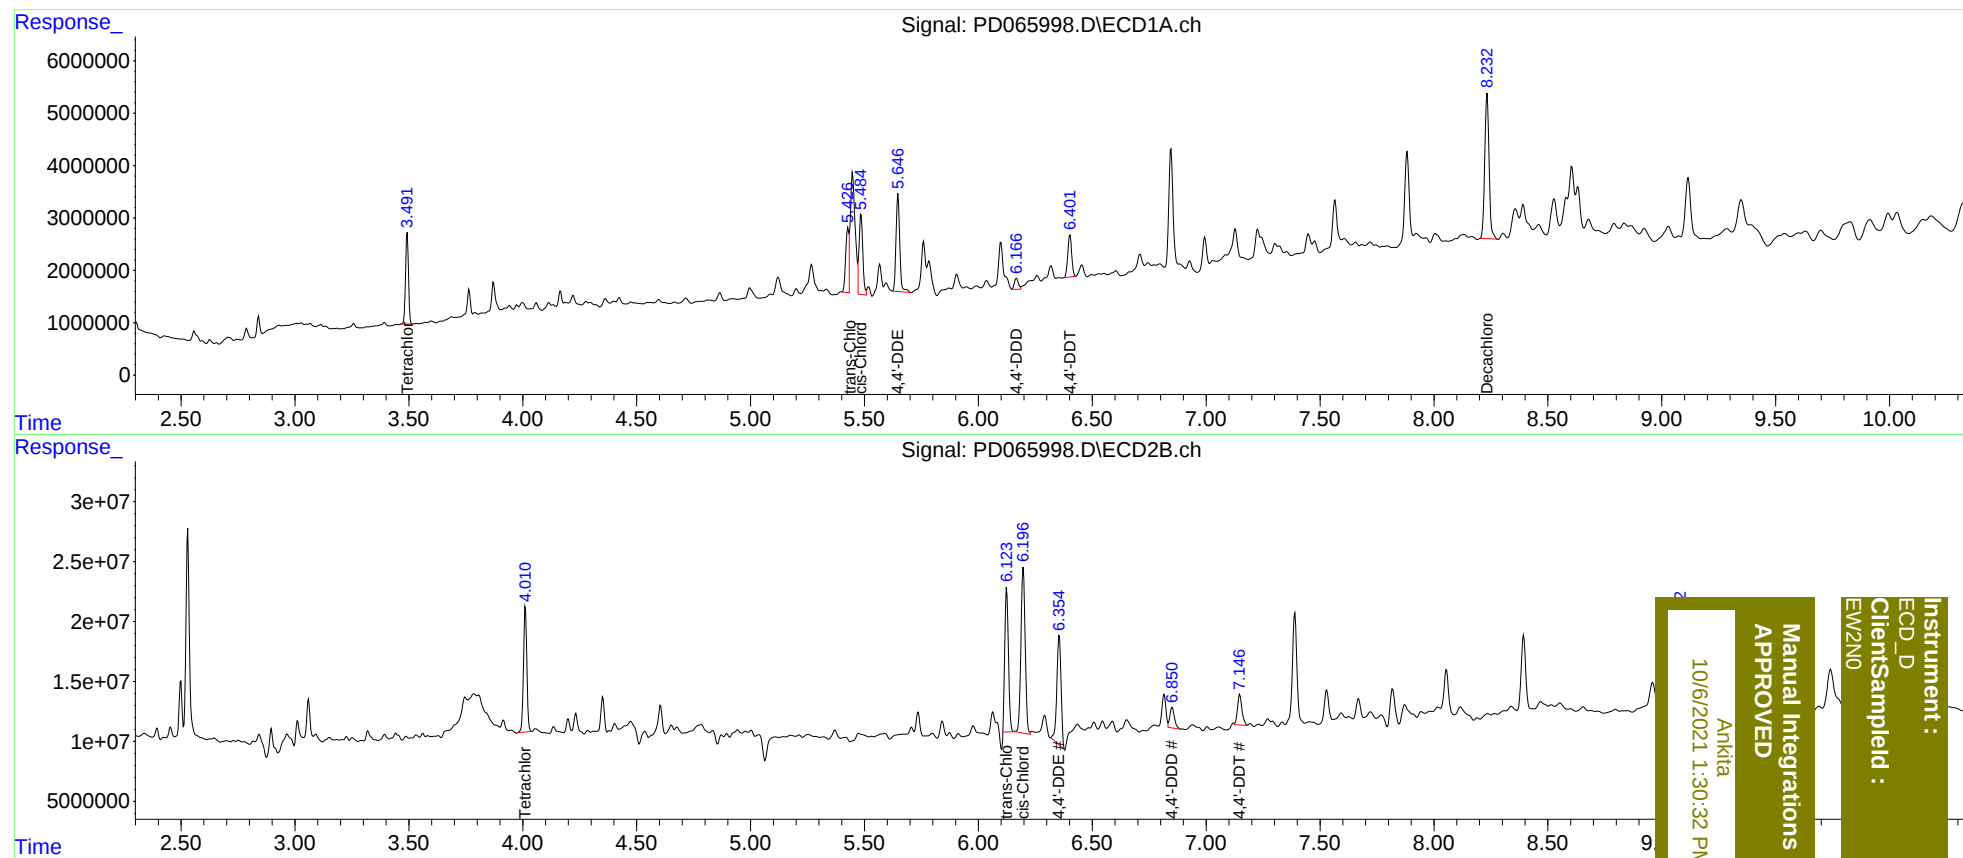

Manual Integrations
APPROVED

Ankita
10/6/2021 1:30:32 PM

Instrument :
ECD_D
Client Sample :
EW2N0