

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
 Data File : PD065994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2021 12:37
 Operator : AR\AJ
 Sample : M3877-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW2M6

Manual Integrations
 APPROVED

Ankita
 10/6/2021 1:30:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 05:00:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 04 09:46:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.493	4.012	16692077	115.8E6	19.286	16.285
2) SA Decachlor...	8.233	9.083	39428410	162.2E6	26.665	37.505m#
Target Compounds						
10) B trans-Chl...	5.428	6.123	12593141	138.0E6	9.666	19.364m#
11) B cis-Chlor...	5.485	6.197	20004067	199.3E6	15.375	28.525 #
12) B 4,4'-DDE	5.648	6.355	22825640	134.9E6	19.150	20.695
17) MA 4,4'-DDT	6.402	7.148	8696101	29104791	7.498	5.379 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093021\
Data File : PD065994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2021 12:37
Operator : AR\AJ
Sample : M3877-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 05:00:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092021CLP.M
Quant Title : GC Extractables
QLast Update : Mon Oct 04 09:46:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

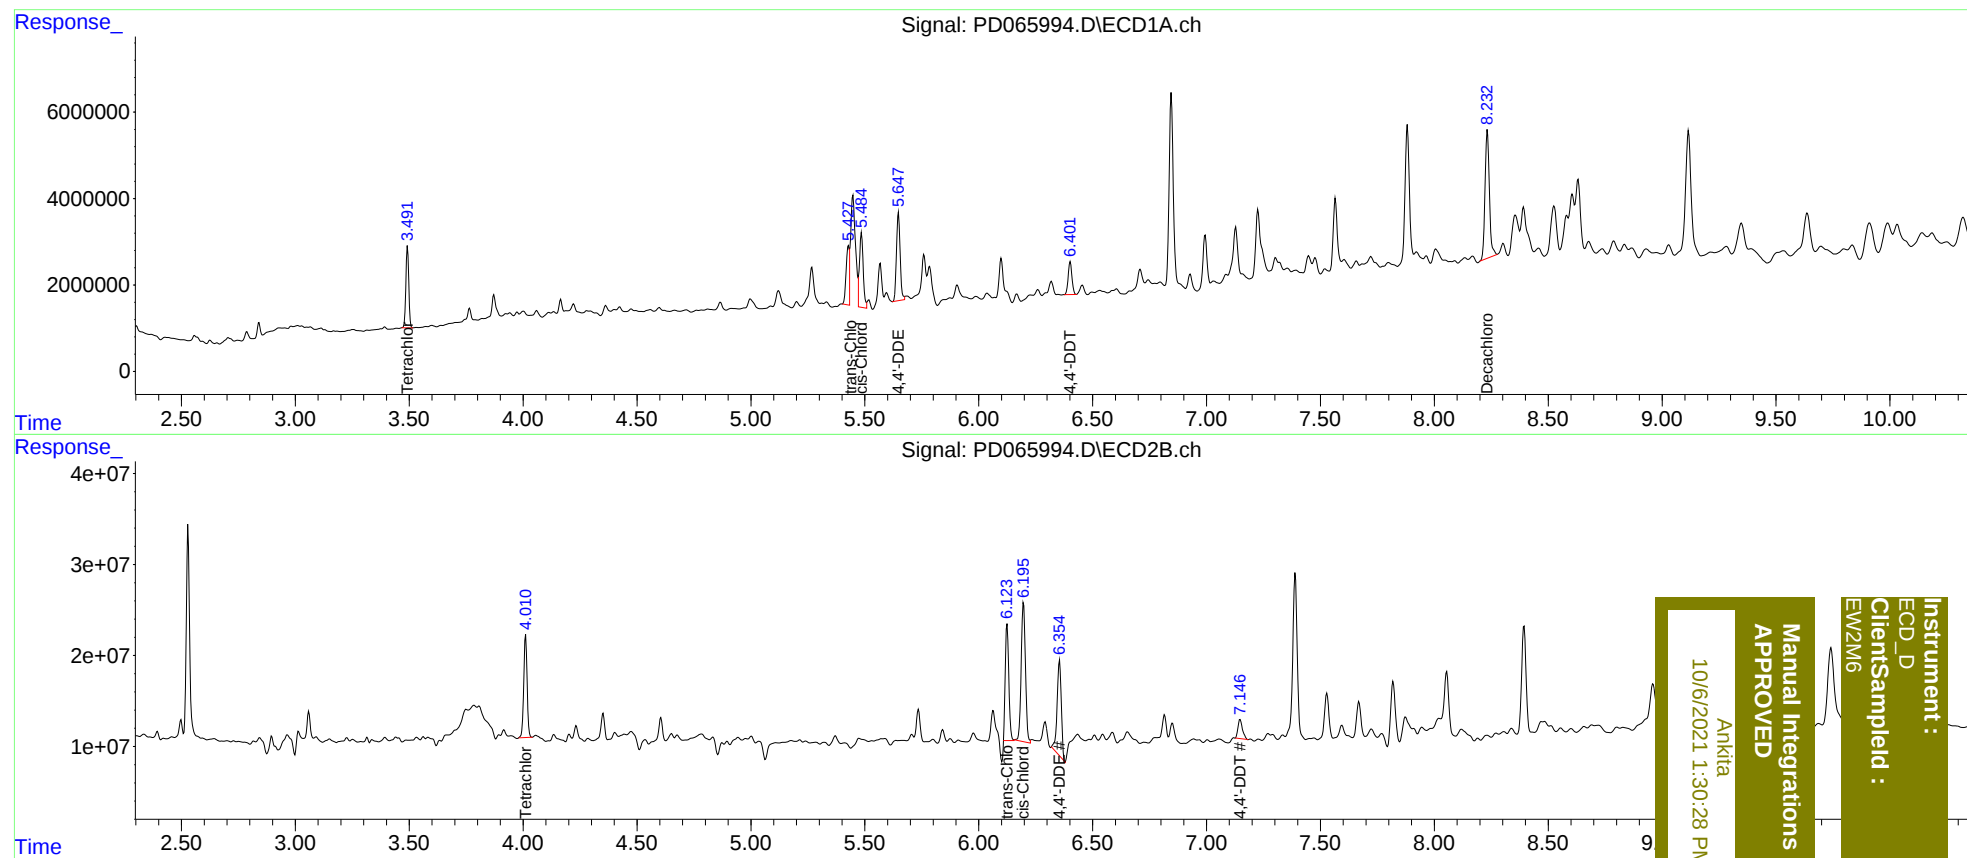

Manual Integrations
APPROVED

10/6/2021 1:30:28 PM

Ankita

Instrument :
ECD_D
ClientSampled :
EW2M6