

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
 Data File : PD072130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 11:58
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 12:09:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 30 11:50:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	13768068	156.8E6	4.745	5.486
28)	SA Decachlor...	7.989	9.085	12603459	51607868	5.625	5.709
Target Compounds							
23)	Chlordane-1	3.813	4.723	5016090	55891269	52.011	59.606
24)	Chlordane-2	4.396	5.255	5820570	42311713	57.339	63.451
25)	Chlordane-3	5.032	5.968	15310547	128.6E6	47.524	59.831 #
26)	Chlordane-4	5.096	6.046	14522814	151.8E6	49.143	60.592
27)	Chlordane-5	5.998	6.908	5319521	26758381	48.834	54.443


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
Data File : PD072130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 11:58
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 12:09:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
Quant Title : GC Extractables
QLast Update : Fri Sep 30 11:50:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

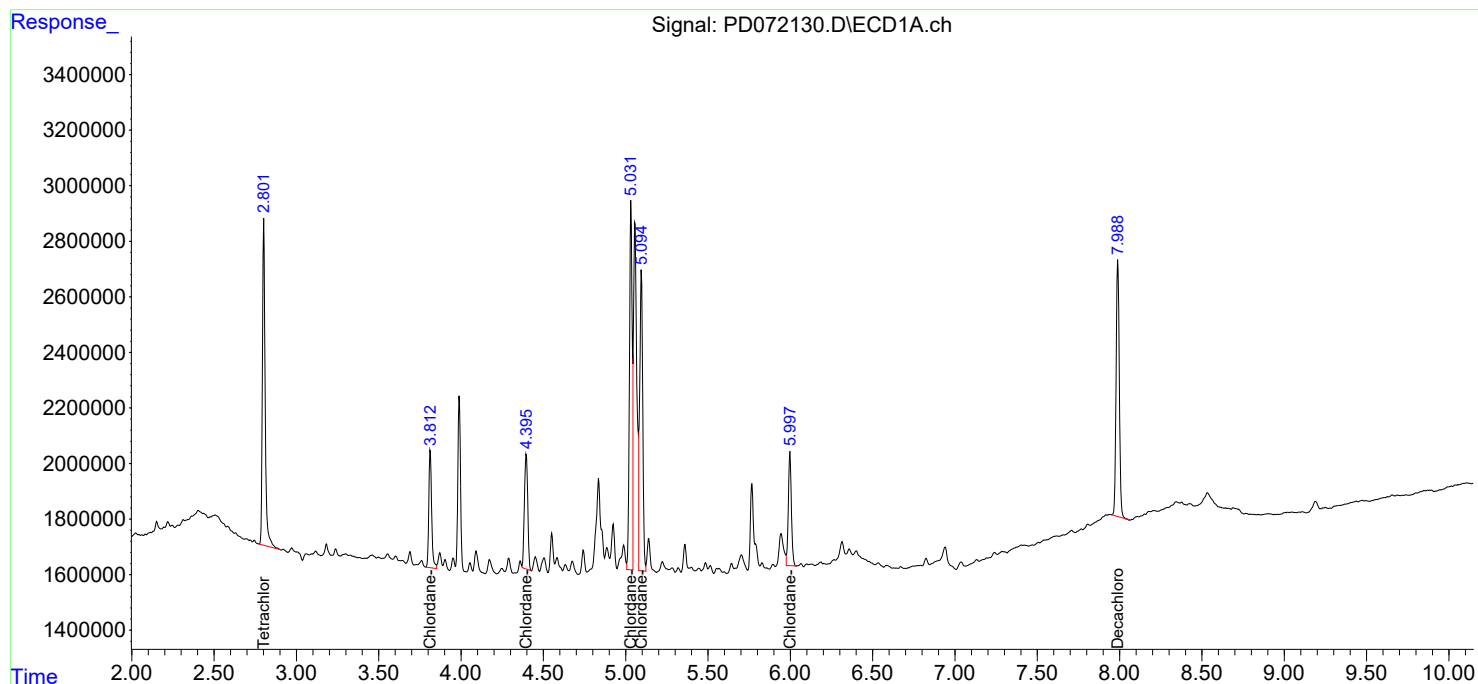


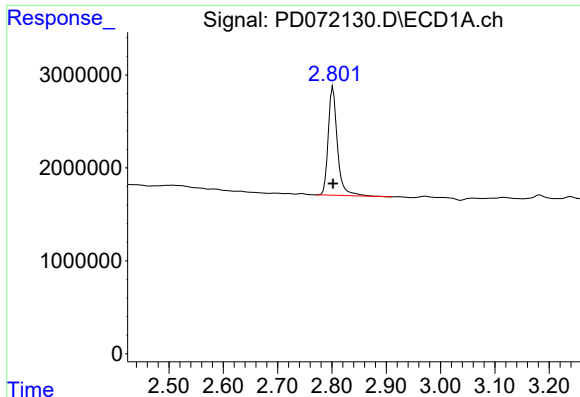

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 13768068
Conc: 4.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

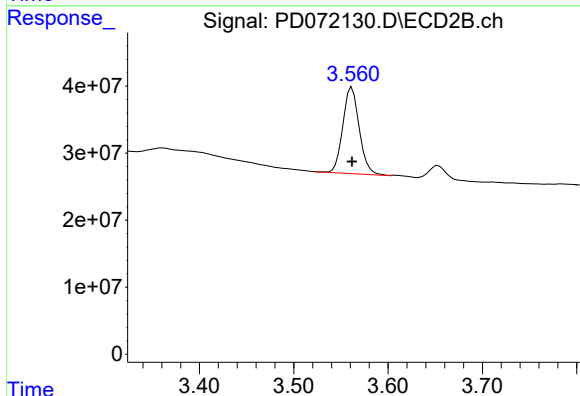


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 156843302
Conc: 5.49 ng/ml

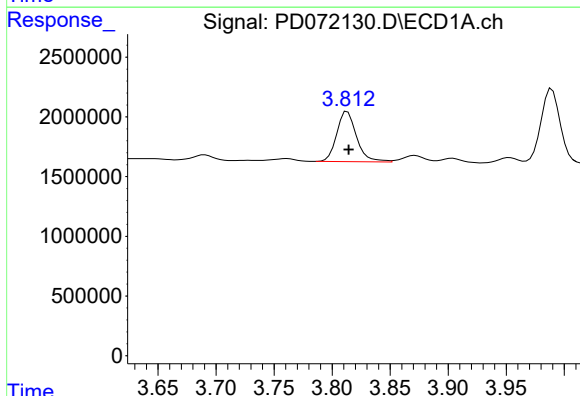


#23 Chlordane-1

R.T.: 3.813 min
Delta R.T.: -0.001 min
Response: 5016090
Conc: 52.01 ng/ml

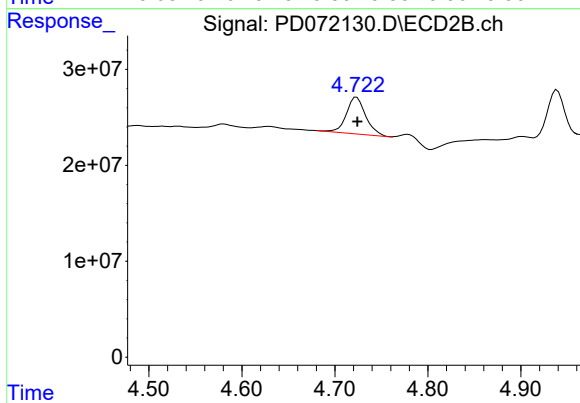

#23 Chlordane-1


R.T.: 4.723 min
Delta R.T.: -0.001 min
Response: 55891269
Conc: 59.61 ng/ml

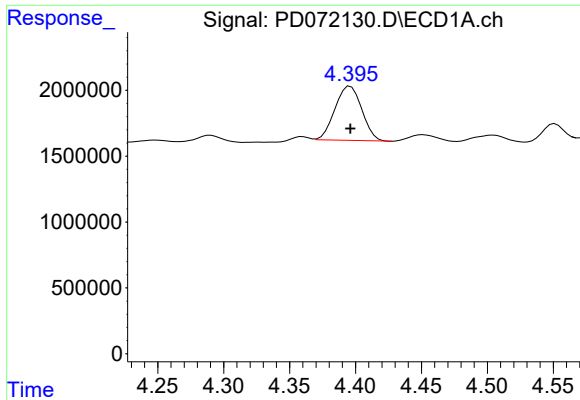

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 5820570
Conc: 57.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

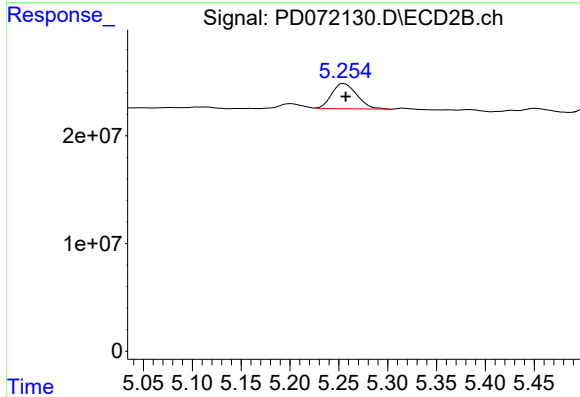


#24 Chlordane-2

R.T.: 5.255 min
Delta R.T.: -0.002 min
Response: 42311713
Conc: 63.45 ng/ml

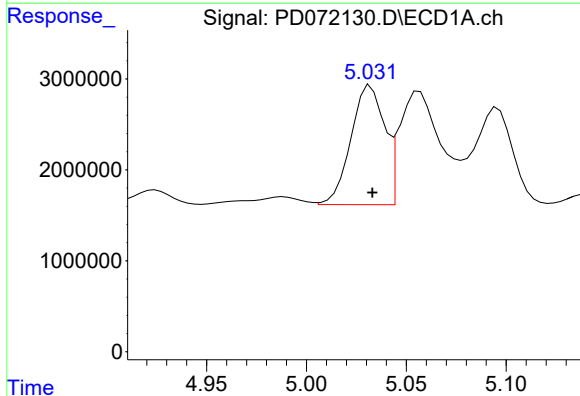


#25 Chlordane-3

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 15310547
Conc: 47.52 ng/ml

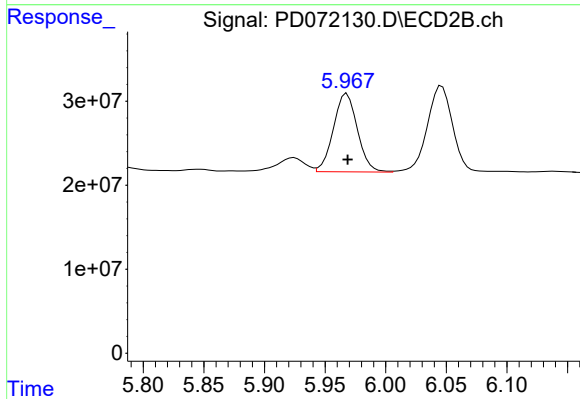

#25 Chlordane-3


R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 128641654
Conc: 59.83 ng/ml

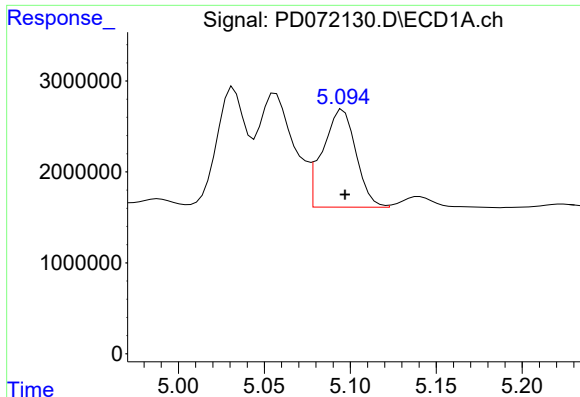

#26 Chlordane-4


R.T.: 5.096 min
Delta R.T.: -0.001 min
Response: 14522814
Conc: 49.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

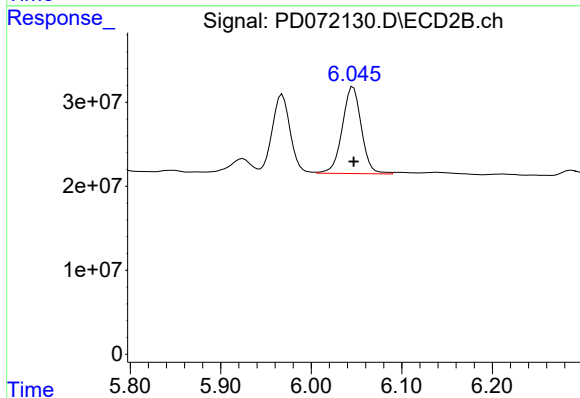


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 151805692
Conc: 60.59 ng/ml

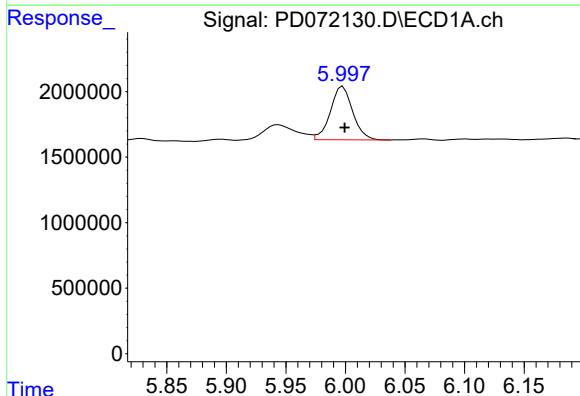


#27 Chlordane-5

R.T.: 5.998 min
Delta R.T.: -0.001 min
Response: 5319521
Conc: 48.83 ng/ml

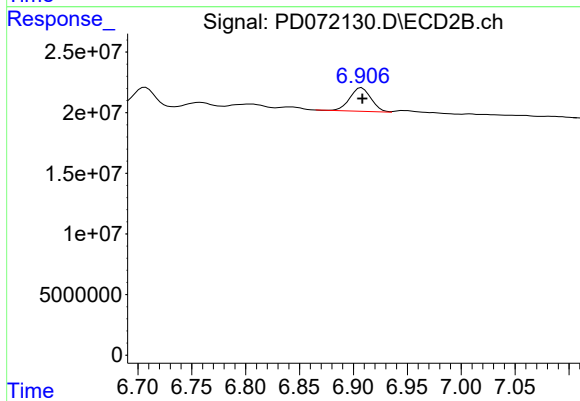

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 26758381
Conc: 54.44 ng/ml

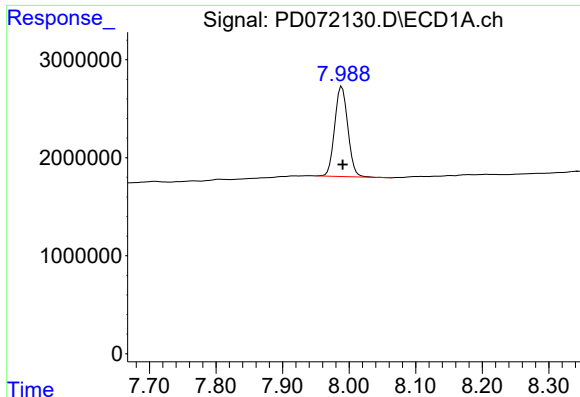

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.001 min
Response: 12603459
Conc: 5.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

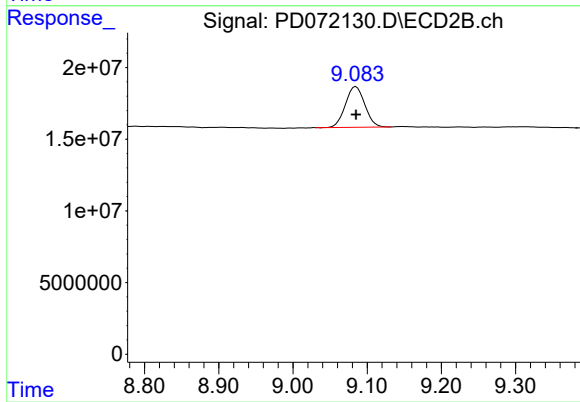

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 51607868
Conc: 5.71 ng/ml