

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
 Data File : PD072120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 09:42
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 16:03:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 30 14:13:47 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.803	3.562	57789937	732.5E6	23.261	24.640
28)	SA Decachlor...	7.990	9.085	52938260	224.9E6	23.086	23.681
Target Compounds							
9)	A Endosulfan I	5.153	6.101	33071607	192.8E6	11.188	12.574
10)	B gamma-Chl...	5.033	5.968	36309503	207.8E6	11.202	12.615
12)	B 4,4'-DDE	5.288	6.218	65076880	353.9E6	22.125	23.250
13)	MA Dieldrin	5.420	6.378	70762325	375.6E6	22.758	23.855
19)	B Endosulfa...	6.397	7.201	52255337	248.8E6	20.693	21.564
20)	A Methoxychlor	6.677	7.530	148.3E6	634.1E6	107.122	102.426
21)	B Endrin ke...	6.906	7.692	64504809	296.2E6	22.449	23.156



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
Data File : PD072120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 09:42
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 16:03:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
Quant Title : GC Extractables
QLast Update : Fri Sep 30 14:13:47 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

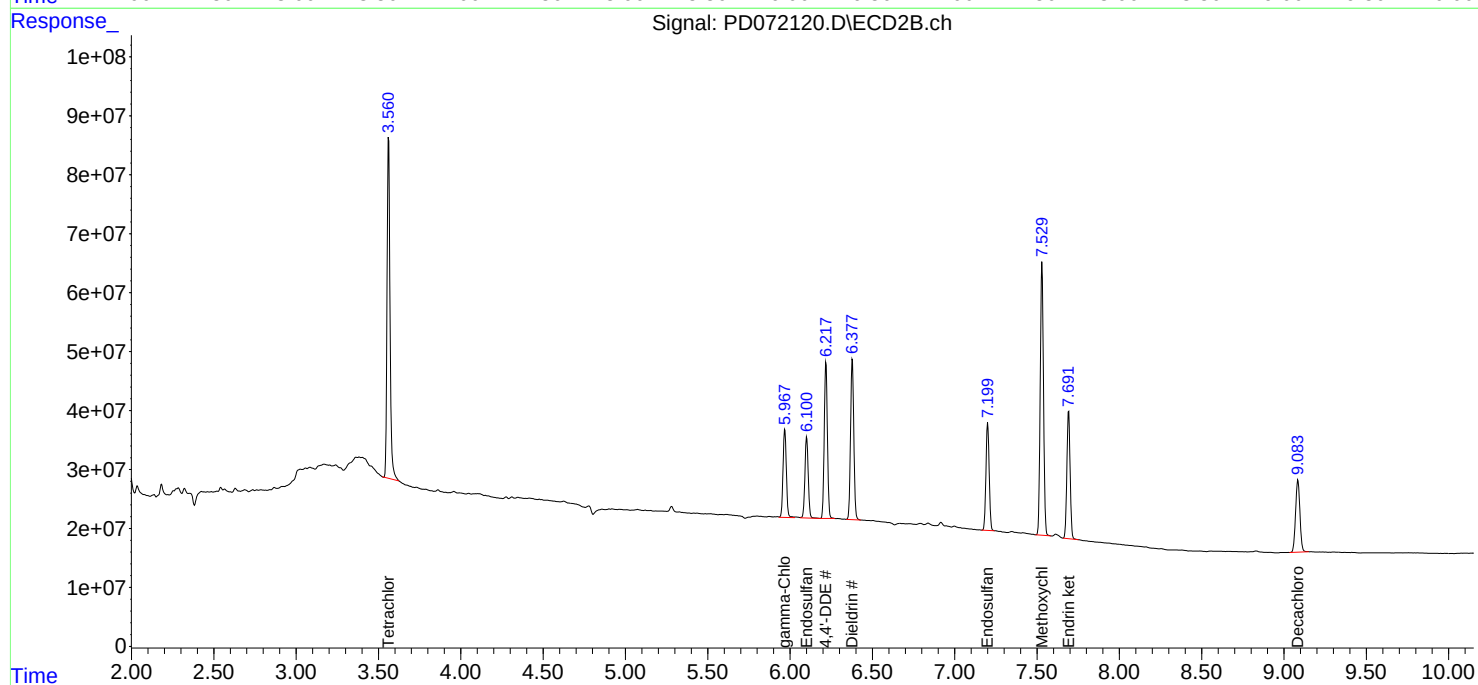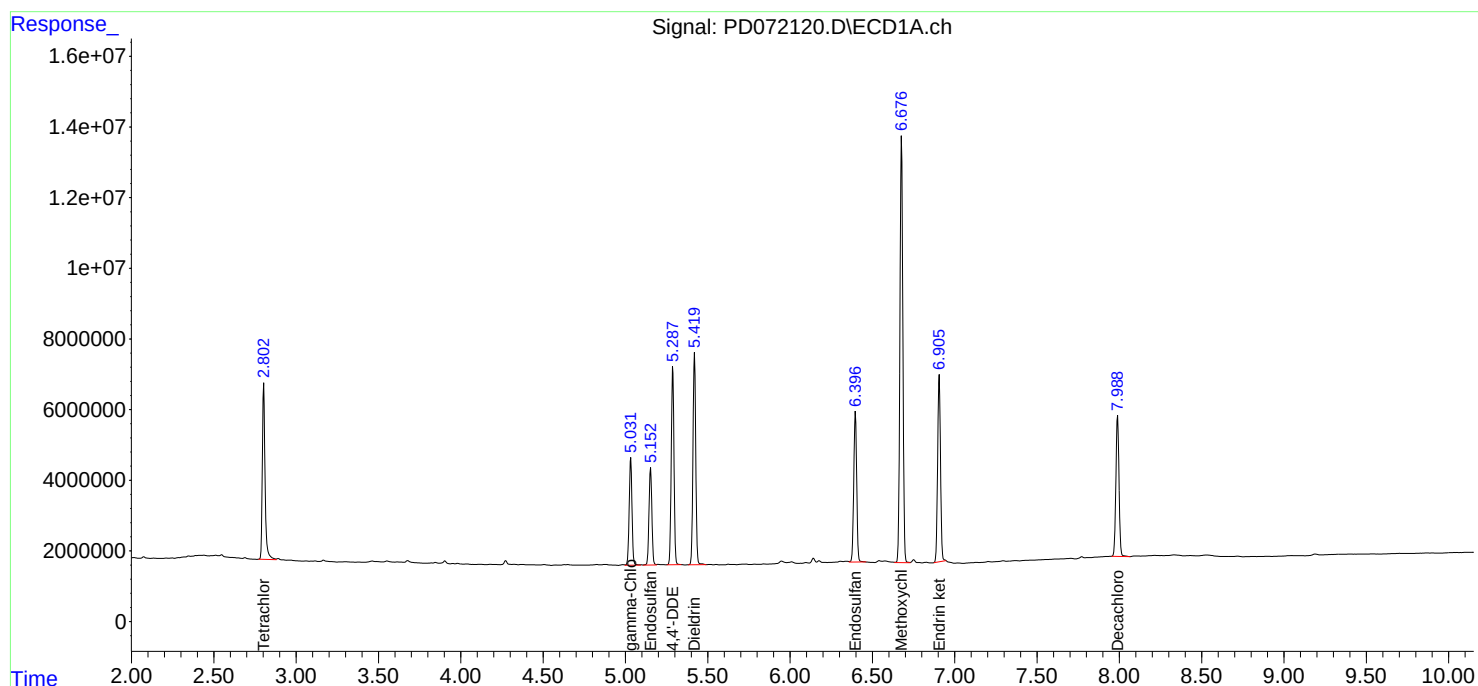


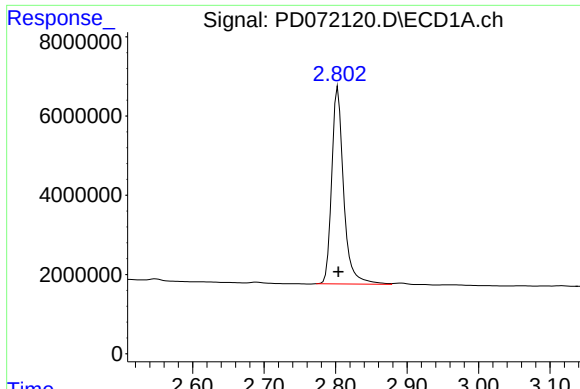

#1 Tetrachloro-m-xylene


R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 57789937
Conc: 23.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

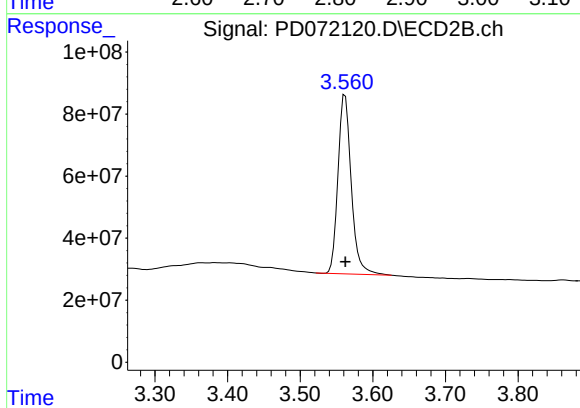


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 732497503
Conc: 24.64 ng/ml

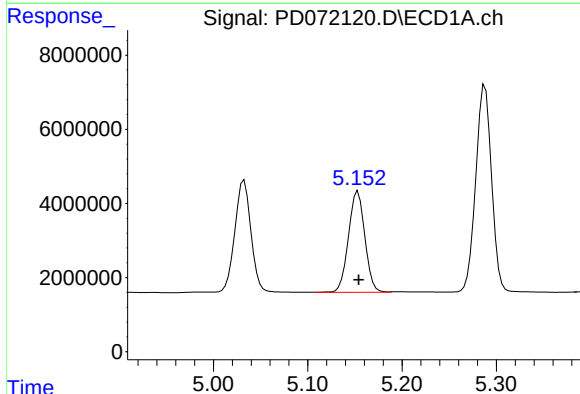


#9 Endosulfan I

R.T.: 5.153 min
Delta R.T.: 0.000 min
Response: 33071607
Conc: 11.19 ng/ml

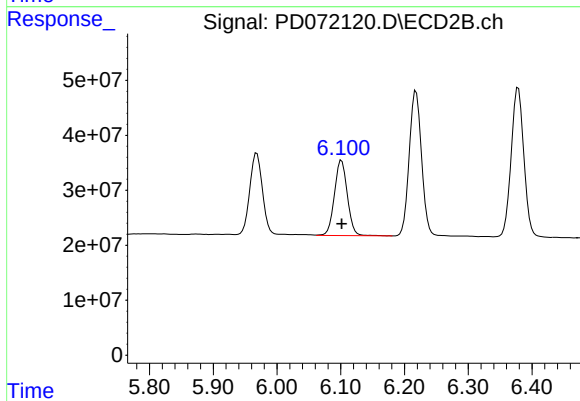

#9 Endosulfan I


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 192816750
Conc: 12.57 ng/ml

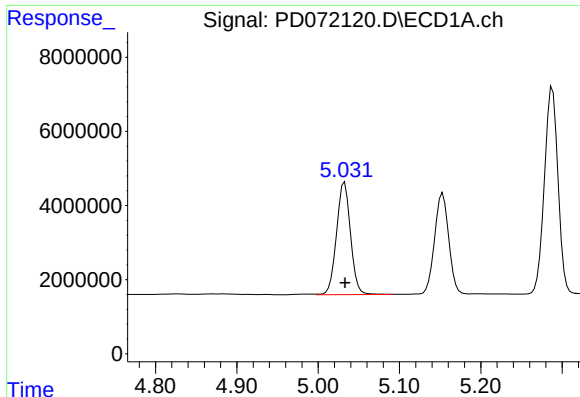

#10 gamma-Chlordane


R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 36309503
Conc: 11.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

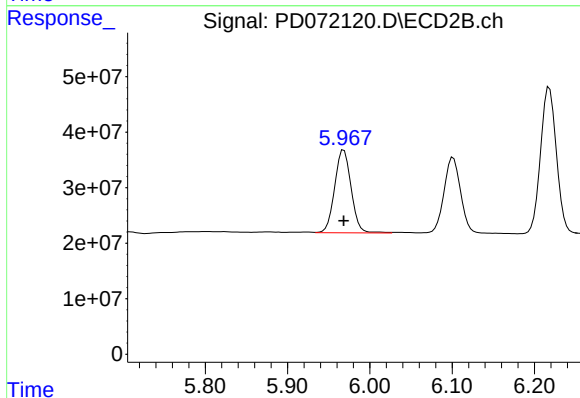


#10 gamma-Chlordane

R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 207799089
Conc: 12.61 ng/ml

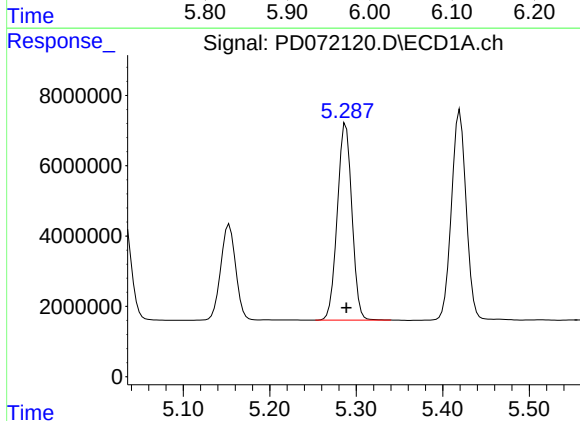


#12 4,4'-DDE

R.T.: 5.288 min
Delta R.T.: 0.000 min
Response: 65076880
Conc: 22.12 ng/ml

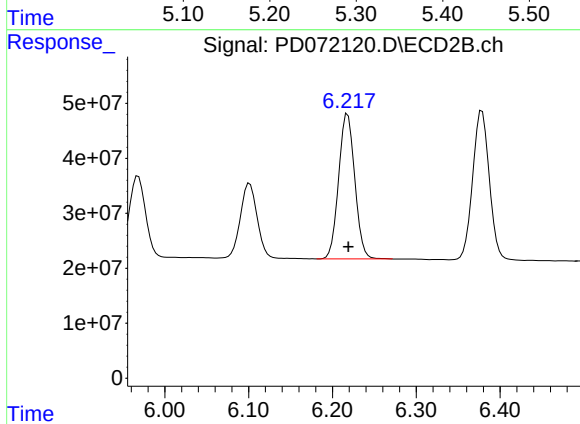

#12 4,4'-DDE


R.T.: 6.218 min
Delta R.T.: 0.000 min
Response: 353851388
Conc: 23.25 ng/ml

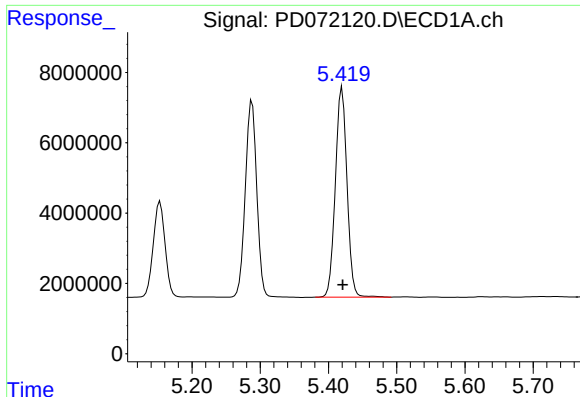

#13 Dieldrin


R.T.: 5.420 min
Delta R.T.: -0.001 min
Response: 70762325
Conc: 22.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

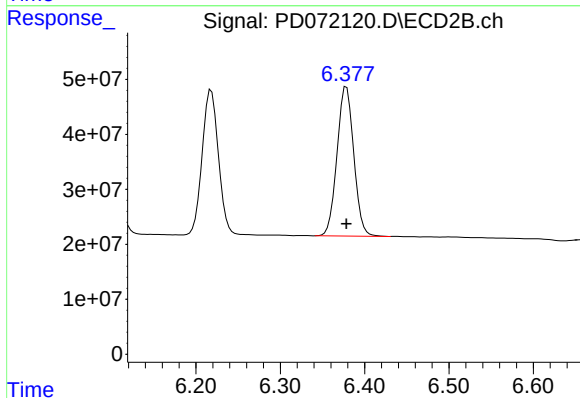


#13 Dieldrin

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 375554834
Conc: 23.85 ng/ml

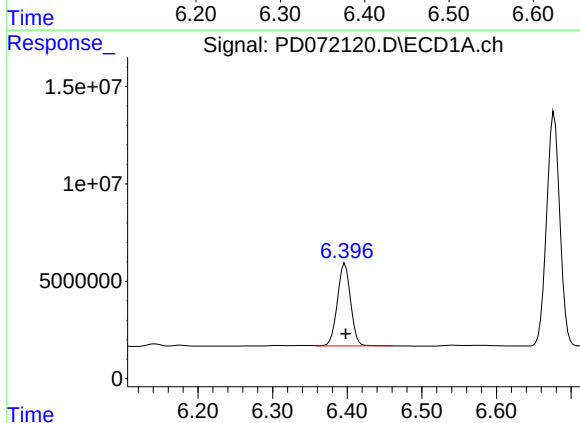


#19 Endosulfan Sulfate

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 52255337
Conc: 20.69 ng/ml

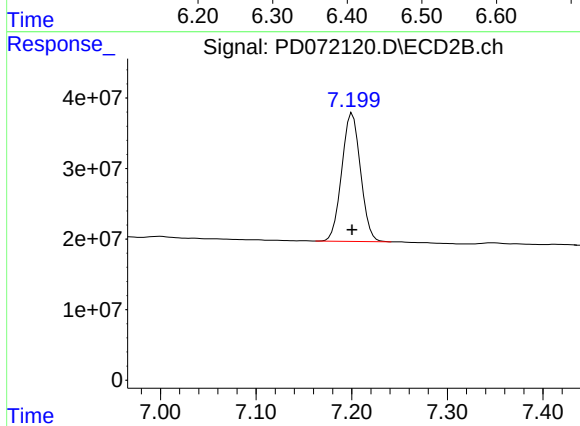

#19 Endosulfan Sulfate


R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 248762903
Conc: 21.56 ng/ml

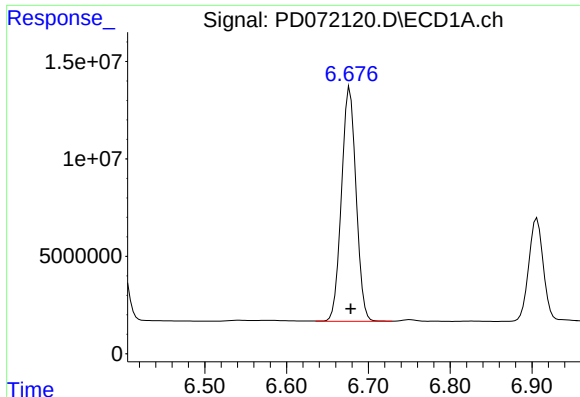

#20 Methoxychlor


R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 148293881
Conc: 107.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

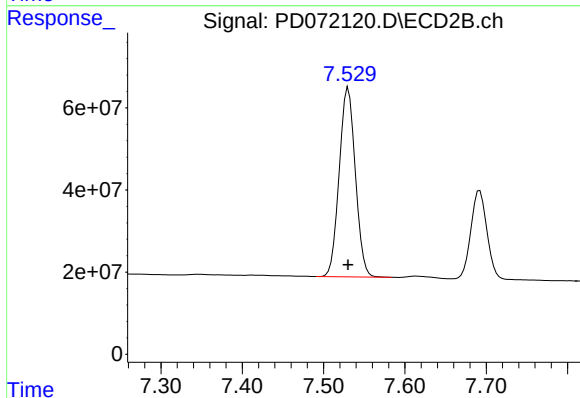


#20 Methoxychlor

R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 634148274
Conc: 102.43 ng/ml

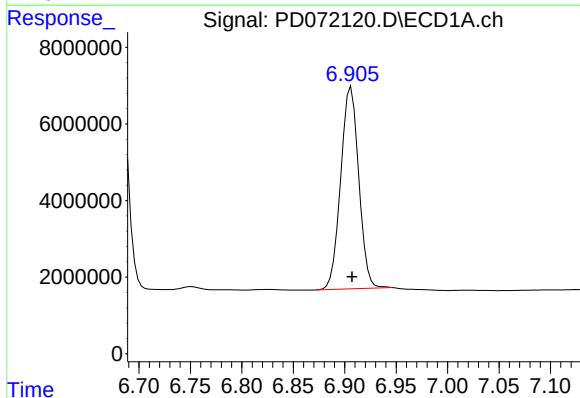


#21 Endrin ketone

R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 64504809
Conc: 22.45 ng/ml

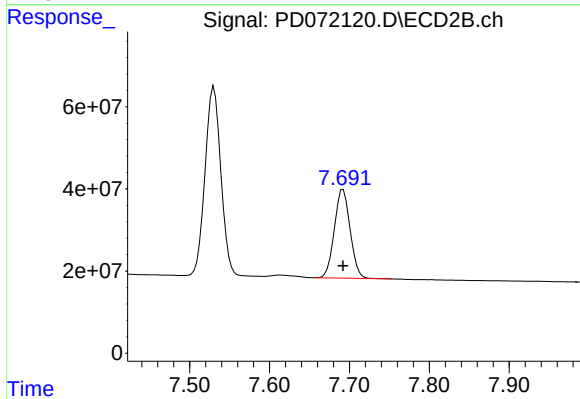

#21 Endrin ketone


R.T.: 7.692 min
Delta R.T.: 0.000 min
Response: 296220086
Conc: 23.16 ng/ml

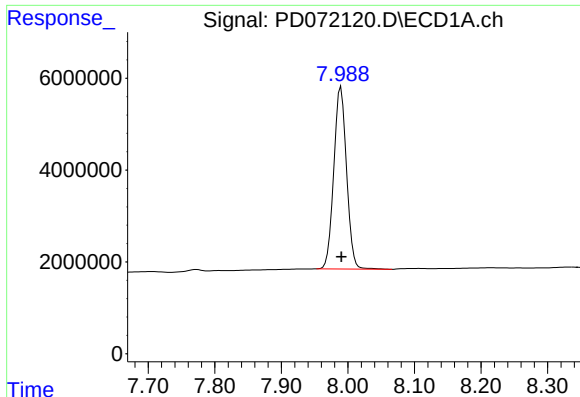

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: 0.000 min
Response: 52938260
Conc: 23.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

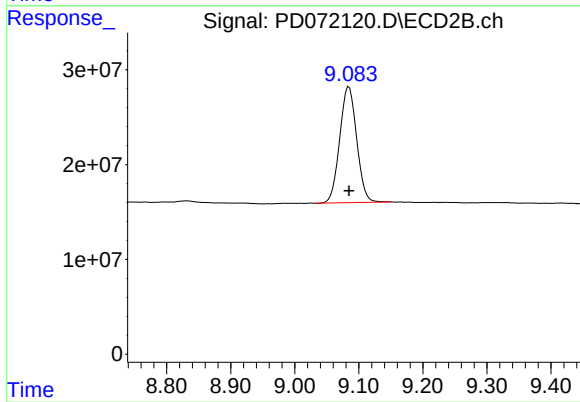

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 224862917
Conc: 23.68 ng/ml