

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
 Data File : PD072127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 11:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 11:52:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 30 11:50:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	218.8E6	2103.0E6	75.327	73.472
28)	SA Decachlor...	7.991	9.084	164.6E6	656.0E6	73.073	71.719
Target Compounds							
23)	Chlordane-1	3.814	4.724	72010423	683.0E6	747.418	722.639
24)	Chlordane-2	4.396	5.256	73713302	479.1E6	724.237	709.199
25)	Chlordane-3	5.033	5.968	242.8E6	1569.8E6	756.950	727.502
26)	Chlordane-4	5.097	6.047	219.3E6	1826.5E6	747.220	726.729
27)	Chlordane-5	5.999	6.908	81324086	361.0E6	746.927	728.348


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
Data File : PD072127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 11:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 11:52:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
Quant Title : GC Extractables
QLast Update : Fri Sep 30 11:50:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

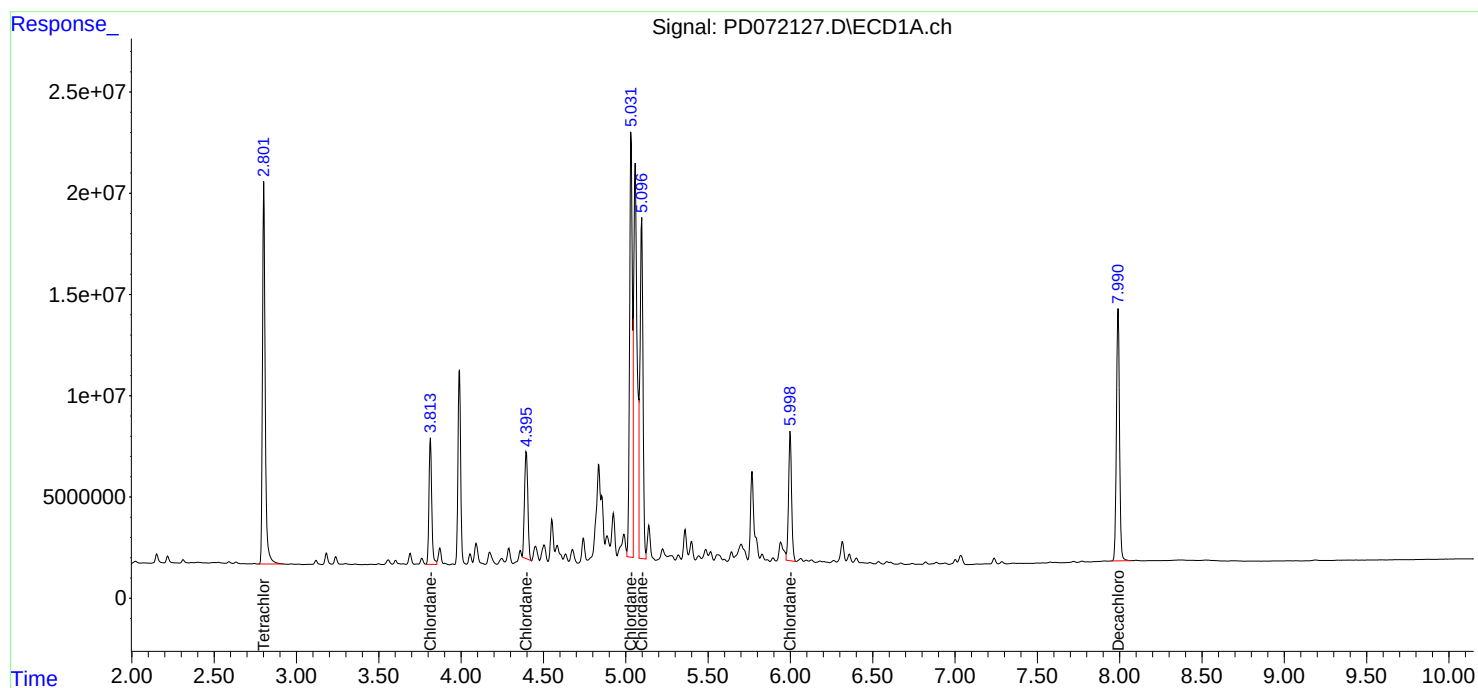


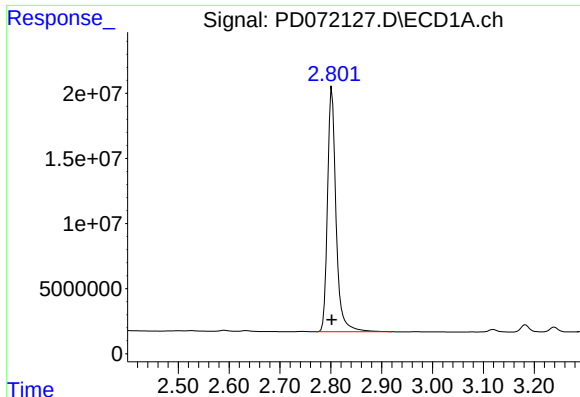

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 218809190
Conc: 75.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

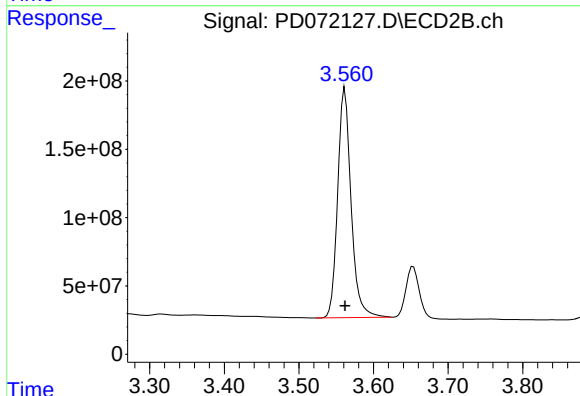


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 2102968516
Conc: 73.47 ng/ml

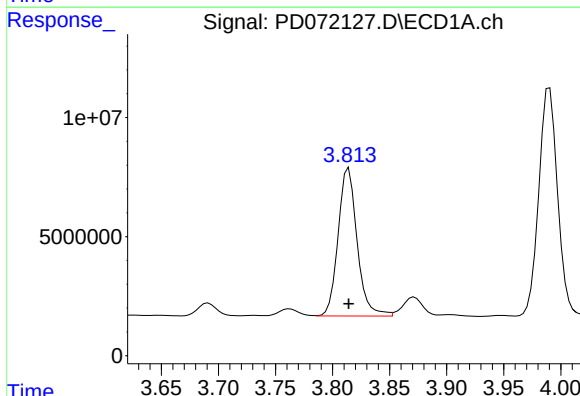


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 72010423
Conc: 747.42 ng/ml

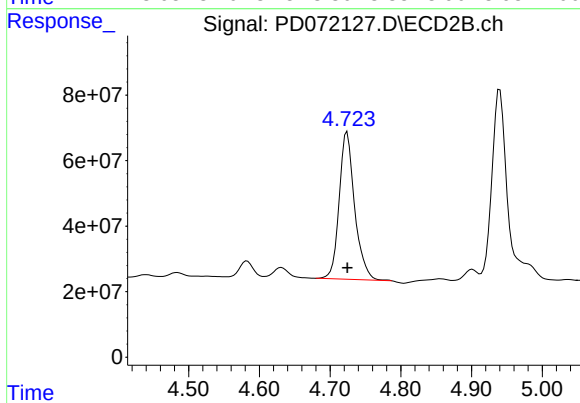

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 683047776
Conc: 722.64 ng/ml

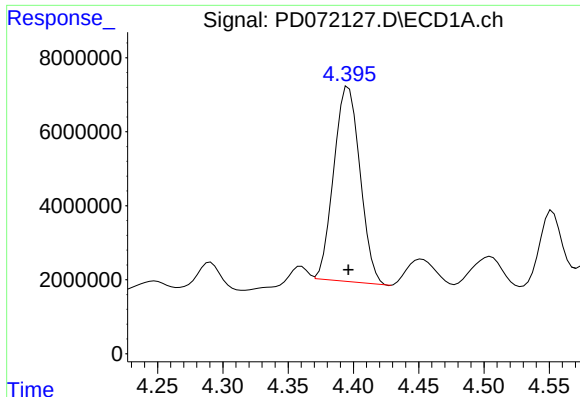

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 73713302
Conc: 724.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

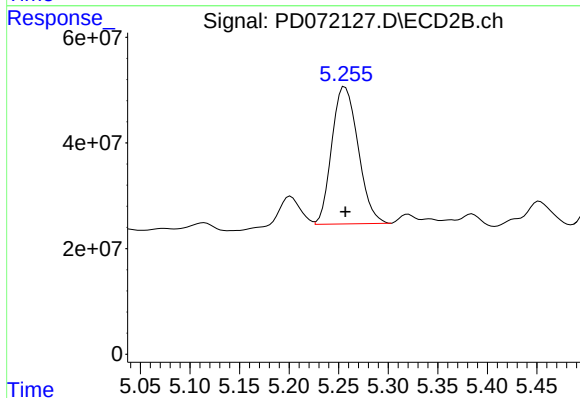


#24 Chlordane-2

R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 479143825
Conc: 709.20 ng/ml

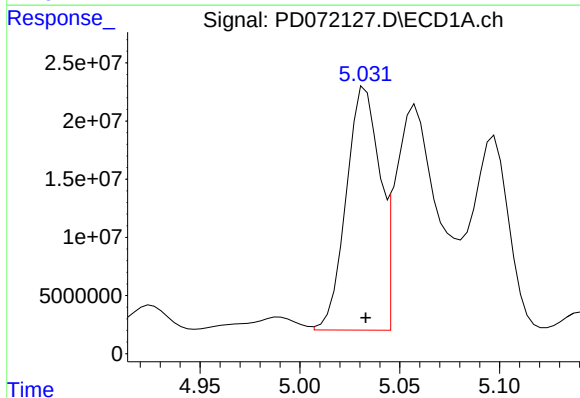


#25 Chlordane-3

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 242766214
Conc: 756.95 ng/ml

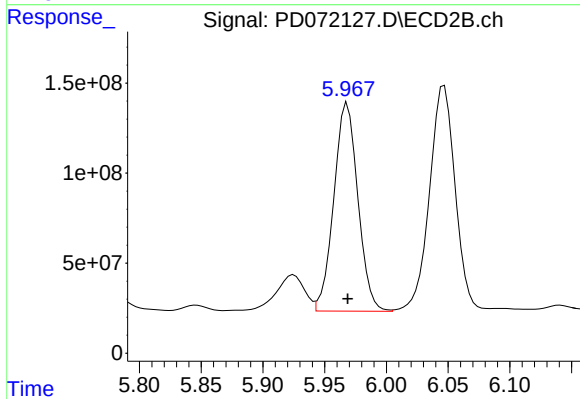

#25 Chlordane-3


R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 1569818906
Conc: 727.50 ng/ml

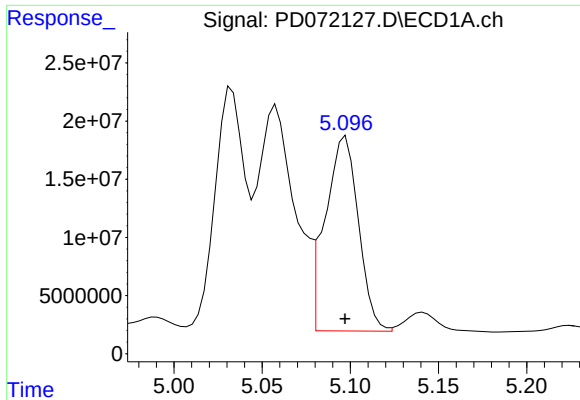

#26 Chlordane-4


R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 219267774
Conc: 747.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

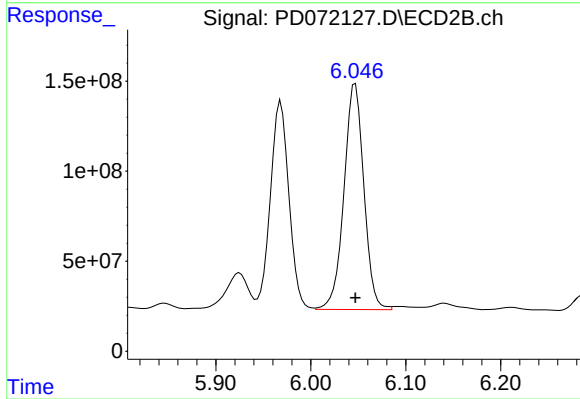


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 1826458150
Conc: 726.73 ng/ml

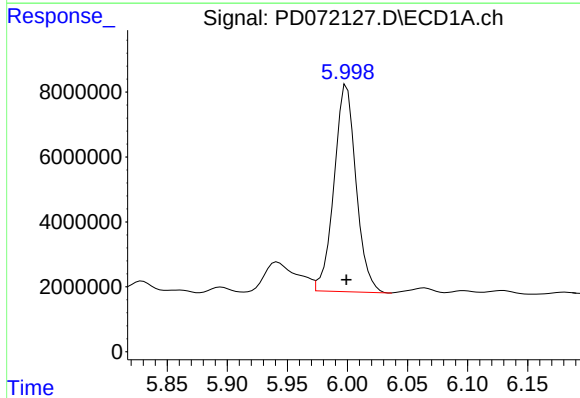


#27 Chlordane-5

R.T.: 5.999 min
Delta R.T.: 0.000 min
Response: 81324086
Conc: 746.93 ng/ml

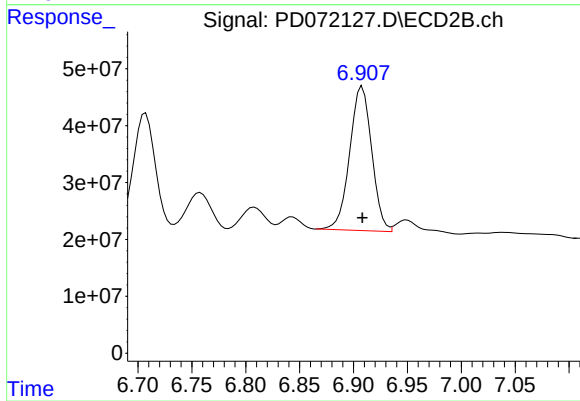

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 360982902
Conc: 728.35 ng/ml

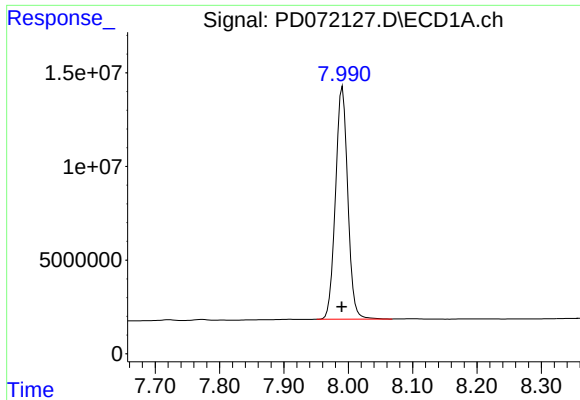

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 164556936
Conc: 73.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

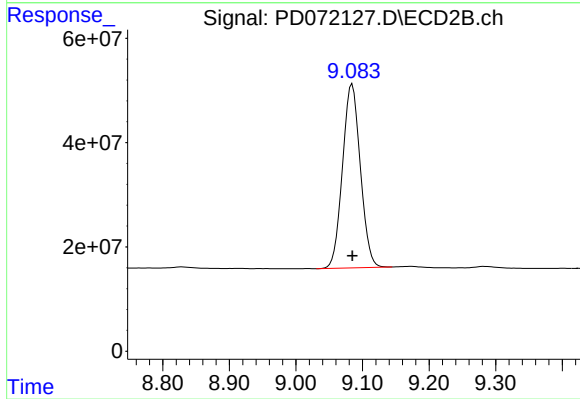

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 655991639
Conc: 71.72 ng/ml