

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
 Data File : PD072128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 11:31
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 11:50:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 30 11:50:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	145.2E6	1431.1E6	50.000	50.000
28)	SA Decachlor...	7.990	9.085	112.6E6	457.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.814	4.724	48172795	472.6E6	500.000	500.000
24)	Chlordane-2	4.396	5.257	50890349	337.8E6	500.000	500.000
25)	Chlordane-3	5.033	5.969	160.4E6	1078.9E6	500.000	500.000
26)	Chlordane-4	5.097	6.047	146.7E6	1256.6E6	500.000	500.000
27)	Chlordane-5	5.999	6.908	54439139	247.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
Data File : PD072128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 11:31
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 11:50:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
Quant Title : GC Extractables
QLast Update : Fri Sep 30 11:50:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

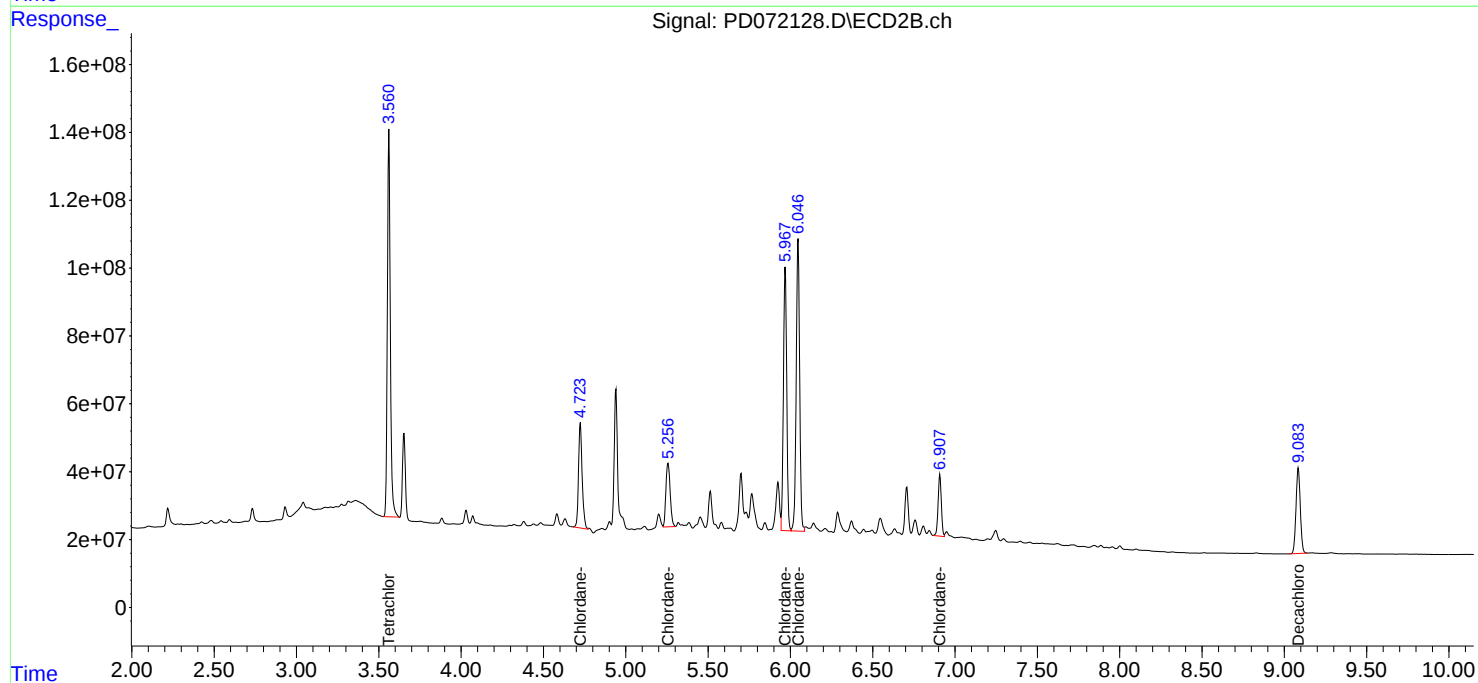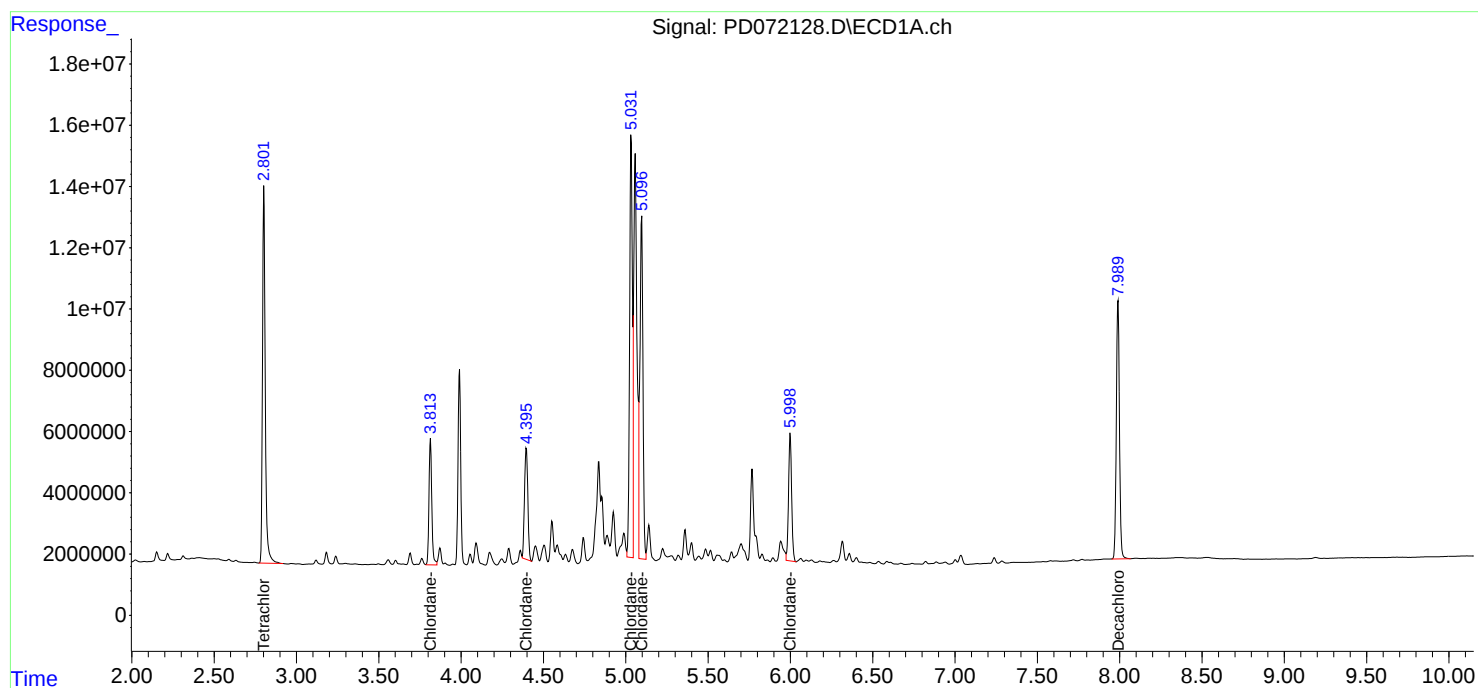


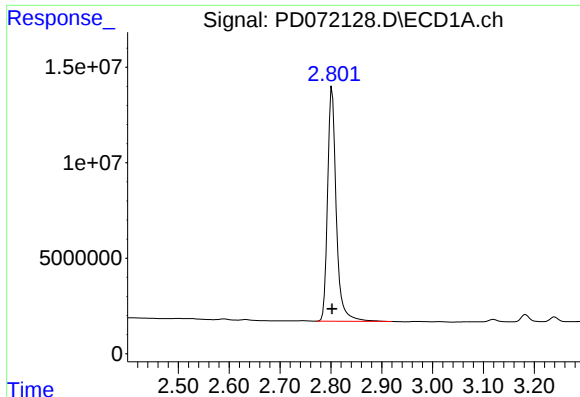

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 145238948
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

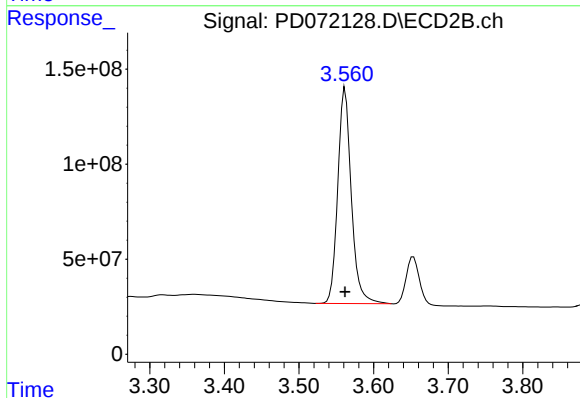


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 1431127582
Conc: 50.00 ng/ml

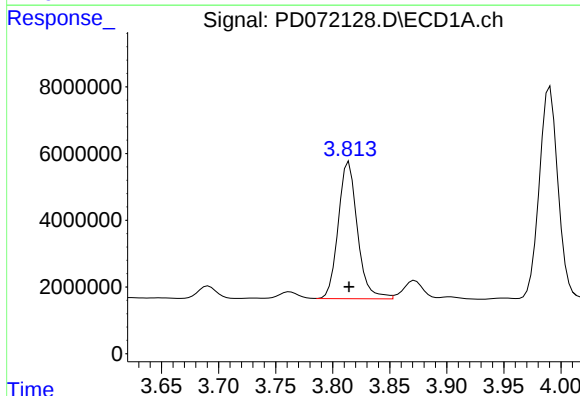


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 48172795
Conc: 500.00 ng/ml

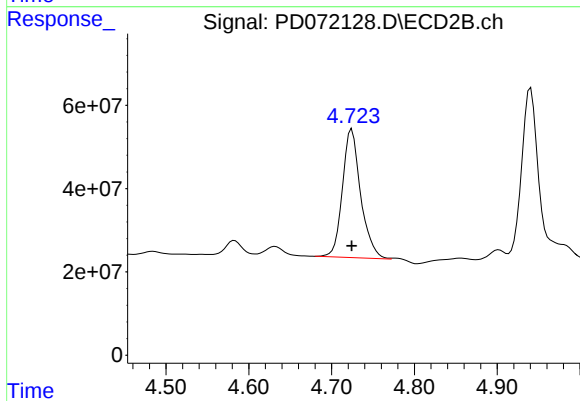

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 472606600
Conc: 500.00 ng/ml

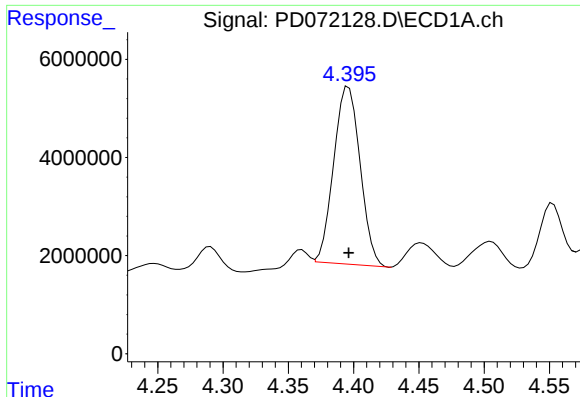

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 50890349
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

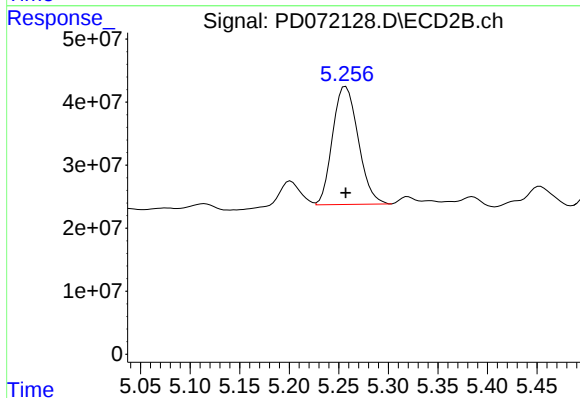


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 337806213
Conc: 500.00 ng/ml

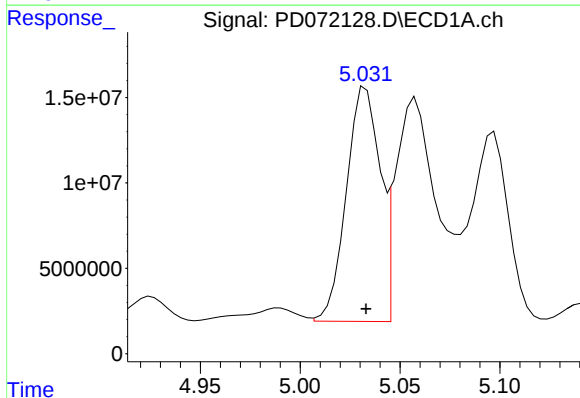


#25 Chlordane-3

R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 160358166
Conc: 500.00 ng/ml

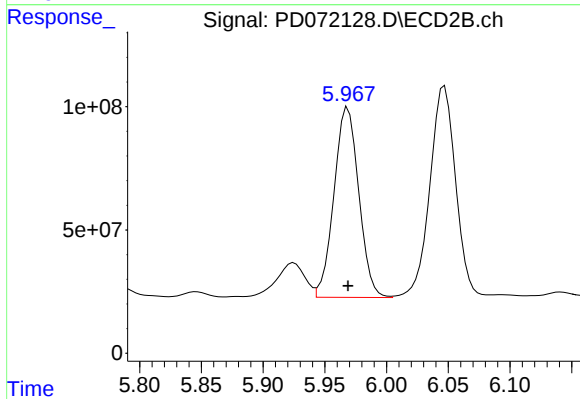

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 1078910008
Conc: 500.00 ng/ml

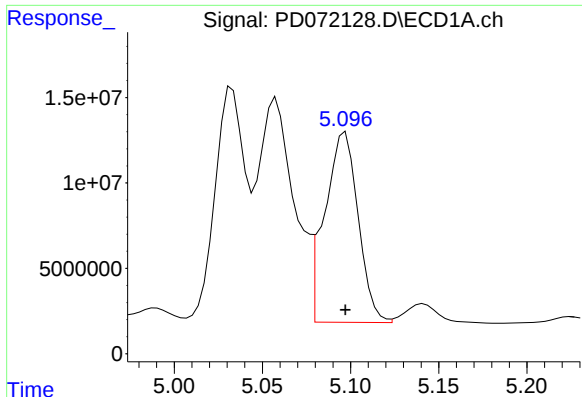

#26 Chlordane-4


R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 146722380
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

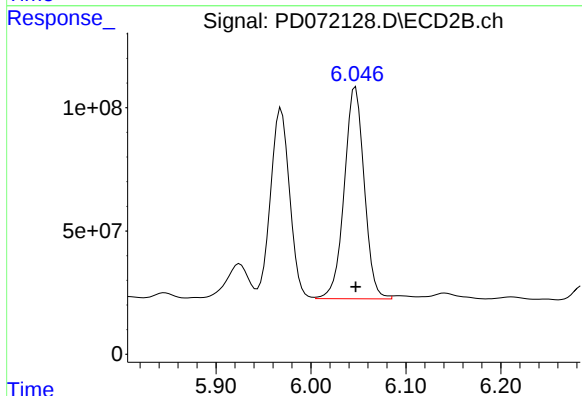


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 1256628902
Conc: 500.00 ng/ml

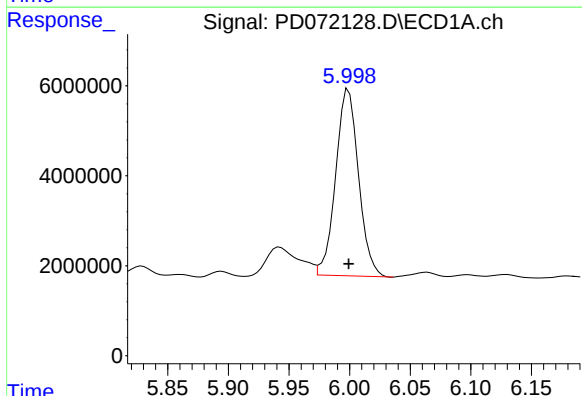


#27 Chlordane-5

R.T.: 5.999 min
Delta R.T.: 0.000 min
Response: 54439139
Conc: 500.00 ng/ml

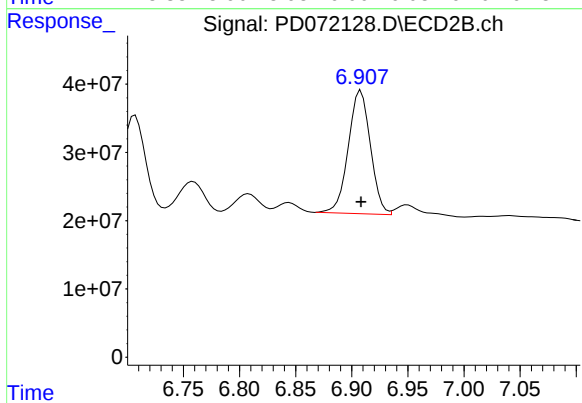

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 247809401
Conc: 500.00 ng/ml

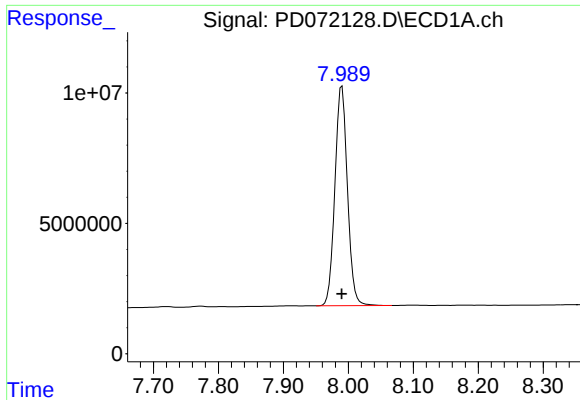

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: 0.000 min
Response: 112597040
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

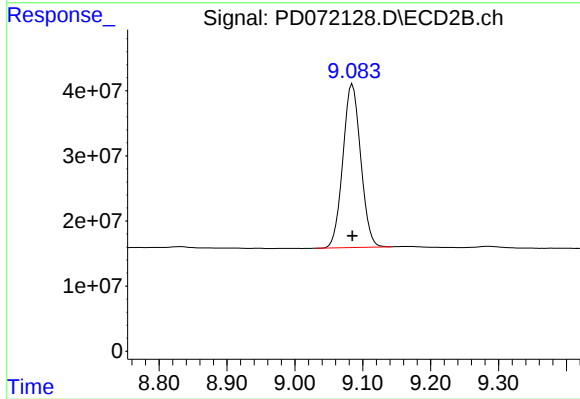

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 457336422
Conc: 50.00 ng/ml