

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
 Data File : PD072137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2022 13:58
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD093022CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 16:04:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 30 14:13:47 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	148.2E6	1443.7E6	59.637	48.566
28)	SA Decachlor...	7.989	9.083	123.0E6	462.9E6	53.638	48.745
Target Compounds							
23)	Chlordane-1	3.814	4.724	49251375	479.0E6	506.601	491.935
24)	Chlordane-2	4.396	5.257	51960134	344.3E6	497.266	489.944
25)	Chlordane-3	5.032	5.968	165.5E6	1082.9E6	518.954	484.586
26)	Chlordane-4	5.096	6.046	152.4E6	1262.7E6	517.311	483.524
27)	Chlordane-5	5.998	6.908	55840118	248.4E6	515.026	496.484



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093022\
Data File : PD072137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2022 13:58
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD093022CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 16:04:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093022.M
Quant Title : GC Extractables
QLast Update : Fri Sep 30 14:13:47 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

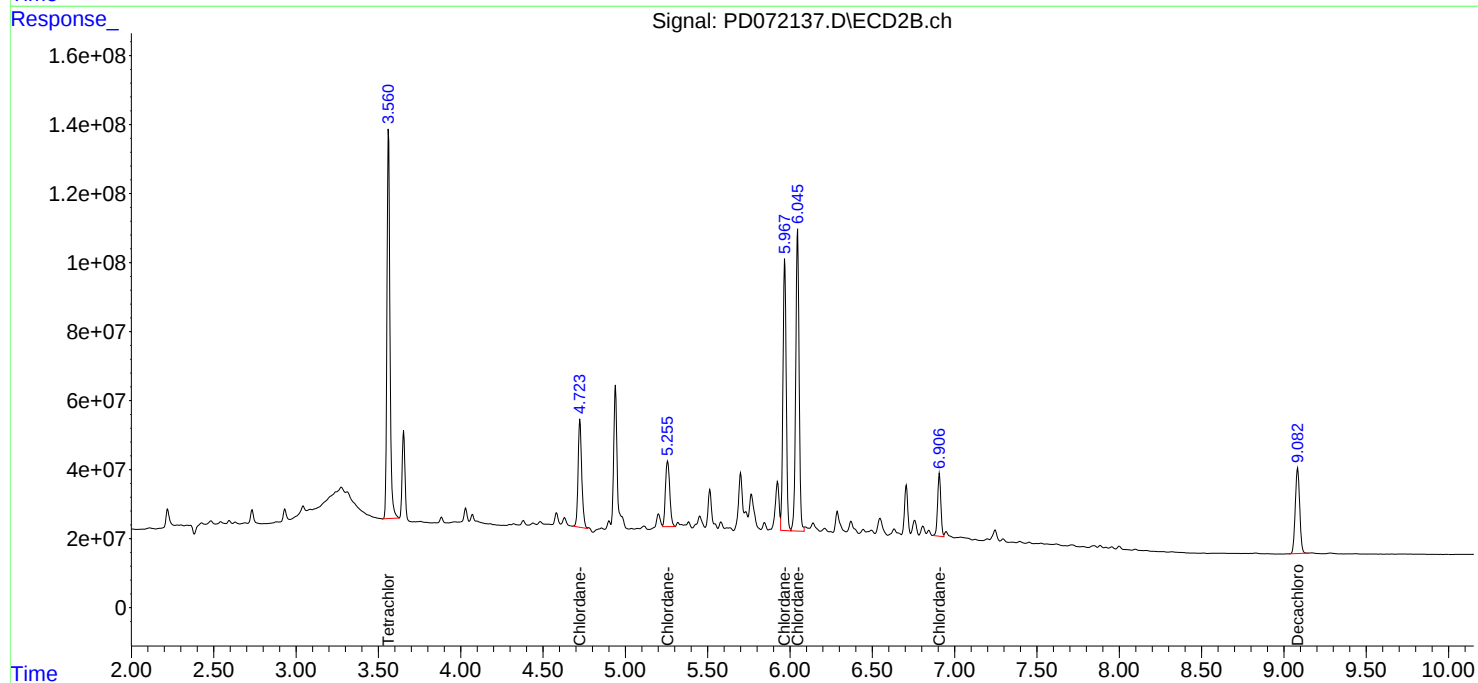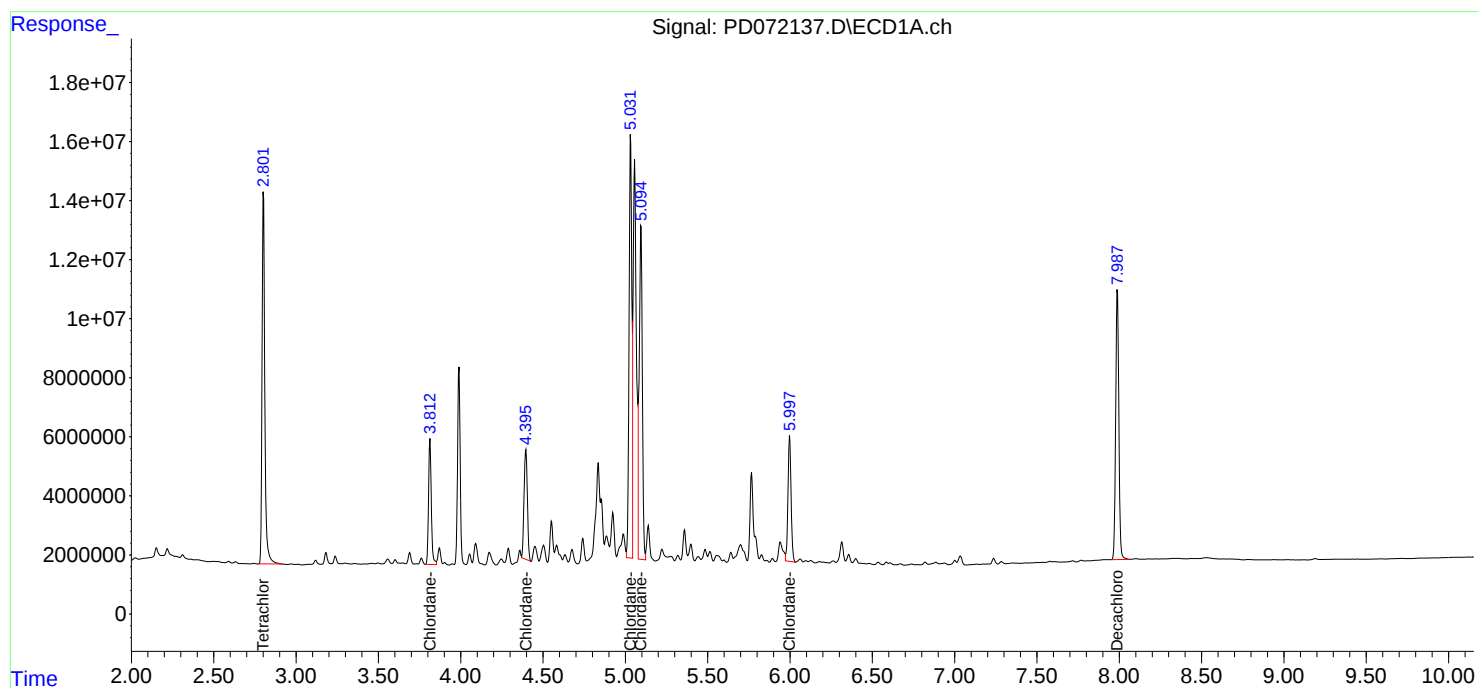


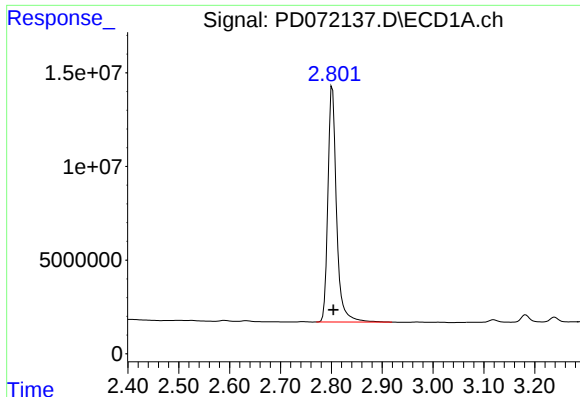

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: -0.002 min
Response: 148164783
Conc: 59.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093022CHLOR

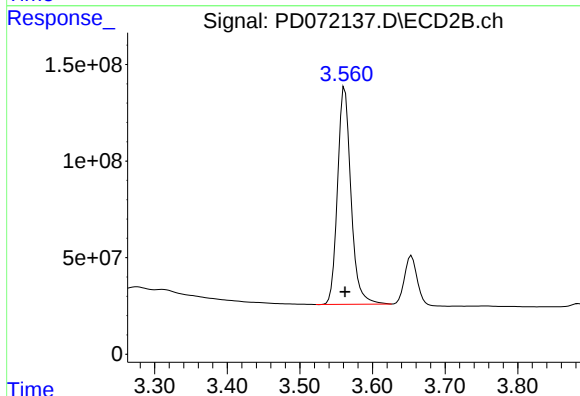


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 1443743012
Conc: 48.57 ng/ml

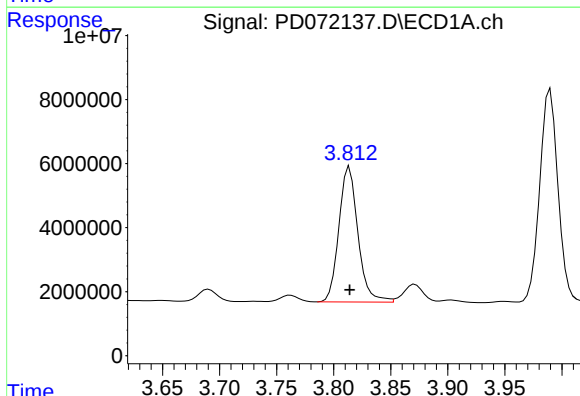


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 49251375
Conc: 506.60 ng/ml

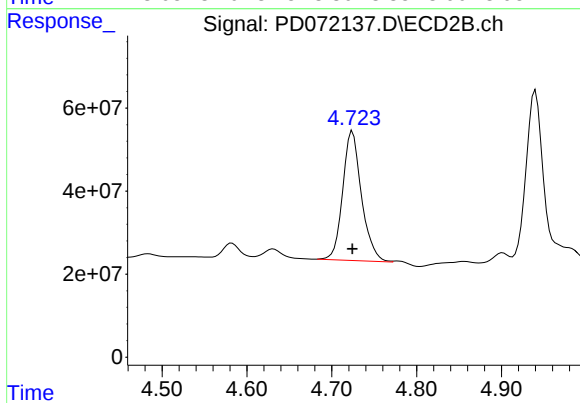

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 479002799
Conc: 491.93 ng/ml

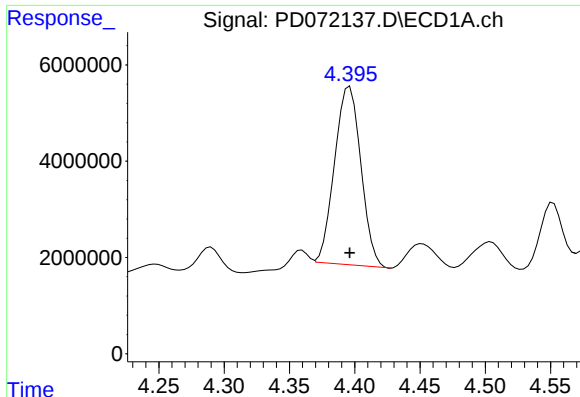

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 51960134
Conc: 497.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093022CHLOR

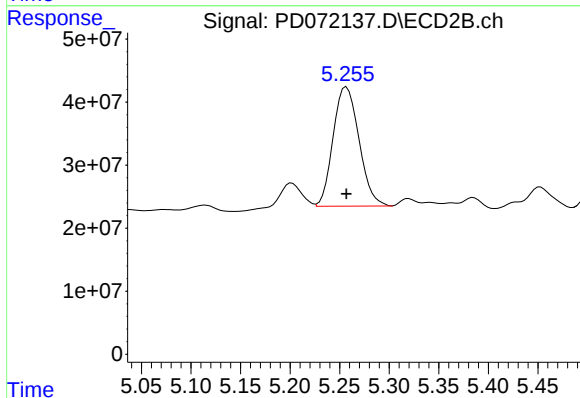


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 344292064
Conc: 489.94 ng/ml

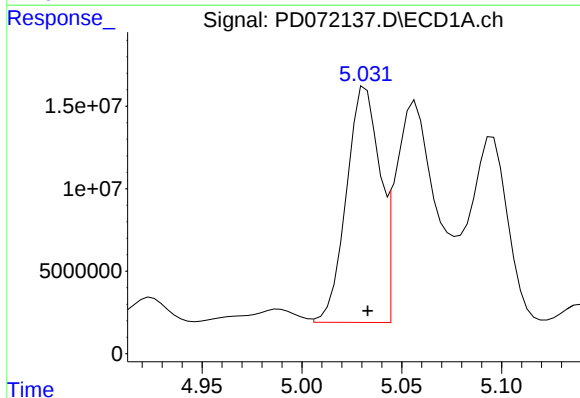


#25 Chlordane-3

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 165533763
Conc: 518.95 ng/ml

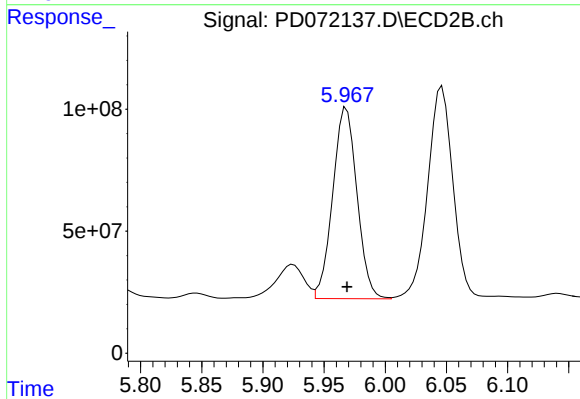

#25 Chlordane-3


R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 1082872354
Conc: 484.59 ng/ml

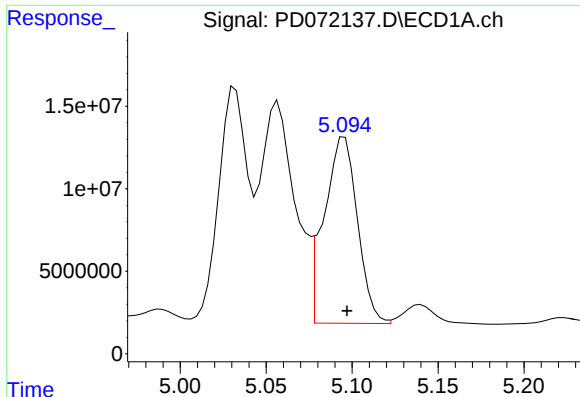

#26 Chlordane-4


R.T.: 5.096 min
Delta R.T.: -0.001 min
Response: 152351999
Conc: 517.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093022CHLOR

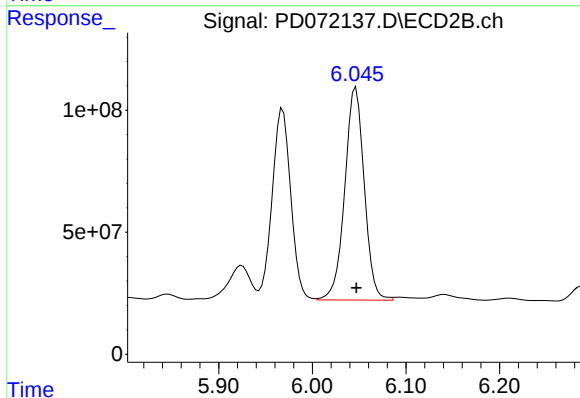


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1262732268
Conc: 483.52 ng/ml

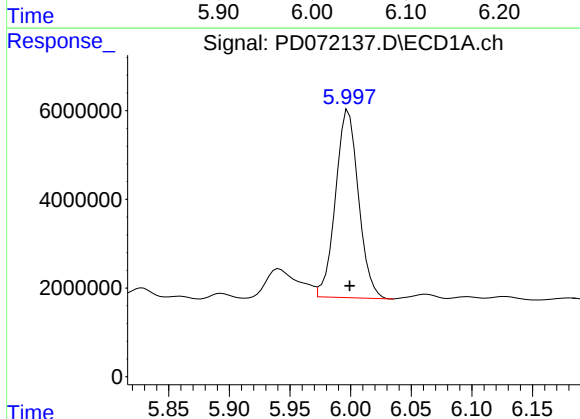


#27 Chlordane-5

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 55840118
Conc: 515.03 ng/ml

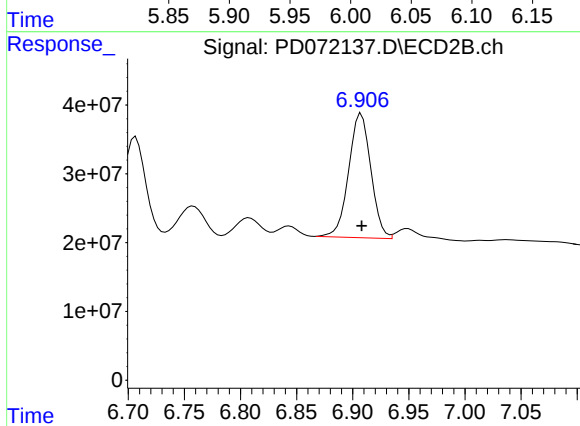

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 248354150
Conc: 496.48 ng/ml

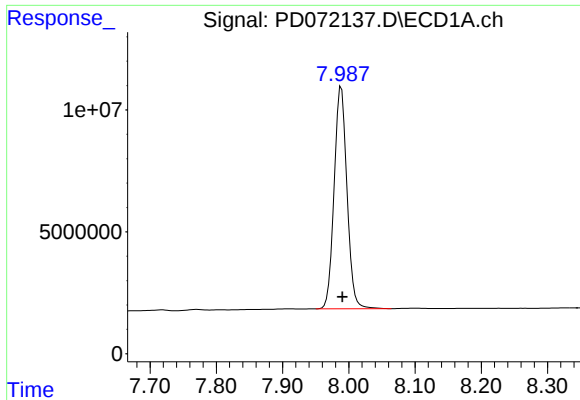

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.002 min
Response: 122993993
Conc: 53.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD093022CHLOR

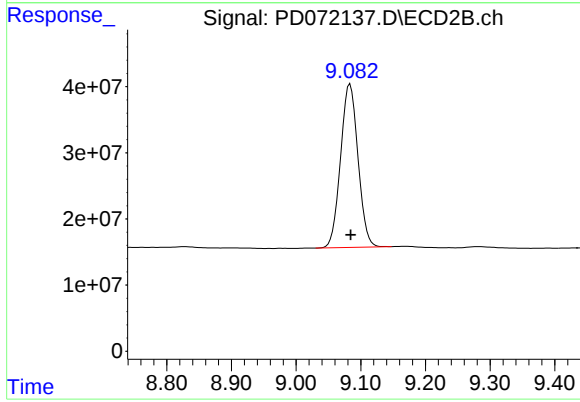

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 462856685
Conc: 48.74 ng/ml