

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093024\
 Data File : PD085805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2024 23:16
 Operator : AR\AJ
 Sample : P4019-06RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA9RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/01/2024
 Supervised By : Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 21:27:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.435	2.887	14735007	1413.0E6	14.065m	333.715m#
2) SA Decachlor...	8.889	8.061	15623687	28440541	10.599m	7.356m#
Target Compounds						
2) A alpha-BHC	3.886	3.386	78099475	256.7E6	42.913	39.750
7) B delta-BHC	4.644	4.251	164.5E6	300.3E6	92.941	50.363 #
11) B cis-Chlor...	5.892	5.184	22604861	72782319	14.495	13.169

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093024\
Data File : PD085805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 23:16
Operator : AR\AJ
Sample : P4019-06RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 21:27:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

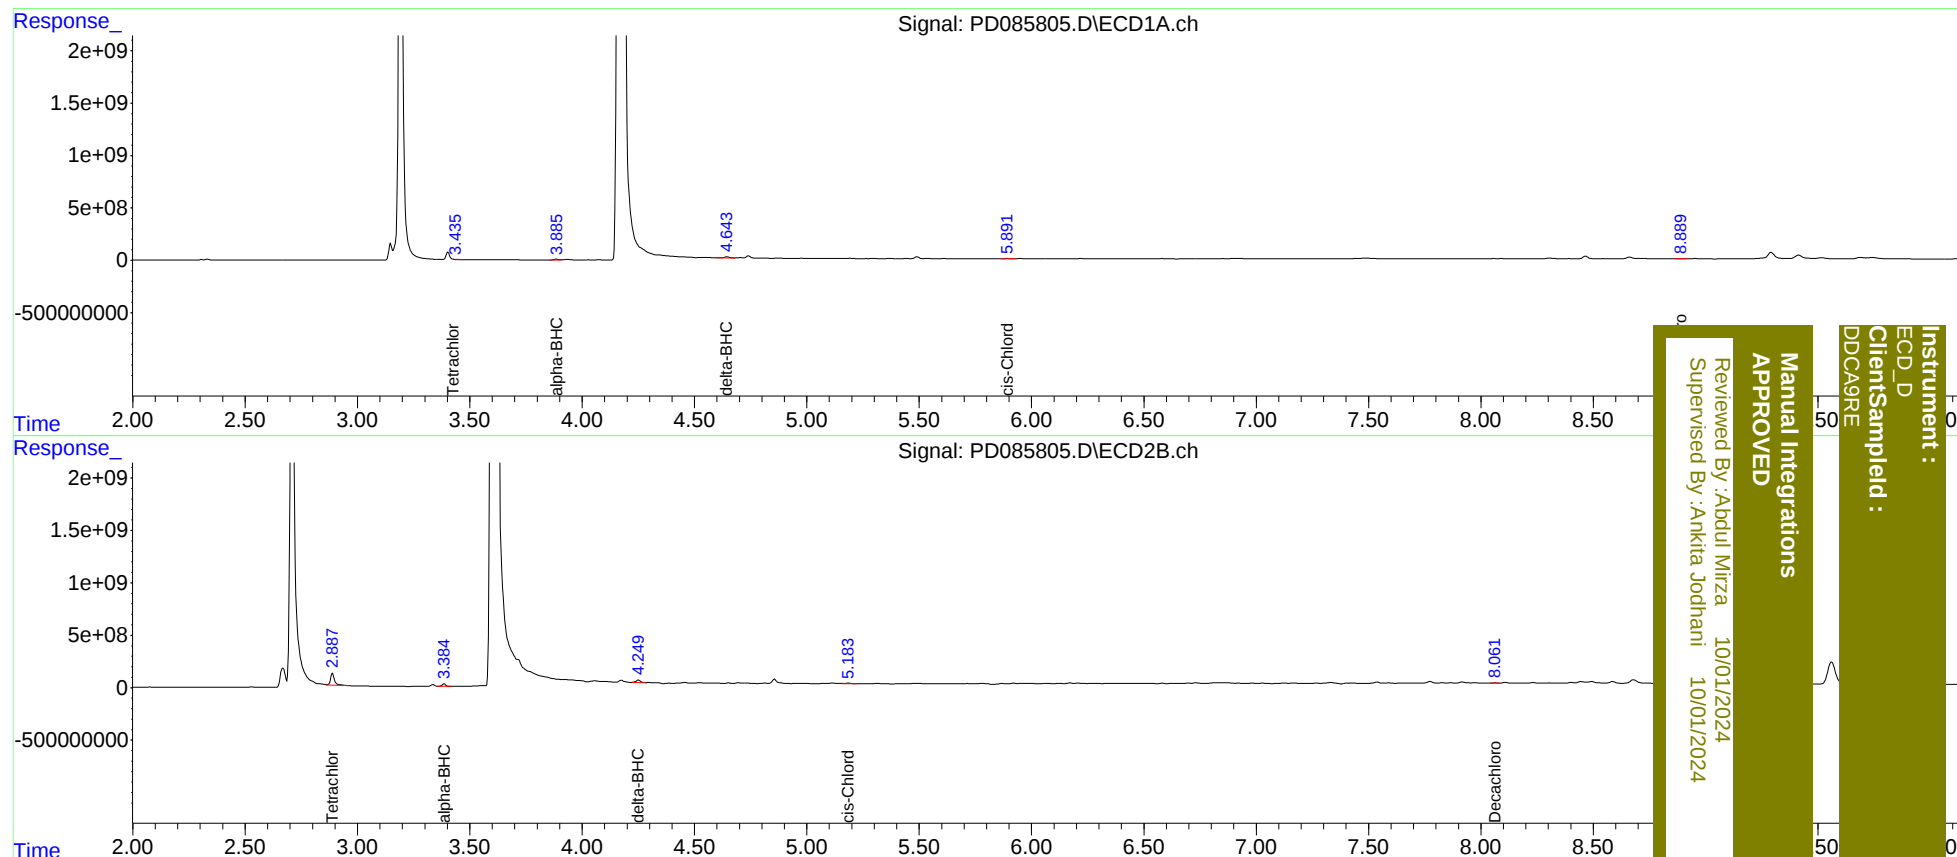

Instrument :
ECD_D
ClientSampled :
DDCA9RE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/01/2024
Supervised By :Ankita Jodhani 10/01/2024