

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093024\
 Data File : PD085819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 02:24
 Operator : AR\AJ
 Sample : P4019-02DL 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC38DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/01/2024
 Supervised By : Ankita Jodhani 10/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 21:32:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 27 15:18:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.879	5333391	34838029	5.091m	8.228 #
27)	SA Decachlor...	8.889	8.063	1364073	13943305	0.925	3.606 #
Target Compounds							
2)	A alpha-BHC	3.866	3.376	6903758	18146700	3.793m	2.810m#
7)	B delta-BHC	4.663	4.255	6741702	346790	3.809	<MDL m#
11)	B cis-Chlor...	5.892	0.000	265868	0	0.170	N.D. #
14)	MA Endrin	6.448	5.799	-465287	57572761	N.D.	12.828
16)	A 4,4'-DDD	0.000	5.980f	0	917036	N.D.	0.216
17)	MA 4,4'-DDT	0.000	6.124f	0	2690567	N.D.	0.616

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD093024\
Data File : PD085819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 02:24
Operator : AR\AJ
Sample : P4019-02DL 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 21:32:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 27 15:18:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

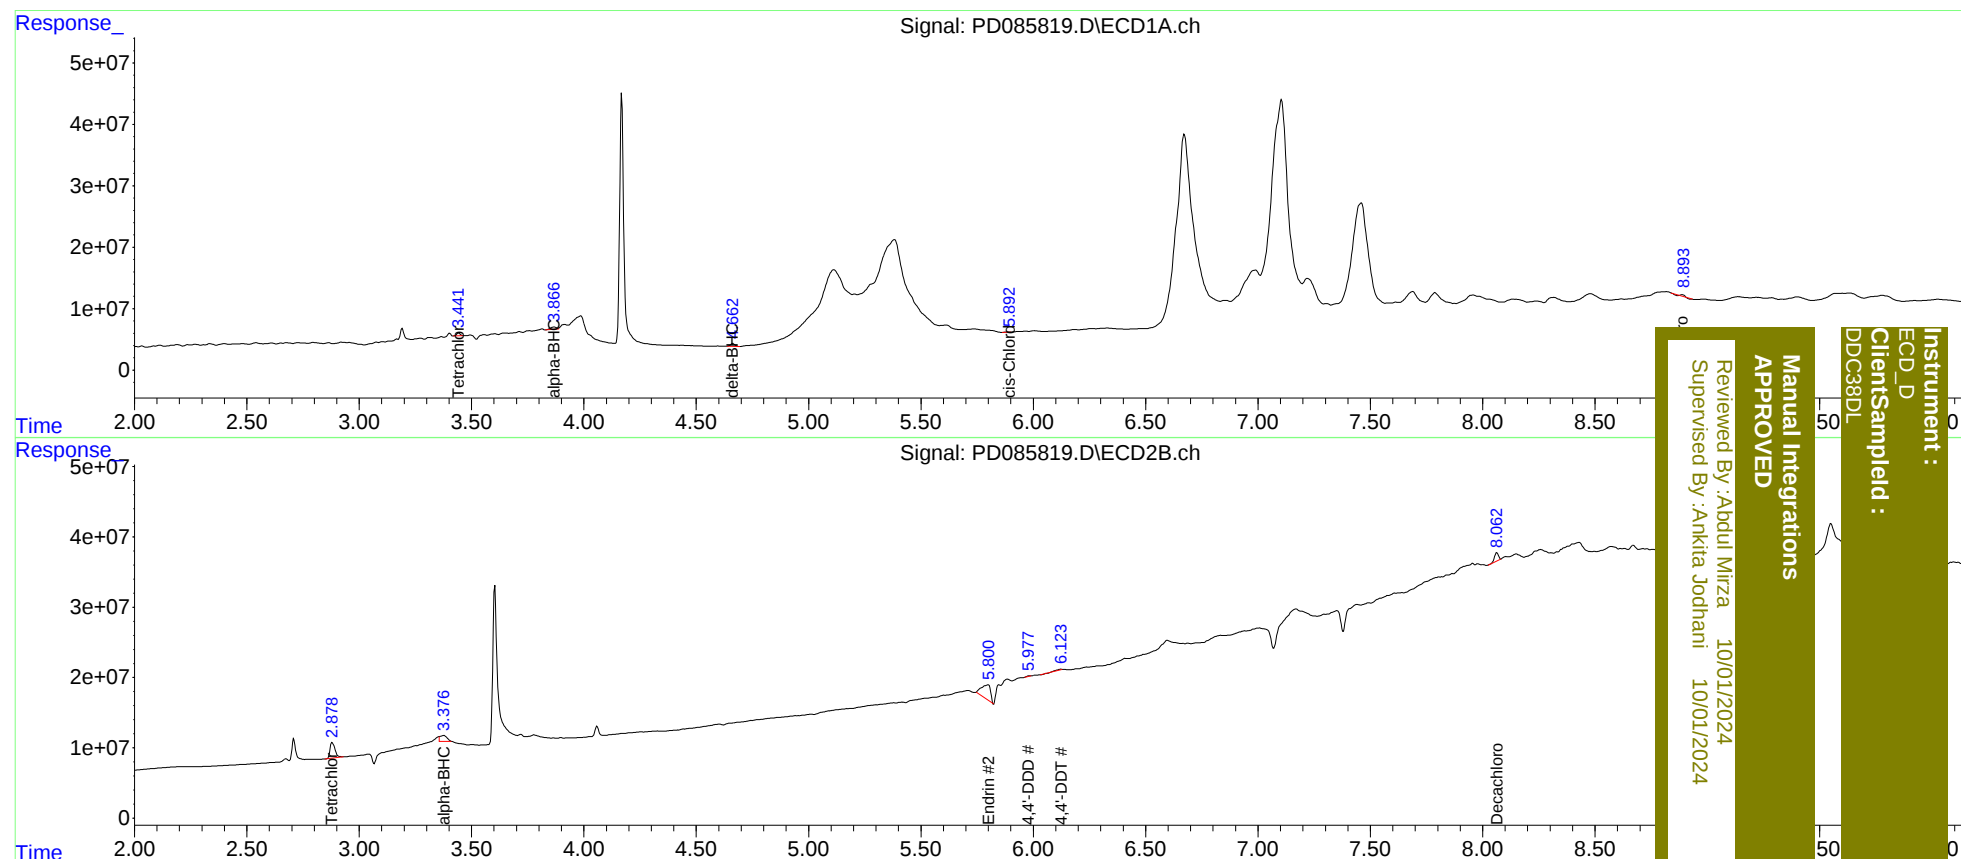

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/01/2024
Supervised By: Ankita Jodhani 10/01/2024

Instrument :
ECD_D
ClientSampled :
DDC38DL