

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100119\
 Data File : PD055071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2019 12:48
 Operator : SG\AJ
 Sample : PIBLK43
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK43

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:13:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.962	16434462	23940530	21.602	23.329
27)	SA Decachlor...	7.970	8.996	32102390	45430855	38.100	38.994
Target Compounds							
2)	A alpha-BHC	3.725	4.387f	172706	-109580	0.156	N.D. #
18)	B Endrin al...	6.280f	0.000	1158221	0	1.592	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100119\
Data File : PD055071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 12:48
Operator : SG\AJ
Sample : PIBLK43
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:13:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

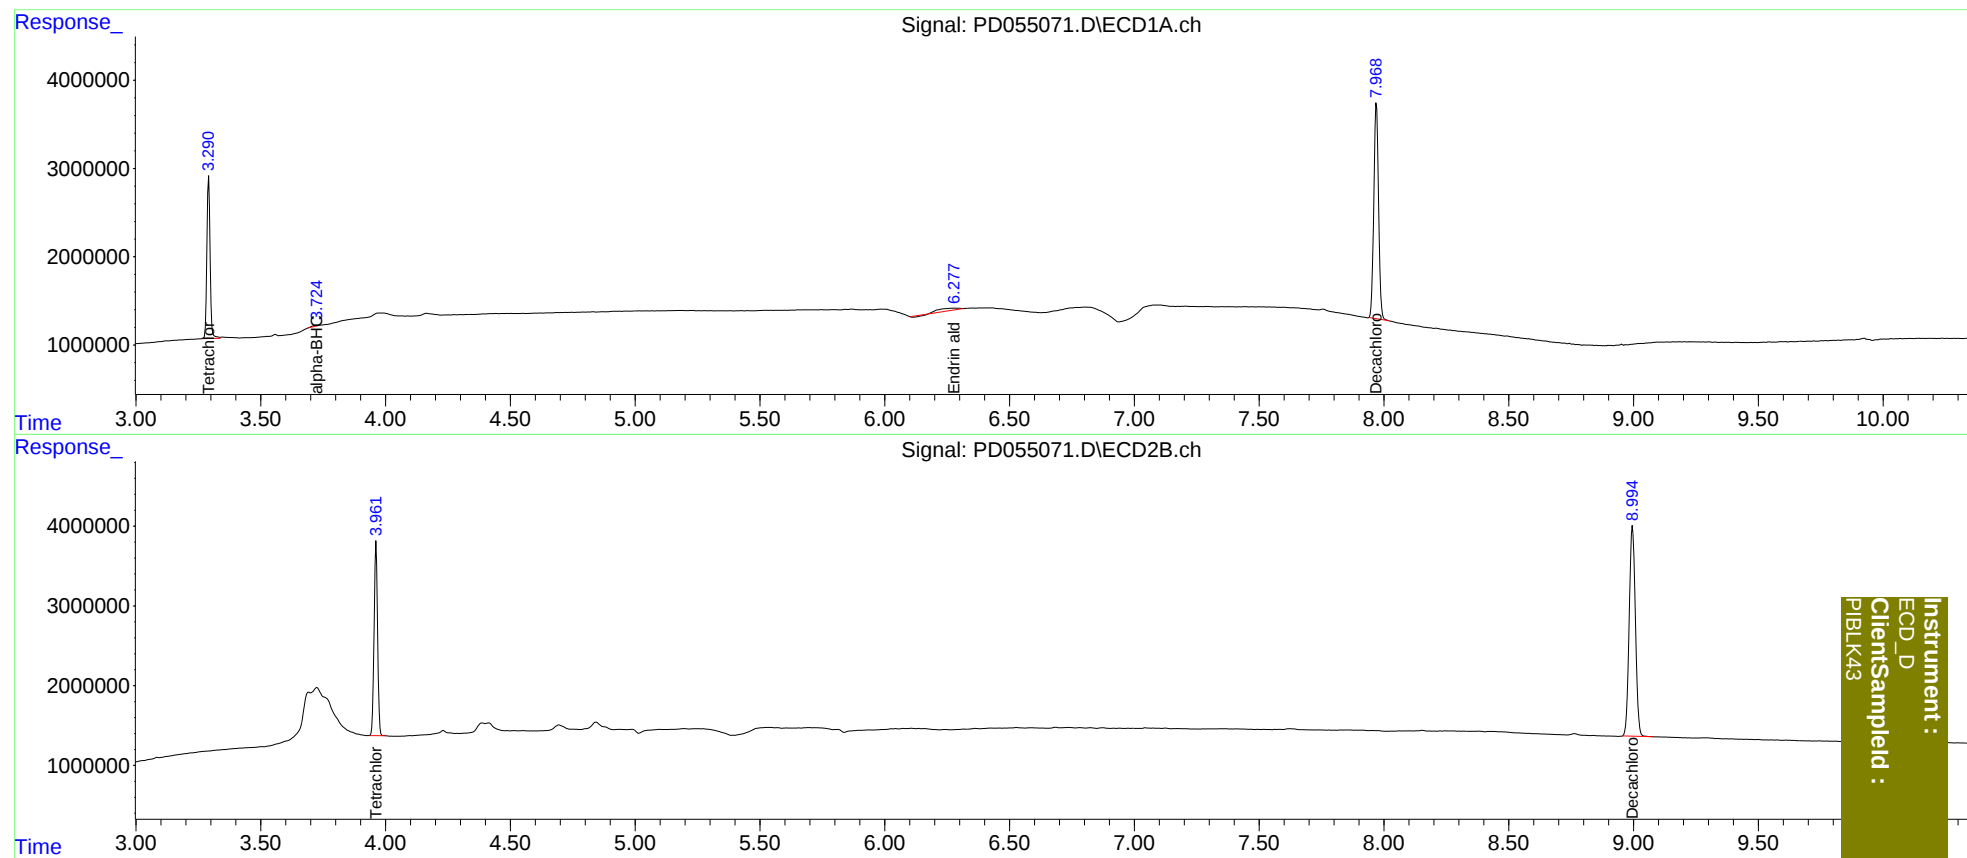


Instrument :
ECD_D
ClientSampled :
PIBLK43

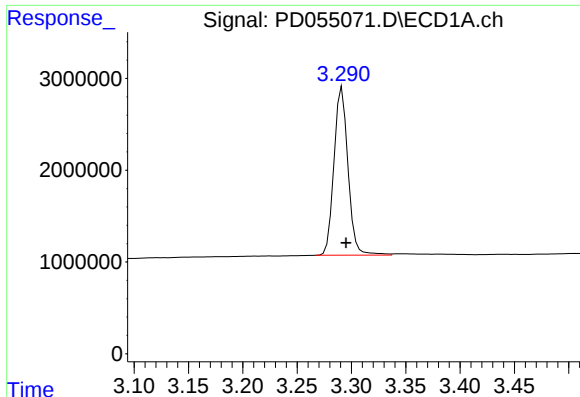

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: -0.003 min
Response: 16434462
Conc: 21.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

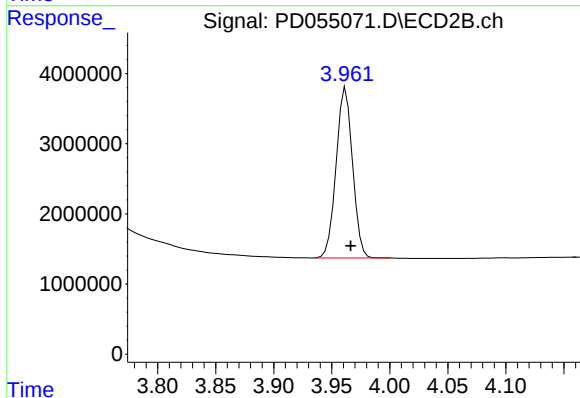


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 23940530
Conc: 23.33 ng/ml

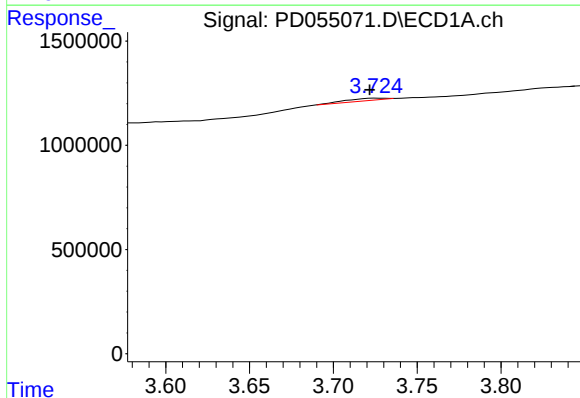


#2 alpha-BHC

R.T.: 3.725 min
Delta R.T.: 0.004 min
Response: 172706
Conc: 0.16 ng/ml

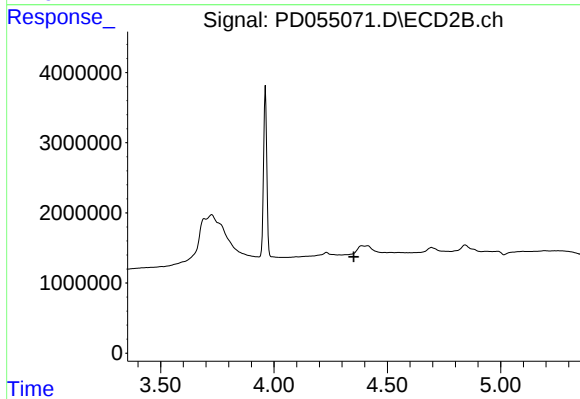

#2 alpha-BHC


R.T.: 4.387 min
Delta R.T.: 0.034 min
Response: -109580
Conc: N.D.

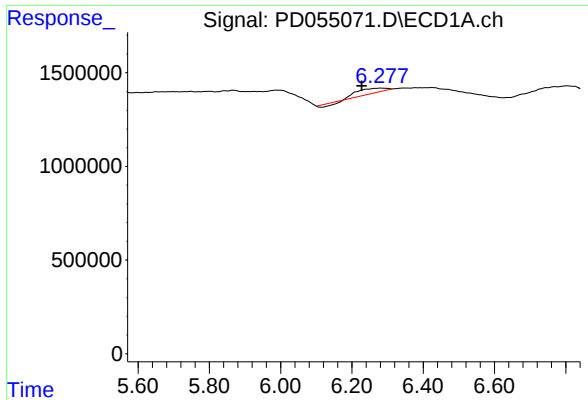

#18 Endrin aldehyde


R.T.: 6.280 min
Delta R.T.: 0.052 min
Response: 1158221
Conc: 1.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

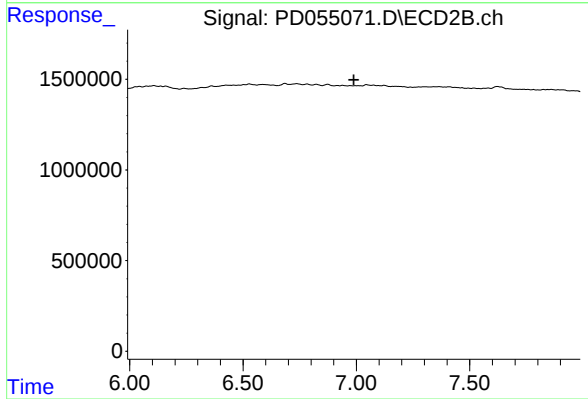


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

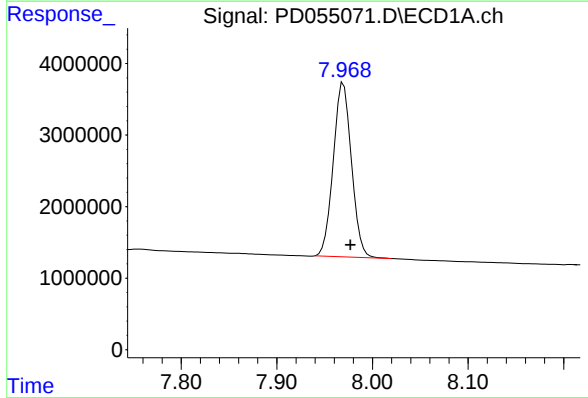

#27 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: -0.007 min
Response: 32102390
Conc: 38.10 ng/ml

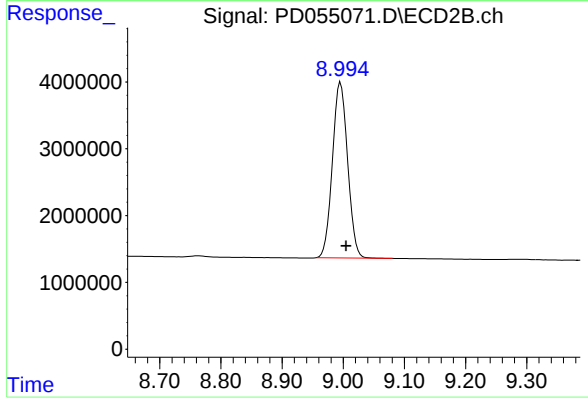

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.009 min
Response: 45430855
Conc: 38.99 ng/ml