

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100119\
Data File : PD055076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 14:49
Operator : SG\AJ
Sample : K5087-12
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual Integrations
APPROVED

Ankita
10/7/2019 10:35:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:14:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

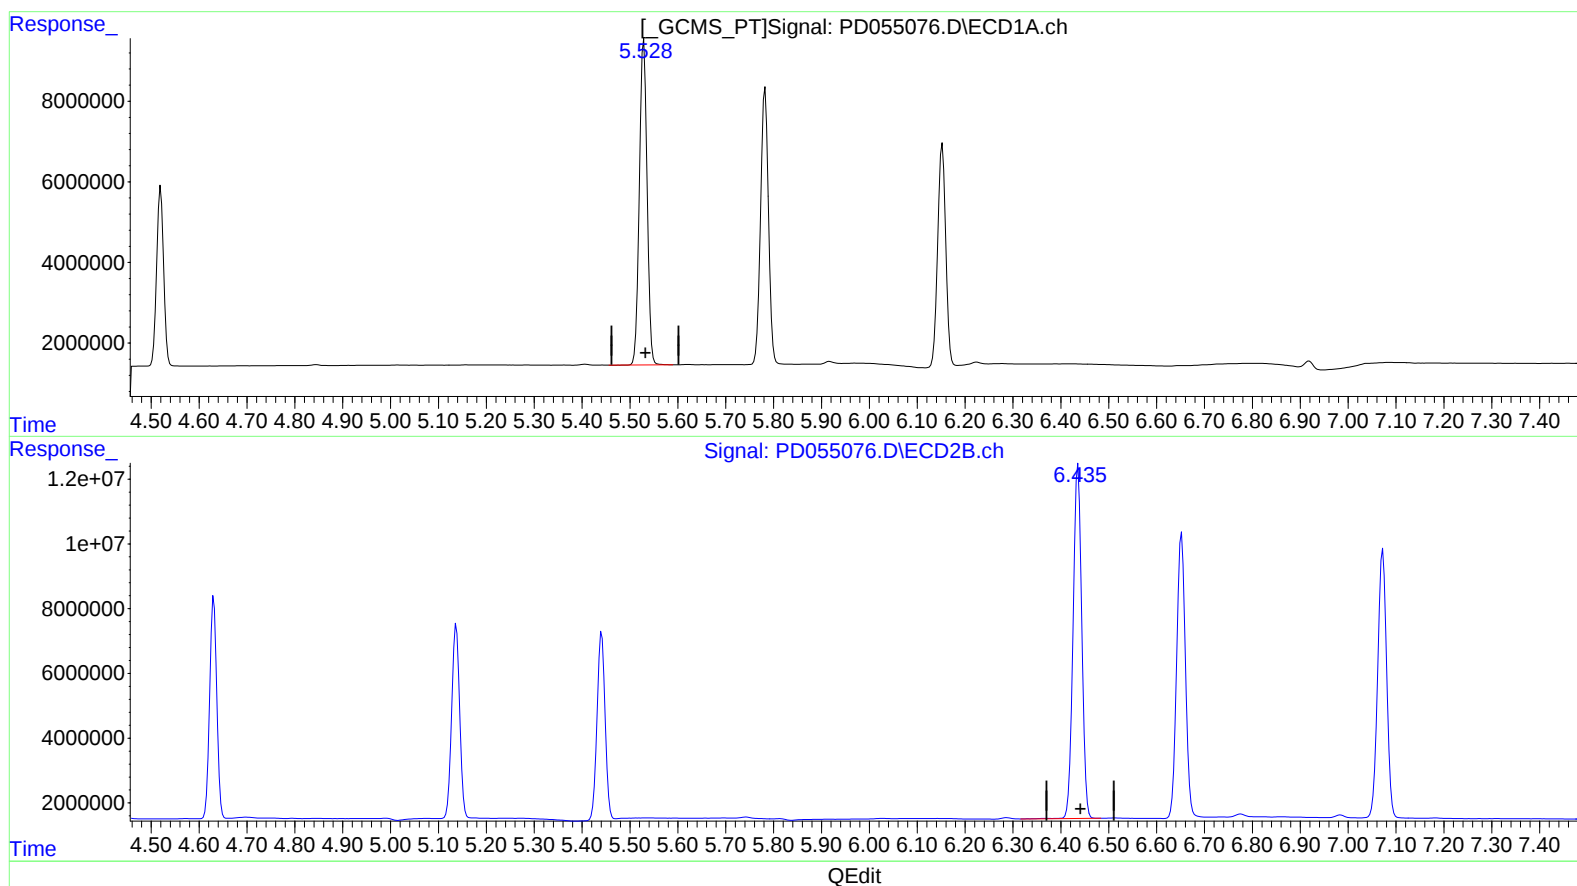

(13) Dieldrin (MA)

5.529min 91.966 ng/ml

response 90525106

(13) Dieldrin #2 (MA)

6.436min 98.069 ng/ml

response 136844280

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100119\
Data File : PD055076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2019 14:49
Operator : SG\AJ
Sample : K5087-12
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PEST-GPC2-BLANK-SPIKE

Manual Integrations
APPROVED

Ankita
10/7/2019 10:35:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:14:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

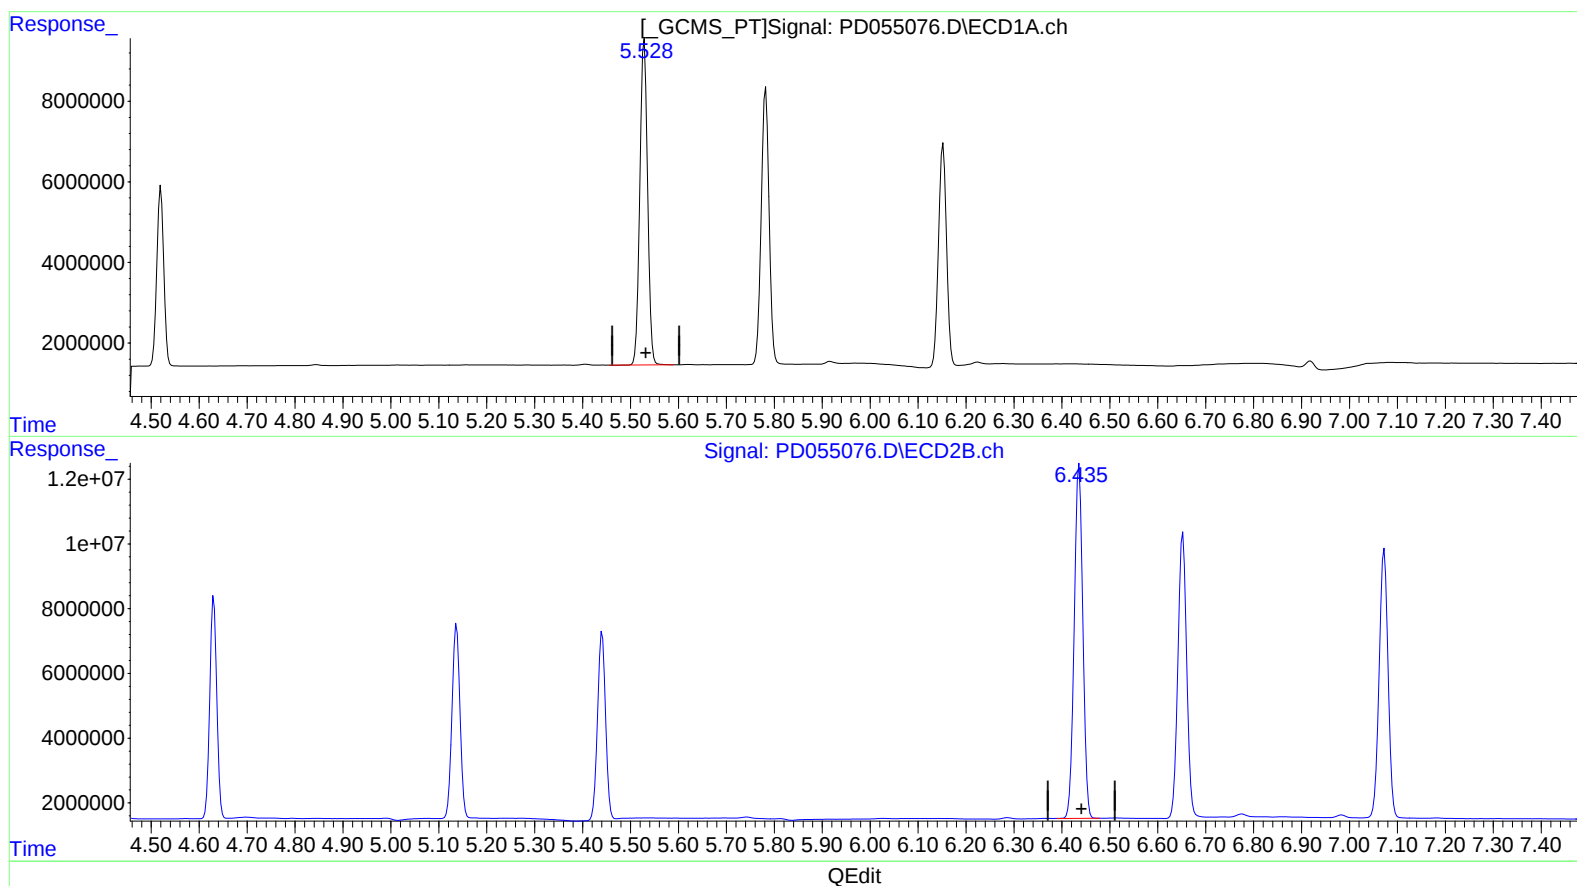

(13) Dieldrin (MA)
5.529min 91.966 ng/ml
response 90525106

(13) Dieldrin #2 (MA)
6.435min 97.777 ng/ml m
response 136437096

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100119\
 Data File : PD055076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2019 14:49
 Operator : SG\AJ
 Sample : K5087-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC2-BLANK-SPIKE

Manual Integrations
 APPROVED

Ankita
 10/7/2019 10:35:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:14:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
3) MA gamma-BHC...	3.995	4.631	47633349	70273004	44.423	50.187
4) MA Heptachlor	4.281	5.137	43297015	69587930	46.803	49.358
5) MB Aldrin	4.520	5.441	44950105	66161531	46.187	50.045
13) MA Dieldrin	5.529	6.435	90525106	136.4E6	91.966	97.777m
14) MA Endrin	5.782	6.653	78627801	111.6E6	94.564	101.327
17) MA 4,4'-DDT	6.152	7.073	63979699	107.3E6	95.991	98.045

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

3
 AJ
 20/11/19