

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2024 23:26
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 00:58:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 00:57:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	2.878	5886742	22168067	5.151	5.168
27)	SA Decachlor...	8.914	8.064	18791631	37449894	10.278	10.058
Target Compounds							
2)	A alpha-BHC	3.908	3.387	9387073	31096268	4.597	4.900
3)	MA gamma-BHC...	4.235	3.722	11343239	30103696	5.372	4.956
4)	MA Heptachlor	4.828	4.073	9870490	28782542	4.834	4.957
9)	A Endosulfan I	5.966	5.236	9014441	25114710	4.961	5.009
13)	MA Dieldrin	6.237	5.502	18813082	55607689	9.491	9.897
14)	MA Endrin	6.463	5.780	13950962	48442103	8.867	10.062
16)	A 4,4'-DDD	6.598	5.920	11218283	39005453	8.964	9.856
17)	MA 4,4'-DDT	6.913	6.174	12090479	41549827	8.708	9.705
20)	A Methoxychlor	7.385	6.746	40871331	111.7E6	50.257	53.248


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 23:26
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 00:58:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 00:57:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

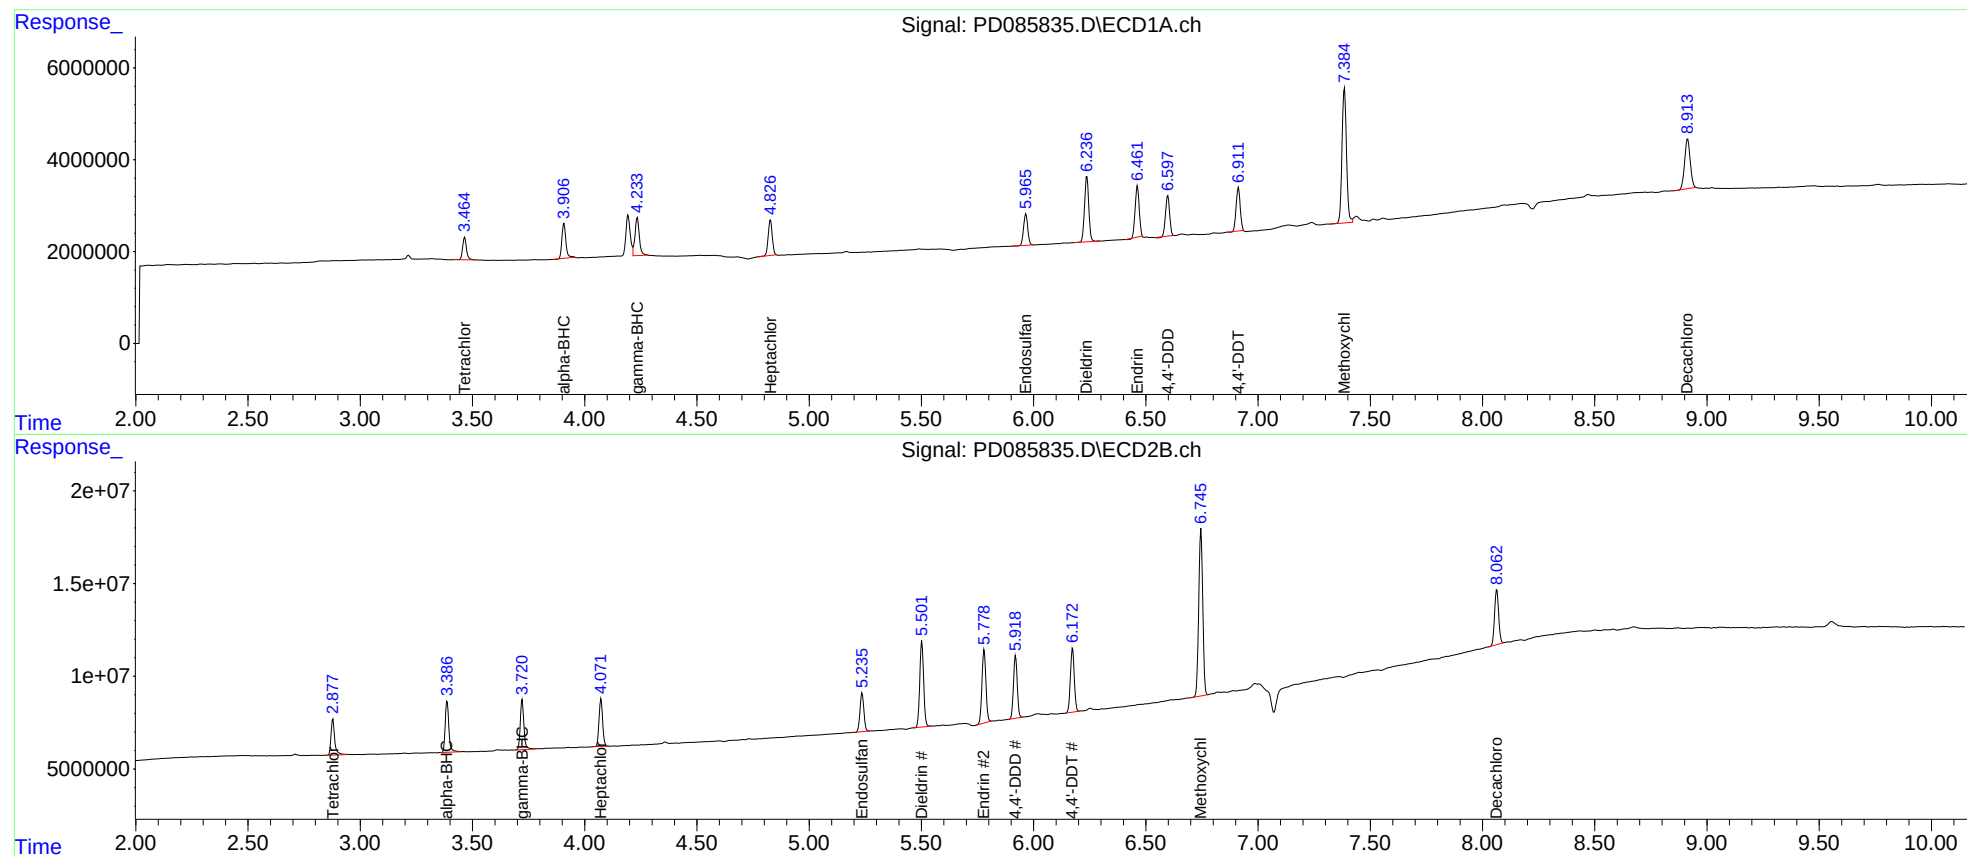

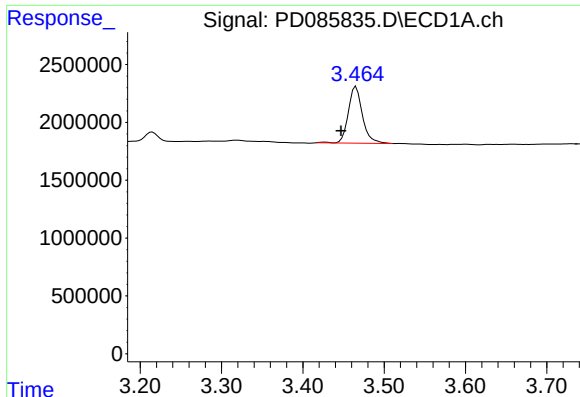


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.018 min
Response: 5886742
Conc: 5.15 ng/ml

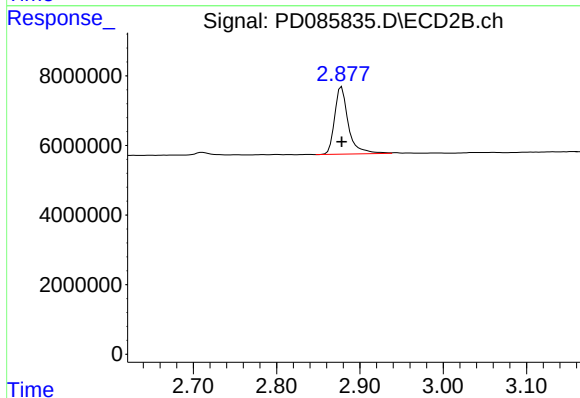


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 22168067
Conc: 5.17 ng/ml

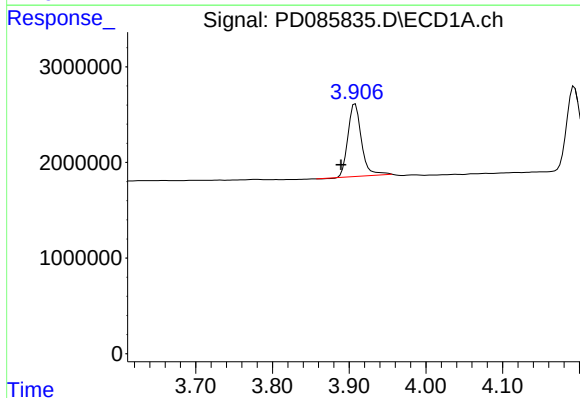


#2 alpha-BHC

R.T.: 3.908 min
Delta R.T.: 0.018 min
Response: 9387073
Conc: 4.60 ng/ml

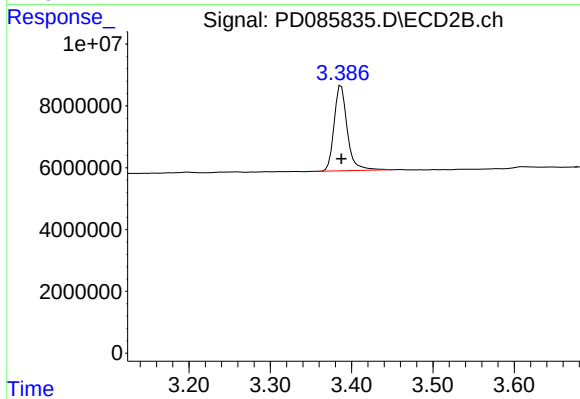


#2 alpha-BHC

R.T.: 3.387 min
Delta R.T.: 0.000 min
Response: 31096268
Conc: 4.90 ng/ml

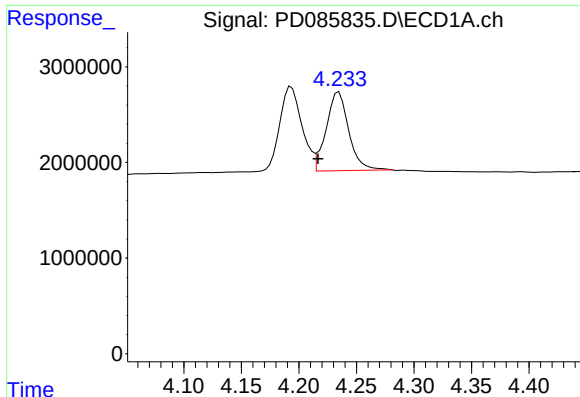


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.018 min
Response: 11343239
Conc: 5.37 ng/ml

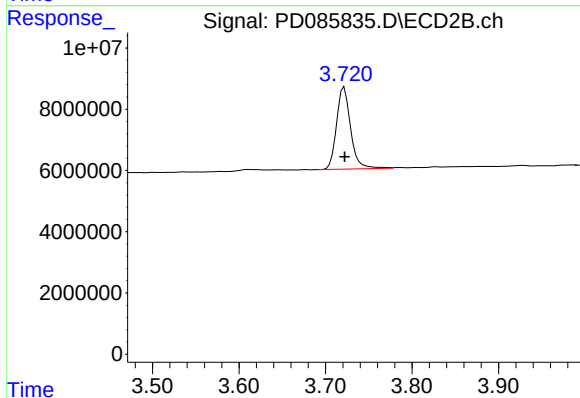


#3 gamma-BHC (Lindane)

R.T.: 3.722 min
Delta R.T.: 0.000 min
Response: 30103696
Conc: 4.96 ng/ml

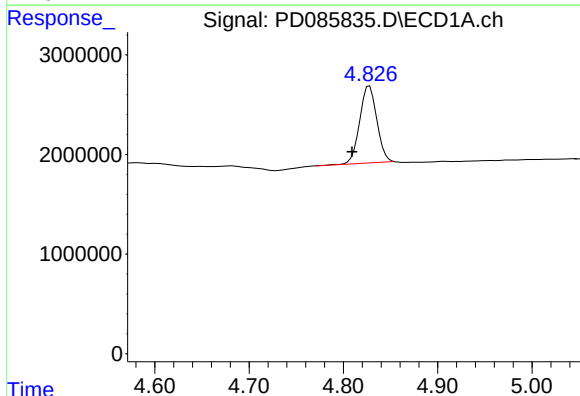


#4 Heptachlor

R.T.: 4.828 min
Delta R.T.: 0.019 min
Response: 9870490
Conc: 4.83 ng/ml

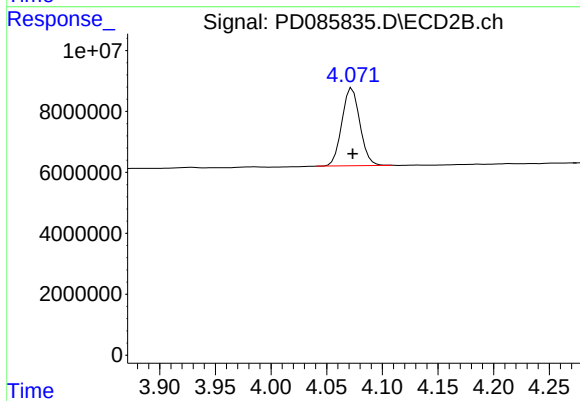


#4 Heptachlor

R.T.: 4.073 min
Delta R.T.: 0.000 min
Response: 28782542
Conc: 4.96 ng/ml

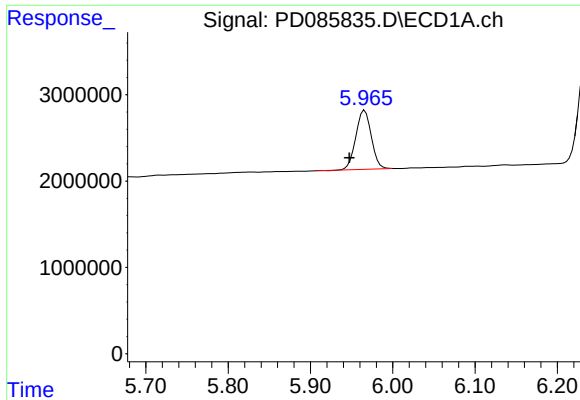


#9 Endosulfan I

R.T.: 5.966 min
Delta R.T.: 0.019 min
Response: 9014441
Conc: 4.96 ng/ml

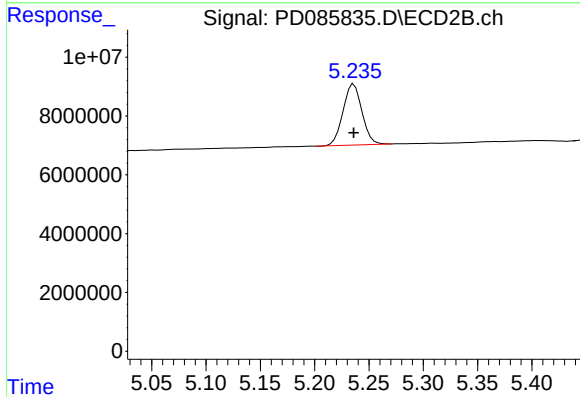


#9 Endosulfan I

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 25114710
Conc: 5.01 ng/ml

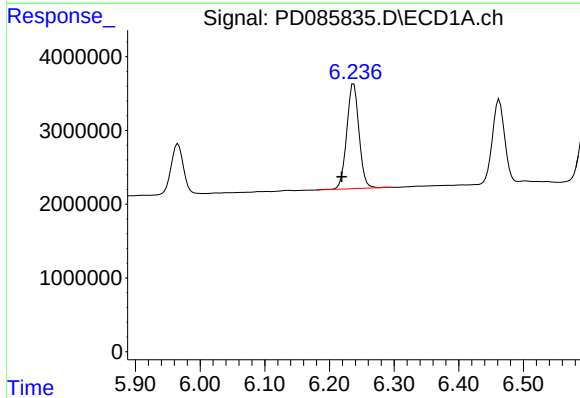


#13 Dieldrin

R.T.: 6.237 min
Delta R.T.: 0.018 min
Response: 18813082
Conc: 9.49 ng/ml

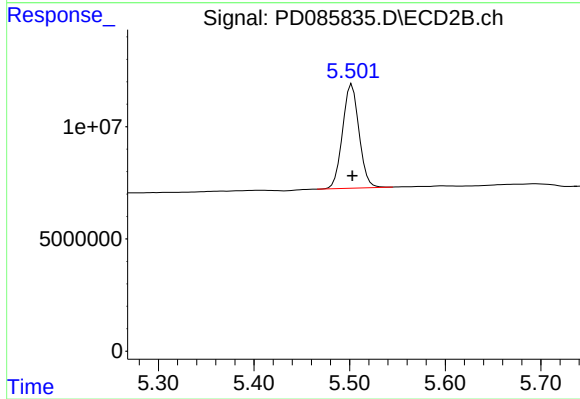


#13 Dieldrin

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 55607689
Conc: 9.90 ng/ml

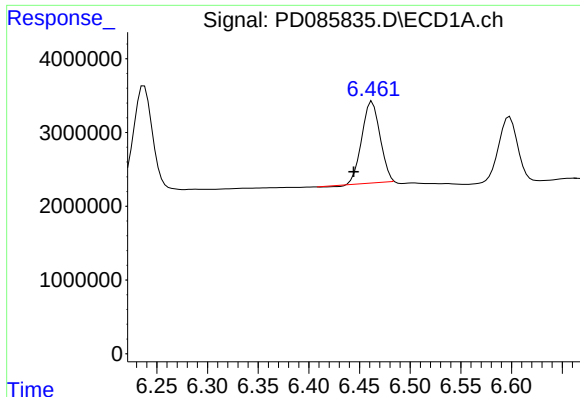


#14 Endrin

R.T.: 6.463 min
Delta R.T.: 0.018 min
Response: 13950962
Conc: 8.87 ng/ml

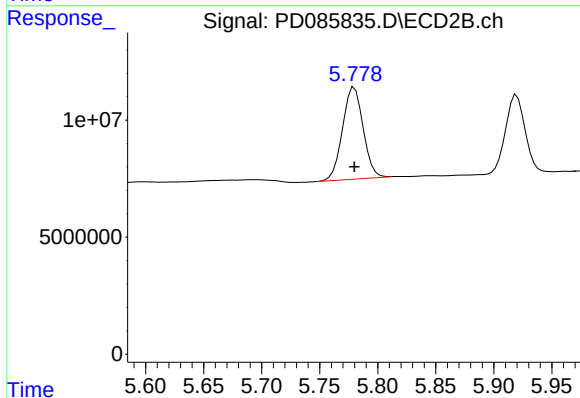


#14 Endrin

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 48442103
Conc: 10.06 ng/ml

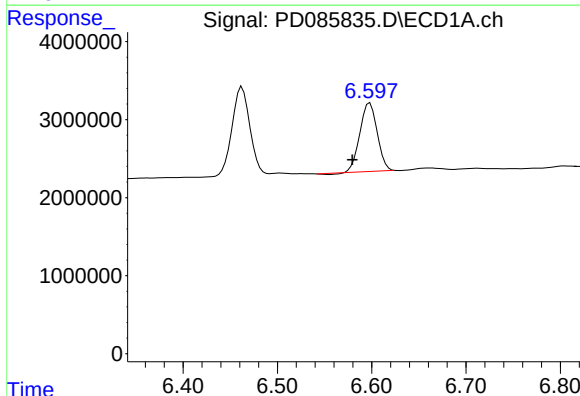


#16 4,4'-DDD

R.T.: 6.598 min
Delta R.T.: 0.019 min
Response: 11218283
Conc: 8.96 ng/ml

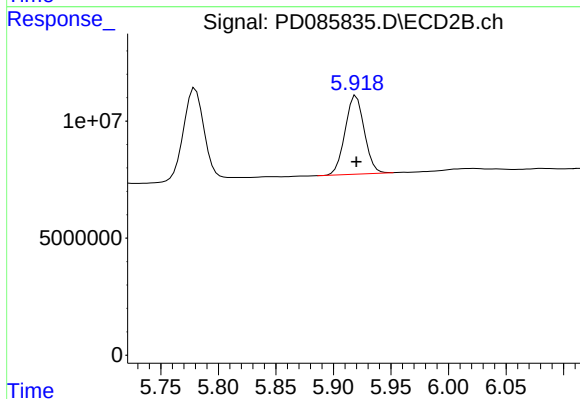


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 39005453
Conc: 9.86 ng/ml

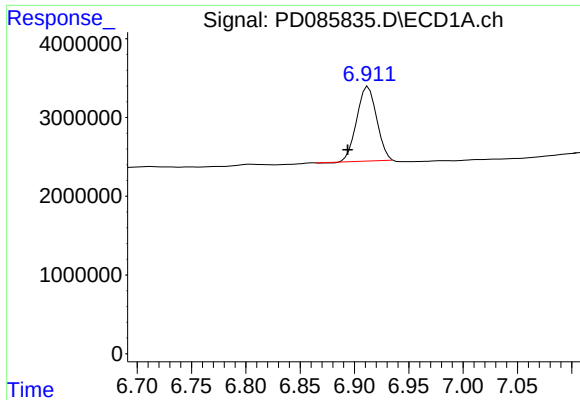


#17 4,4'-DDT

R.T.: 6.913 min
Delta R.T.: 0.019 min
Response: 12090479
Conc: 8.71 ng/ml

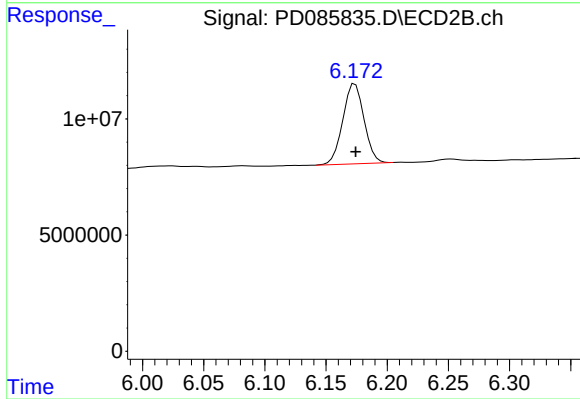


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 41549827
Conc: 9.70 ng/ml

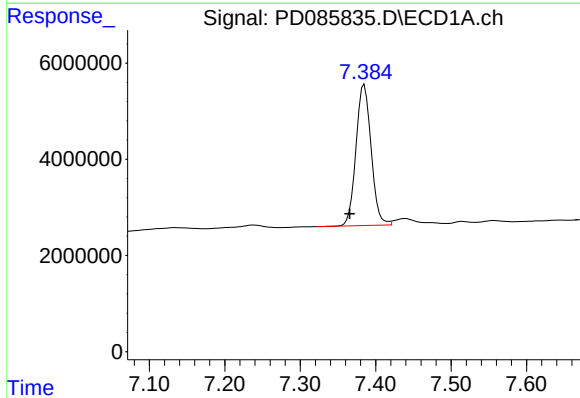


#20 Methoxychlor

R.T.: 7.385 min
Delta R.T.: 0.019 min
Response: 40871331
Conc: 50.26 ng/ml

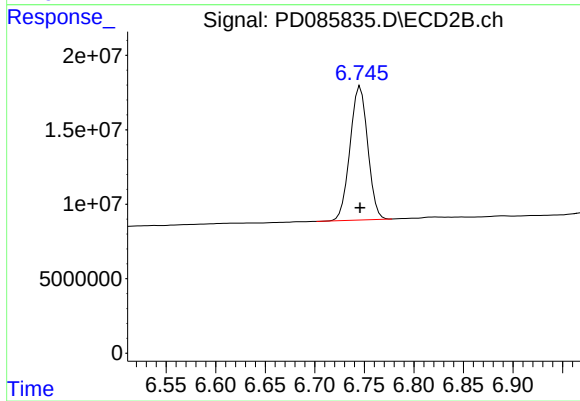


#20 Methoxychlor

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 111731589
Conc: 53.25 ng/ml

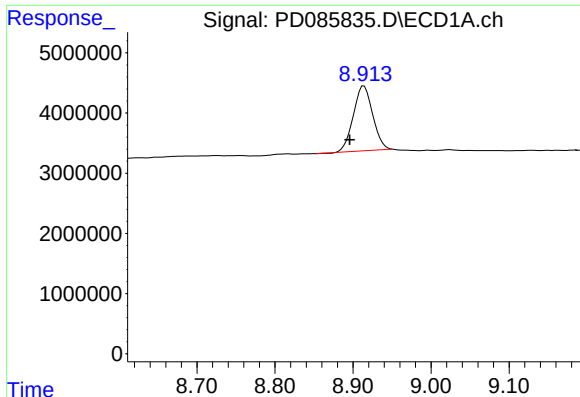

#27 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.018 min
Response: 18791631
Conc: 10.28 ng/ml

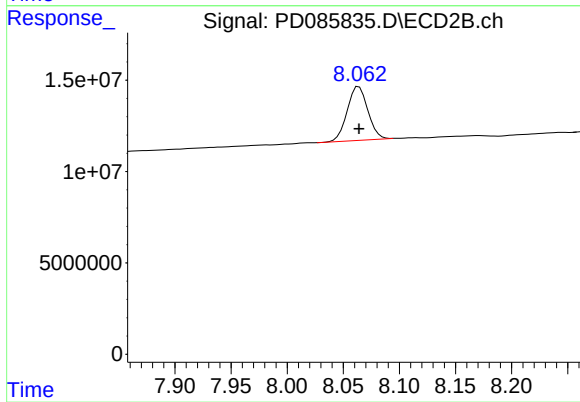

#27 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 37449894
Conc: 10.06 ng/ml