

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2024 23:55
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 00:58:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 00:57:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	2.878	11757457	44166202	10.288	10.297
27)	SA Decachlor...	8.896	8.063	38352265	76728609	20.977	20.608
Target Compounds							
2)	A alpha-BHC	3.889	3.387	19957778	63960927	9.773	10.079
3)	MA gamma-BHC...	4.216	3.722	21999927	61962618	10.419	10.202
4)	MA Heptachlor	4.809	4.073	20372178	59403573	9.977	10.230
9)	A Endosulfan I	5.947	5.236	18410572	51647672	10.133	10.300
13)	MA Dieldrin	6.219	5.503	39151843	113.3E6	19.752	20.166
14)	MA Endrin	6.445	5.780	31022344	98755106	19.717	20.512
16)	A 4,4'-DDD	6.580	5.920	24157728	79837354	19.302	20.174
17)	MA 4,4'-DDT	6.894	6.174	27038724	85586631	19.475	19.990
20)	A Methoxychlor	7.367	6.746	82421548	221.9E6	101.349	105.775


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 23:55
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 00:58:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 00:57:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

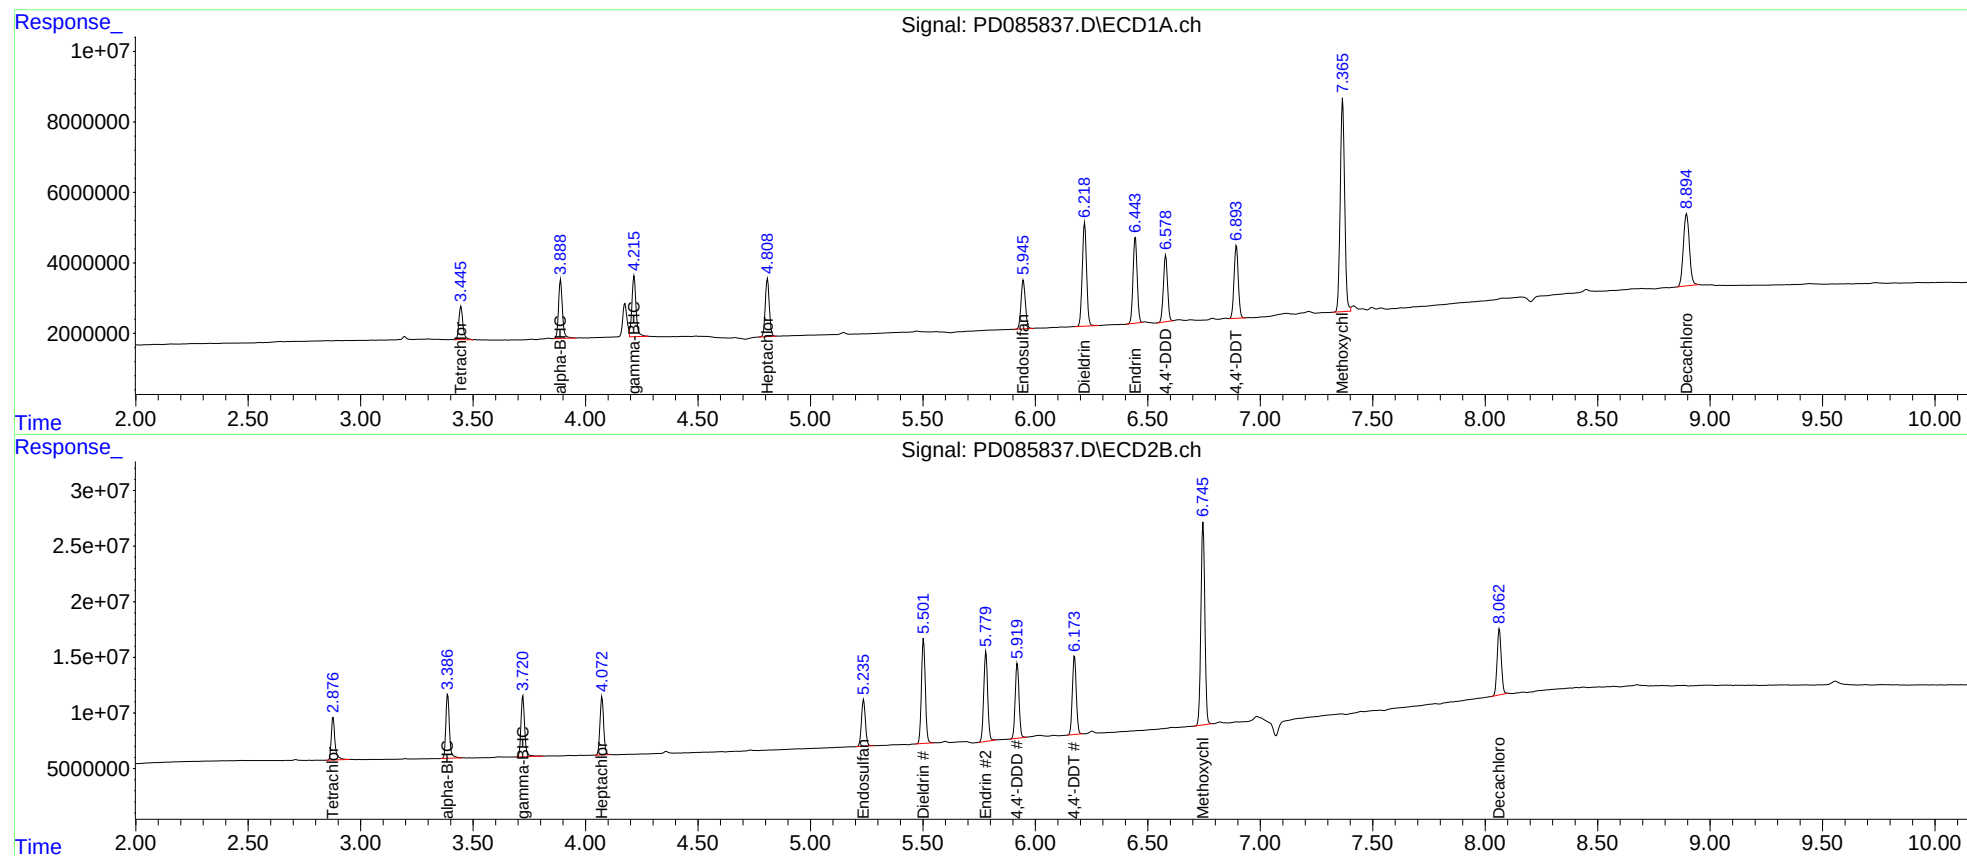

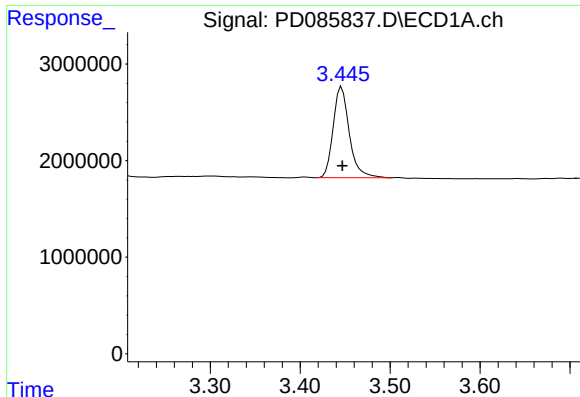


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 11757457
Conc: 10.29 ng/ml

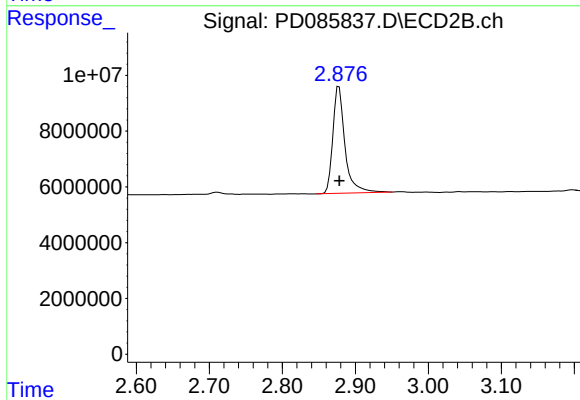


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 44166202
Conc: 10.30 ng/ml

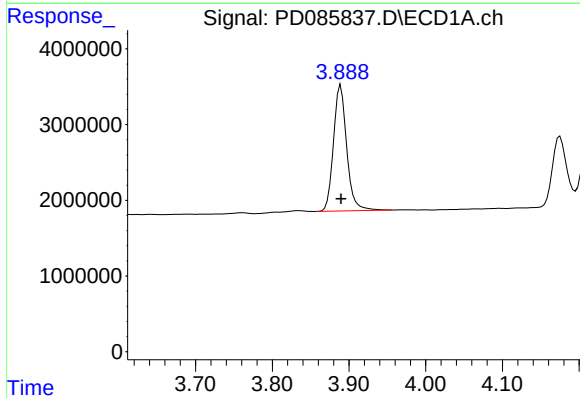


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: 0.000 min
Response: 19957778
Conc: 9.77 ng/ml

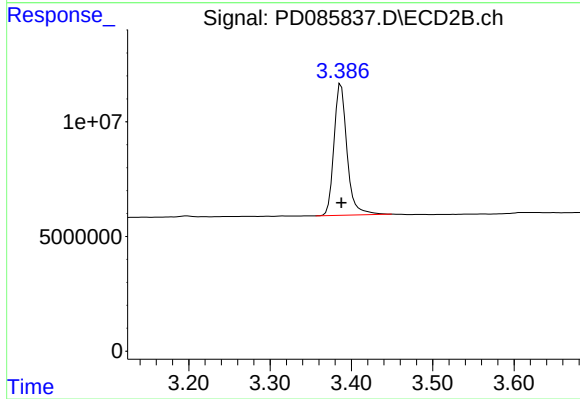


#2 alpha-BHC

R.T.: 3.387 min
Delta R.T.: 0.000 min
Response: 63960927
Conc: 10.08 ng/ml

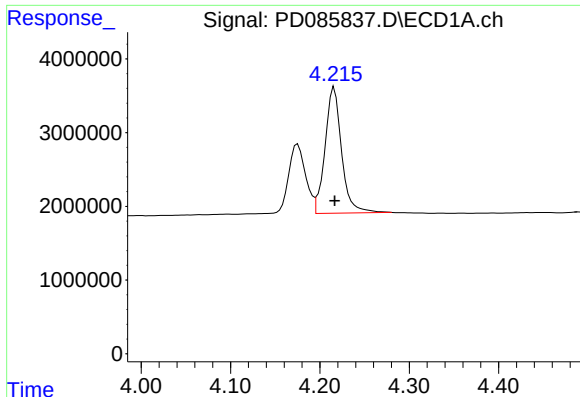


#3 gamma-BHC (Lindane)

R.T.: 4.216 min
Delta R.T.: 0.000 min
Response: 21999927
Conc: 10.42 ng/ml

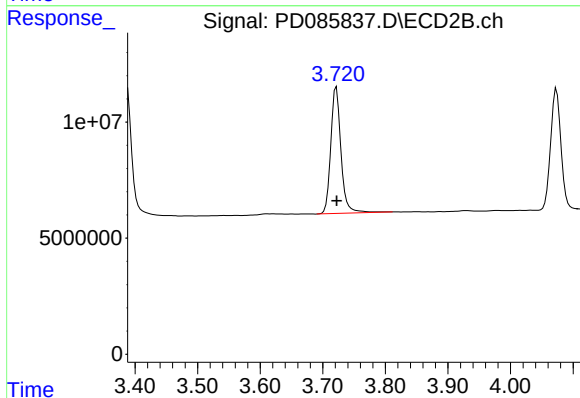


#3 gamma-BHC (Lindane)

R.T.: 3.722 min
Delta R.T.: 0.000 min
Response: 61962618
Conc: 10.20 ng/ml

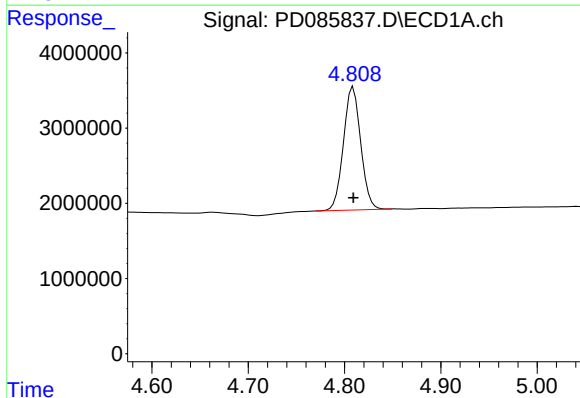


#4 Heptachlor

R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 20372178
Conc: 9.98 ng/ml

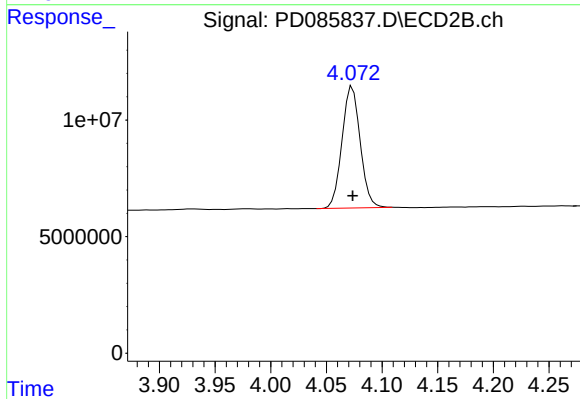


#4 Heptachlor

R.T.: 4.073 min
Delta R.T.: 0.000 min
Response: 59403573
Conc: 10.23 ng/ml

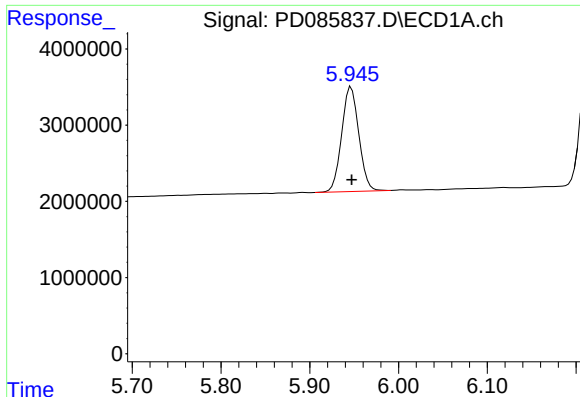


#9 Endosulfan I

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 18410572
Conc: 10.13 ng/ml

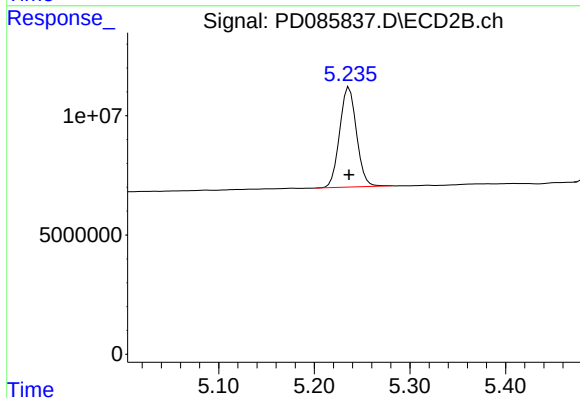


#9 Endosulfan I

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 51647672
Conc: 10.30 ng/ml

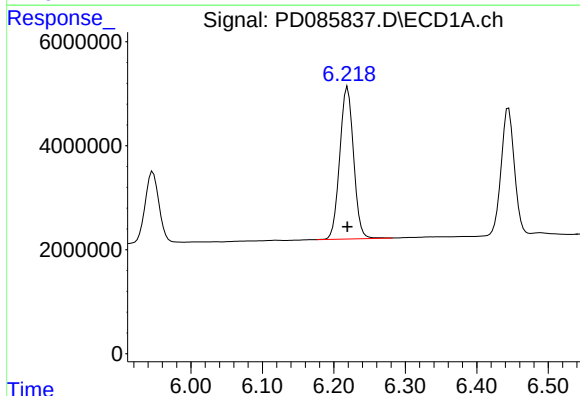


#13 Dieldrin

R.T.: 6.219 min
Delta R.T.: 0.000 min
Response: 39151843
Conc: 19.75 ng/ml

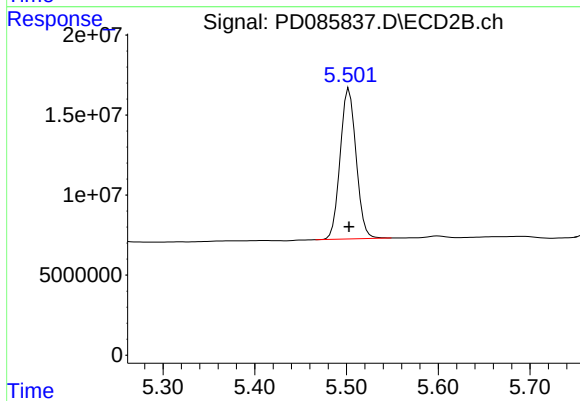


#13 Dieldrin

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 113307778
Conc: 20.17 ng/ml

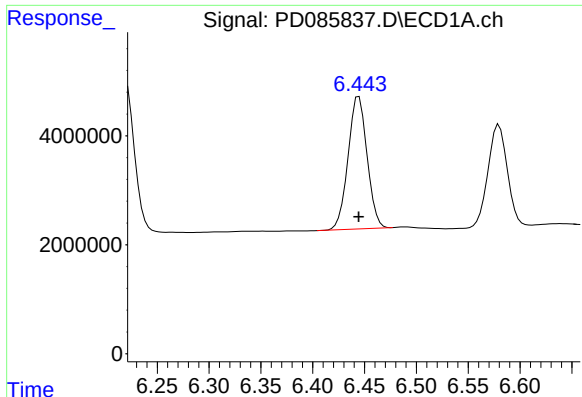


#14 Endrin

R.T.: 6.445 min
Delta R.T.: 0.000 min
Response: 31022344
Conc: 19.72 ng/ml

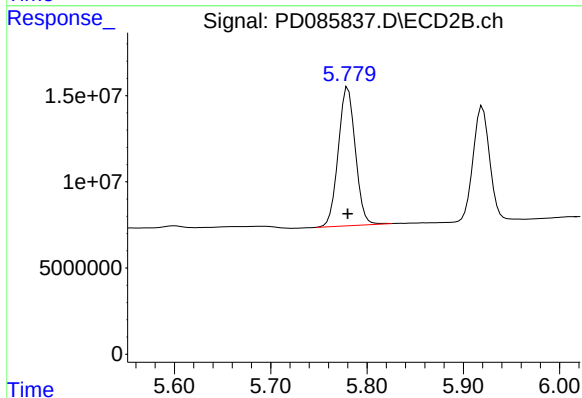


#14 Endrin

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 98755106
Conc: 20.51 ng/ml

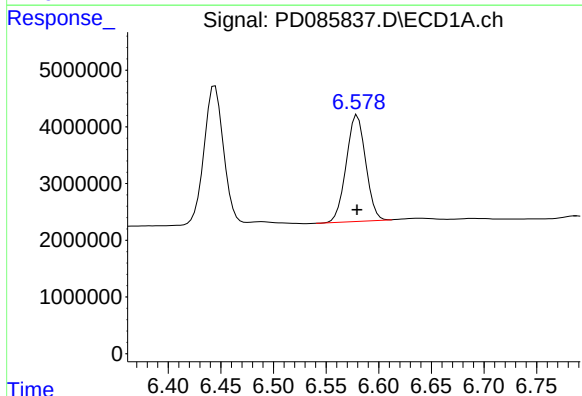


#16 4,4'-DDD

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 24157728
Conc: 19.30 ng/ml

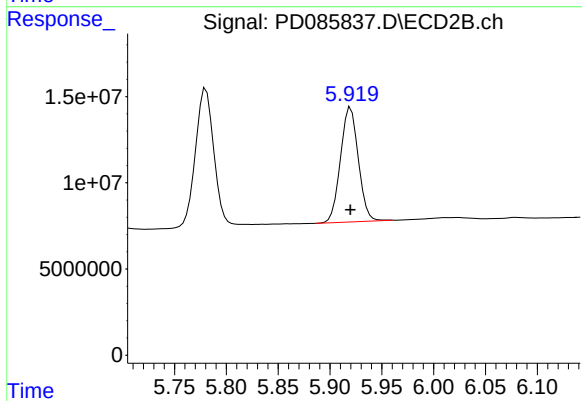


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 79837354
Conc: 20.17 ng/ml

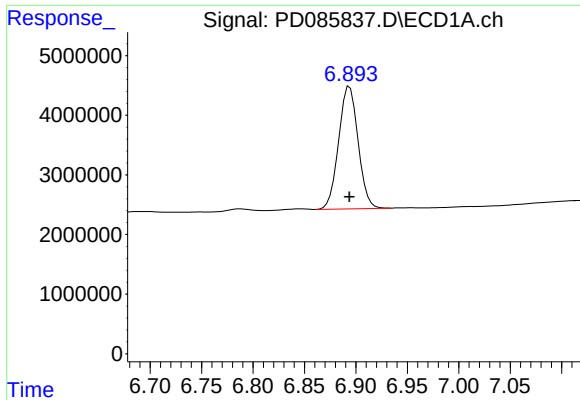


#17 4,4'-DDT

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 27038724
Conc: 19.47 ng/ml

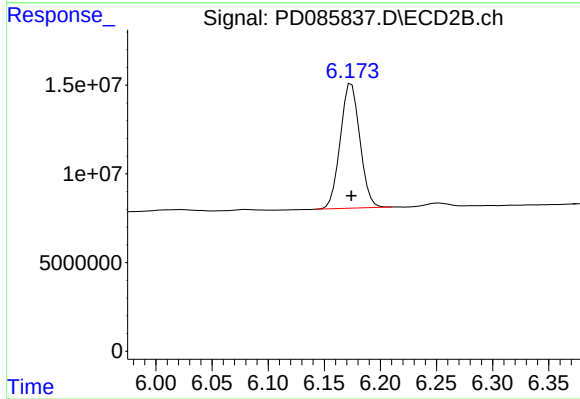


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 85586631
Conc: 19.99 ng/ml

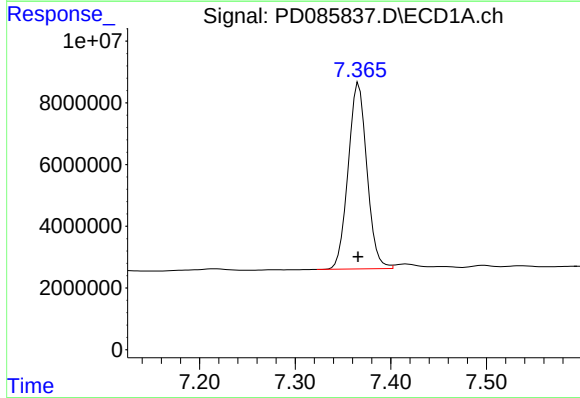


#20 Methoxychlor

R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 82421548
Conc: 101.35 ng/ml

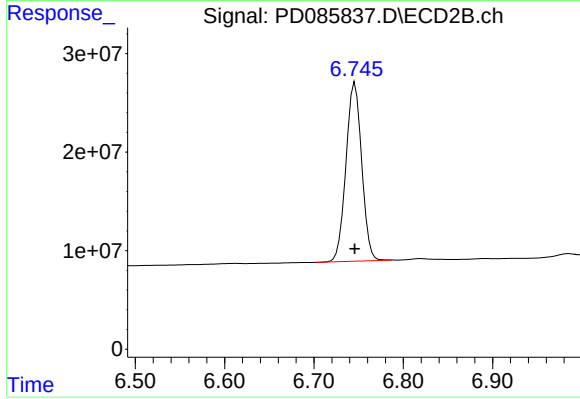


#20 Methoxychlor

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 221949836
Conc: 105.78 ng/ml

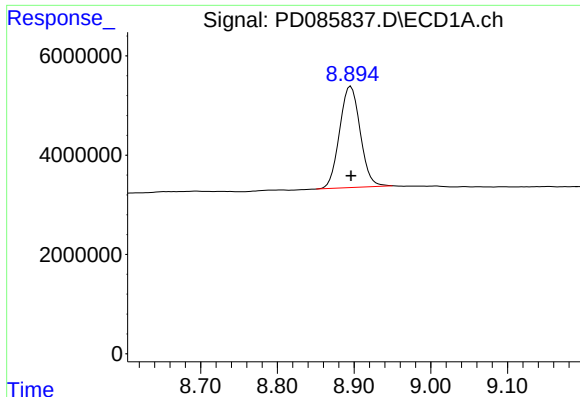

#27 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 38352265
Conc: 20.98 ng/ml

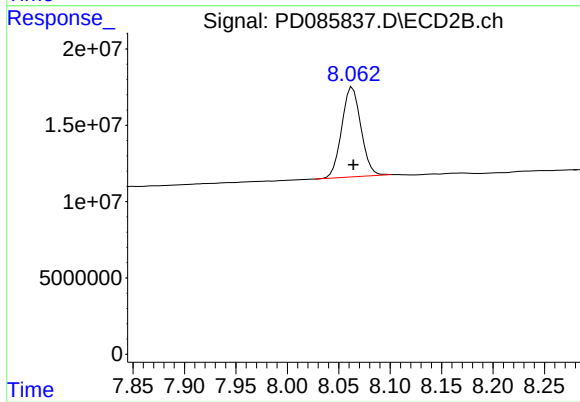

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 76728609
Conc: 20.61 ng/ml