

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 00:25
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 00:58:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 00:57:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	2.878	22855558	85782996	20.000	20.000
27)	SA Decachlor...	8.896	8.064	73130363	148.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.889	3.388	40841843	126.9E6	20.000	20.000
3)	MA gamma-BHC...	4.217	3.722	42231067	121.5E6	20.000	20.000
4)	MA Heptachlor	4.809	4.073	40839994	116.1E6	20.000	20.000
9)	A Endosulfan I	5.947	5.236	36337773	100.3E6	20.000	20.000
13)	MA Dieldrin	6.219	5.503	79285654	224.8E6	40.000	40.000
14)	MA Endrin	6.444	5.780	62935512	192.6E6	40.000	40.000
16)	A 4,4'-DDD	6.579	5.920	50061984	158.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.894	6.174	55535952	171.3E6	40.000	40.000
20)	A Methoxychlor	7.366	6.746	162.6E6	419.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 00:25
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 00:58:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 00:57:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

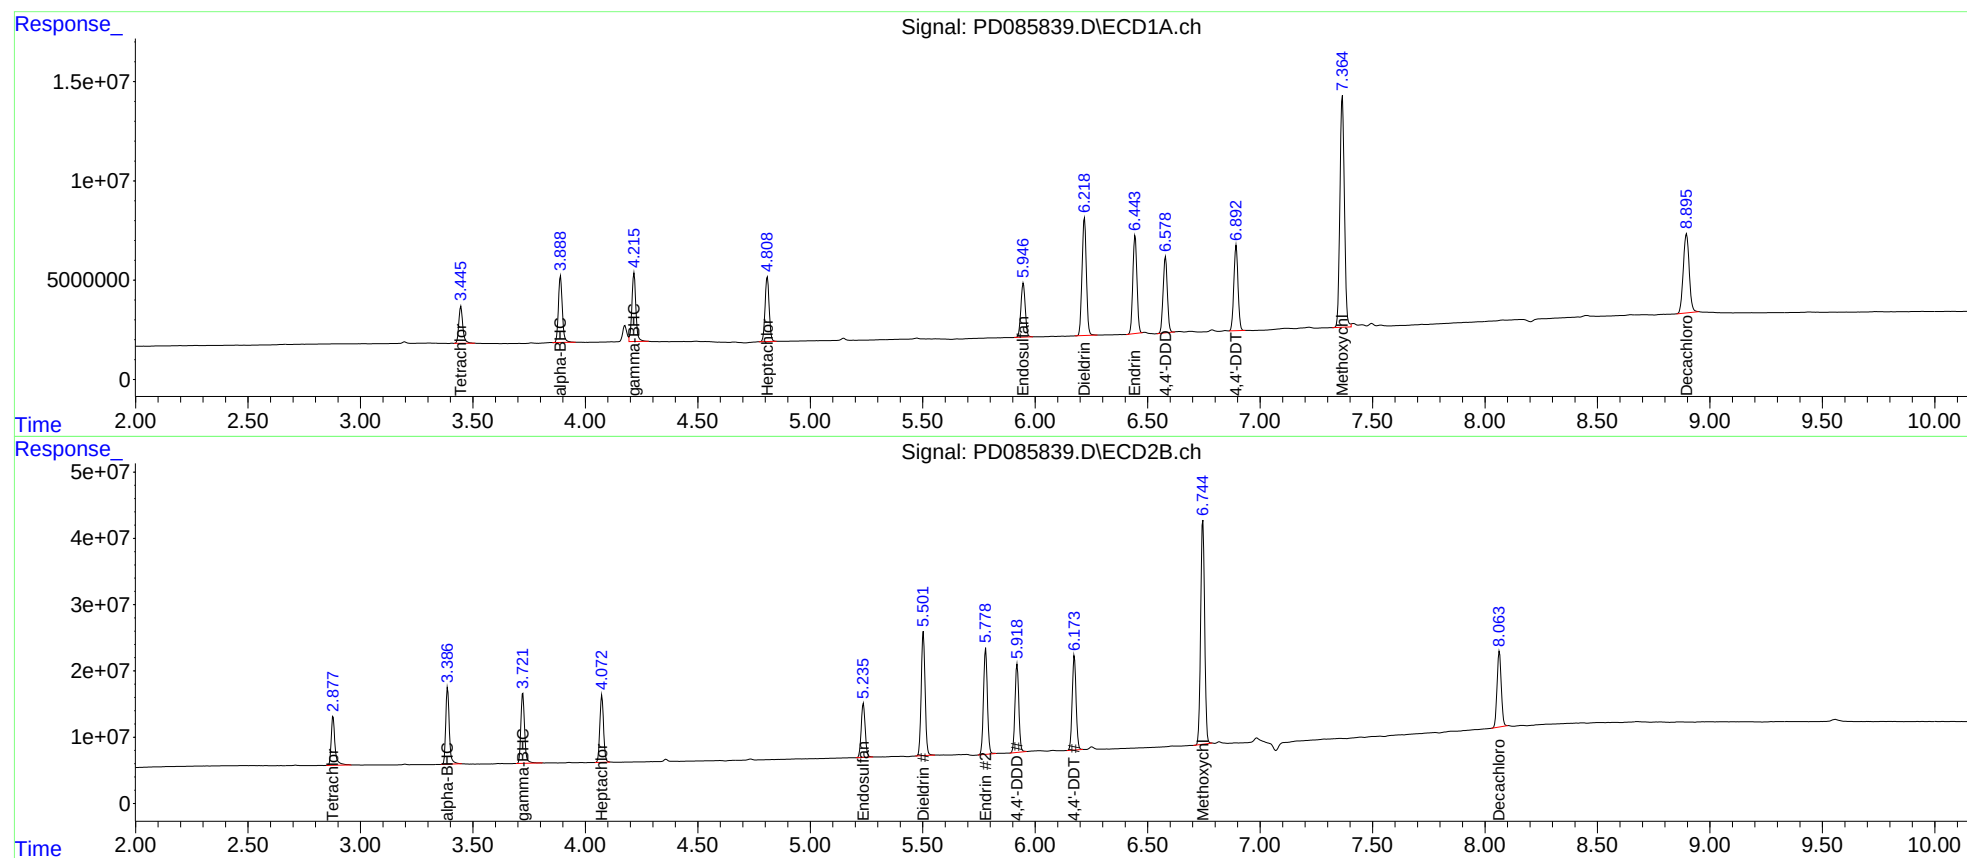

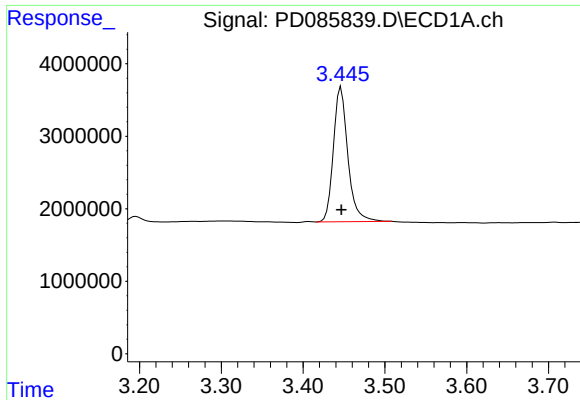


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 22855558
Conc: 20.00 ng/ml

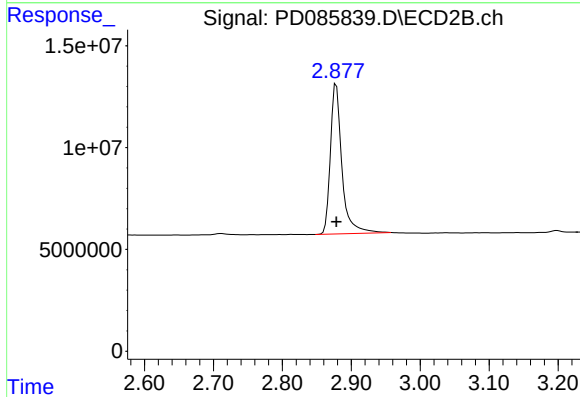


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 85782996
Conc: 20.00 ng/ml

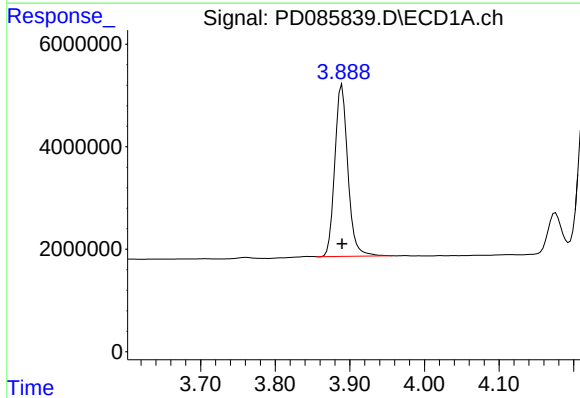


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: 0.000 min
Response: 40841843
Conc: 20.00 ng/ml

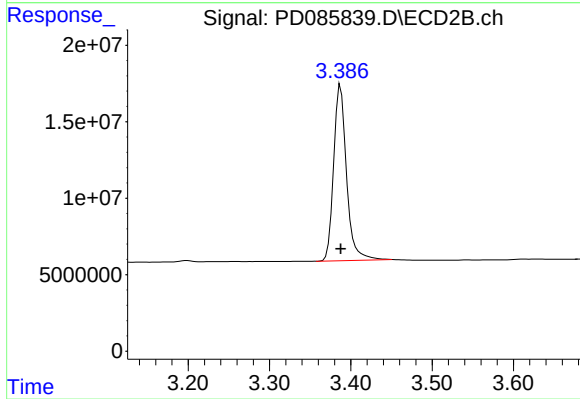


#2 alpha-BHC

R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 126918857
Conc: 20.00 ng/ml

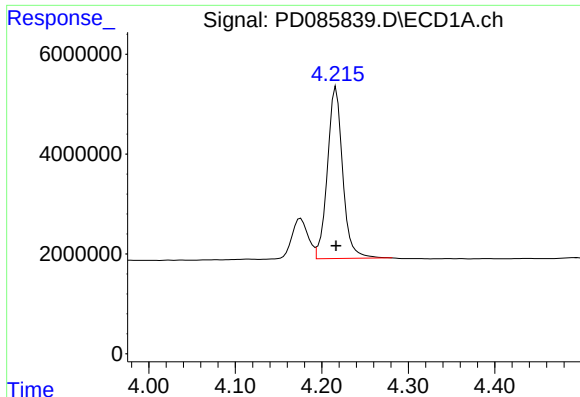


#3 gamma-BHC (Lindane)

R.T.: 4.217 min
Delta R.T.: 0.000 min
Response: 42231067
Conc: 20.00 ng/ml

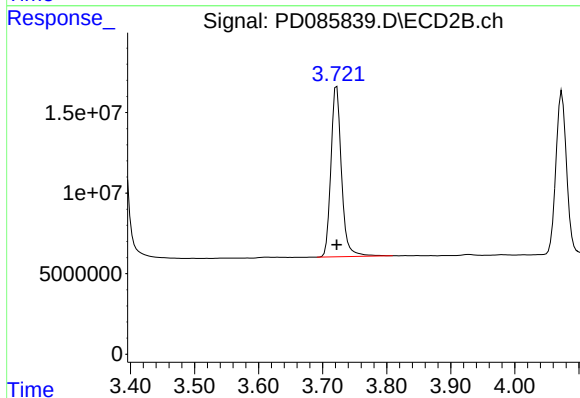


#3 gamma-BHC (Lindane)

R.T.: 3.722 min
Delta R.T.: 0.000 min
Response: 121471589
Conc: 20.00 ng/ml

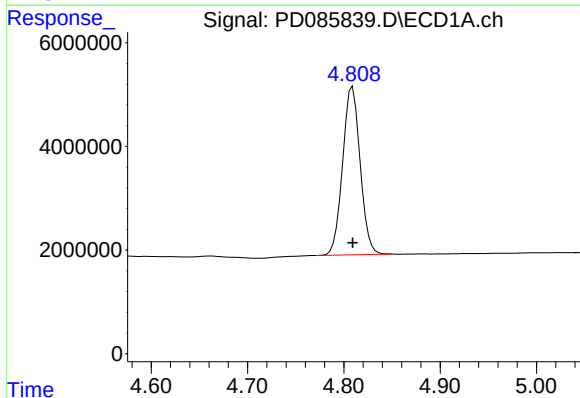


#4 Heptachlor

R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 40839994
Conc: 20.00 ng/ml

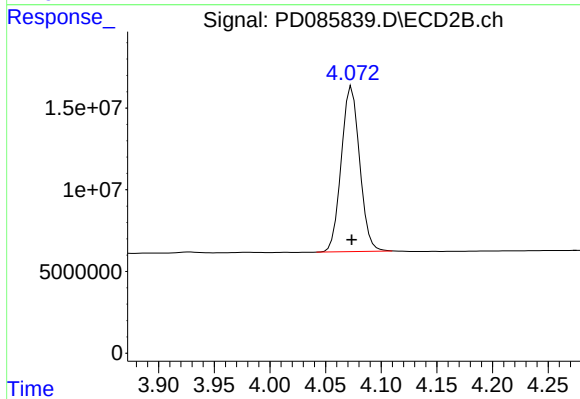


#4 Heptachlor

R.T.: 4.073 min
Delta R.T.: 0.000 min
Response: 116137079
Conc: 20.00 ng/ml

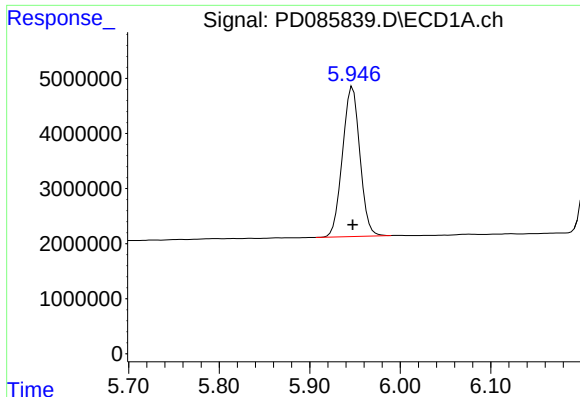


#9 Endosulfan I

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 36337773
Conc: 20.00 ng/ml

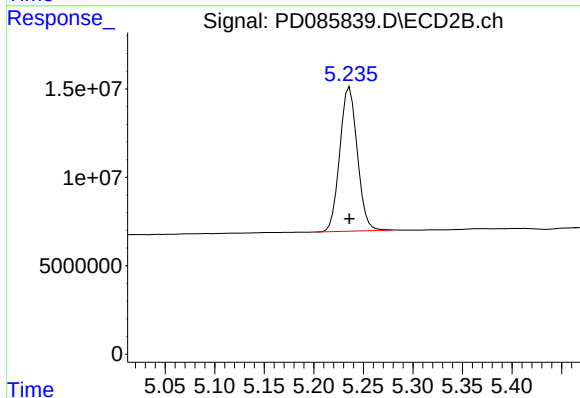


#9 Endosulfan I

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 100286402
Conc: 20.00 ng/ml

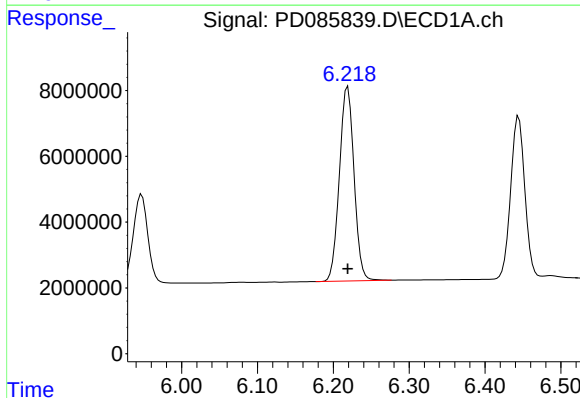


#13 Dieldrin

R.T.: 6.219 min
Delta R.T.: 0.000 min
Response: 79285654
Conc: 40.00 ng/ml

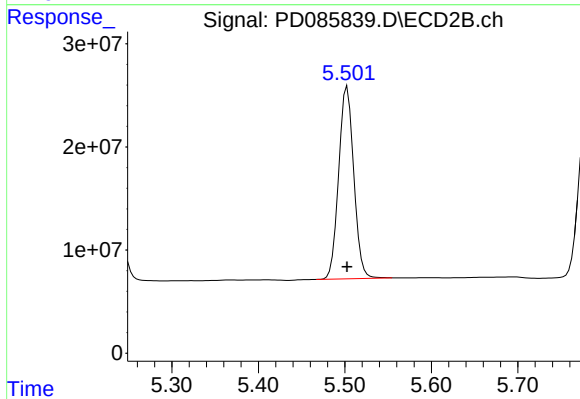


#13 Dieldrin

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 224754311
Conc: 40.00 ng/ml

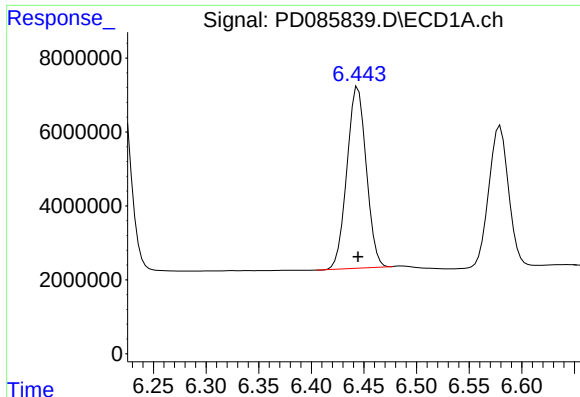


#14 Endrin

R.T.: 6.444 min
Delta R.T.: 0.000 min
Response: 62935512
Conc: 40.00 ng/ml

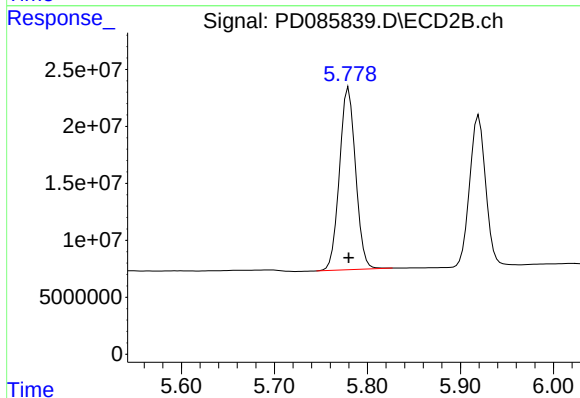


#14 Endrin

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 192579458
Conc: 40.00 ng/ml

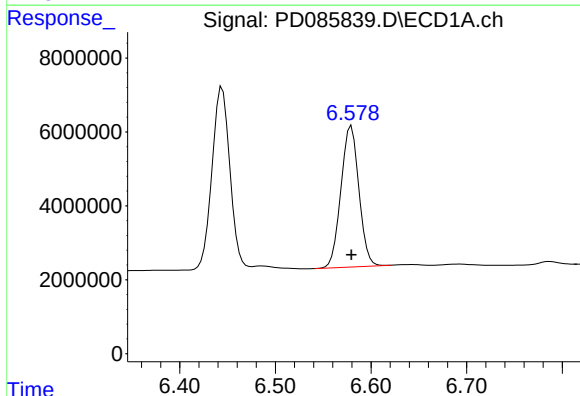


#16 4,4'-DDD

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 50061984
Conc: 40.00 ng/ml

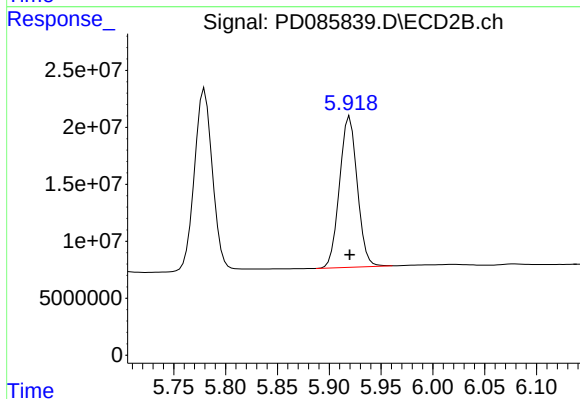


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 158298938
Conc: 40.00 ng/ml

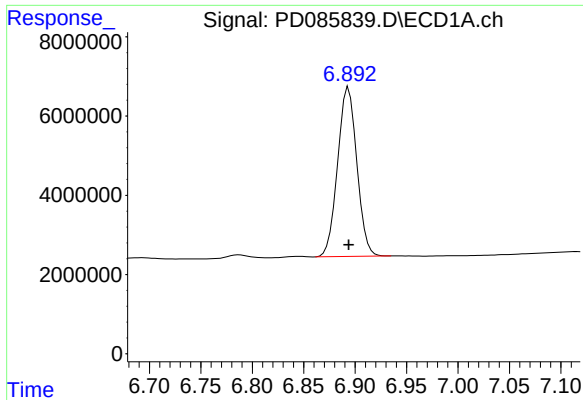


#17 4,4'-DDT

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 55535952
Conc: 40.00 ng/ml

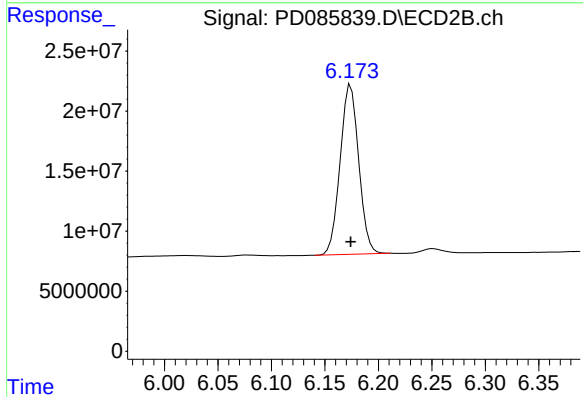


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 171256627
Conc: 40.00 ng/ml

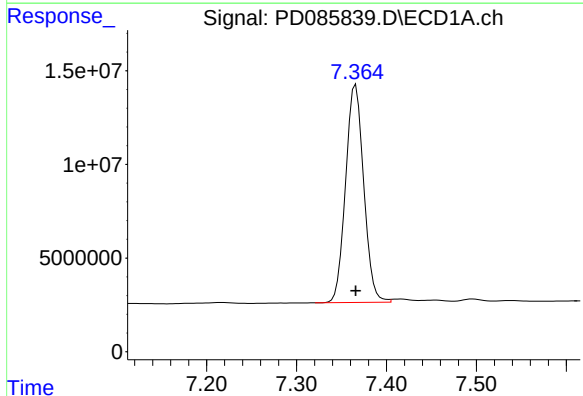


#20 Methoxychlor

R.T.: 7.366 min
Delta R.T.: 0.000 min
Response: 162648814
Conc: 200.00 ng/ml

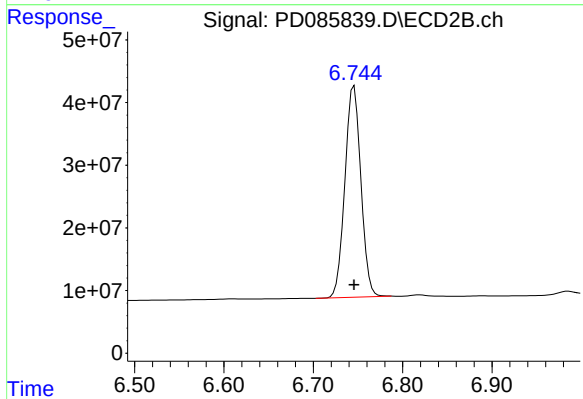


#20 Methoxychlor

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 419662424
Conc: 200.00 ng/ml

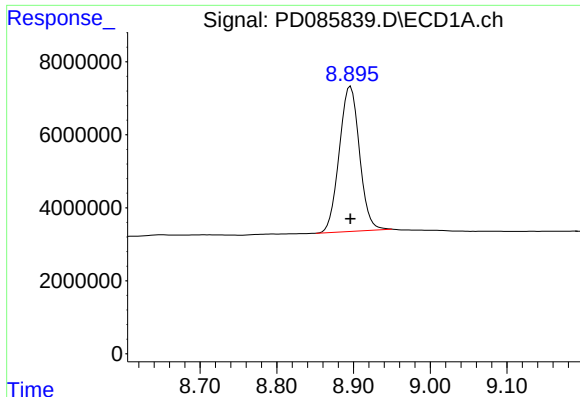

#27 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 73130363
Conc: 40.00 ng/ml

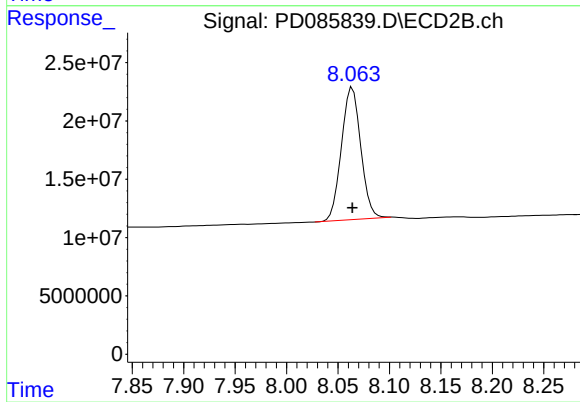

#27 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 148929903
Conc: 40.00 ng/ml