

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 00:55
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:09:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 01:01:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	2.878	44990934	164.7E6	38.783	37.766
27) SA Decachlor...	8.894	8.064	140.0E6	289.1E6	75.515	77.424
Target Compounds						
2) A alpha-BHC	3.888	3.388	87452378	253.0E6	44.624	40.270
3) MA gamma-BHC...	4.215	3.722	85664580	240.0E6	39.114	39.696
4) MA Heptachlor	4.808	4.074	83033501	227.6E6	41.350	39.364
9) A Endosulfan I	5.946	5.236	72792511	196.3E6	40.219	39.105
13) MA Dieldrin	6.218	5.503	165.8E6	442.5E6	85.820	79.163
14) MA Endrin	6.443	5.780	130.8E6	379.1E6	88.140	78.491
16) A 4,4'-DDD	6.578	5.920	104.6E6	314.3E6	88.156	80.000
17) MA 4,4'-DDT	6.893	6.174	115.7E6	342.9E6	89.059	81.284
20) A Methoxychlor	7.365	6.745	327.7E6	788.9E6	401.870	364.120


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 00:55
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:09:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 01:01:30 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

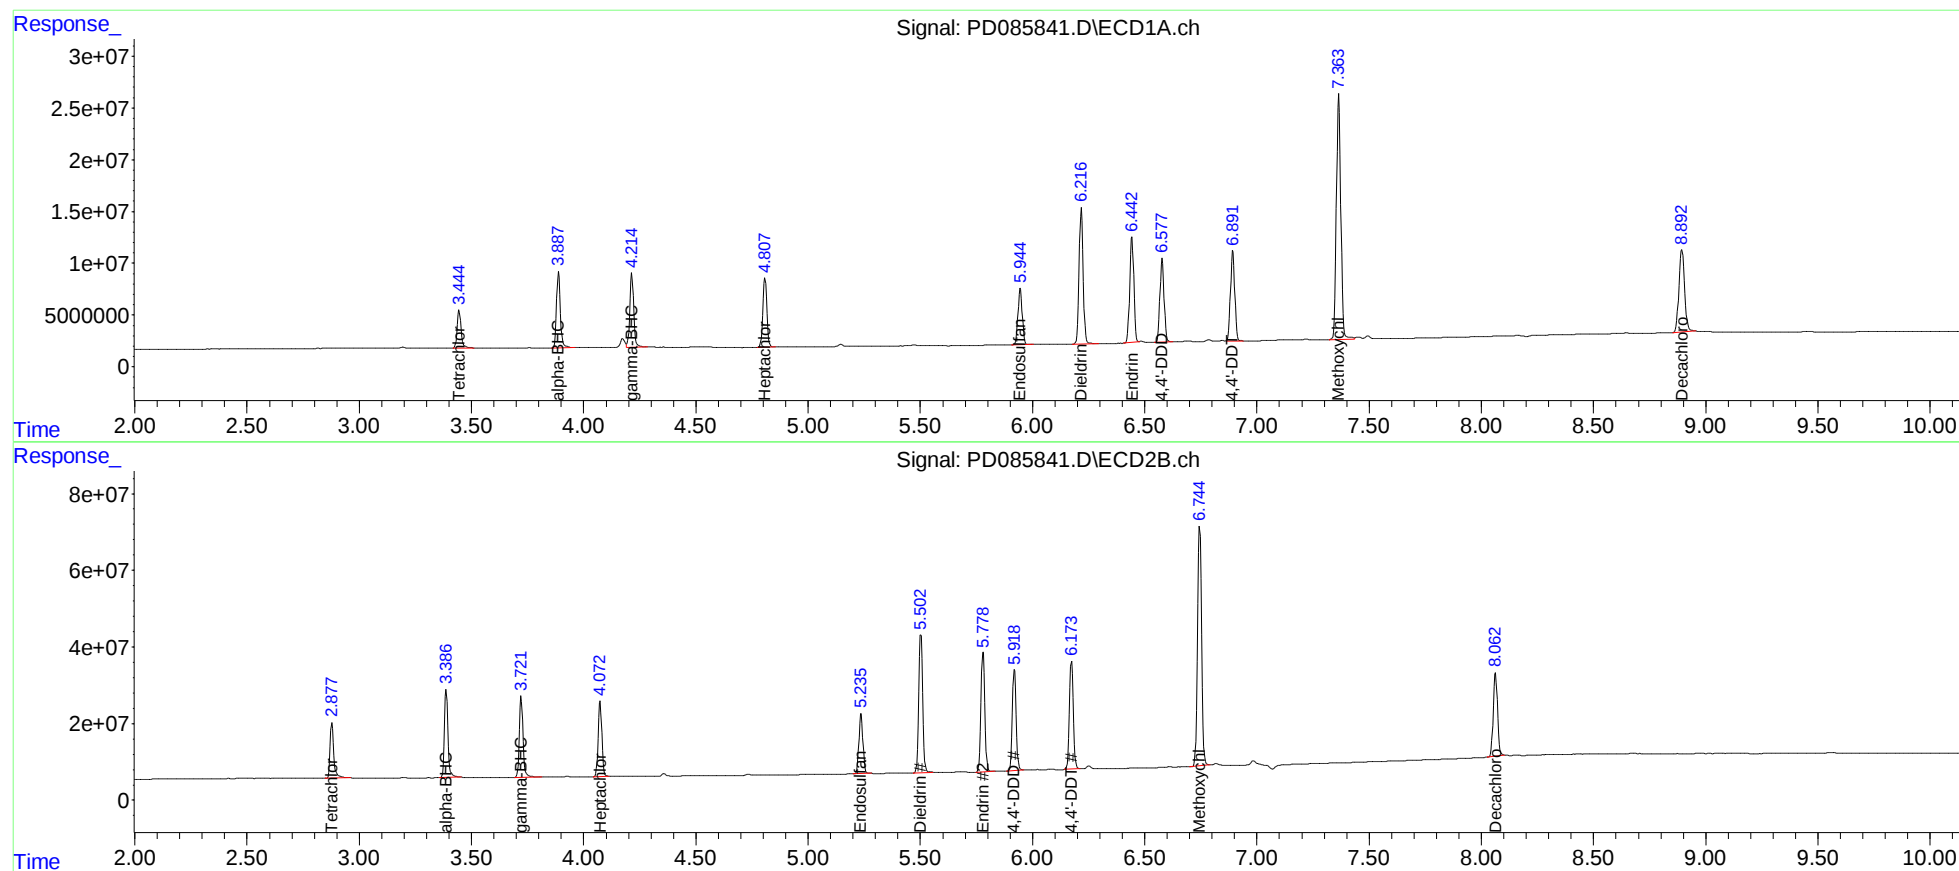

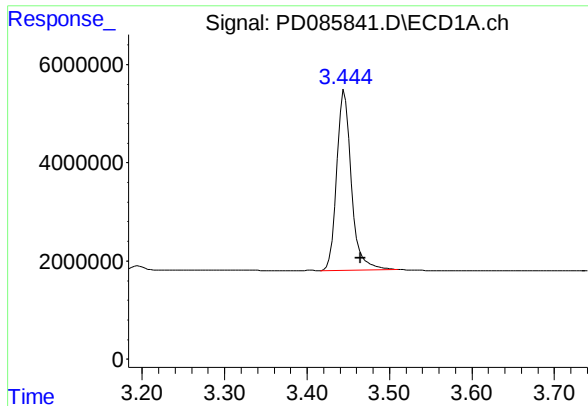


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: -0.020 min
Response: 44990934
Conc: 38.78 ng/ml

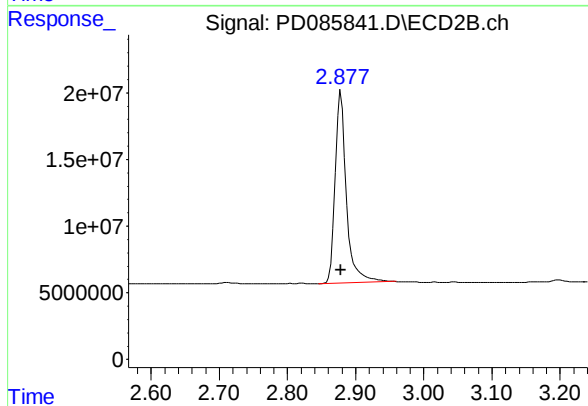


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 164711549
Conc: 37.77 ng/ml

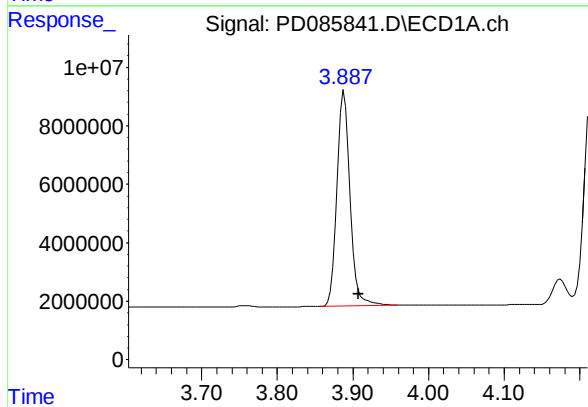


#2 alpha-BHC

R.T.: 3.888 min
Delta R.T.: -0.019 min
Response: 87452378
Conc: 44.62 ng/ml

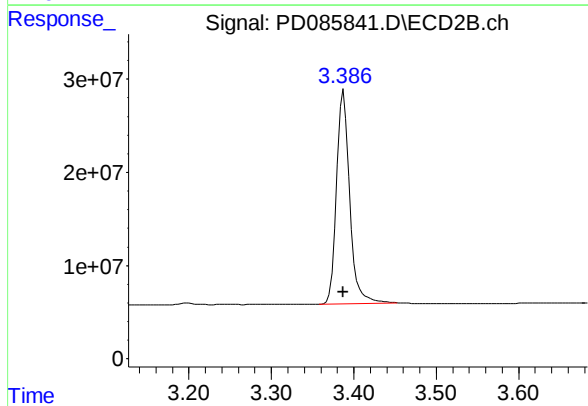


#2 alpha-BHC

R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 253002591
Conc: 40.27 ng/ml

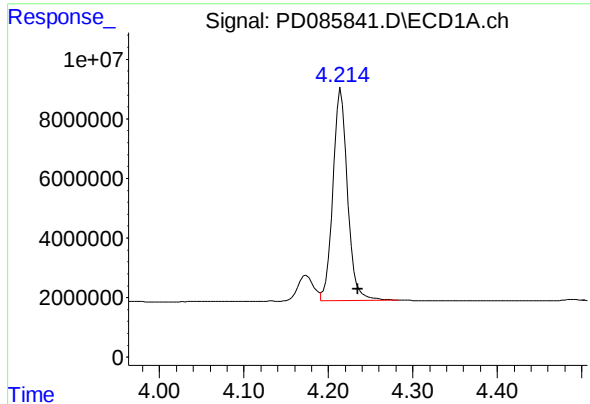


#3 gamma-BHC (Lindane)

R.T.: 4.215 min
Delta R.T.: -0.020 min
Response: 85664580
Conc: 39.11 ng/ml

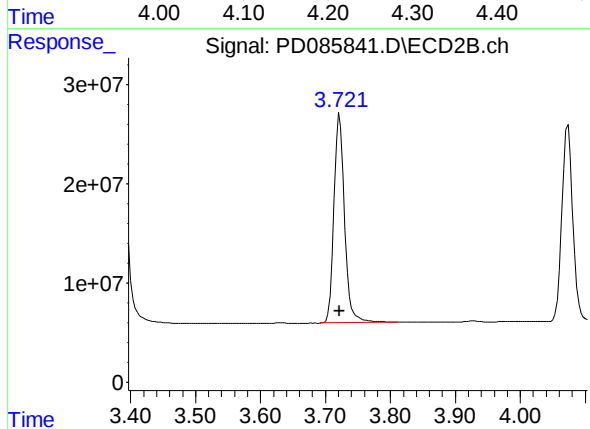


#3 gamma-BHC (Lindane)

R.T.: 3.722 min
Delta R.T.: 0.000 min
Response: 240049626
Conc: 39.70 ng/ml

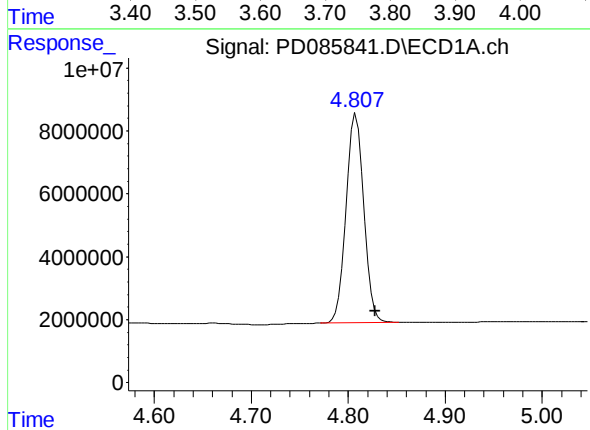


#4 Heptachlor

R.T.: 4.808 min
Delta R.T.: -0.020 min
Response: 83033501
Conc: 41.35 ng/ml

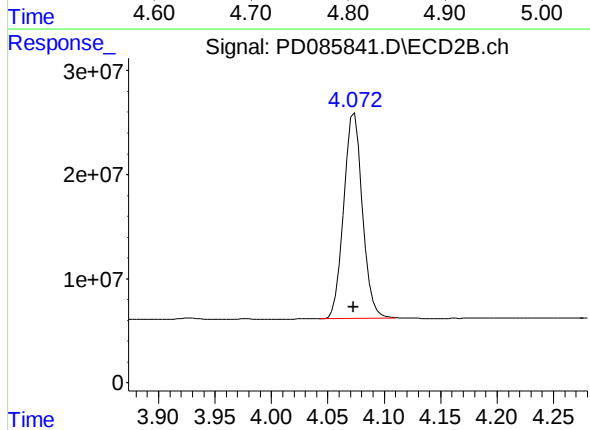


#4 Heptachlor

R.T.: 4.074 min
Delta R.T.: 0.000 min
Response: 227590289
Conc: 39.36 ng/ml

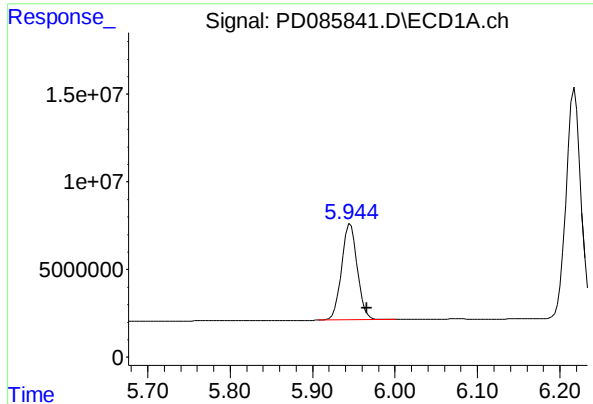


#9 Endosulfan I

R.T.: 5.946 min
Delta R.T.: -0.020 min
Response: 72792511
Conc: 40.22 ng/ml

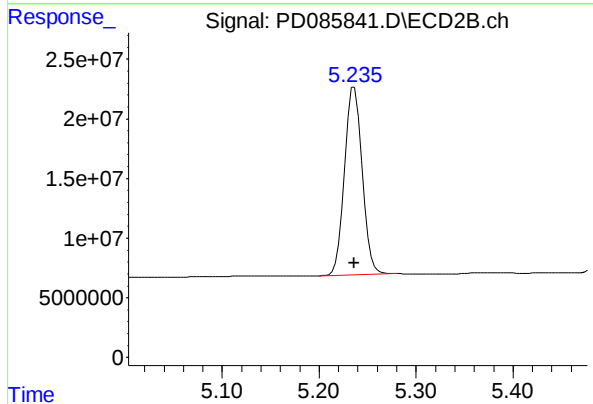


#9 Endosulfan I

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 196253989
Conc: 39.11 ng/ml

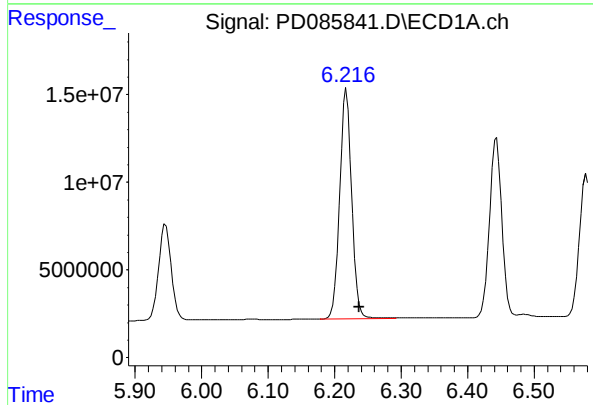


#13 Dieldrin

R.T.: 6.218 min
Delta R.T.: -0.020 min
Response: 165779897
Conc: 85.82 ng/ml

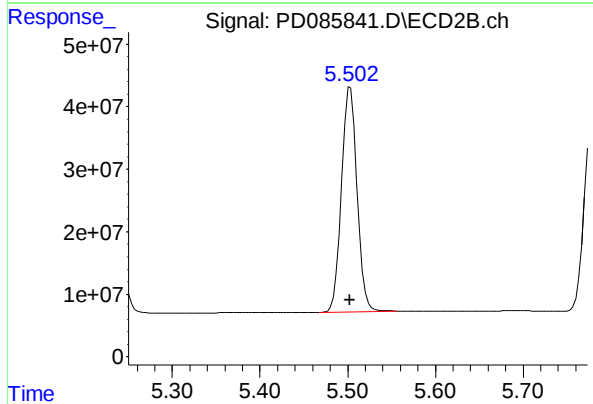


#13 Dieldrin

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 442506074
Conc: 79.16 ng/ml

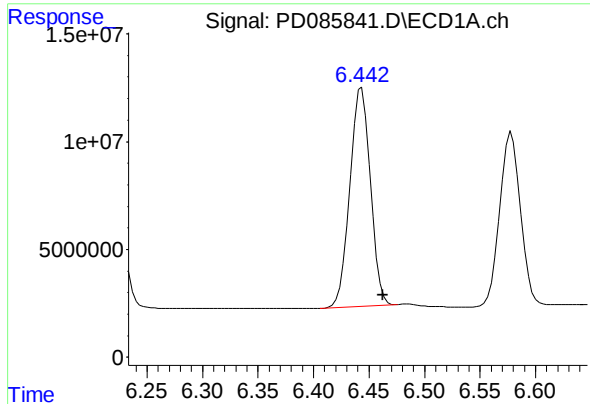


#14 Endrin

R.T.: 6.443 min
Delta R.T.: -0.019 min
Response: 130821490
Conc: 88.14 ng/ml

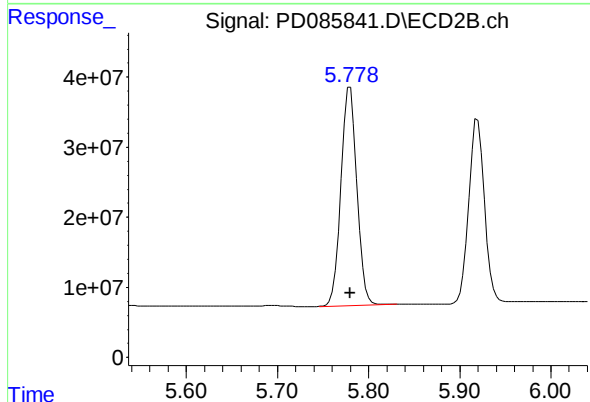


#14 Endrin

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 379060721
Conc: 78.49 ng/ml

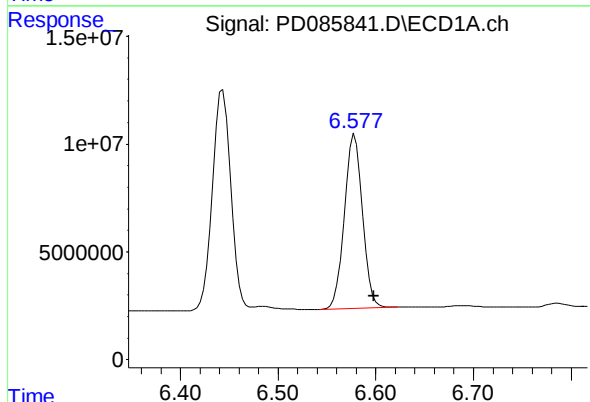


#16 4,4'-DDD

R.T.: 6.578 min
Delta R.T.: -0.020 min
Response: 104613222
Conc: 88.16 ng/ml

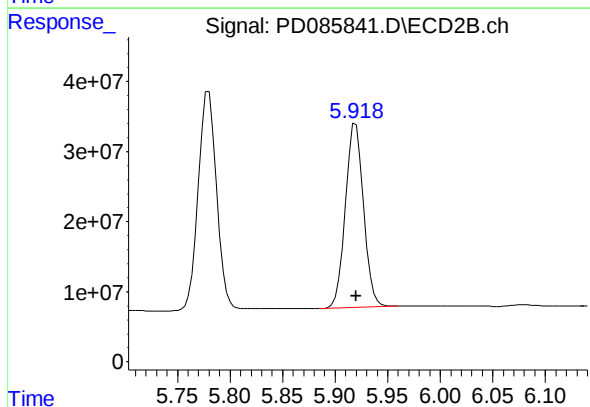


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 314322479
Conc: 80.00 ng/ml

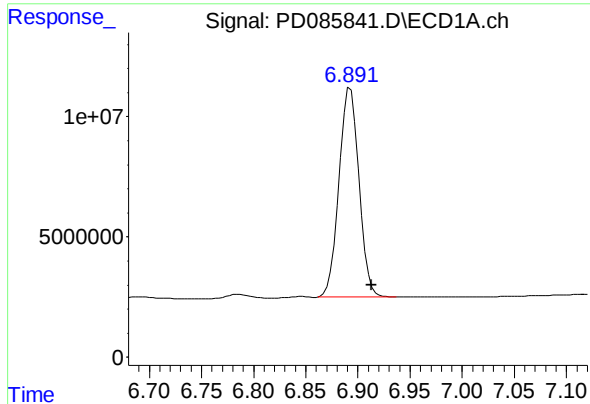


#17 4,4'-DDT

R.T.: 6.893 min
Delta R.T.: -0.020 min
Response: 115663619
Conc: 89.06 ng/ml

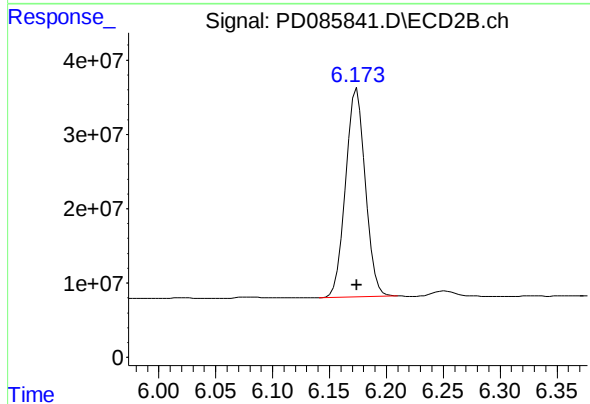


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 342873124
Conc: 81.28 ng/ml

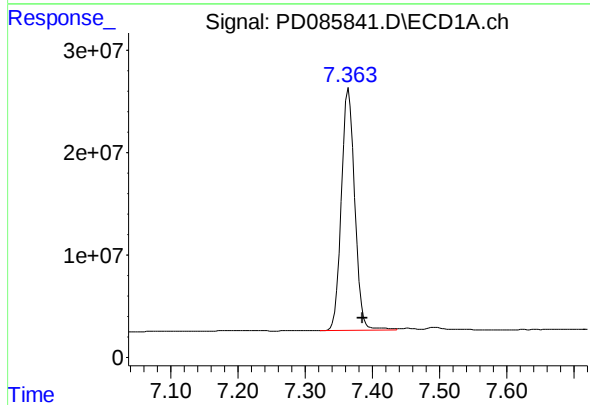


#20 Methoxychlor

R.T.: 7.365 min
Delta R.T.: -0.020 min
Response: 327659018
Conc: 401.87 ng/ml

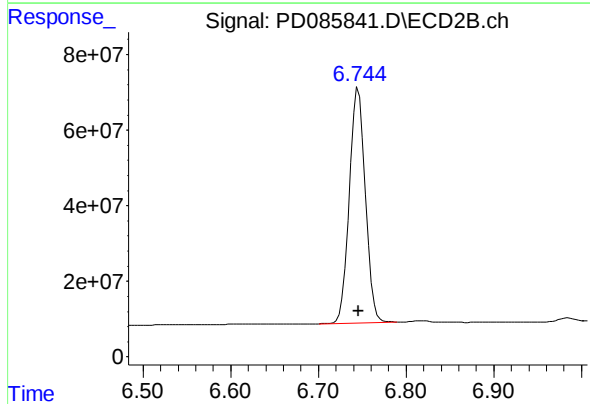


#20 Methoxychlor

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 788856842
Conc: 364.12 ng/ml

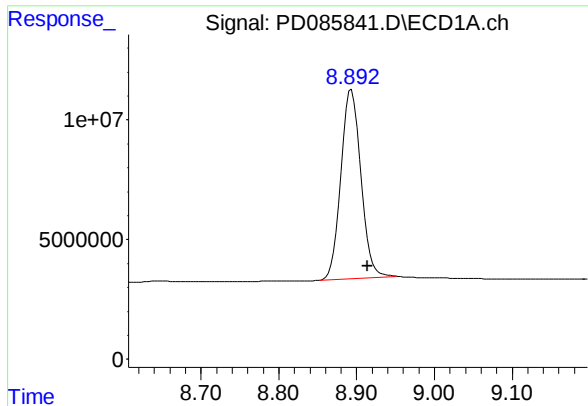

#27 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.021 min
Response: 139982465
Conc: 75.51 ng/ml

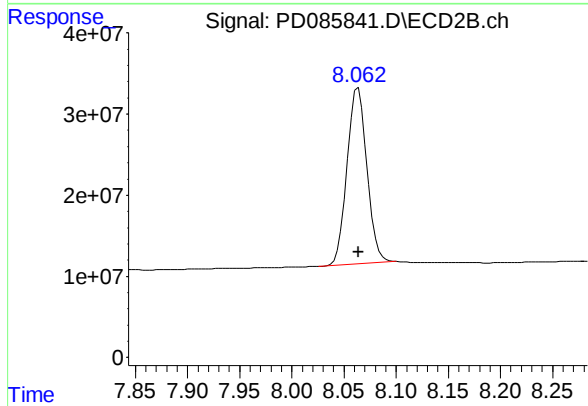

#27 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 289109823
Conc: 77.42 ng/ml