

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 01:10
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 02:11:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 02:08:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	2.878	44824695	165.0E6	38.765	38.524
27)	SA Decachlor...	8.894	8.064	139.9E6	290.9E6	76.034	77.414
Target Compounds							
5)	MB Aldrin	5.147	4.359	83938017	230.3E6	40.536	38.939
6)	B beta-BHC	4.402	4.016	34179277	100.6E6	38.255	38.112
7)	B delta-BHC	4.646	4.252	77682949	234.0E6	41.641	39.266
8)	B Heptachlo...	5.566	4.862	75205861	211.2E6	40.110	38.603
10)	B trans-Chl...	5.820	5.114	73423960	209.3E6	39.695	38.869
11)	B cis-Chlor...	5.900	5.179	75887261	213.0E6	39.621	38.629
12)	B 4,4'-DDE	6.072	5.364	135.2E6	383.2E6	83.467	79.154
15)	B Endosulfa...	6.656	6.072	133.8E6	356.2E6	79.751	77.395
18)	B Endrin al...	6.785	6.251	103.3E6	279.4E6	78.506	76.850
19)	B Endosulfa...	7.018	6.475	124.8E6	332.4E6	79.315	76.992
21)	B Endrin ke...	7.495	6.985	138.6E6	393.5E6	80.000	75.897


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 01:10
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 02:11:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 02:08:19 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

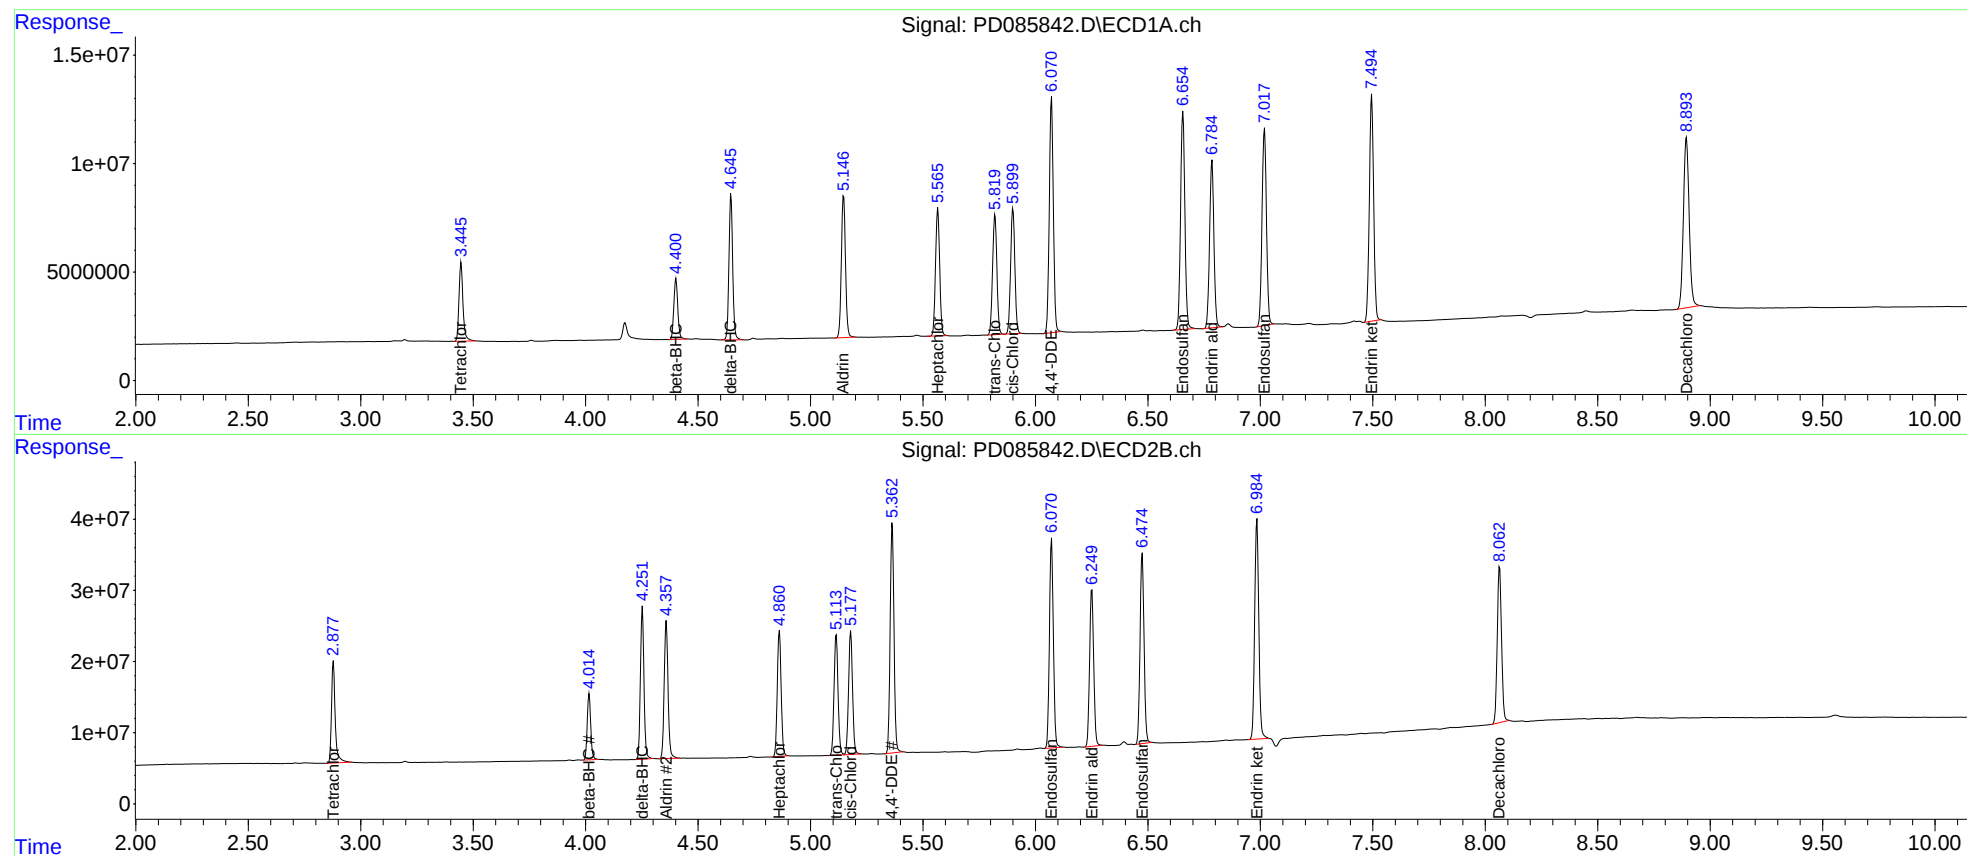

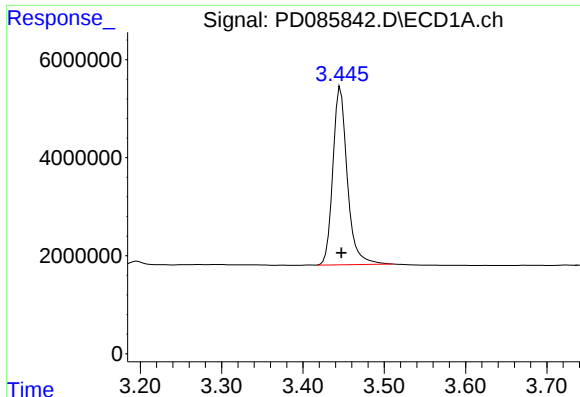


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 44824695
Conc: 38.77 ng/ml

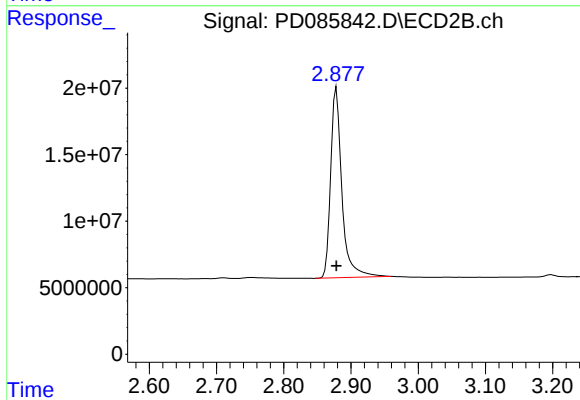


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 164975846
Conc: 38.52 ng/ml

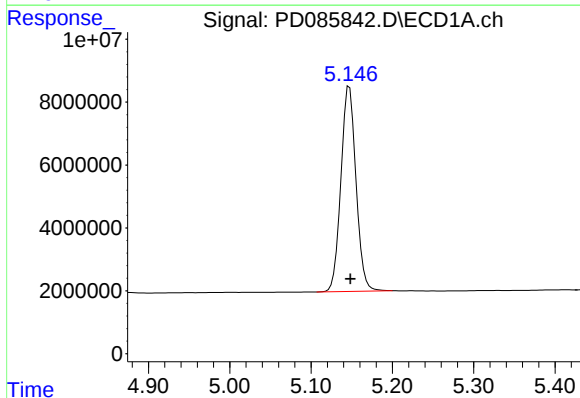


#5 Aldrin

R.T.: 5.147 min
Delta R.T.: -0.001 min
Response: 83938017
Conc: 40.54 ng/ml

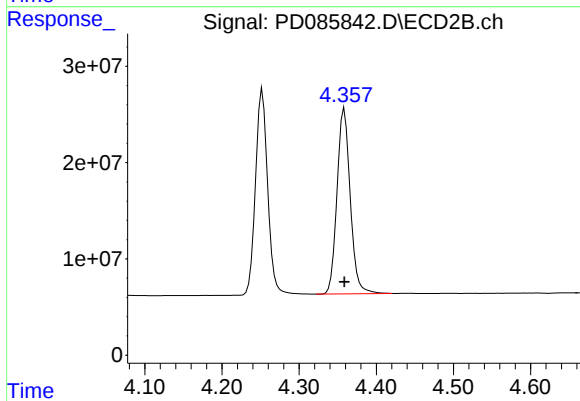


#5 Aldrin

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 230287575
Conc: 38.94 ng/ml

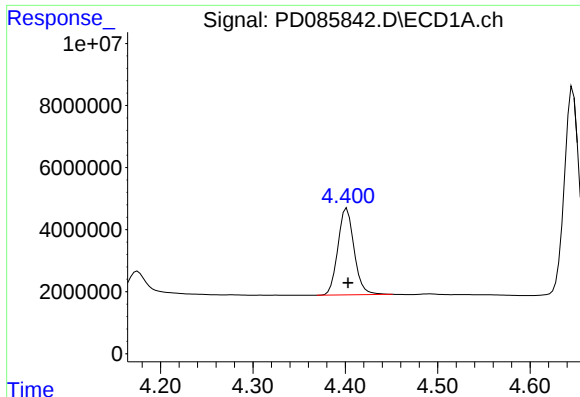


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.001 min
Response: 34179277
Conc: 38.26 ng/ml

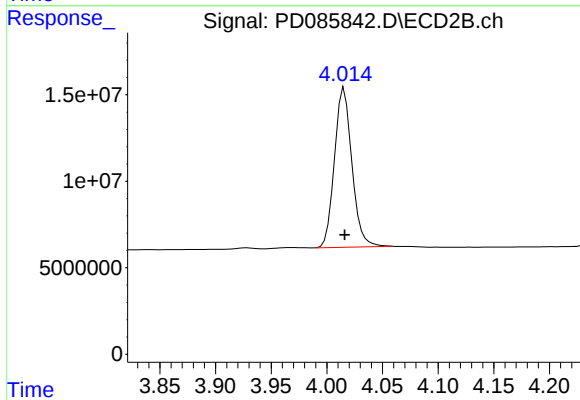


#6 beta-BHC

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 100609043
Conc: 38.11 ng/ml

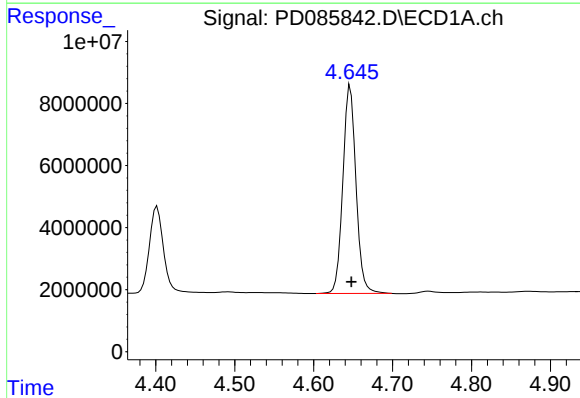


#7 delta-BHC

R.T.: 4.646 min
Delta R.T.: -0.002 min
Response: 77682949
Conc: 41.64 ng/ml

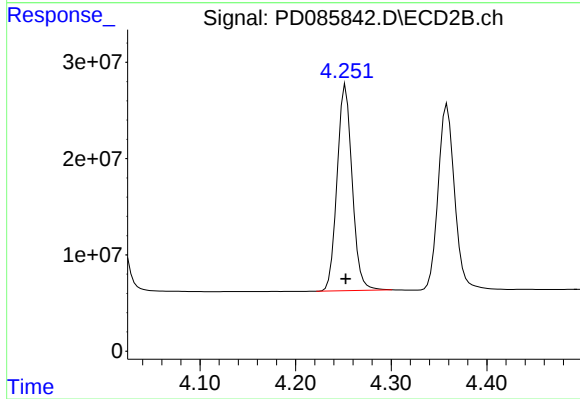


#7 delta-BHC

R.T.: 4.252 min
Delta R.T.: 0.000 min
Response: 234005608
Conc: 39.27 ng/ml

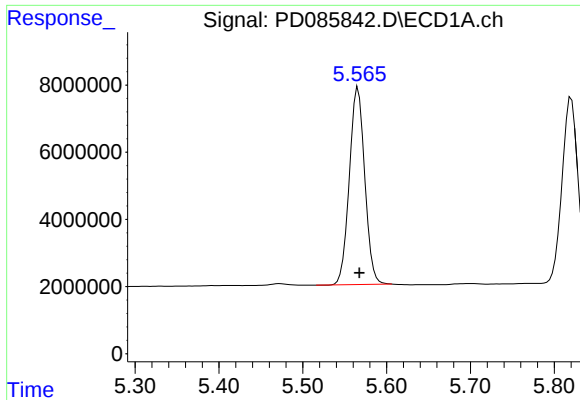


#8 Heptachlor epoxide

R.T.: 5.566 min
Delta R.T.: -0.001 min
Response: 75205861
Conc: 40.11 ng/ml

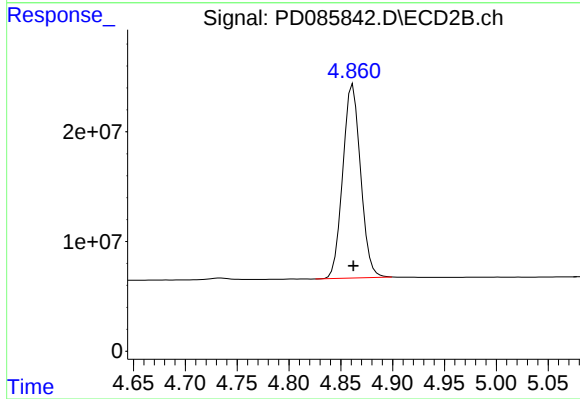


#8 Heptachlor epoxide

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 211156851
Conc: 38.60 ng/ml

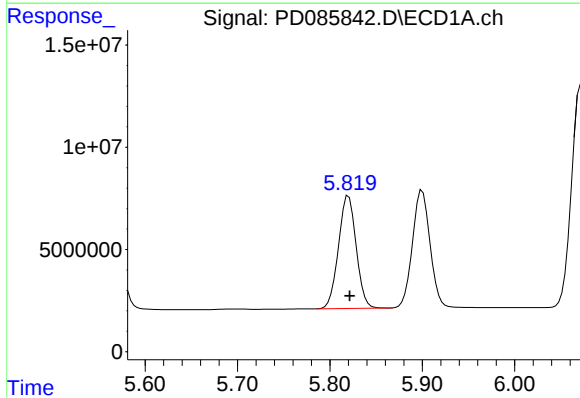


#10 trans-Chlordane

R.T.: 5.820 min
Delta R.T.: -0.001 min
Response: 73423960
Conc: 39.70 ng/ml

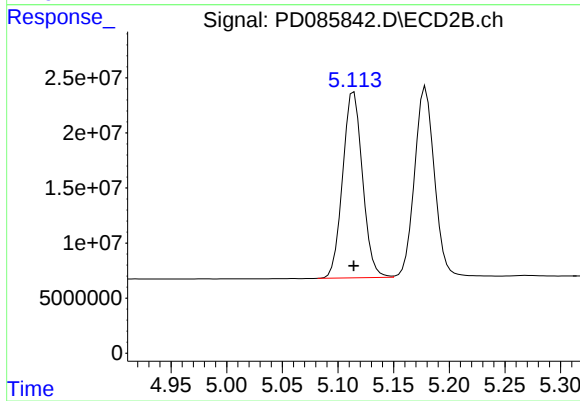


#10 trans-Chlordane

R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 209279533
Conc: 38.87 ng/ml

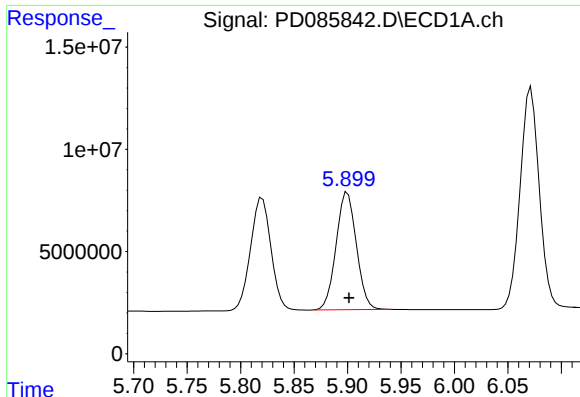


#11 cis-Chlordane

R.T.: 5.900 min
Delta R.T.: -0.002 min
Response: 75887261
Conc: 39.62 ng/ml

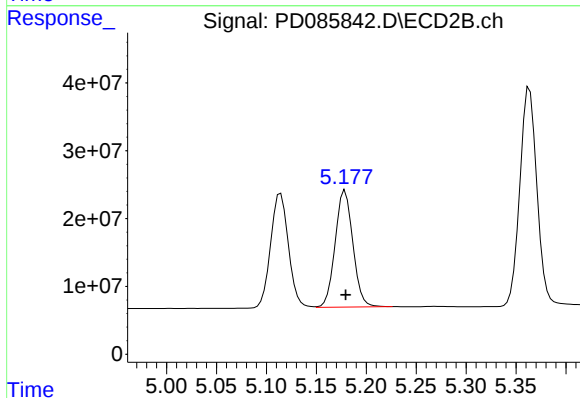


#11 cis-Chlordane

R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 212953239
Conc: 38.63 ng/ml

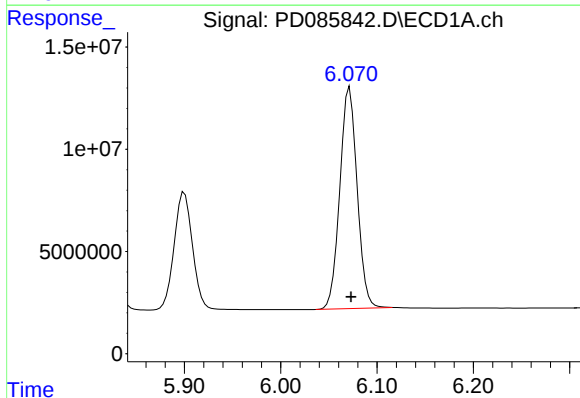


#12 4,4'-DDE

R.T.: 6.072 min
Delta R.T.: -0.001 min
Response: 135174218
Conc: 83.47 ng/ml

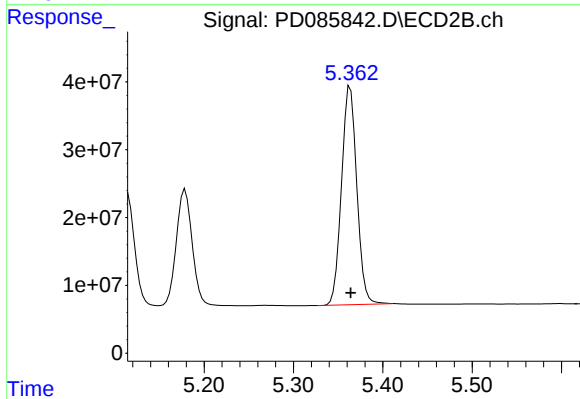


#12 4,4'-DDE

R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 383153569
Conc: 79.15 ng/ml

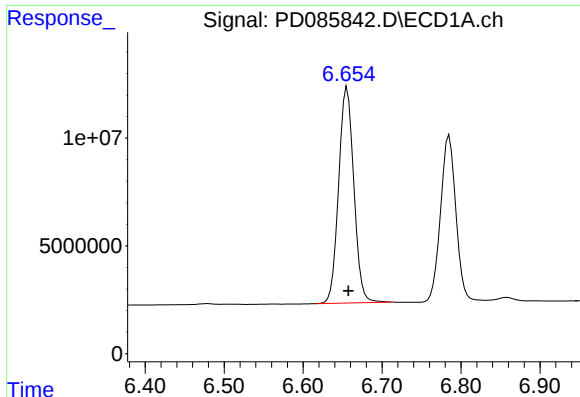


#15 Endosulfan II

R.T.: 6.656 min
Delta R.T.: -0.002 min
Response: 133759567
Conc: 79.75 ng/ml

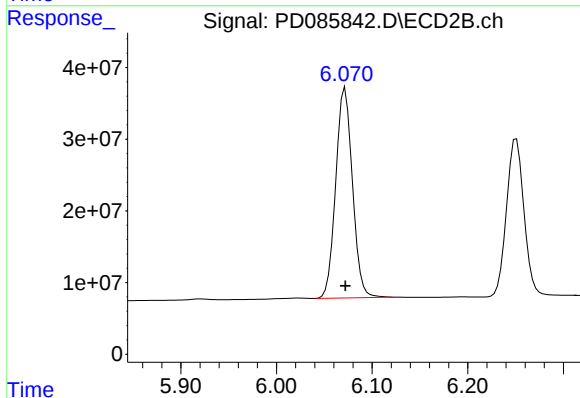


#15 Endosulfan II

R.T.: 6.072 min
Delta R.T.: 0.000 min
Response: 356191583
Conc: 77.40 ng/ml

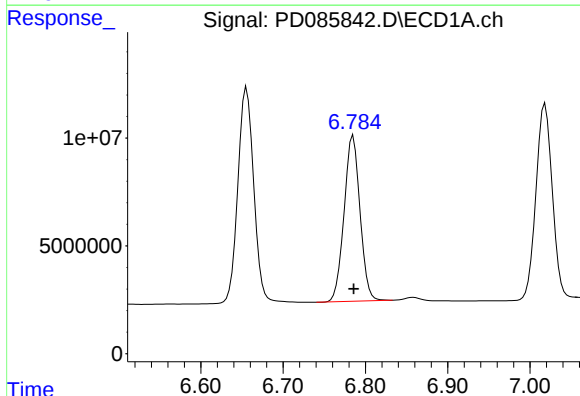


#18 Endrin aldehyde

R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 103311658
Conc: 78.51 ng/ml

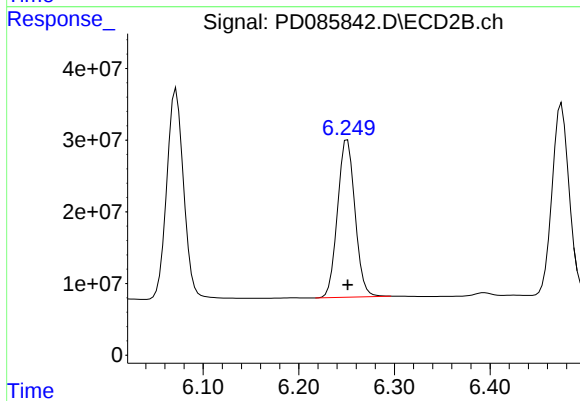


#18 Endrin aldehyde

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 279354344
Conc: 76.85 ng/ml

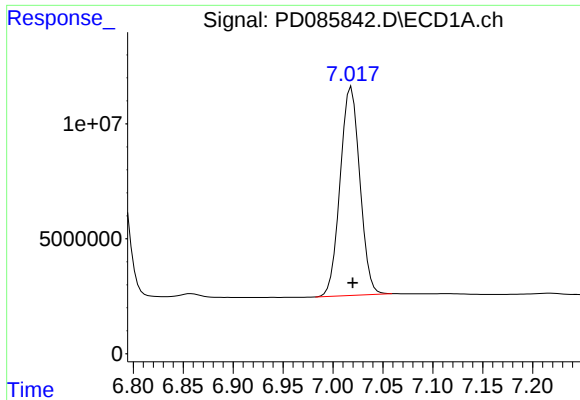


#19 Endosulfan Sulfate

R.T.: 7.018 min
Delta R.T.: -0.001 min
Response: 124809844
Conc: 79.32 ng/ml

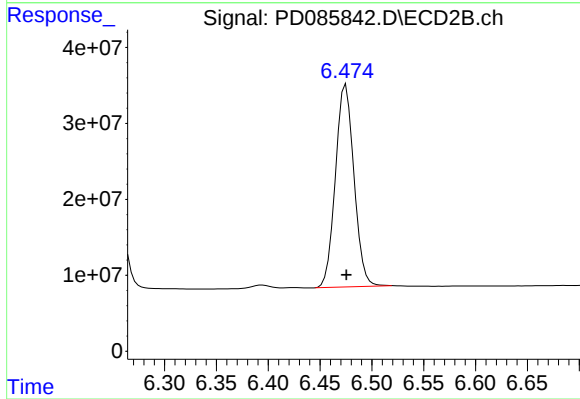


#19 Endosulfan Sulfate

R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 332442555
Conc: 76.99 ng/ml

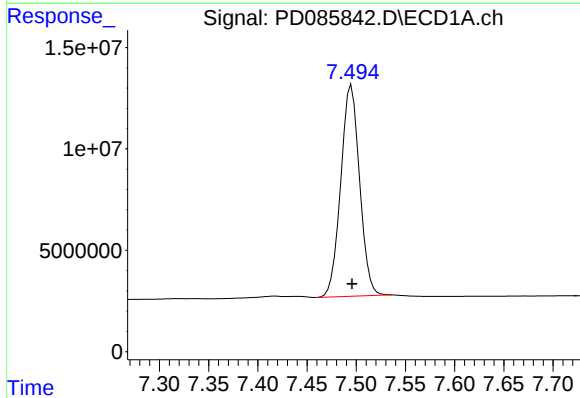


#21 Endrin ketone

R.T.: 7.495 min
Delta R.T.: 0.000 min
Response: 138649559
Conc: 80.00 ng/ml

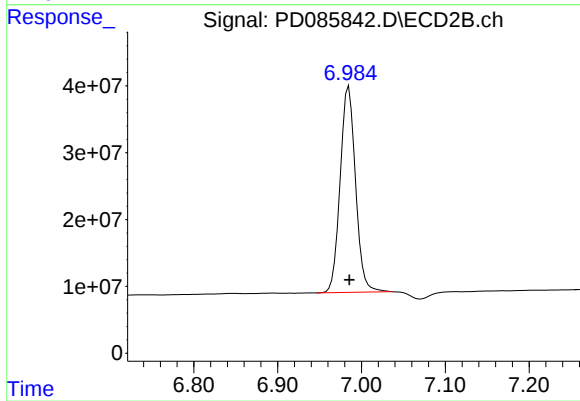


#21 Endrin ketone

R.T.: 6.985 min
Delta R.T.: 0.000 min
Response: 393481007
Conc: 75.90 ng/ml

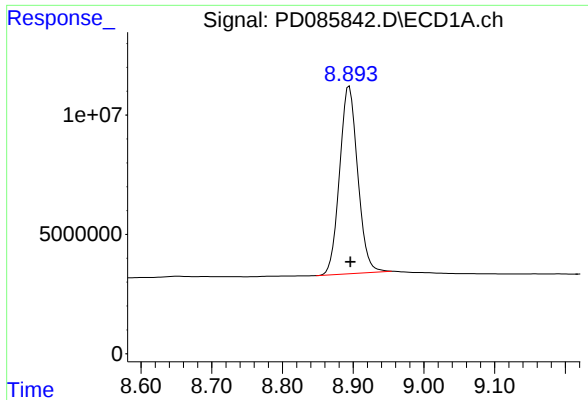

#27 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 139914026
Conc: 76.03 ng/ml

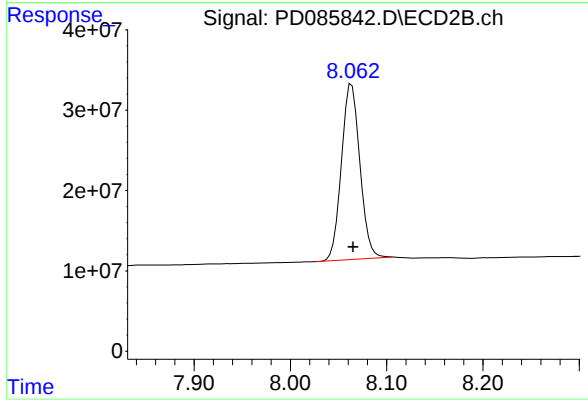

#27 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: -0.001 min
Response: 290948819
Conc: 77.41 ng/ml