

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 01:25
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:40:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 01:10:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	2.878	87968205	315.6E6	76.607	73.746
27)	SA Decachlor...	8.895	8.065	266.8E6	553.7E6	146.685	149.882
Target Compounds							
2)	A alpha-BHC	3.890	3.388	184.7E6	500.9E6	90.738	79.554
3)	MA gamma-BHC...	4.217	3.722	175.7E6	471.0E6	80.833	78.092
4)	MA Heptachlor	4.809	4.074	172.6E6	444.3E6	84.995	77.257
9)	A Endosulfan I	5.947	5.237	145.0E6	375.9E6	79.980	75.455
13)	MA Dieldrin	6.219	5.503	340.0E6	853.9E6	171.833	153.302
14)	MA Endrin	6.444	5.781	272.1E6	736.6E6	177.331	153.494
16)	A 4,4'-DDD	6.580	5.920	215.5E6	604.9E6	175.605	153.964
17)	MA 4,4'-DDT	6.893	6.175	240.3E6	666.7E6	178.299	157.201
20)	A Methoxychlor	7.366	6.746	652.6E6	1433.0E6	799.175	681.853


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 01:25
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:40:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 01:10:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

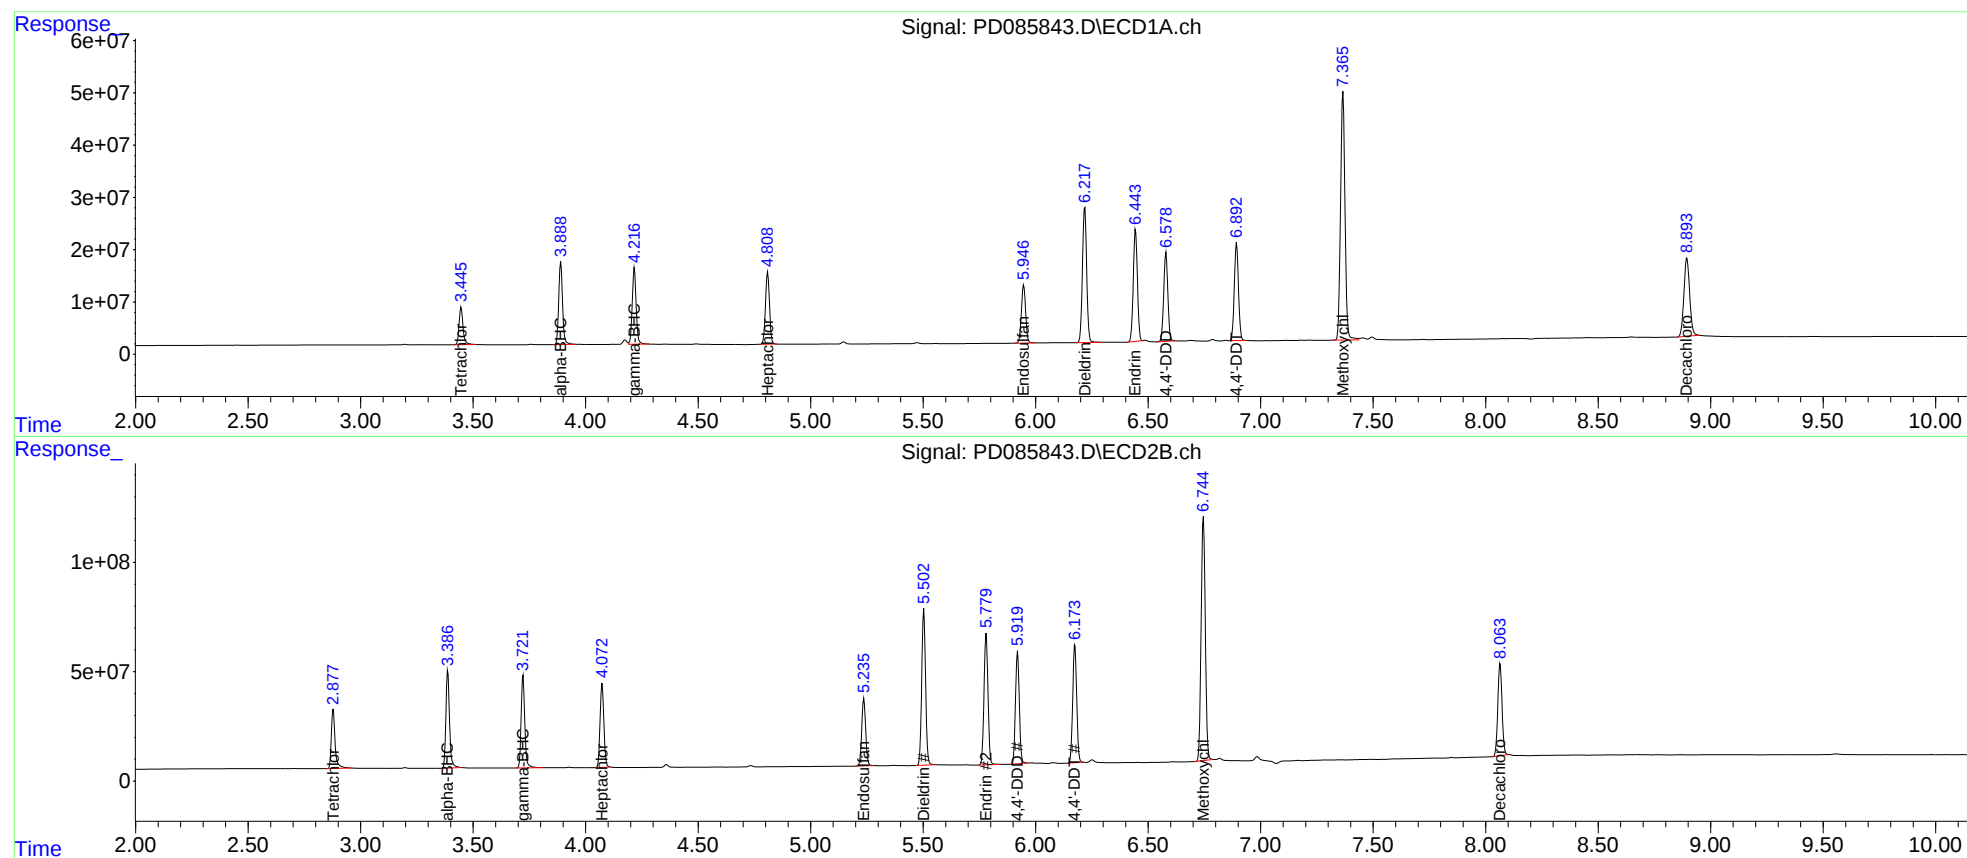

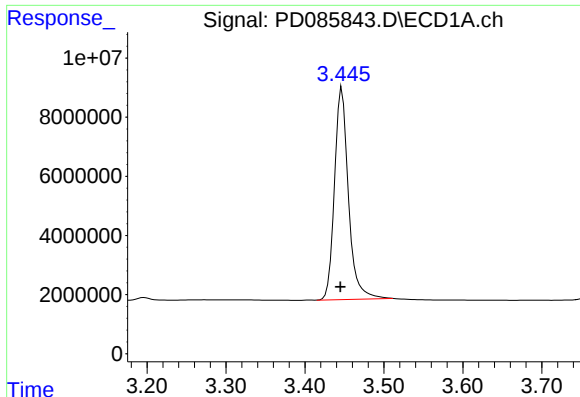


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.002 min
Response: 87968205
Conc: 76.61 ng/ml

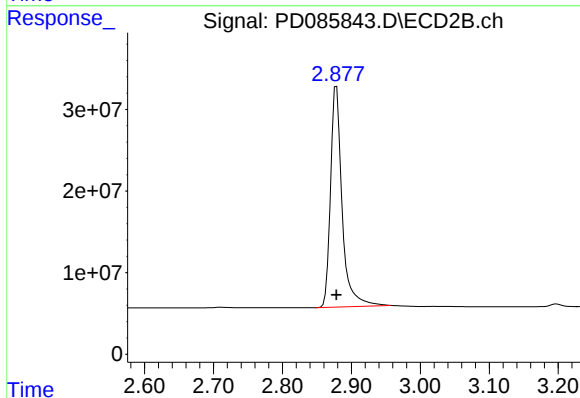


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 315647330
Conc: 73.75 ng/ml

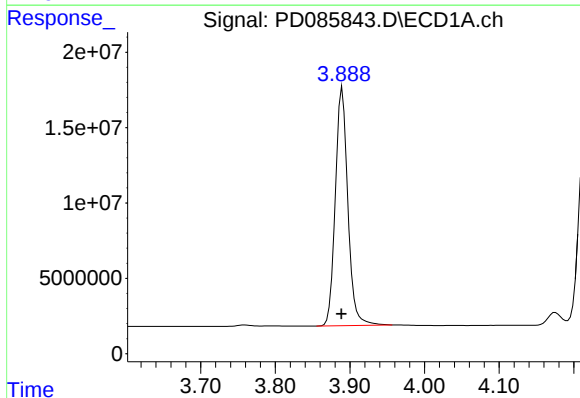


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.001 min
Response: 184676139
Conc: 90.74 ng/ml

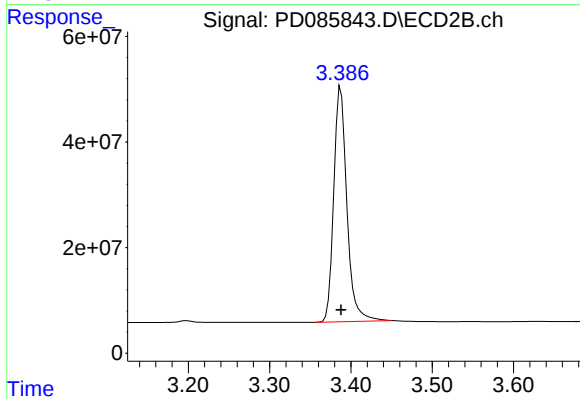

#2 alpha-BHC

R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 500931400
Conc: 79.55 ng/ml

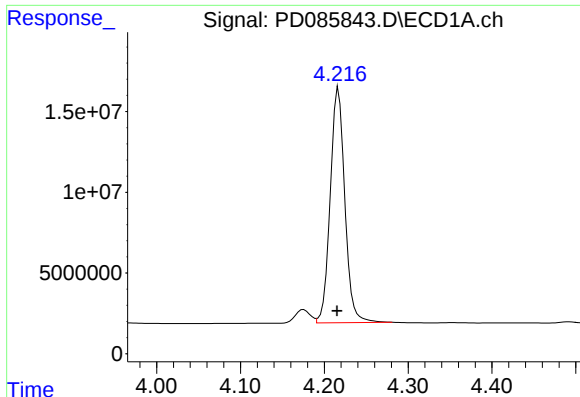


#3 gamma-BHC (Lindane)

R.T.: 4.217 min

Delta R.T.: 0.002 min

Response: 175725761

Conc: 80.83 ng/ml

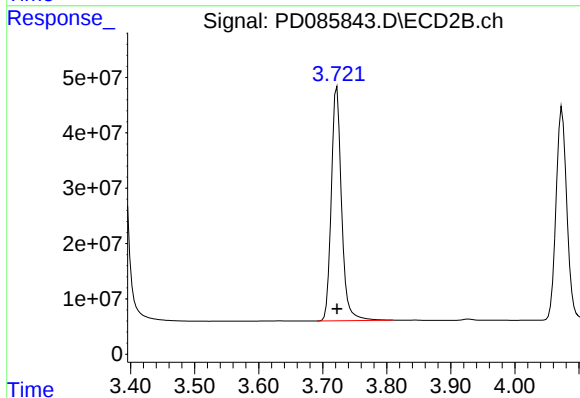


#3 gamma-BHC (Lindane)

R.T.: 3.722 min

Delta R.T.: 0.000 min

Response: 471042423

Conc: 78.09 ng/ml

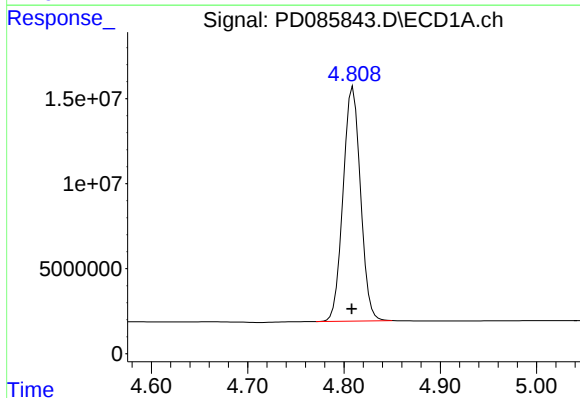


#4 Heptachlor

R.T.: 4.809 min

Delta R.T.: 0.001 min

Response: 172593722

Conc: 84.99 ng/ml

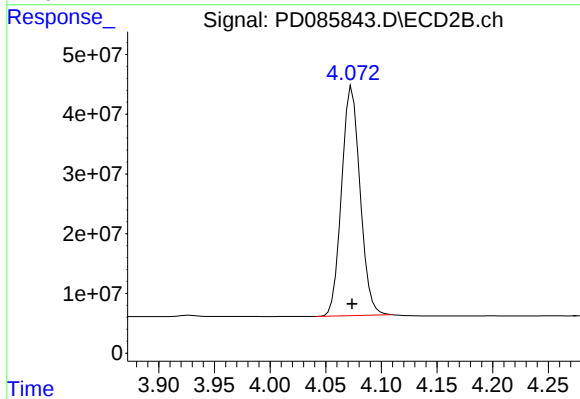


#4 Heptachlor

R.T.: 4.074 min

Delta R.T.: 0.000 min


Response: 444307697

Conc: 77.26 ng/ml

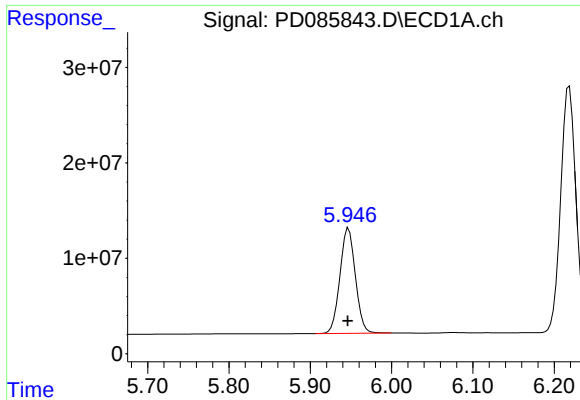


#9 Endosulfan I

R.T.: 5.947 min
Delta R.T.: 0.001 min
Response: 145019869
Conc: 79.98 ng/ml

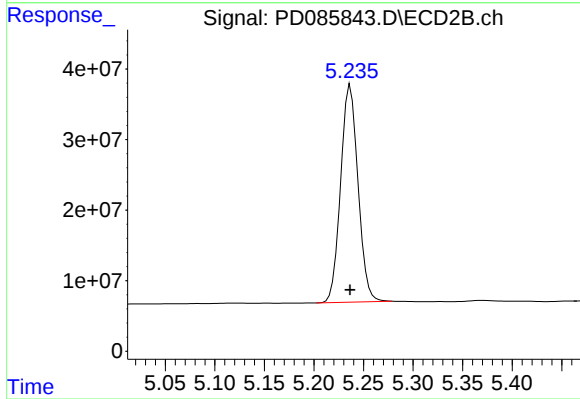


#9 Endosulfan I

R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 375856929
Conc: 75.46 ng/ml

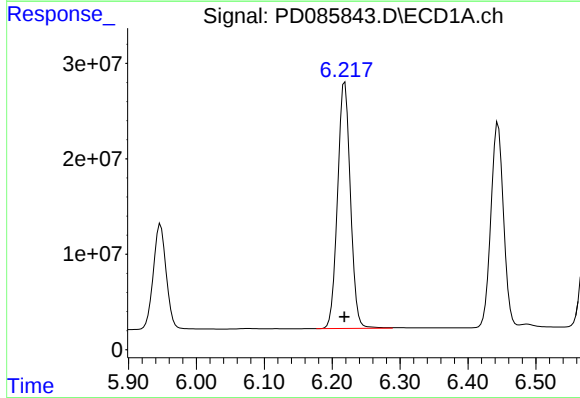


#13 Dieldrin

R.T.: 6.219 min
Delta R.T.: 0.000 min
Response: 339982012
Conc: 171.83 ng/ml

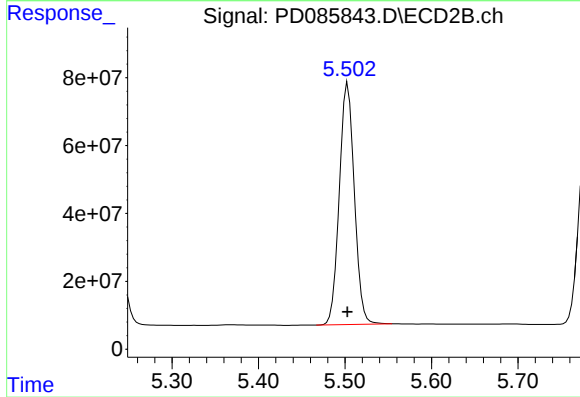


#13 Dieldrin

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 853938723
Conc: 153.30 ng/ml

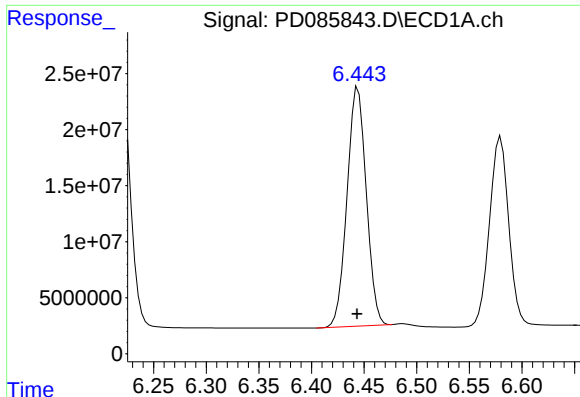


#14 Endrin

R.T.: 6.444 min
Delta R.T.: 0.000 min
Response: 272129475
Conc: 177.33 ng/ml

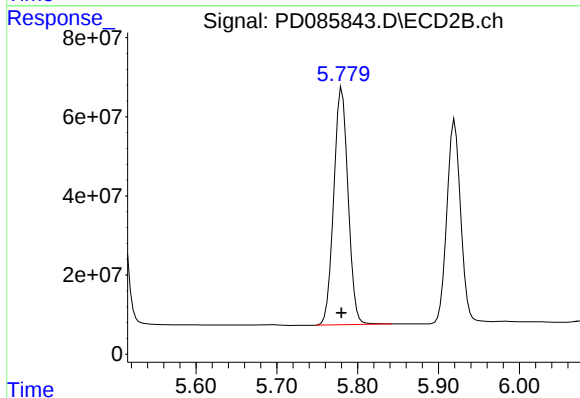


#14 Endrin

R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 736615701
Conc: 153.49 ng/ml

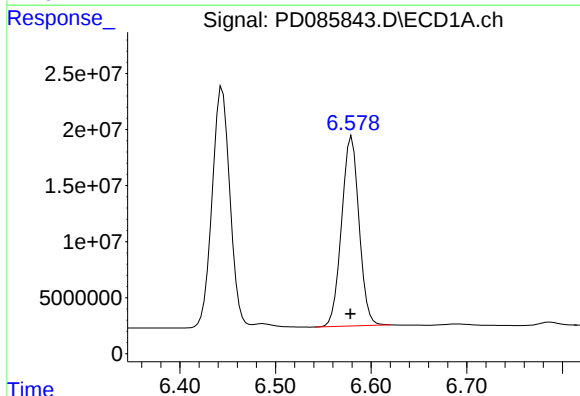


#16 4,4'-DDD

R.T.: 6.580 min
Delta R.T.: 0.001 min
Response: 215469950
Conc: 175.61 ng/ml

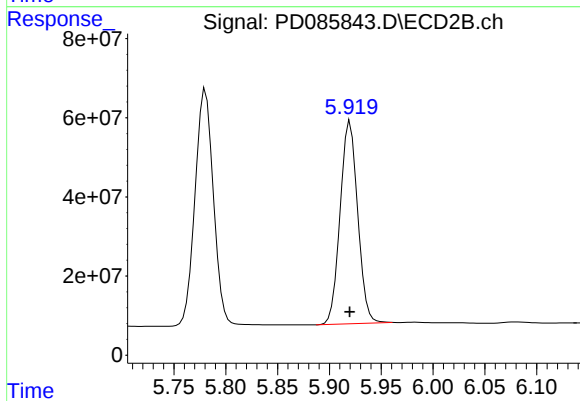


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 604928128
Conc: 153.96 ng/ml

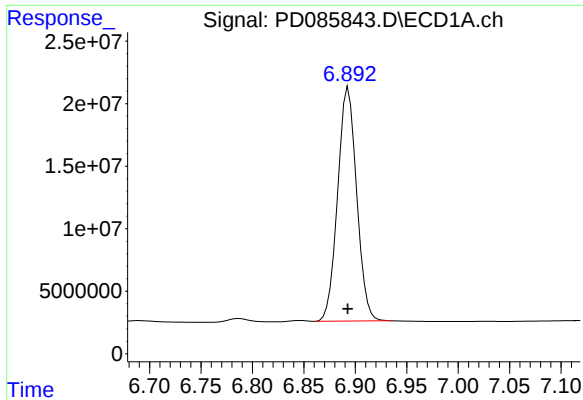


#17 4,4'-DDT

R.T.: 6.893 min
Delta R.T.: 0.000 min
Response: 240301618
Conc: 178.30 ng/ml

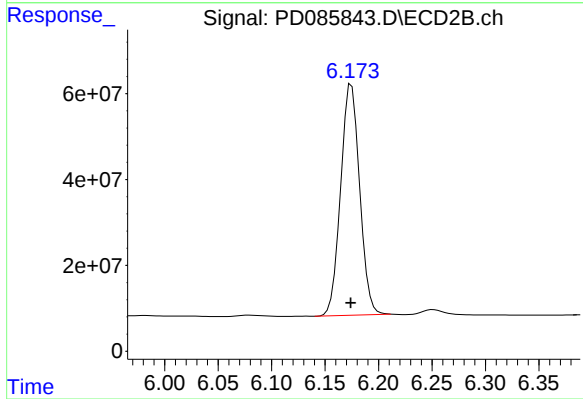


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 666652269
Conc: 157.20 ng/ml

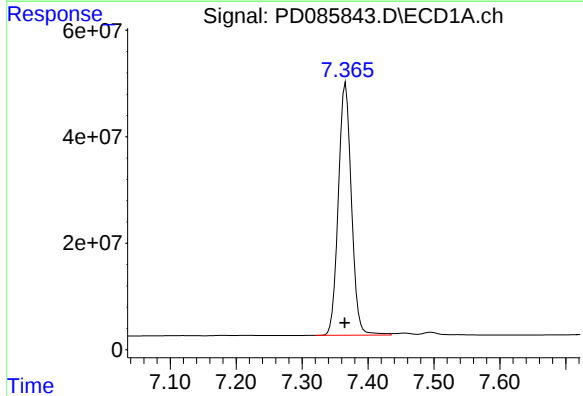


#20 Methoxychlor

R.T.: 7.366 min
Delta R.T.: 0.002 min
Response: 652610950
Conc: 799.17 ng/ml

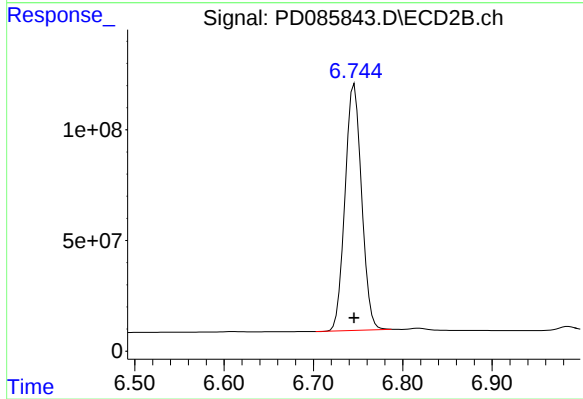


#20 Methoxychlor

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 1433047828
Conc: 681.85 ng/ml

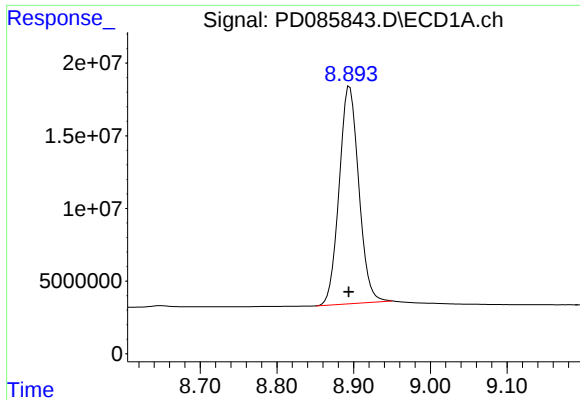

#27 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.001 min
Response: 266829565
Conc: 146.68 ng/ml

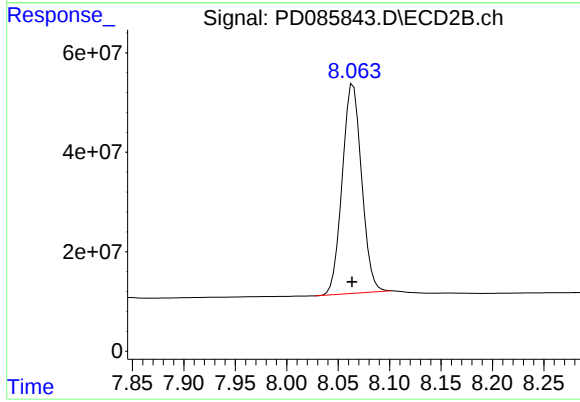

#27 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.001 min
Response: 553667854
Conc: 149.88 ng/ml