

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
 Data File : PD085828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2024 21:32
 Operator : AR\AJ
 Sample : RESC047
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 20:27:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	2.878	24662247	91133666	21.557	21.491
27)	SA Decachlor...	8.896	8.063	78368296	160.6E6	43.092	43.683
Target Compounds							
2)	A alpha-BHC	3.889	3.388	19297563	61394488	9.269	9.730
3)	MA gamma-BHC...	4.216	3.722	22600034	58452214	10.350	9.684
4)	MA Heptachlor	4.809	4.073	19581565	56991985	9.518	9.913
5)	MB Aldrin	5.147	4.359	24767465	71275971	11.800	12.130
6)	B beta-BHC	4.402	4.016	11048780	32849059	12.381	12.551
7)	B delta-BHC	4.646	4.252	22788074	75065028	11.860	12.649
8)	B Heptachlo...	5.566	4.862	22110148	64508349	11.581	11.882
9)	A Endosulfan I	5.946	5.236	17620114	49152368	9.688	9.907
10)	B trans-Chl...	5.820	5.115	21465418	63346610	11.533	11.829
11)	B cis-Chlor...	5.901	5.179	22317984	64573574	11.567	11.760
12)	B 4,4'-DDE	6.072	5.364	37188946	113.7E6	22.624	23.530
13)	MA Dieldrin	6.219	5.503	37482170	108.7E6	18.707	19.606
14)	MA Endrin	6.444	5.780	30033080	96365540	18.905	20.128
15)	B Endosulfa...	6.656	6.072	40259913	109.3E6	23.670	24.048
16)	A 4,4'-DDD	6.579	5.919	23740268	77293710	19.036	19.758
17)	MA 4,4'-DDT	6.893	6.174	25268083	82633197	18.176	19.518
18)	B Endrin al...	6.785	6.251	32301633	90965062	24.546	25.231
19)	B Endosulfa...	7.019	6.475	38328834	104.8E6	24.341	24.541
20)	A Methoxychlor	7.366	6.746	79166437	213.2E6	96.785	103.335
21)	B Endrin ke...	7.495	6.985	41427589	130.8E6	23.960	24.966

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 21:32
Operator : AR\AJ
Sample : RESC047
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:27:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

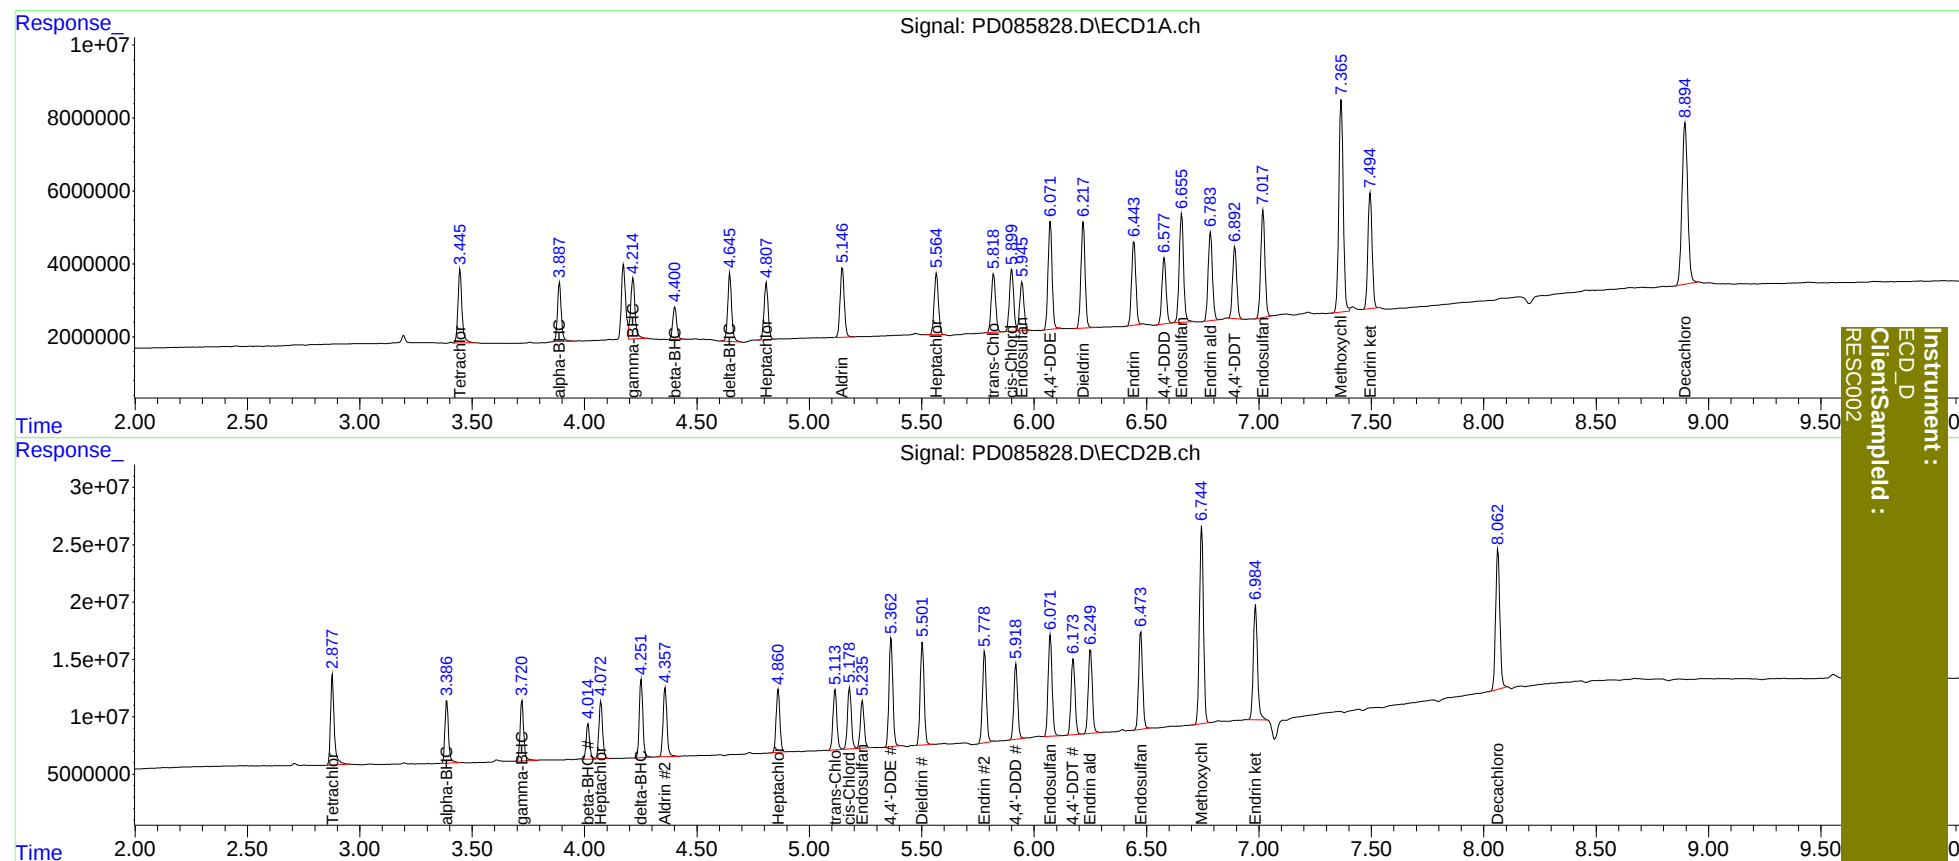

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085828.D
Acq On : 30 Sep 2024 21:32
Operator : AR\AJ
Sample : RESC047
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Title : GC Extractables
Last Update : Tue Oct 01 08:04:20 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.446	3.889	100.00%
3.889	4.216	100.00%
4.216	4.402	100.00%
4.402	4.646	100.00%
4.646	4.809	100.00%
4.809	5.147	100.00%
5.147	5.566	100.00%
5.566	5.820	100.00%
5.820	5.901	100.00%
5.901	5.946	93.44%
5.946	6.072	100.00%
6.072	6.219	100.00%
6.219	6.444	100.00%
6.444	6.579	100.00%
6.579	6.656	100.00%
6.656	6.785	100.00%
6.785	6.893	100.00%
6.893	7.019	100.00%
7.019	7.366	100.00%
7.366	7.495	100.00%
7.495	8.896	100.00%

Signal #2


2.878	3.388	100.00%
3.388	3.722	100.00%
3.722	4.016	100.00%
4.016	4.073	99.50%
4.073	4.252	100.00%
4.252	4.359	100.00%
4.359	4.862	100.00%
4.862	5.115	100.00%
5.115	5.179	98.97%
5.179	5.236	100.00%
5.236	5.364	100.00%
5.364	5.503	100.00%
5.503	5.780	100.00%
5.780	5.919	100.00%
5.919	6.072	100.00%
6.072	6.174	100.00%
6.174	6.251	100.00%
6.251	6.475	100.00%
6.475	6.746	100.00%
6.746	6.985	100.00%
6.985	8.063	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 21:32
Operator : AR\AJ
Sample : RESC047
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:27:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

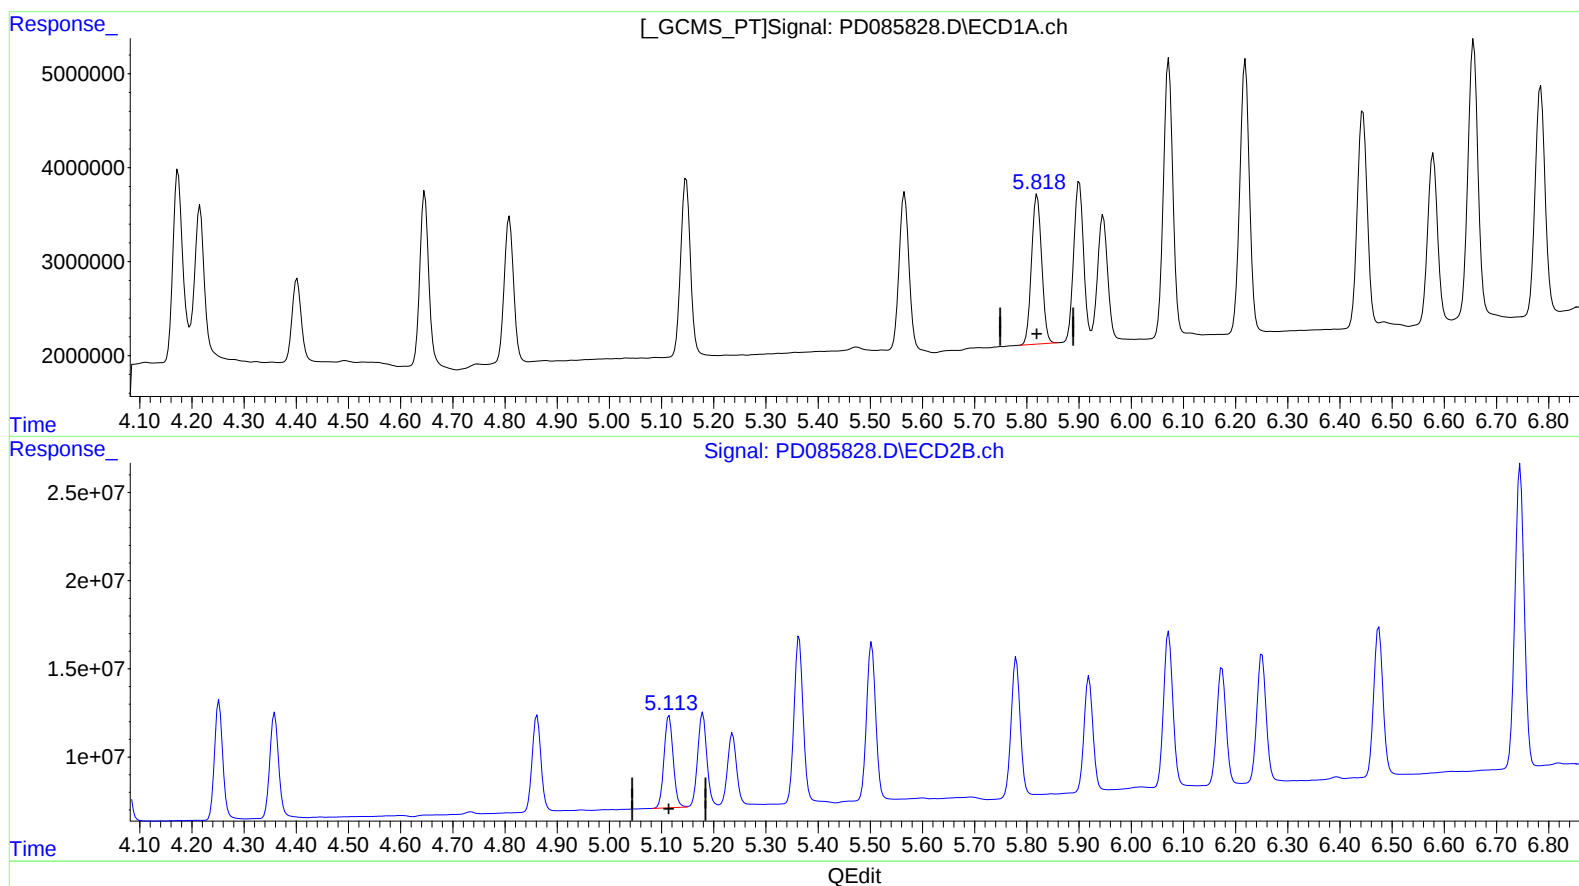

(10) trans-Chlordane (B)

5.820min 11.533 ng/ml

response 21465418

(10) trans-Chlordane #2 (B)

5.115min 11.829 ng/ml


response 63346610

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 21:32
Operator : AR\AJ
Sample : RESC047
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:27:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

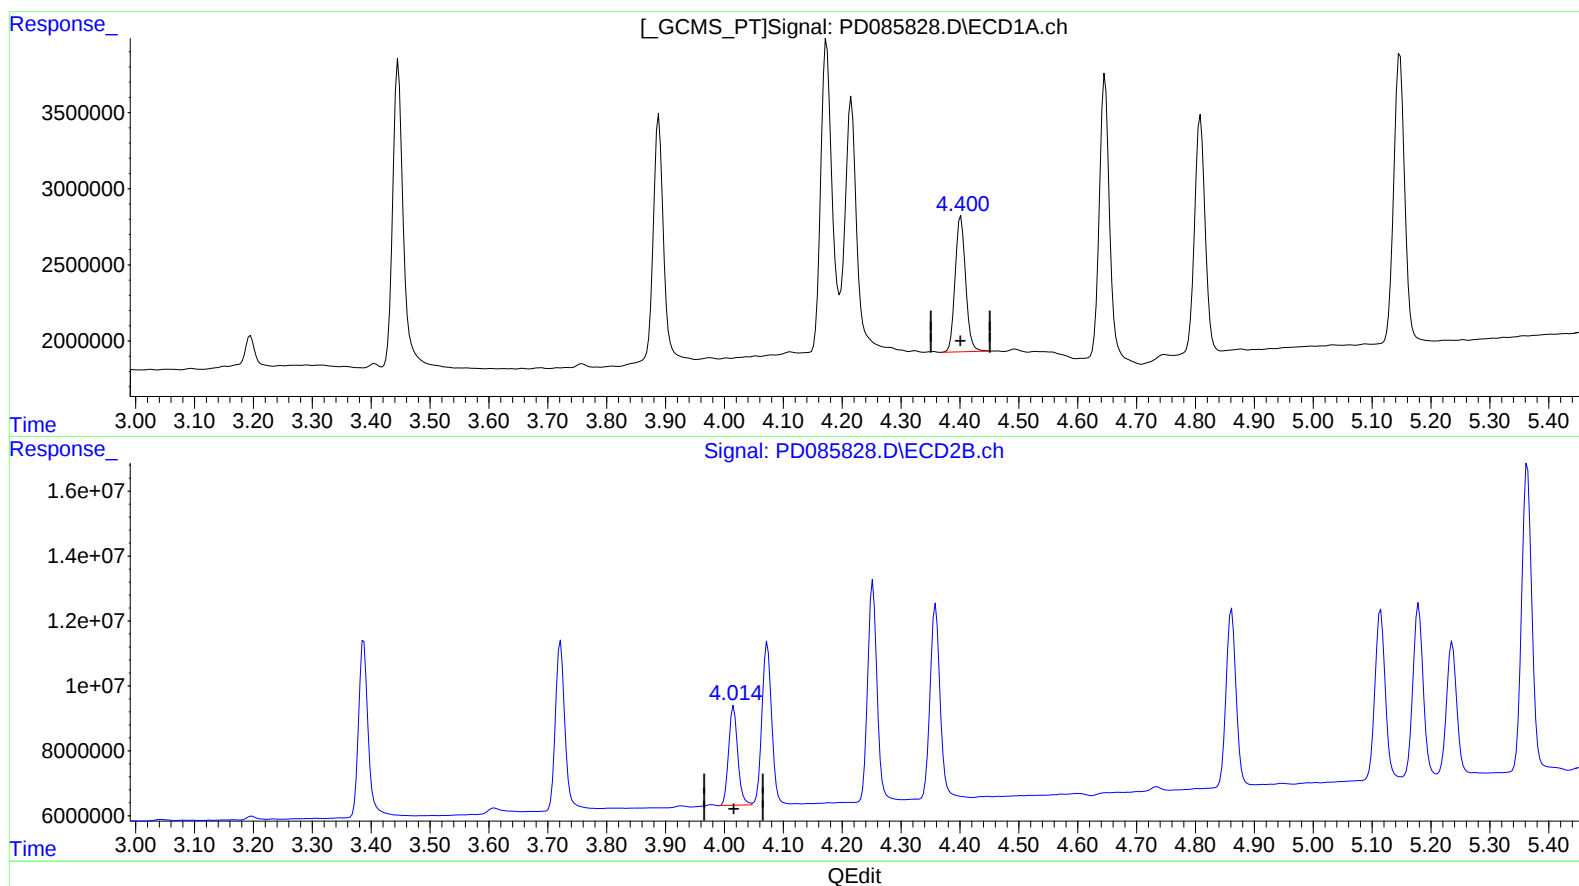

(6) beta-BHC (B)
4.402min 12.381 ng/ml
response 11048780


(6) beta-BHC #2 (B)
4.016min 12.551 ng/ml
response 32849059

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100124\
Data File : PD085828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2024 21:32
Operator : AR\AJ
Sample : RESC047
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:27:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

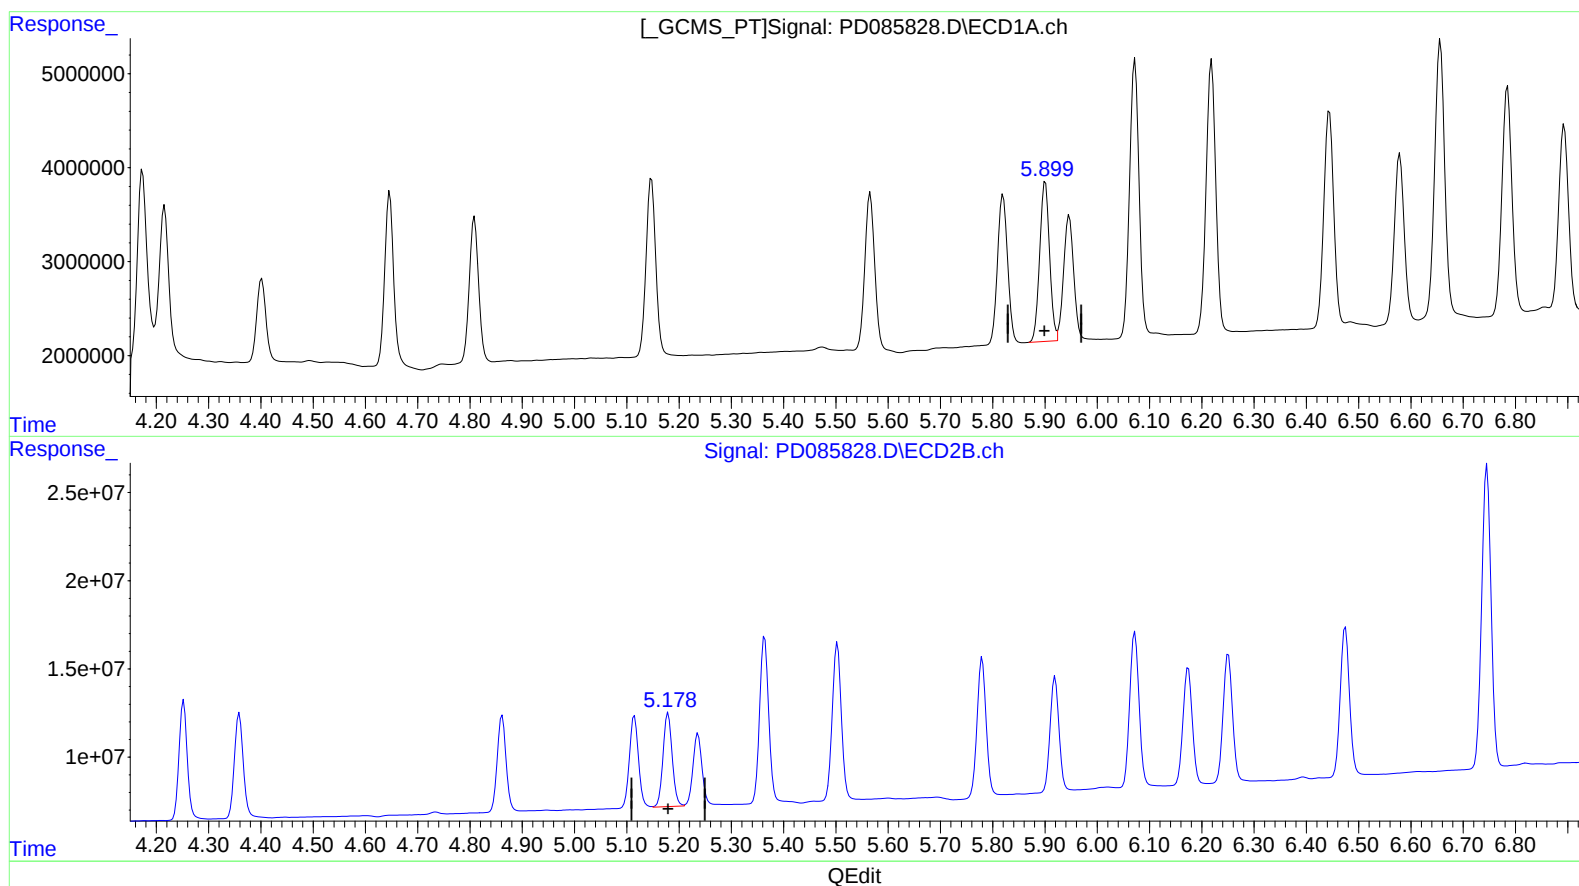

(11) cis-Chlordane (B)

5.901min 11.567 ng/ml

response 22317984

(11) cis-Chlordane #2 (B)

5.179min 11.760 ng/ml

response 64573574