

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
 Data File : PD059461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 17:55
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:08:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:07:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.512	4.026	15472974	21027738	10.678	10.586
27)	SA Decachlor...	8.319	9.113	23172467	31402701	22.107	21.181
Target Compounds							
2)	A alpha-BHC	3.954	4.417	22026900	30054413	10.355	10.332
3)	MA gamma-BHC...	4.241	4.703	20613333	27377716	10.563	10.237
4)	MA Heptachlor	4.550	5.215	20329550	29638579	10.411	11.606
9)	A Endosulfan I	5.593	6.266	15872991	21171773	10.588	10.446
13)	MA Dieldrin	5.839	6.523	35223240	45934574	21.789	20.654
14)	MA Endrin	6.097	6.742	23298338	29292925	19.683	18.745
16)	A 4,4'-DDD	6.223	6.860	27737900	35724381	21.472	20.798
17)	MA 4,4'-DDT	6.467	7.160	27602158	31792920	20.729	20.010
20)	A Methoxychlor	7.016	7.617	63866935	84386370	102.962	101.471


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
Data File : PD059461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 17:55
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:08:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:07:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

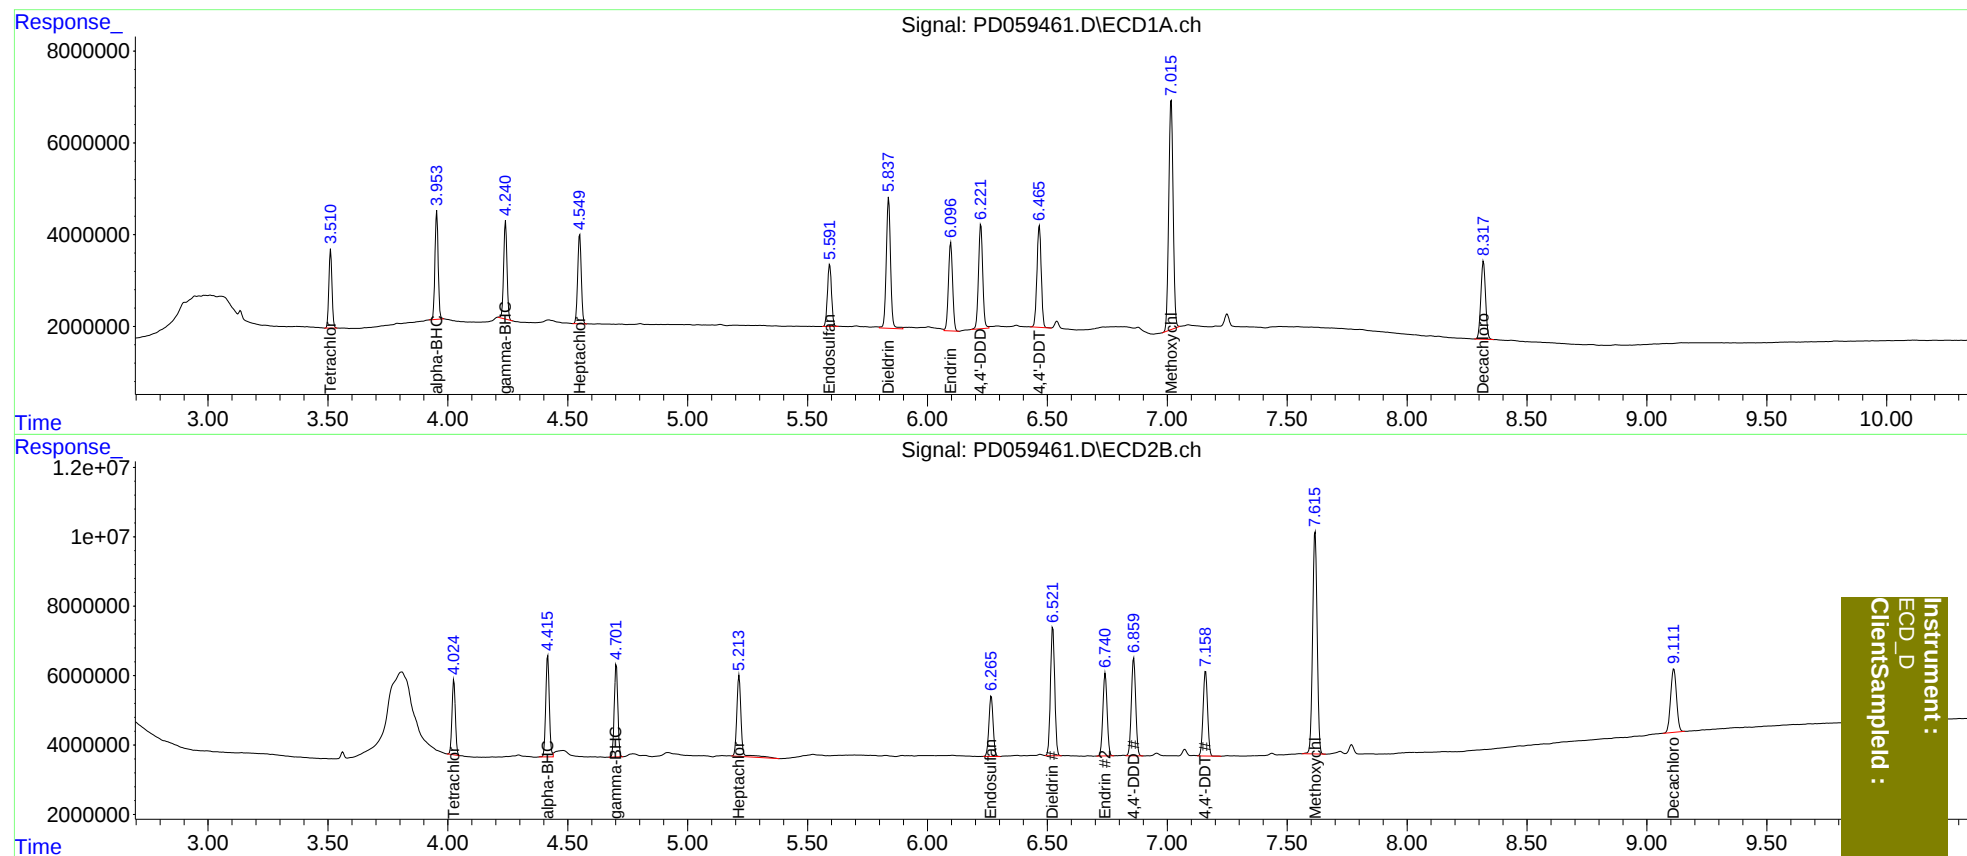


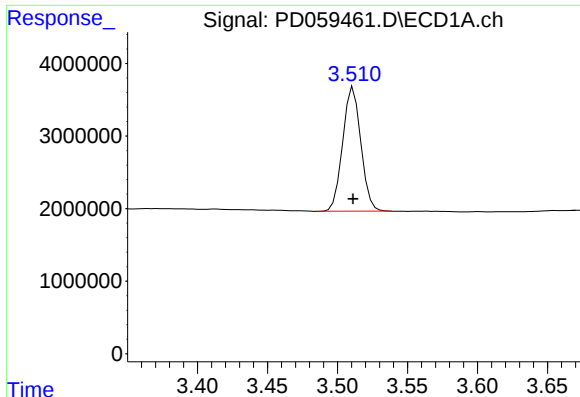

#1 Tetrachloro-m-xylene


R.T.: 3.512 min
Delta R.T.: 0.000 min
Response: 15472974
Conc: 10.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

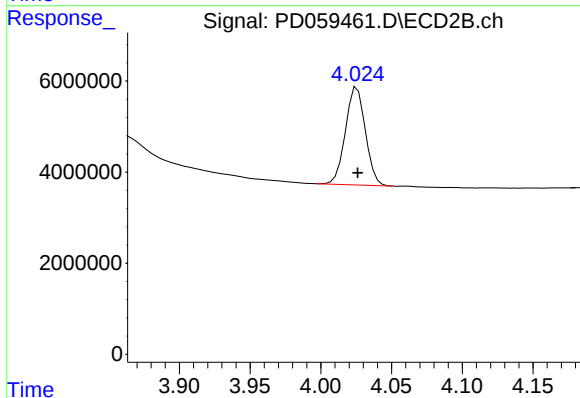


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 21027738
Conc: 10.59 ng/ml

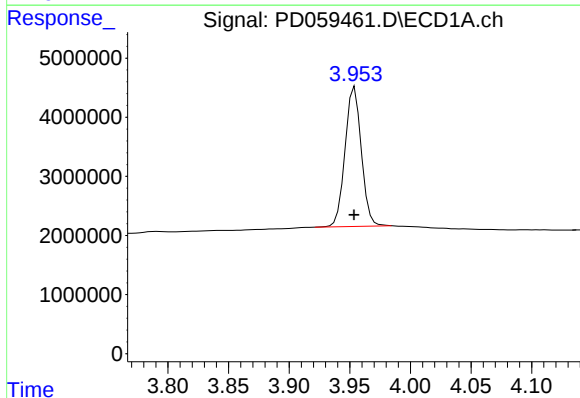


#2 alpha-BHC

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 22026900
Conc: 10.35 ng/ml

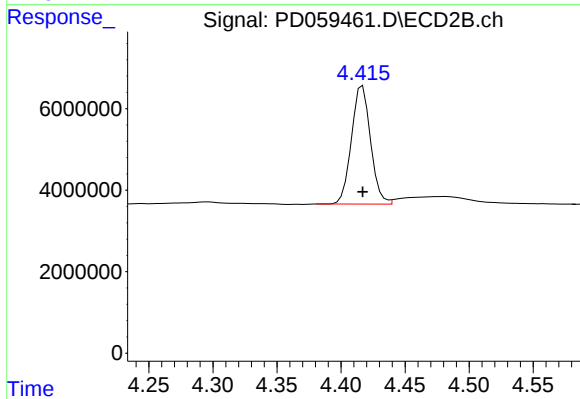

#2 alpha-BHC


R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 30054413
Conc: 10.33 ng/ml

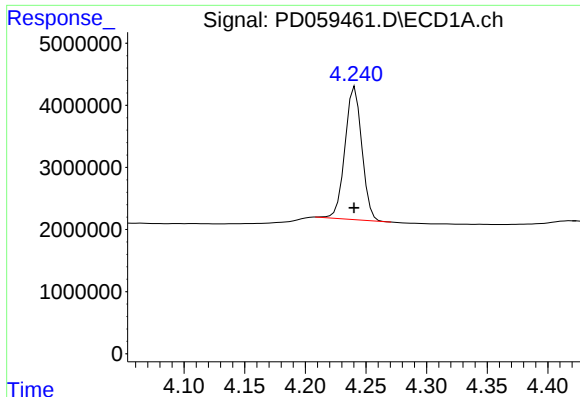

#3 gamma-BHC (Lindane)


R.T.: 4.241 min
Delta R.T.: 0.000 min
Response: 20613333
Conc: 10.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

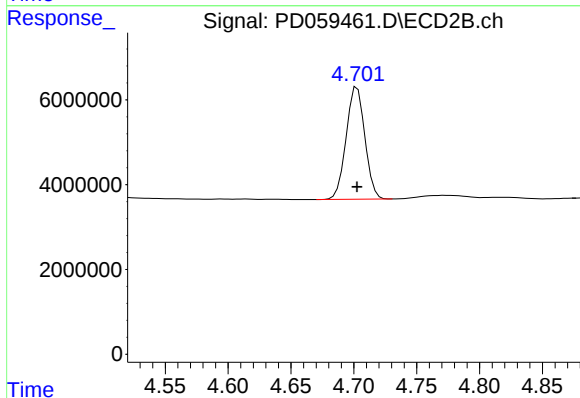


#3 gamma-BHC (Lindane)

R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 27377716
Conc: 10.24 ng/ml

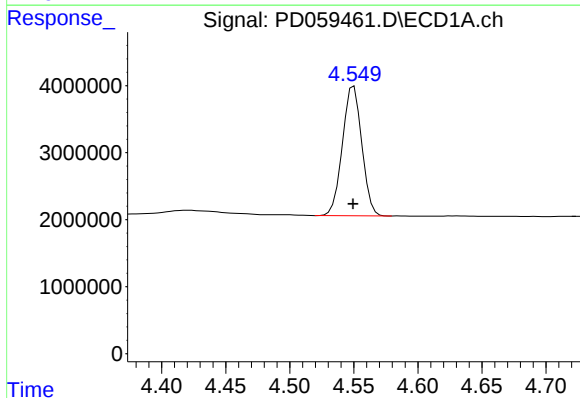


#4 Heptachlor

R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 20329550
Conc: 10.41 ng/ml

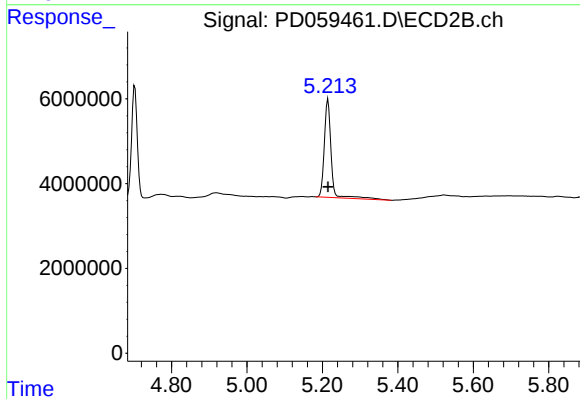

#4 Heptachlor


R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 29638579
Conc: 11.61 ng/ml

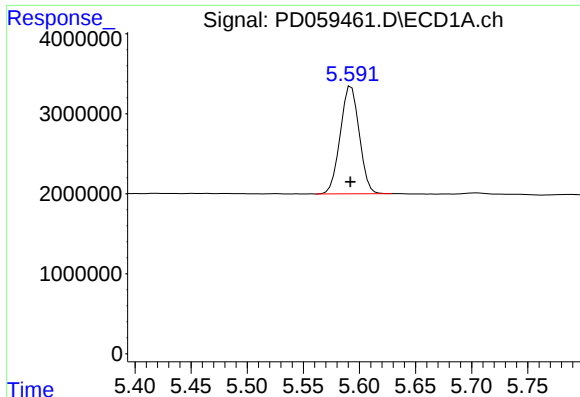

#9 Endosulfan I


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 15872991
Conc: 10.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

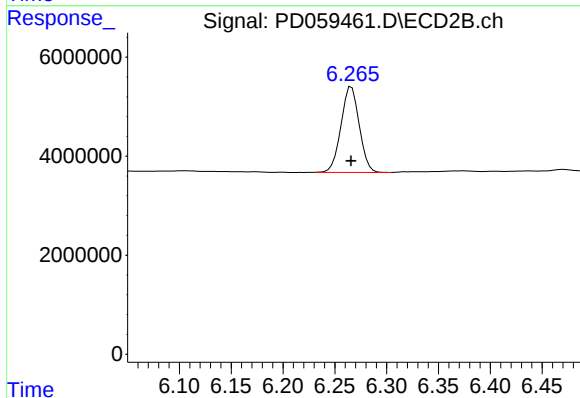


#9 Endosulfan I

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 21171773
Conc: 10.45 ng/ml

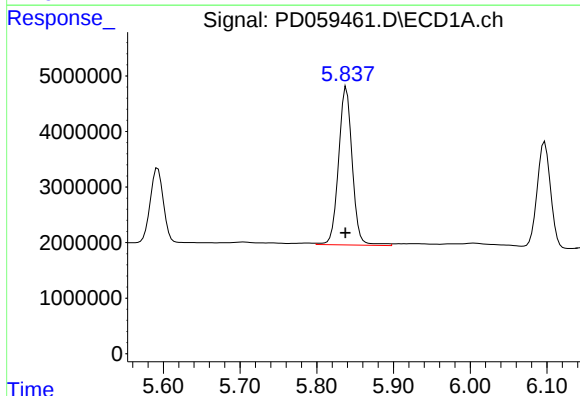


#13 Dieldrin

R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 35223240
Conc: 21.79 ng/ml

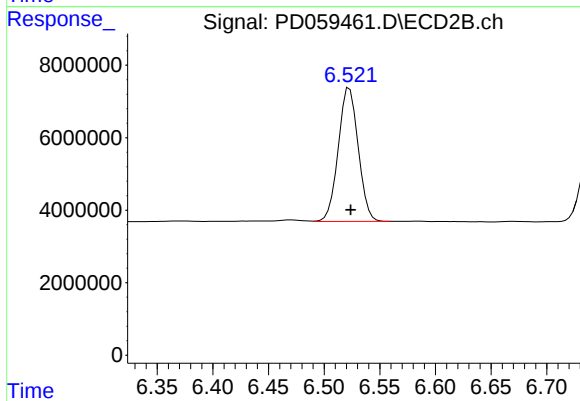

#13 Dieldrin


R.T.: 6.523 min
Delta R.T.: -0.001 min
Response: 45934574
Conc: 20.65 ng/ml

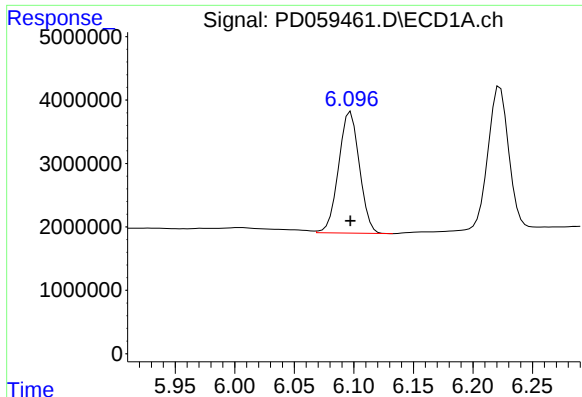

#14 Endrin


R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 23298338
Conc: 19.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

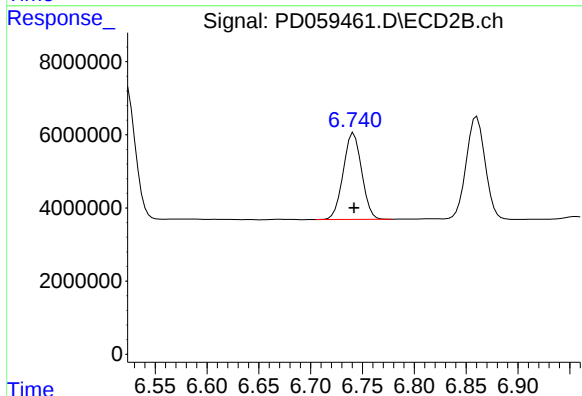


#14 Endrin

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 29292925
Conc: 18.75 ng/ml

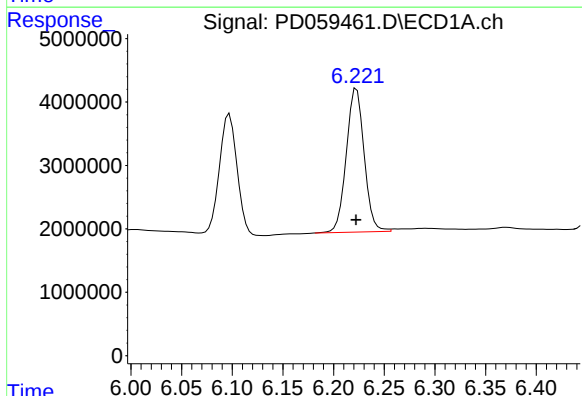


#16 4,4'-DDD

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 27737900
Conc: 21.47 ng/ml

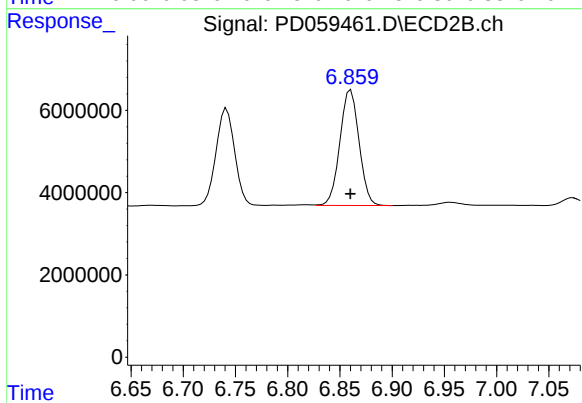

#16 4,4'-DDD


R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 35724381
Conc: 20.80 ng/ml

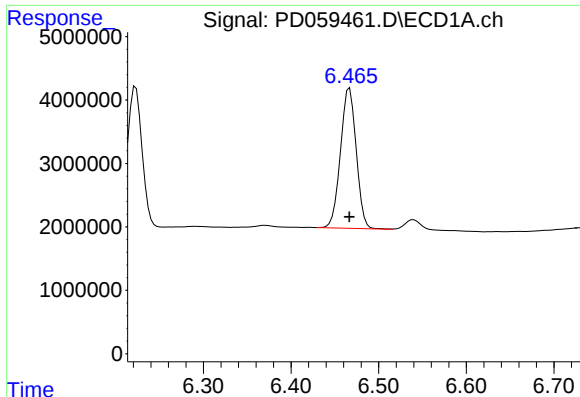

#17 4,4'-DDT


R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 27602158
Conc: 20.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

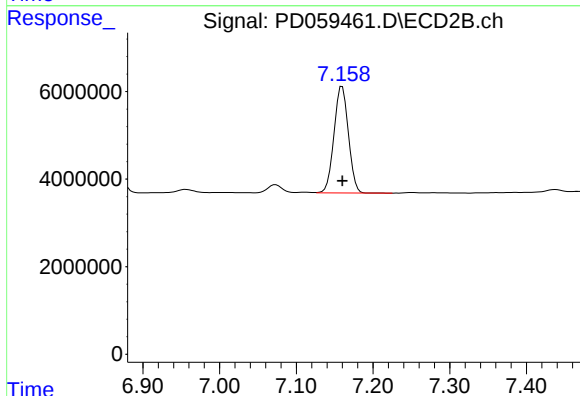


#17 4,4'-DDT

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 31792920
Conc: 20.01 ng/ml

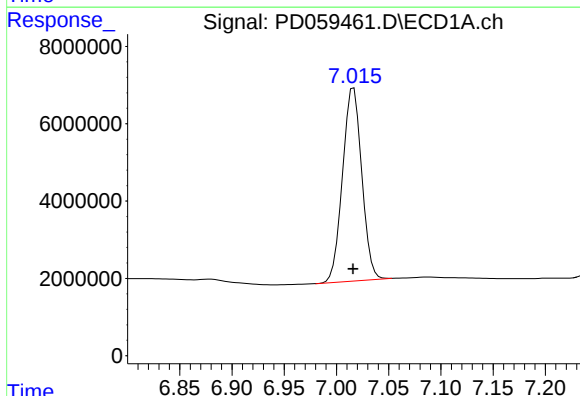


#20 Methoxychlor

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 63866935
Conc: 102.96 ng/ml

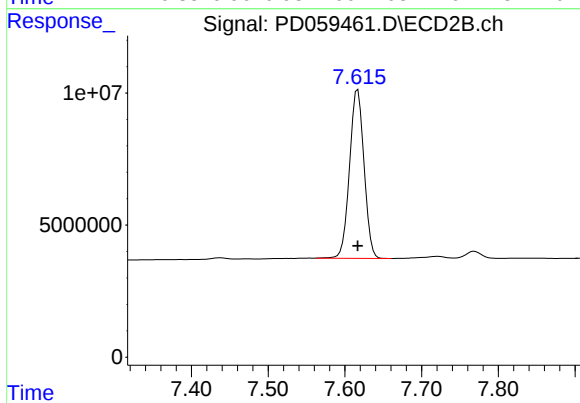

#20 Methoxychlor


R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 84386370
Conc: 101.47 ng/ml

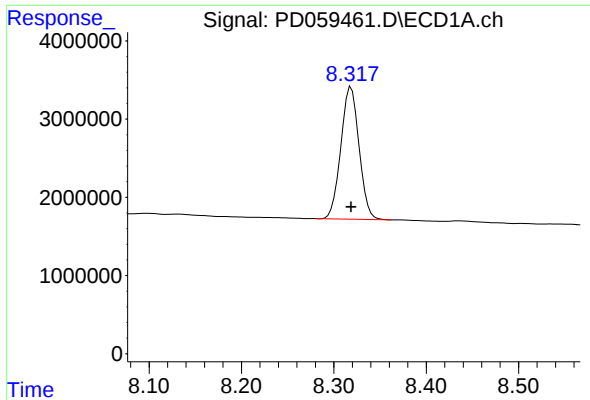

#27 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 23172467
Conc: 22.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

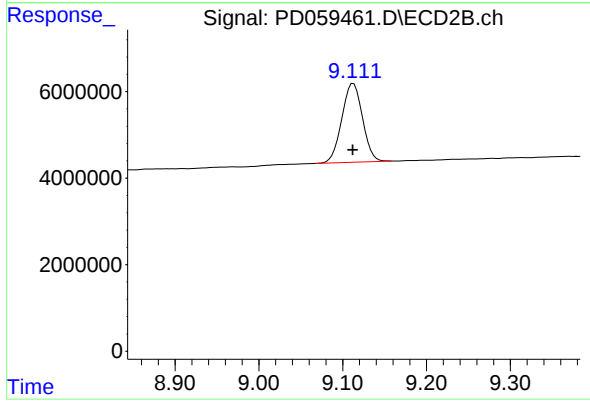

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 31402701
Conc: 21.18 ng/ml