

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
 Data File : PD059463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 18:23
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:08:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:07:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.026	28980480	39727439	20.000	20.000
27)	SA Decachlor...	8.319	9.112	41927544	59303190	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.954	4.417	42544386	58179877	20.000	20.000
3)	MA gamma-BHC...	4.240	4.703	39030931	53485601	20.000	20.000
4)	MA Heptachlor	4.549	5.215	39055333	51072526	20.000	20.000
9)	A Endosulfan I	5.592	6.266	29983414	40534040	20.000	20.000
13)	MA Dieldrin	5.838	6.524	64662955	88958959	40.000	40.000
14)	MA Endrin	6.097	6.742	47348282	62507520	40.000	40.000
16)	A 4,4'-DDD	6.222	6.860	51673298	68706111	40.000	40.000
17)	MA 4,4'-DDT	6.466	7.160	53264010	63554144	40.000	40.000
20)	A Methoxychlor	7.016	7.617	124.1E6	166.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
Data File : PD059463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 18:23
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:08:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:07:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

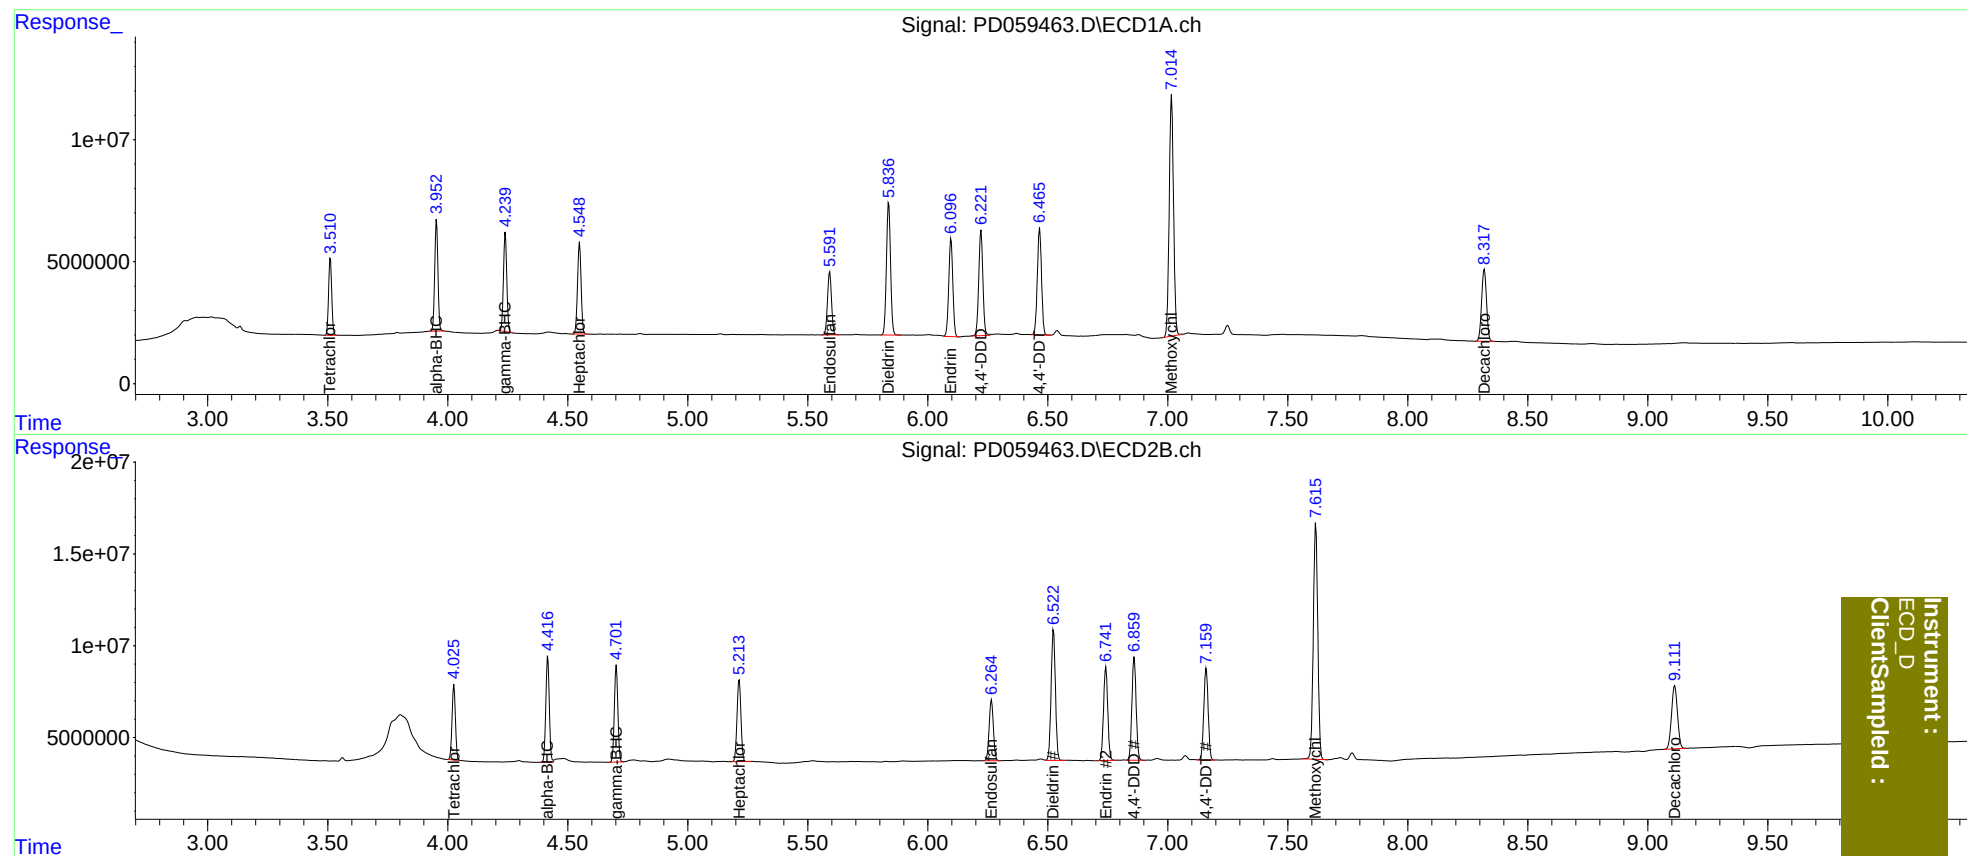


Instrument :
ECD_D
ClientSampled :

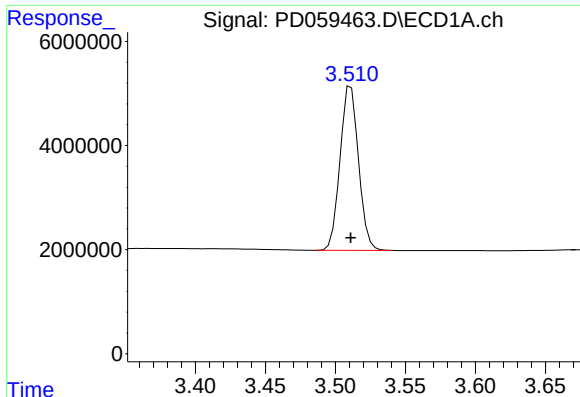

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 28980480
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

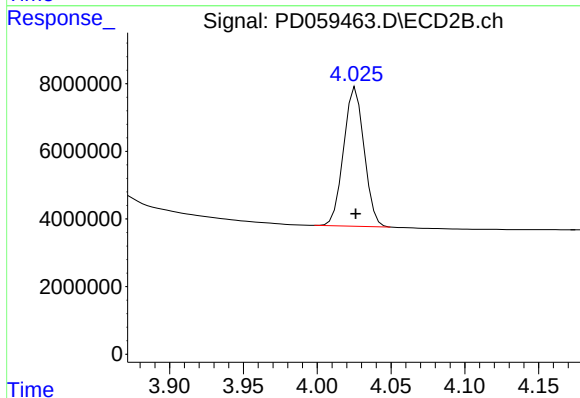


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 39727439
Conc: 20.00 ng/ml

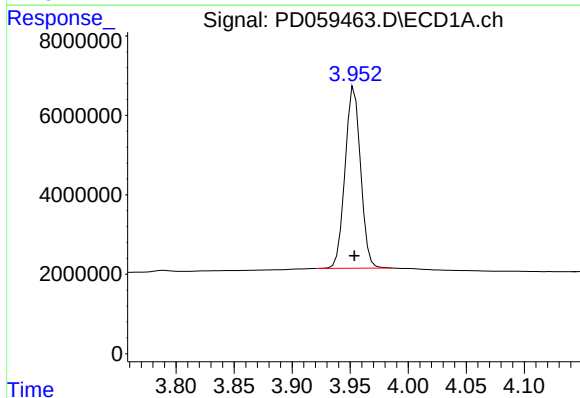


#2 alpha-BHC

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 42544386
Conc: 20.00 ng/ml

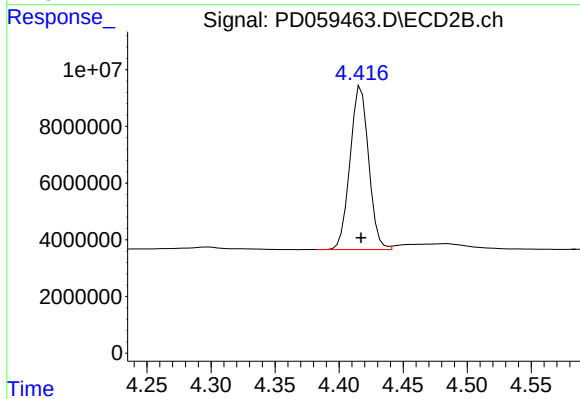

#2 alpha-BHC


R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 58179877
Conc: 20.00 ng/ml

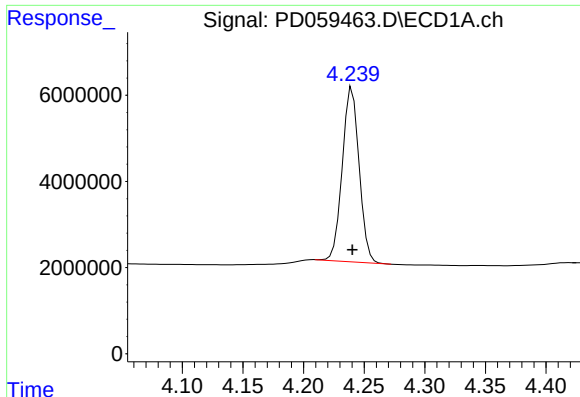

#3 gamma-BHC (Lindane)


R.T.: 4.240 min
Delta R.T.: 0.000 min
Response: 39030931
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

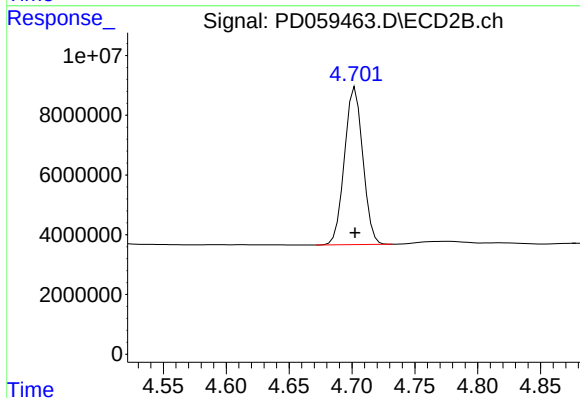


#3 gamma-BHC (Lindane)

R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 53485601
Conc: 20.00 ng/ml

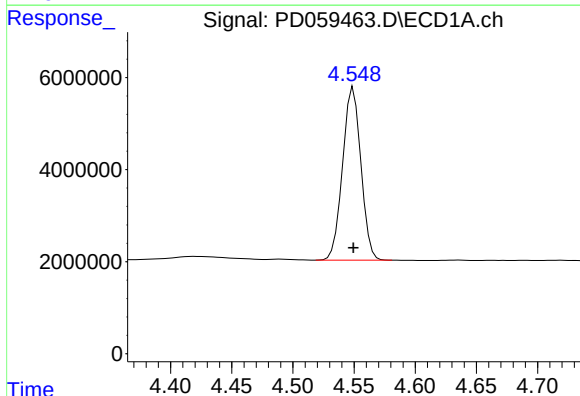


#4 Heptachlor

R.T.: 4.549 min
Delta R.T.: 0.000 min
Response: 39055333
Conc: 20.00 ng/ml

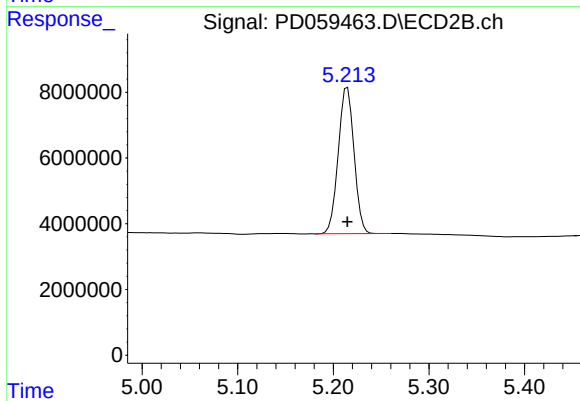

#4 Heptachlor


R.T.: 5.215 min
Delta R.T.: 0.000 min
Response: 51072526
Conc: 20.00 ng/ml

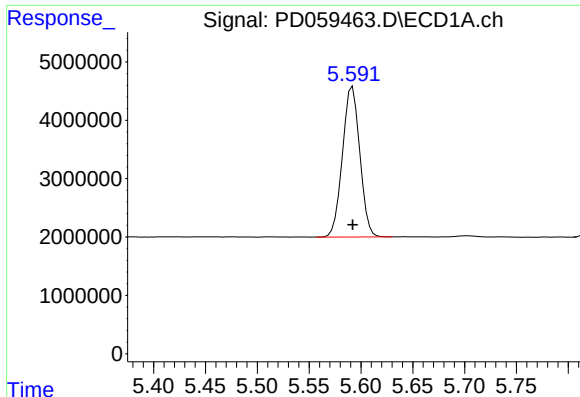

#9 Endosulfan I


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 29983414
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

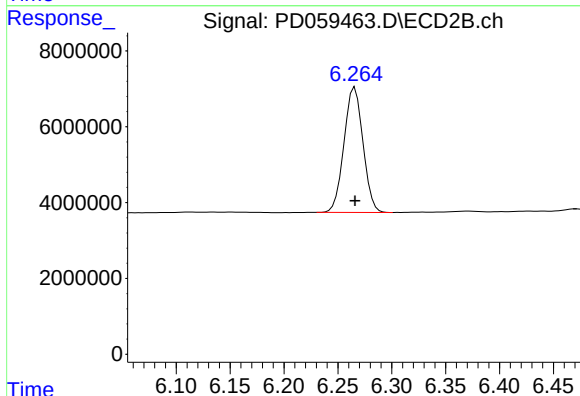


#9 Endosulfan I

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 40534040
Conc: 20.00 ng/ml

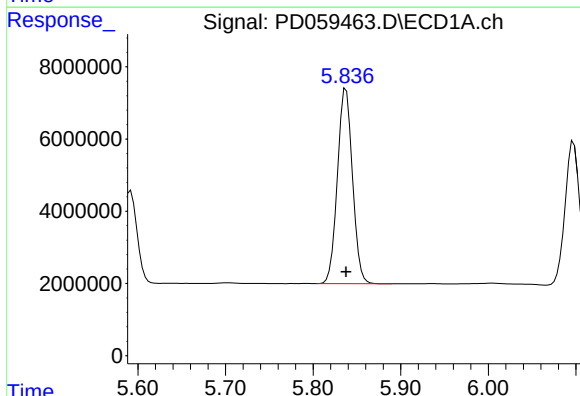


#13 Dieldrin

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 64662955
Conc: 40.00 ng/ml

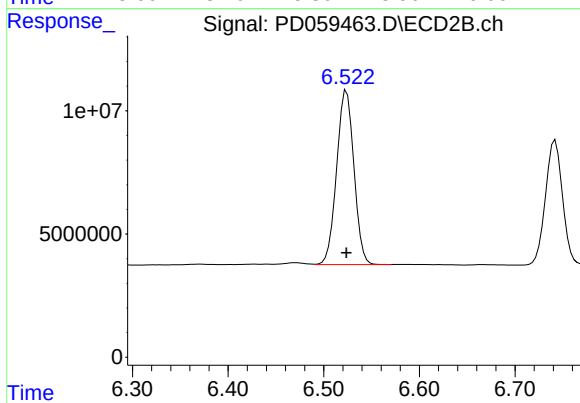

#13 Dieldrin


R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 88958959
Conc: 40.00 ng/ml

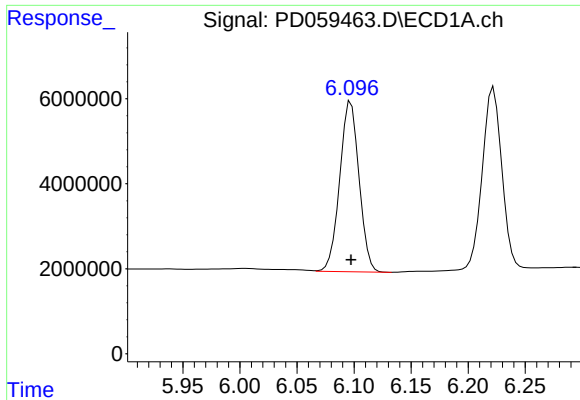

#14 Endrin


R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 47348282
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

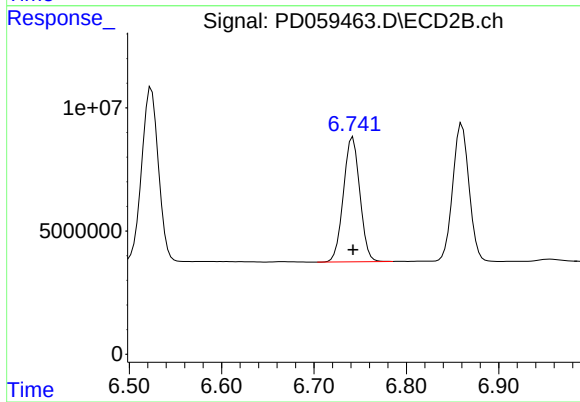


#14 Endrin

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 62507520
Conc: 40.00 ng/ml

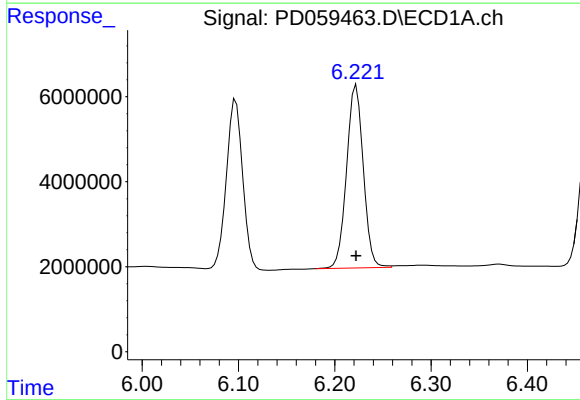


#16 4,4'-DDD

R.T.: 6.222 min
Delta R.T.: 0.000 min
Response: 51673298
Conc: 40.00 ng/ml

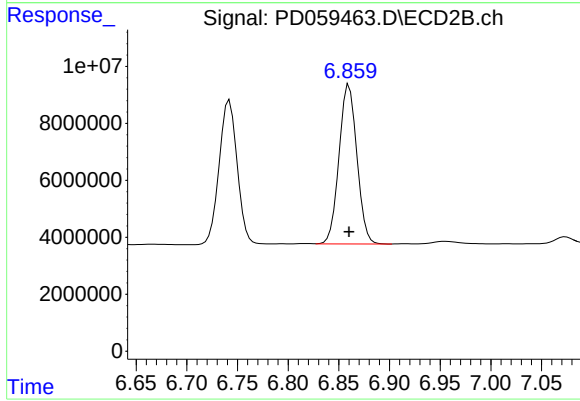

#16 4,4'-DDD


R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 68706111
Conc: 40.00 ng/ml

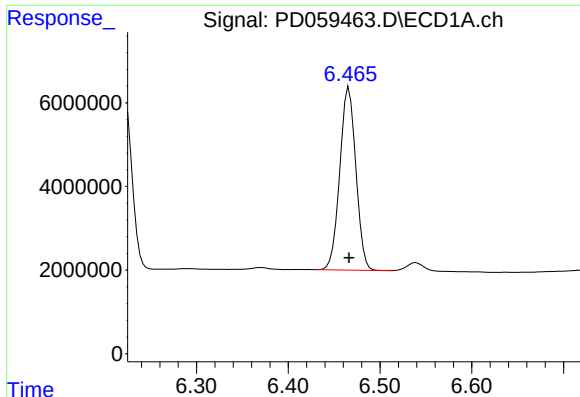

#17 4,4'-DDT


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 53264010
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

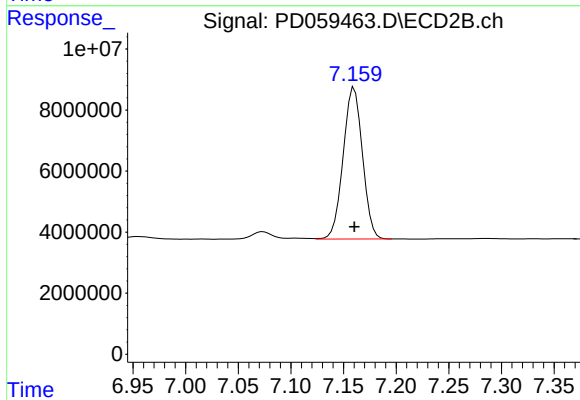


#17 4,4'-DDT

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 63554144
Conc: 40.00 ng/ml

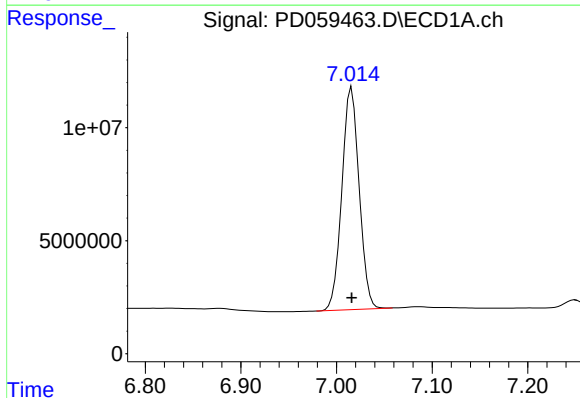


#20 Methoxychlor

R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 124059447
Conc: 200.00 ng/ml

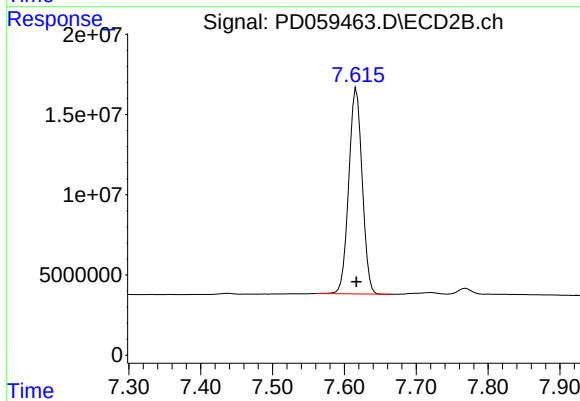

#20 Methoxychlor


R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 166326049
Conc: 200.00 ng/ml

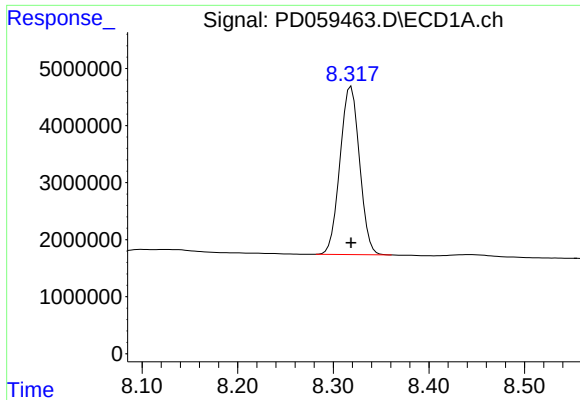

#27 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 41927544
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

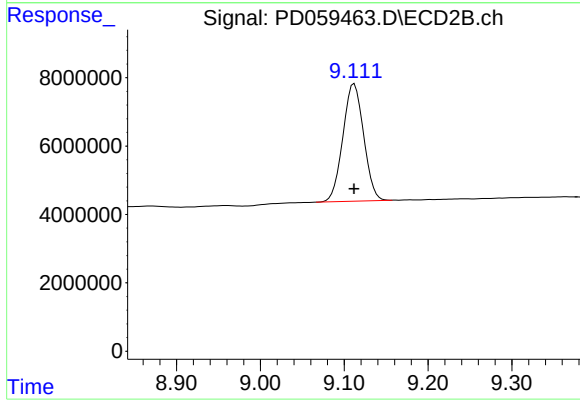

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 59303190
Conc: 40.00 ng/ml