

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
 Data File : PD059465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 18:51
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:09:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:07:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.026	54180999	76126549	37.391	38.324
27)	SA Decachlor...	8.319	9.112	77594081	113.4E6	74.027	76.474
Target Compounds							
2)	A alpha-BHC	3.954	4.417	81811453	114.5E6	38.459	39.352
3)	MA gamma-BHC...	4.240	4.702	74527032	104.0E6	38.189	38.877
4)	MA Heptachlor	4.549	5.214	74722994	97662565	38.265	38.245
9)	A Endosulfan I	5.592	6.266	57073255	78755843	38.070	38.859
13)	MA Dieldrin	5.838	6.523	125.7E6	175.1E6	77.758	78.729
14)	MA Endrin	6.097	6.742	92326193	127.3E6	77.998	81.490
16)	A 4,4'-DDD	6.223	6.860	97529727	135.8E6	75.497	79.036
17)	MA 4,4'-DDT	6.467	7.160	102.5E6	130.5E6	76.996	82.111
20)	A Methoxychlor	7.017	7.616	229.7E6	330.7E6	370.258	397.685


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
Data File : PD059465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 18:51
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:09:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:07:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

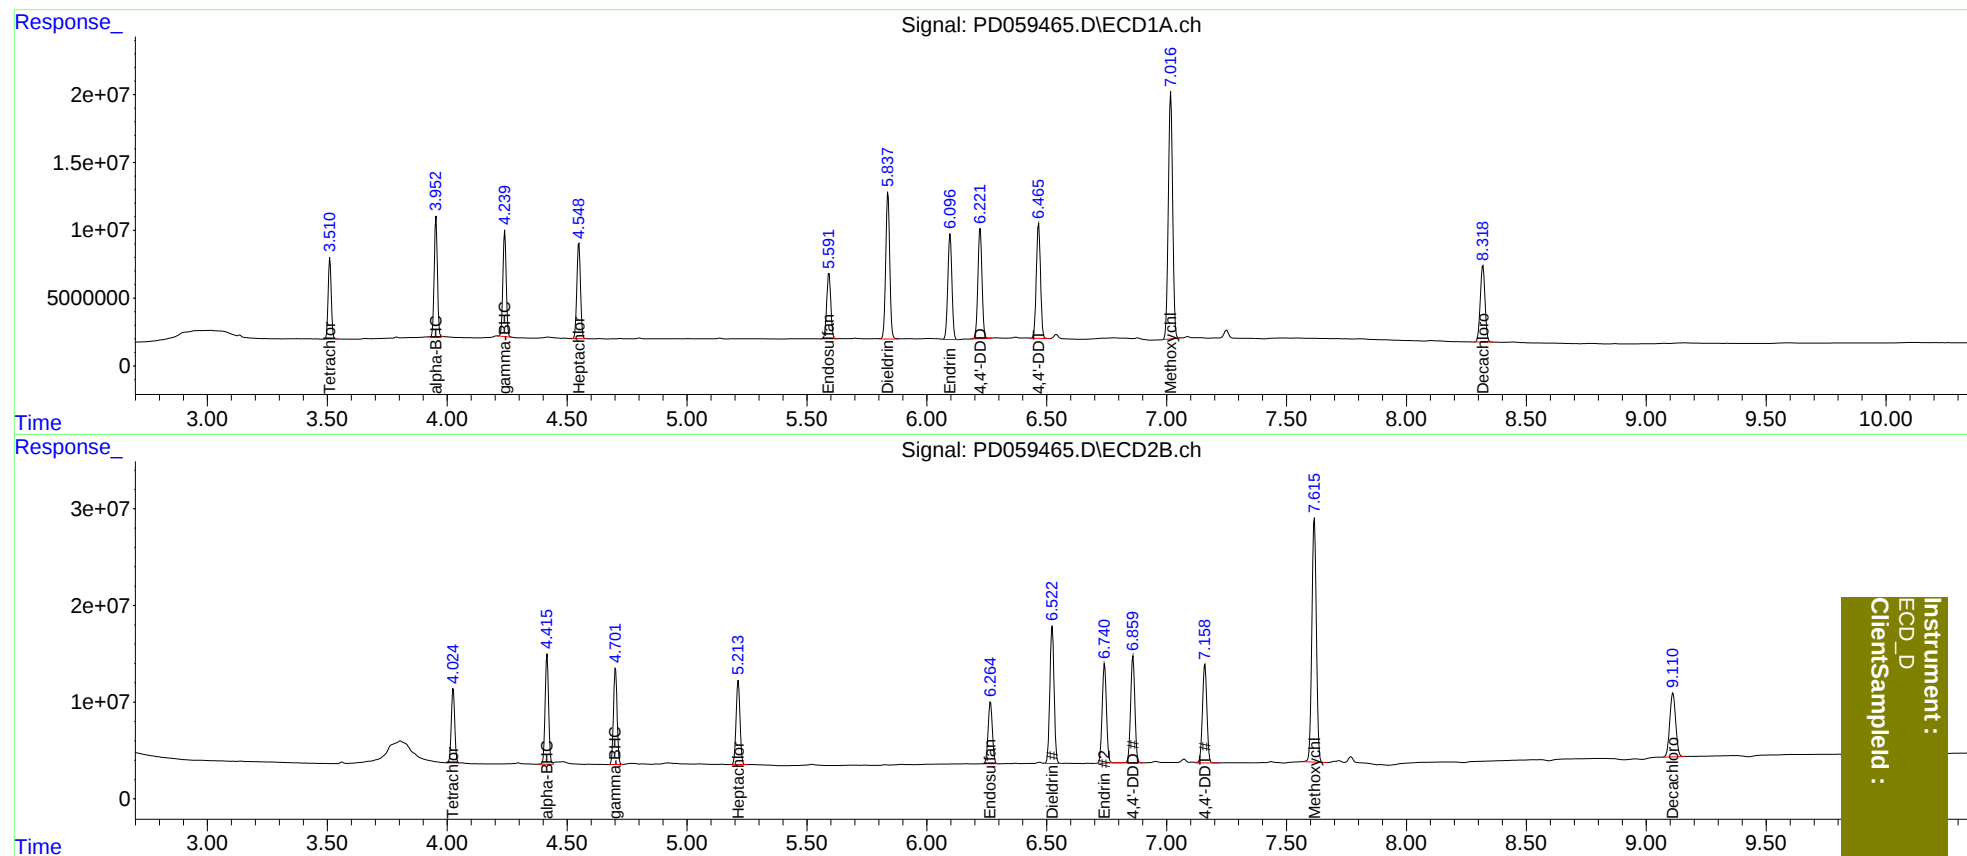


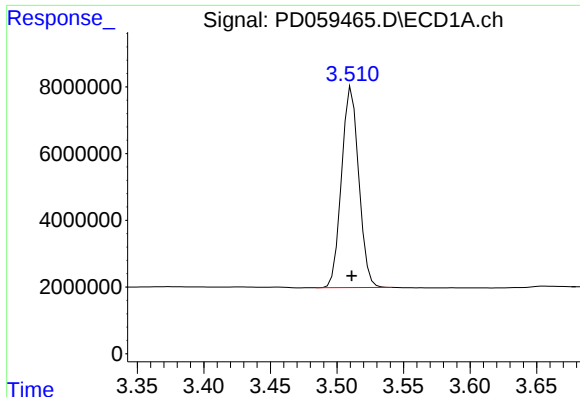

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 54180999
Conc: 37.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

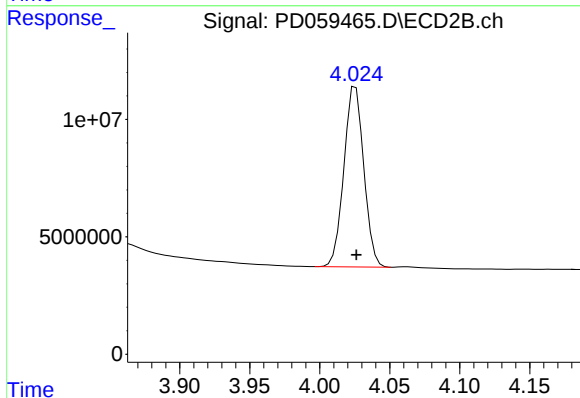


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 76126549
Conc: 38.32 ng/ml

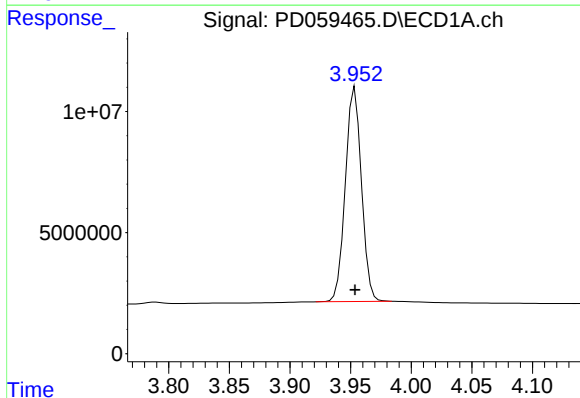


#2 alpha-BHC

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 81811453
Conc: 38.46 ng/ml

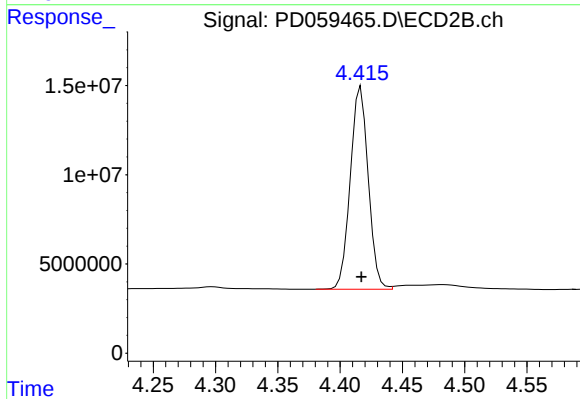

#2 alpha-BHC


R.T.: 4.417 min
Delta R.T.: 0.000 min
Response: 114474102
Conc: 39.35 ng/ml

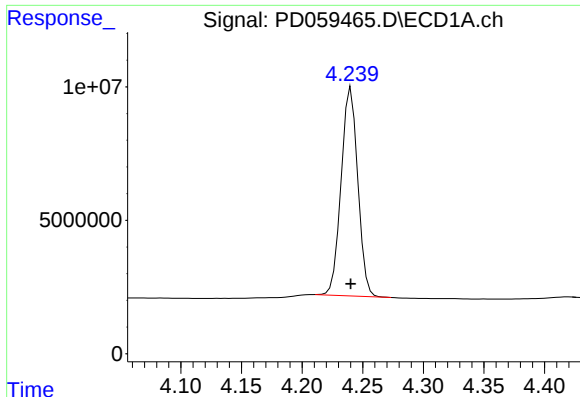

#3 gamma-BHC (Lindane)


R.T.: 4.240 min
Delta R.T.: 0.000 min
Response: 74527032
Conc: 38.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

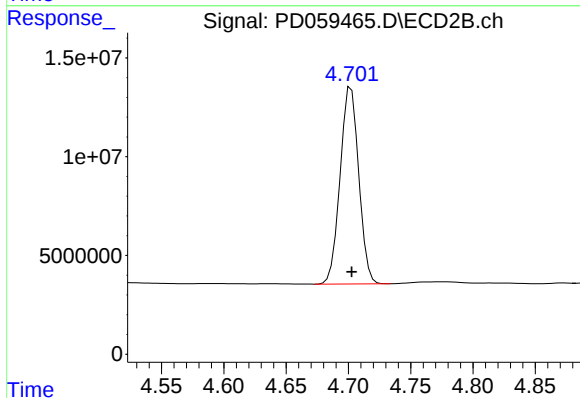


#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 103968943
Conc: 38.88 ng/ml

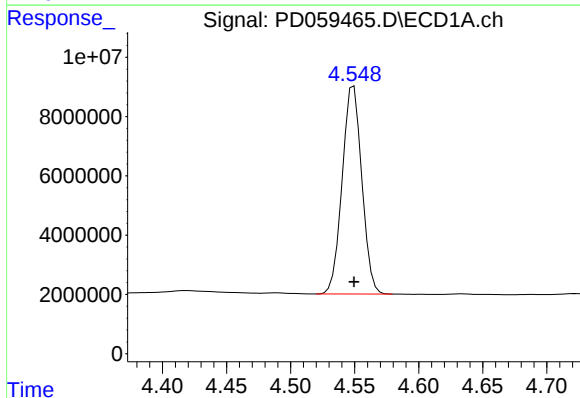


#4 Heptachlor

R.T.: 4.549 min
Delta R.T.: 0.000 min
Response: 74722994
Conc: 38.27 ng/ml

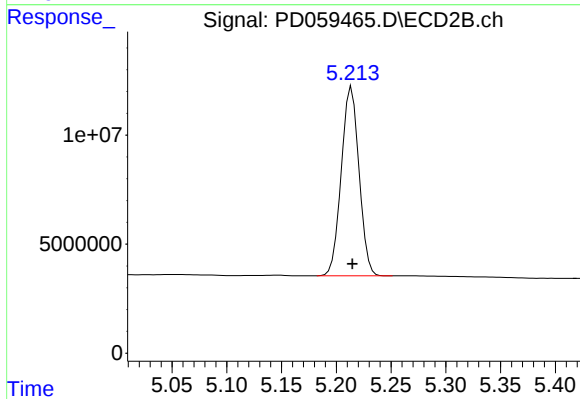

#4 Heptachlor


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 97662565
Conc: 38.24 ng/ml

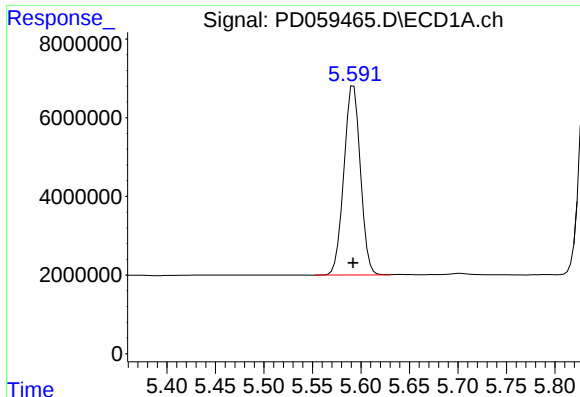

#9 Endosulfan I


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 57073255
Conc: 38.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

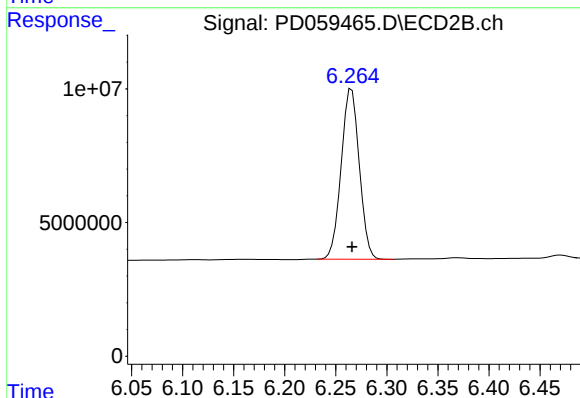


#9 Endosulfan I

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 78755843
Conc: 38.86 ng/ml

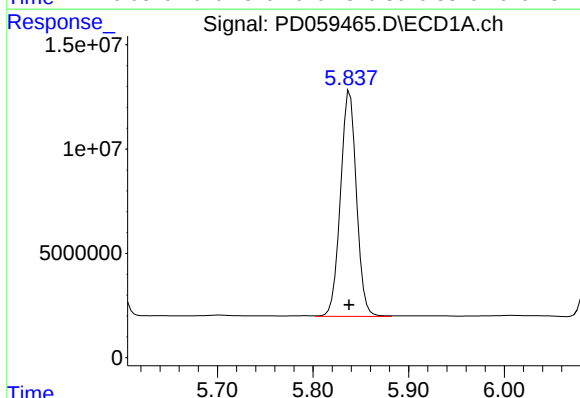


#13 Dieldrin

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 125702296
Conc: 77.76 ng/ml

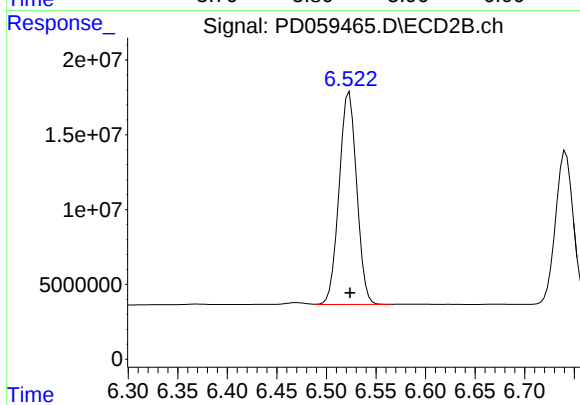

#13 Dieldrin


R.T.: 6.523 min
Delta R.T.: 0.000 min
Response: 175091292
Conc: 78.73 ng/ml

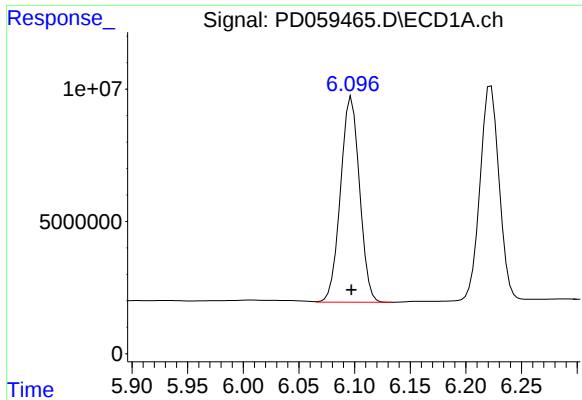

#14 Endrin


R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 92326193
Conc: 78.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

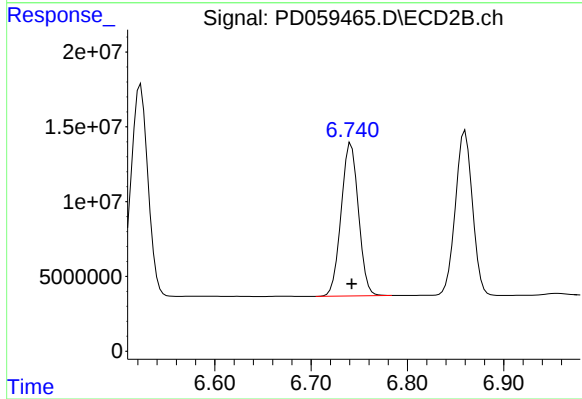


#14 Endrin

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 127343136
Conc: 81.49 ng/ml

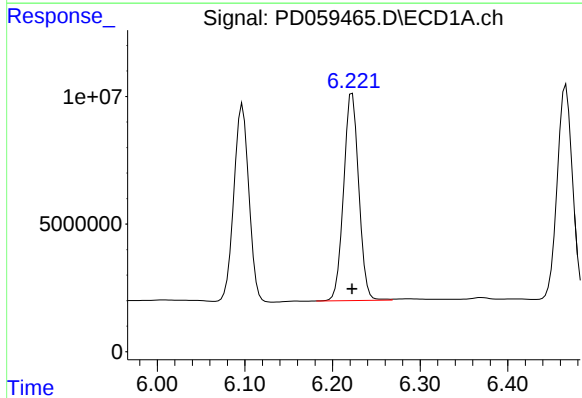


#16 4,4'-DDD

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 97529727
Conc: 75.50 ng/ml

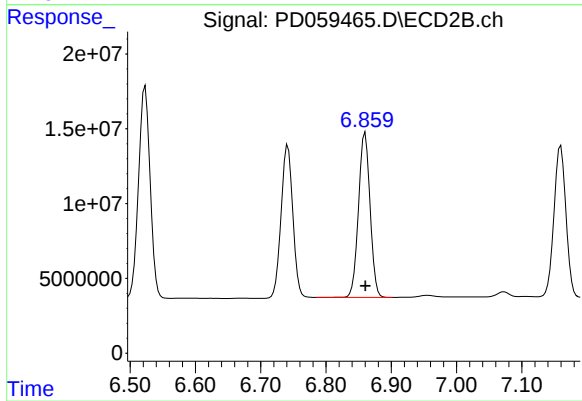

#16 4,4'-DDD


R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 135756592
Conc: 79.04 ng/ml

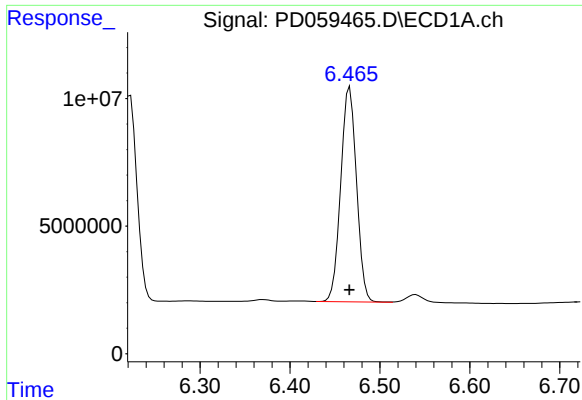

#17 4,4'-DDT


R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 102527948
Conc: 77.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

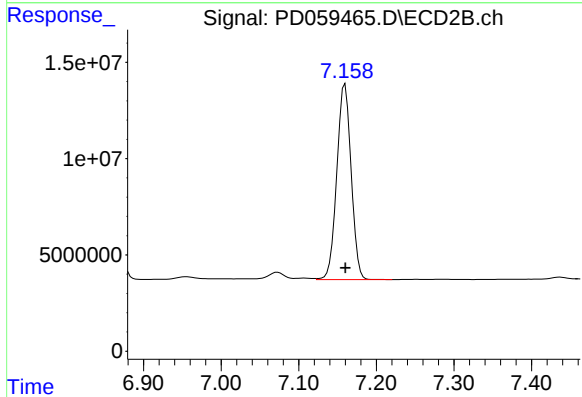


#17 4,4'-DDT

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 130462972
Conc: 82.11 ng/ml

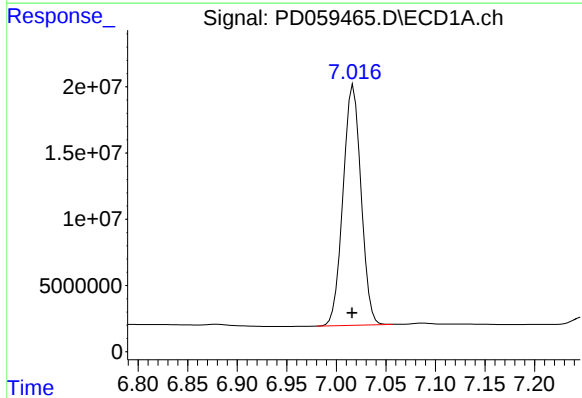


#20 Methoxychlor

R.T.: 7.017 min
Delta R.T.: 0.001 min
Response: 229670116
Conc: 370.26 ng/ml

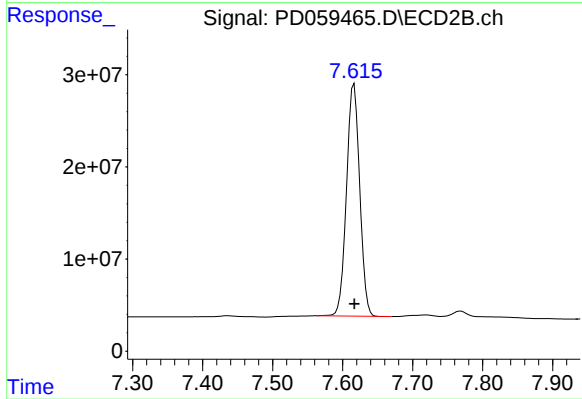

#20 Methoxychlor


R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 330727055
Conc: 397.69 ng/ml

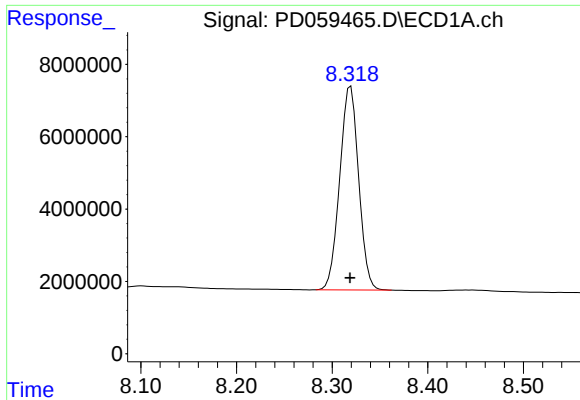

#27 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 77594081
Conc: 74.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

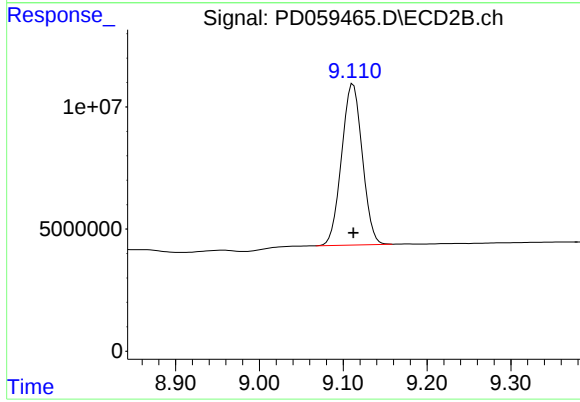

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 113378238
Conc: 76.47 ng/ml