

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
 Data File : PD059467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2020 19:20
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 04:09:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:07:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.025	108.7E6	154.2E6	75.030	77.634
27)	SA Decachlor...	8.319	9.112	145.2E6	218.8E6	138.512	147.560
Target Compounds							
2)	A alpha-BHC	3.954	4.416	168.3E6	236.7E6	79.138	81.385
3)	MA gamma-BHC...	4.241	4.702	151.8E6	215.2E6	77.808	80.487
4)	MA Heptachlor	4.550	5.214	151.1E6	203.1E6	77.371	79.545
9)	A Endosulfan I	5.593	6.266	113.5E6	159.6E6	75.686	78.732
13)	MA Dieldrin	5.839	6.524	253.1E6	356.6E6	156.563	160.338
14)	MA Endrin	6.098	6.742	176.5E6	245.9E6	149.095	157.369
16)	A 4,4'-DDD	6.223	6.861	194.7E6	274.9E6	150.684	160.043
17)	MA 4,4'-DDT	6.467	7.160	209.0E6	262.3E6	156.966	165.113
20)	A Methoxychlor	7.017	7.617	439.0E6	632.2E6	707.710	760.143

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100220\
Data File : PD059467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2020 19:20
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 04:09:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:07:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

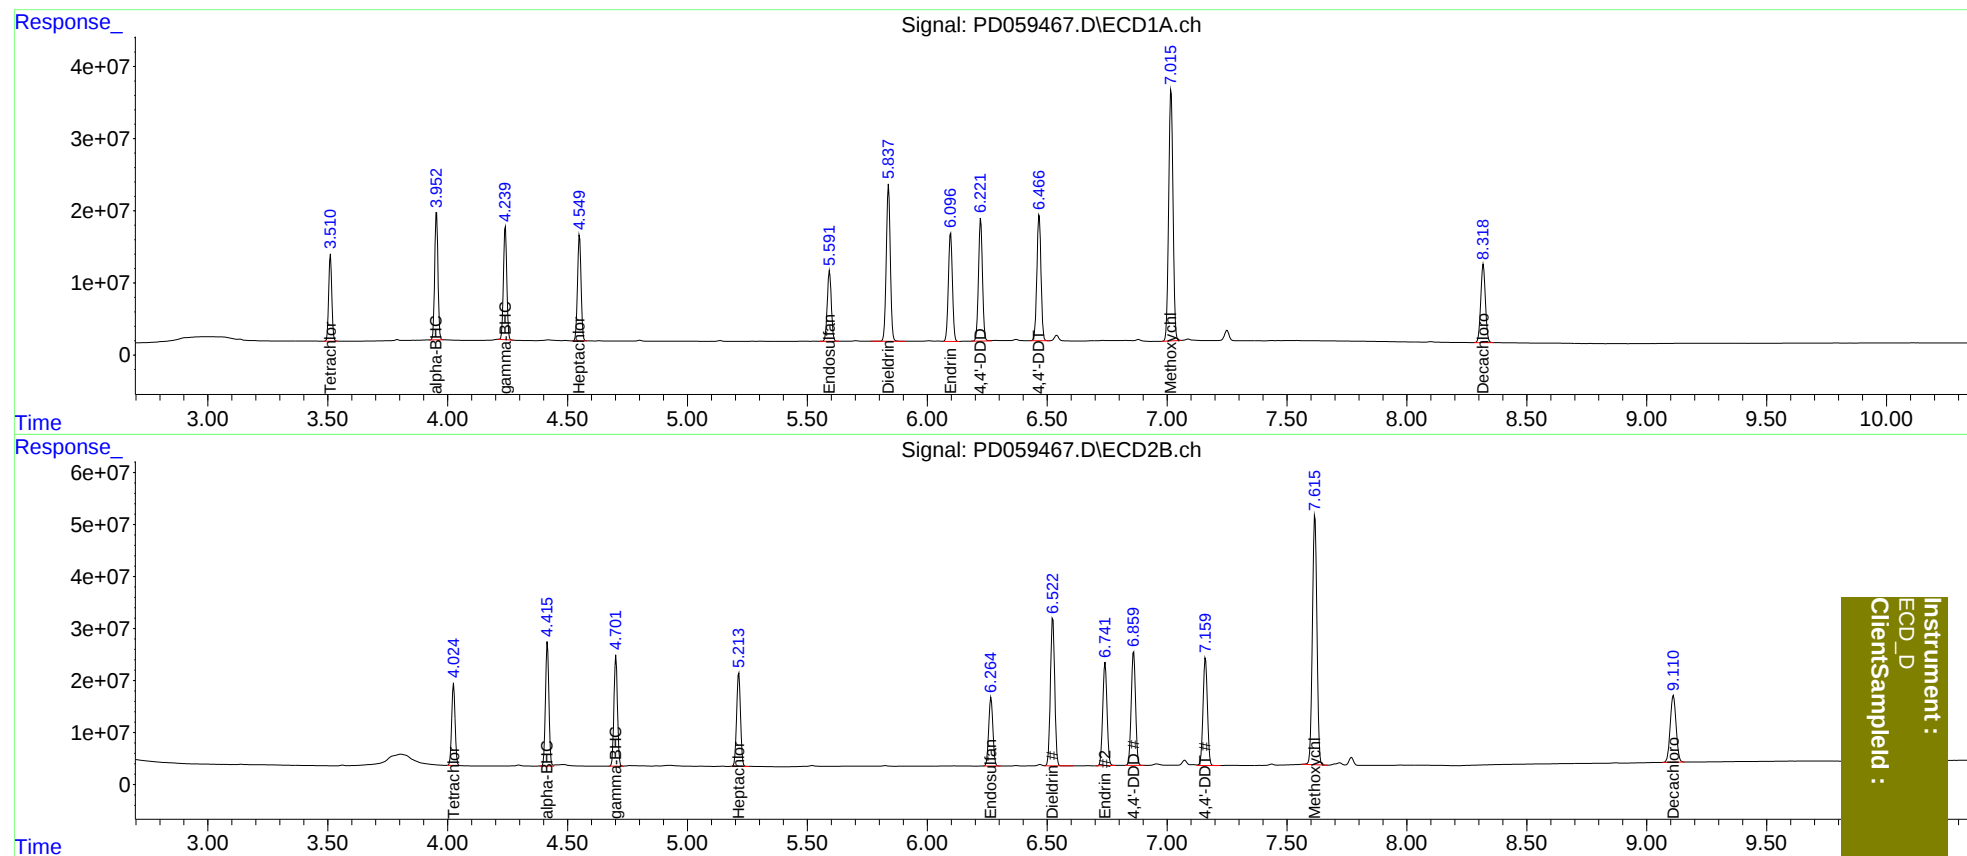


Instrument :
ECD_D
ClientSampled :

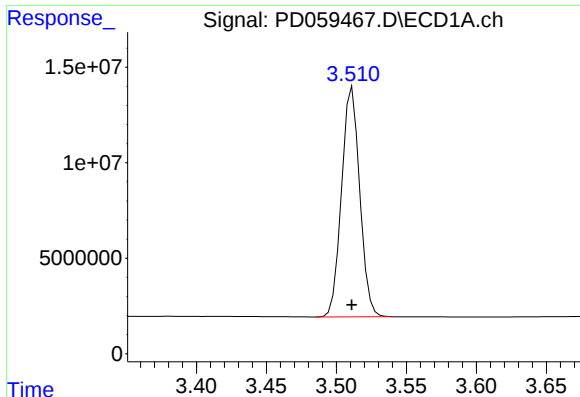

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 108720326
Conc: 75.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

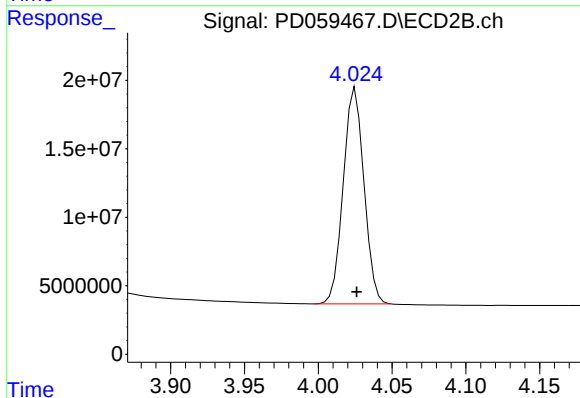


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 154209437
Conc: 77.63 ng/ml

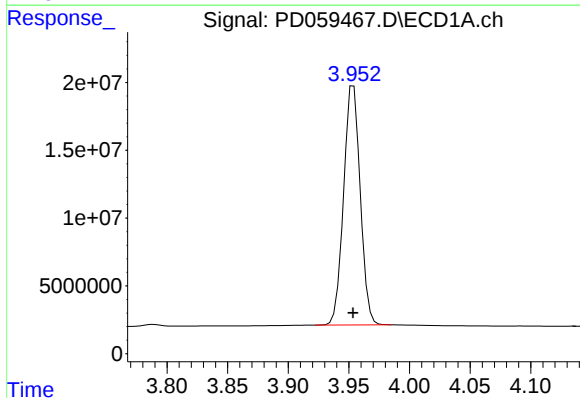


#2 alpha-BHC

R.T.: 3.954 min
Delta R.T.: 0.000 min
Response: 168344833
Conc: 79.14 ng/ml

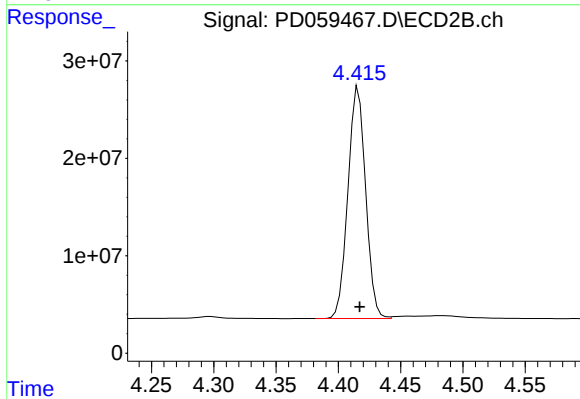

#2 alpha-BHC


R.T.: 4.416 min
Delta R.T.: -0.001 min
Response: 236749670
Conc: 81.39 ng/ml

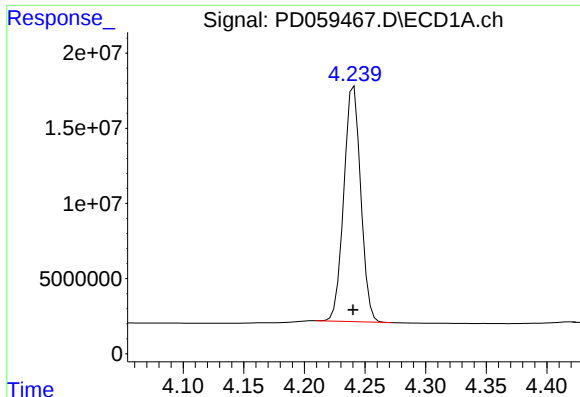

#3 gamma-BHC (Lindane)


R.T.: 4.241 min
Delta R.T.: 0.000 min
Response: 151844974
Conc: 77.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

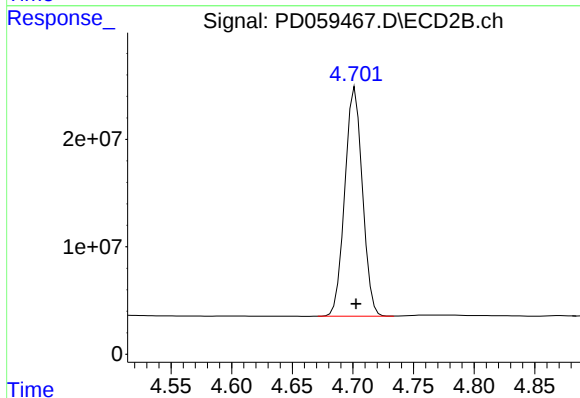


#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 215244341
Conc: 80.49 ng/ml

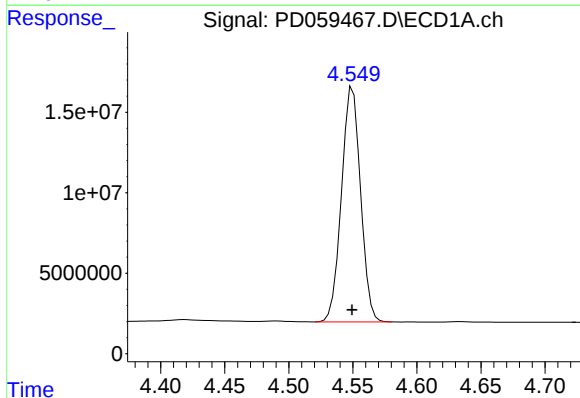


#4 Heptachlor

R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 151088117
Conc: 77.37 ng/ml

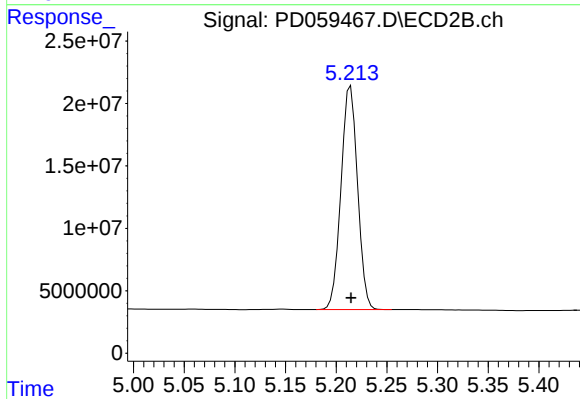

#4 Heptachlor


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 203128731
Conc: 79.55 ng/ml

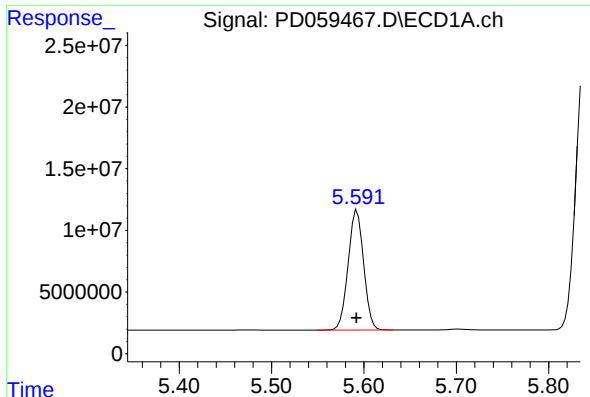

#9 Endosulfan I


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 113465542
Conc: 75.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

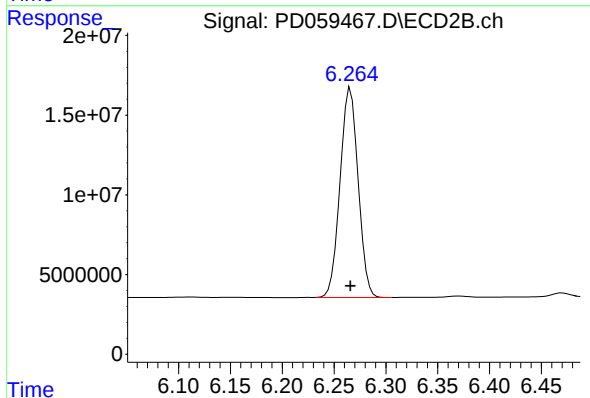


#9 Endosulfan I

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 159566532
Conc: 78.73 ng/ml

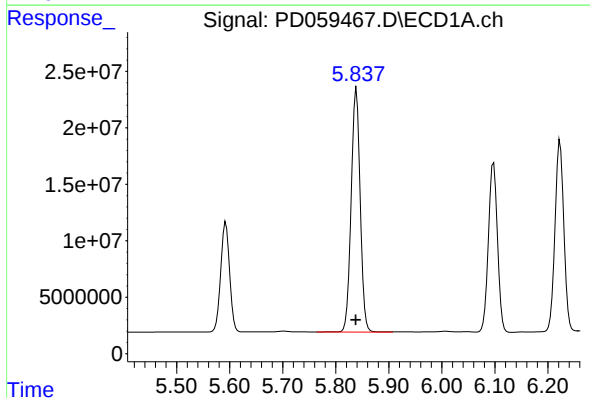


#13 Dieldrin

R.T.: 5.839 min
Delta R.T.: 0.001 min
Response: 253095114
Conc: 156.56 ng/ml

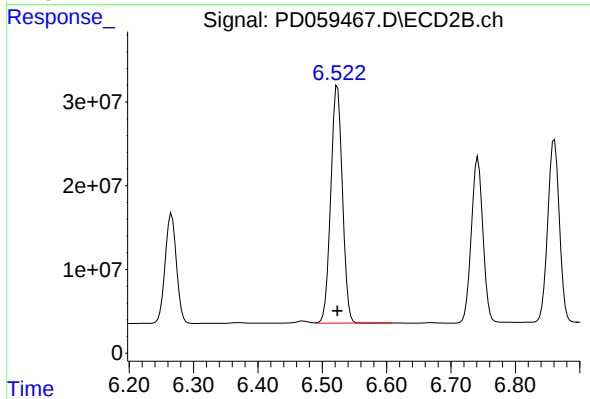

#13 Dieldrin


R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 356586446
Conc: 160.34 ng/ml

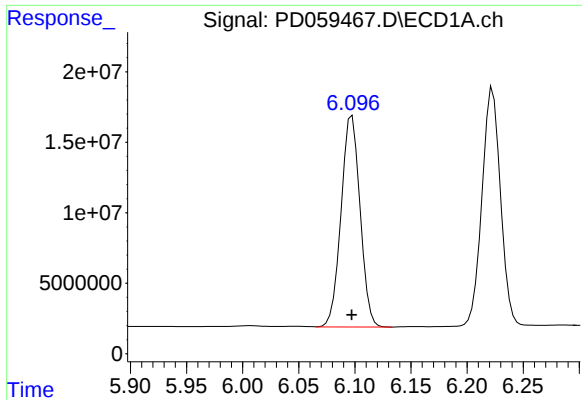

#14 Endrin


R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 176484460
Conc: 149.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

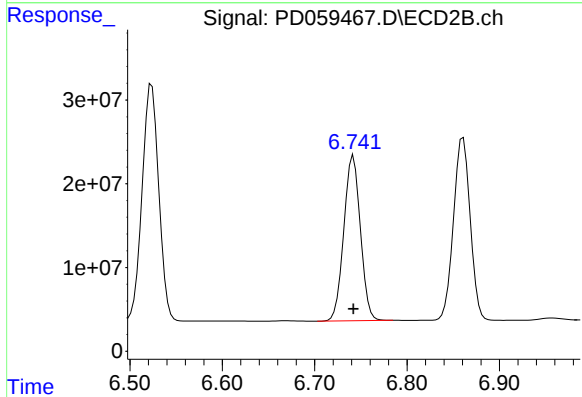


#14 Endrin

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 245917904
Conc: 157.37 ng/ml

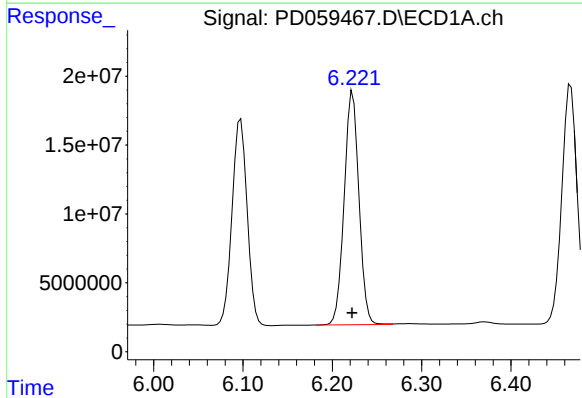


#16 4,4'-DDD

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 194658372
Conc: 150.68 ng/ml

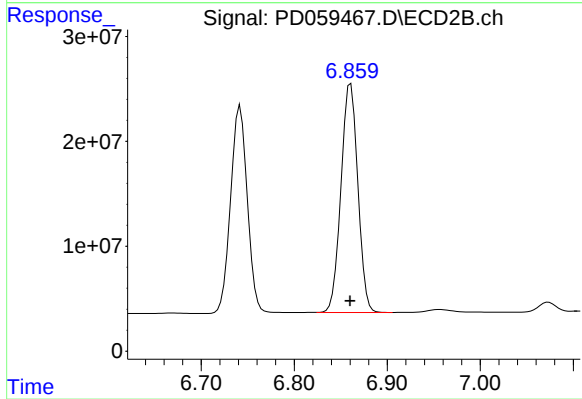

#16 4,4'-DDD


R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 274897868
Conc: 160.04 ng/ml

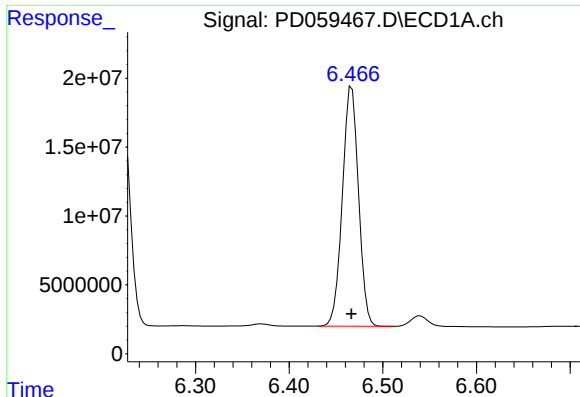

#17 4,4'-DDT


R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 209016438
Conc: 156.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

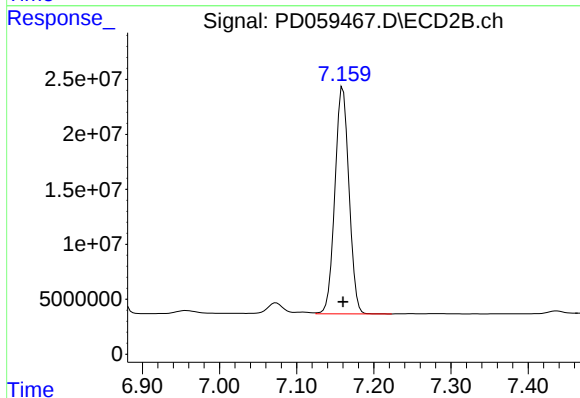


#17 4,4'-DDT

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 262340729
Conc: 165.11 ng/ml

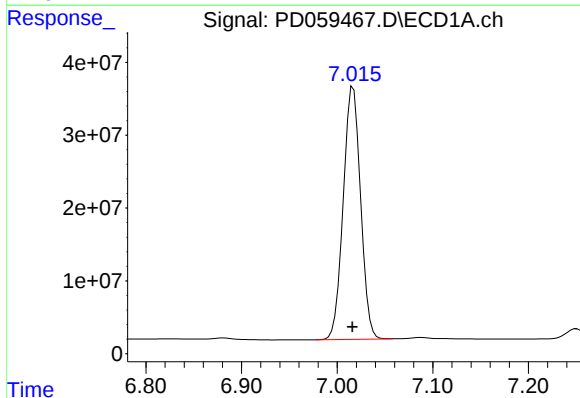


#20 Methoxychlor

R.T.: 7.017 min
Delta R.T.: 0.001 min
Response: 438990686
Conc: 707.71 ng/ml

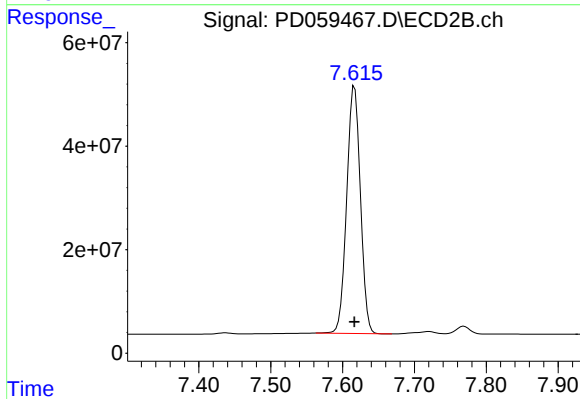

#20 Methoxychlor


R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 632157613
Conc: 760.14 ng/ml

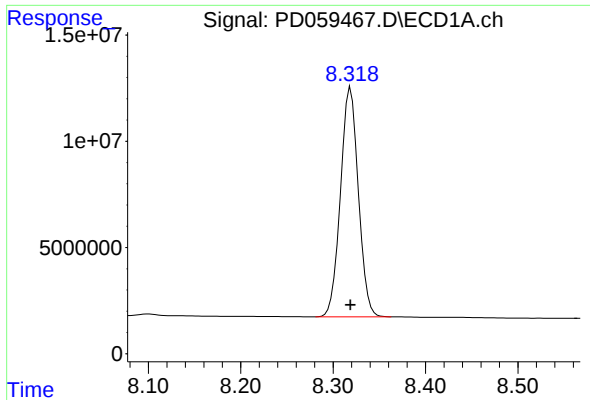

#27 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 145186364
Conc: 138.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

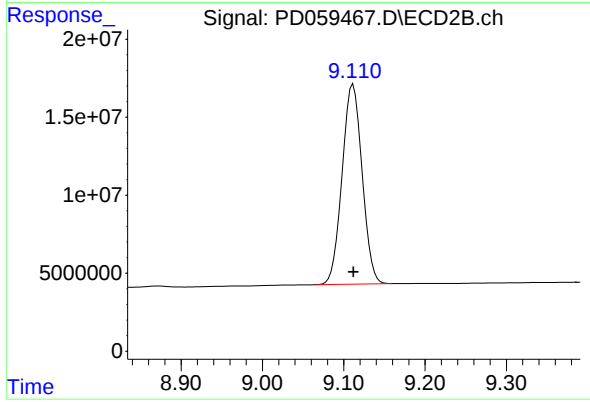

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 218769876
Conc: 147.56 ng/ml