

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100223\
 Data File : PD078515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 11:28
 Operator : AR\AJ
 Sample : 04636-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-03-09272023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/03/2023
 Supervised By :Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 13:16:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.758	25481422	18390683	10.036	11.628
28)	SA Decachlor...	9.083	7.895	30577466	16840736	10.038	9.759
Target Compounds							
11)	B alpha-Chl...	6.030	5.021	3338706	855935	0.938m	0.425m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100223\
Data File : PD078515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 11:28
Operator : AR\AJ
Sample : 04636-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OR-03-09272023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/03/2023
Supervised By : Ankita Jodhani 10/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 13:16:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

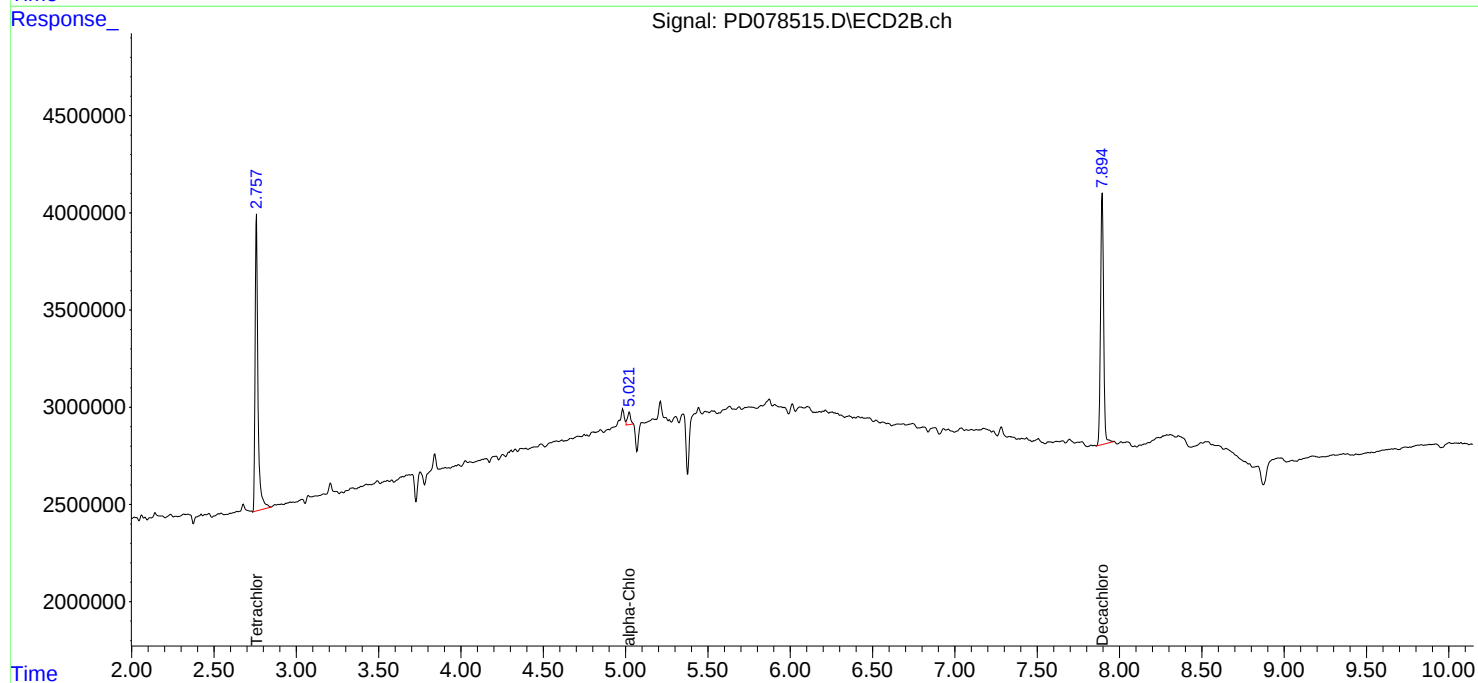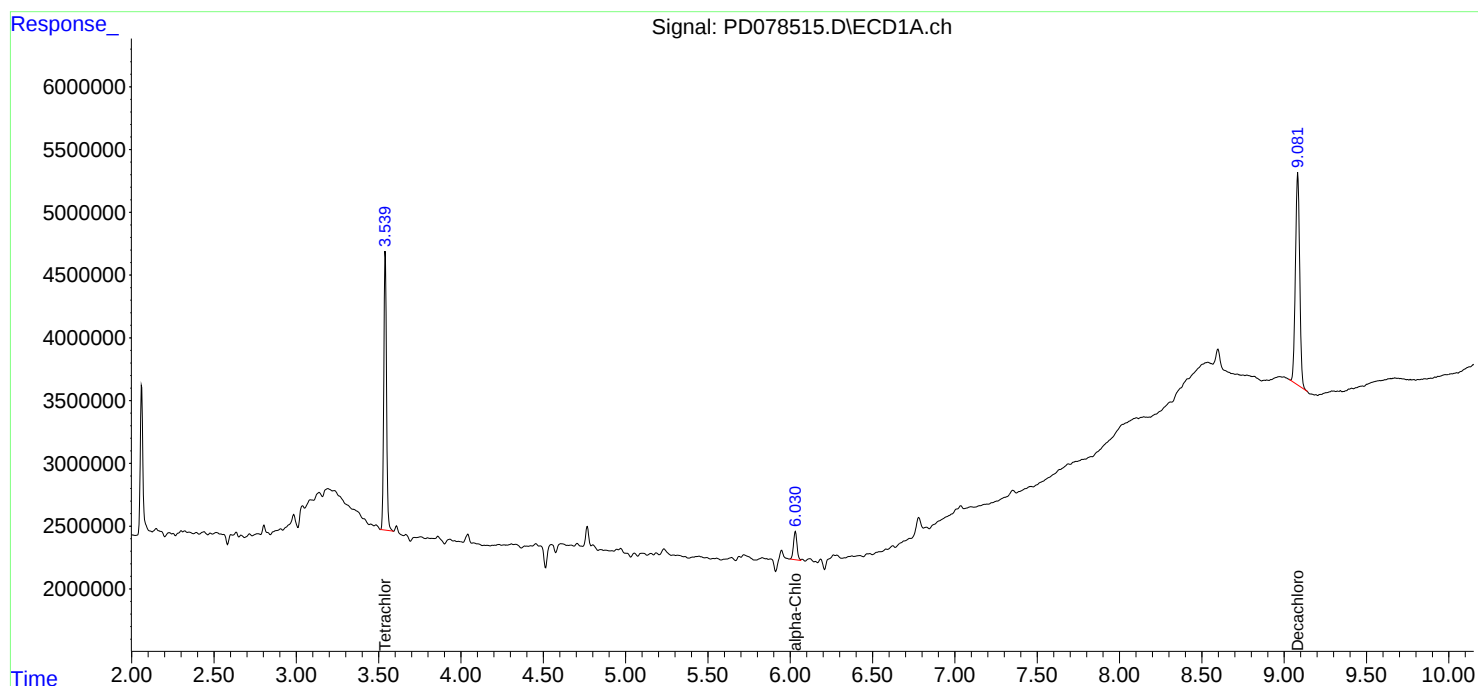

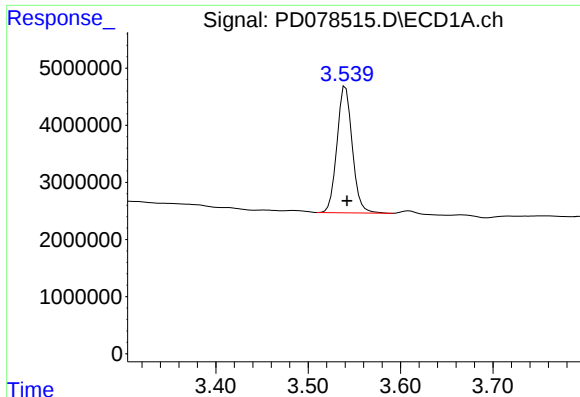


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: -0.001 min
Response: 25481422
Conc: 10.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-03-09272023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023

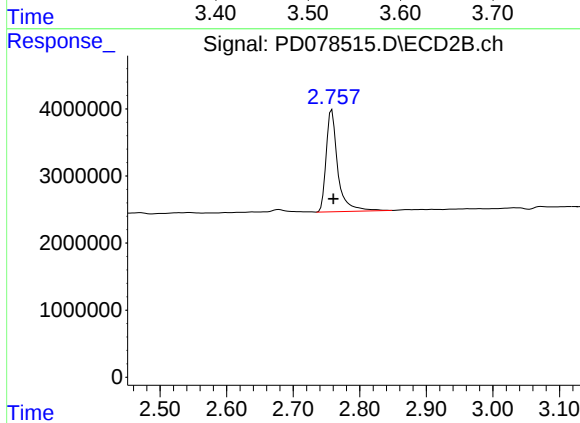


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.002 min
Response: 18390683
Conc: 11.63 ng/ml

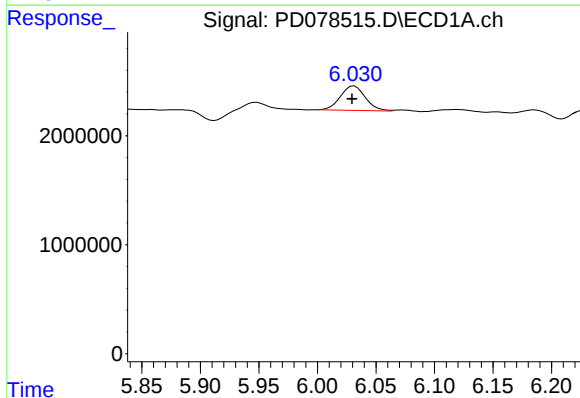


#11 alpha-Chlordane

R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 3338706
Conc: 0.94 ng/ml m

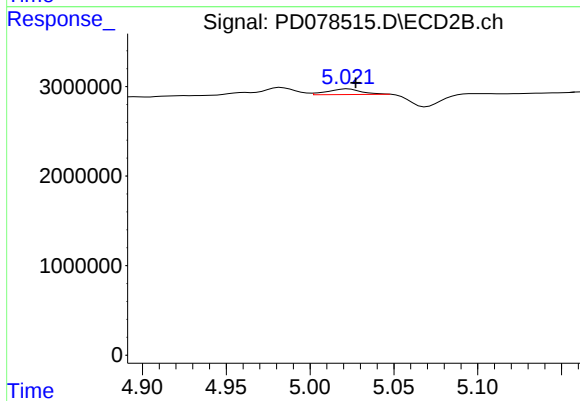

#11 alpha-Chlordane

R.T.: 5.021 min
Delta R.T.: -0.006 min
Response: 855935
Conc: 0.42 ng/ml m

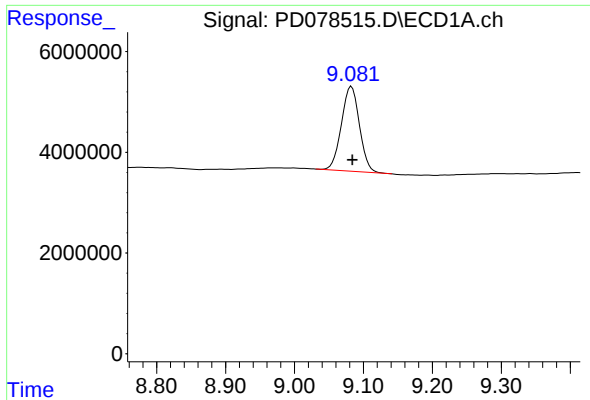


#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 30577466
Conc: 10.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-03-09272023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/03/2023
Supervised By :Ankita Jodhani 10/03/2023

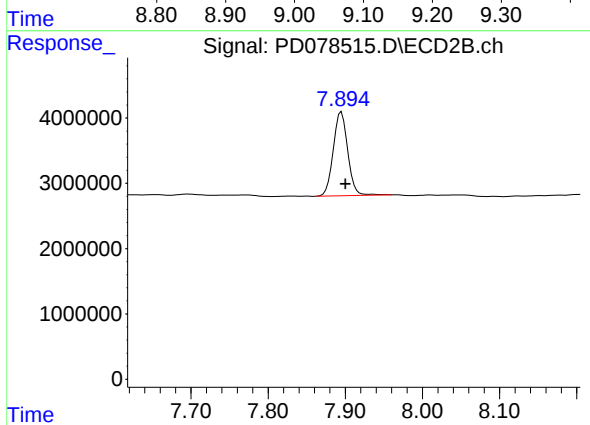

#28 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.005 min
Response: 16840736
Conc: 9.76 ng/ml