

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100319\
 Data File : PD055169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 10:02
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 07:28:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 24 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.733	0.000	261942	0	0.236	N.D.	#
3) MA	gamma-BHC...	3.998	0.000	111398	0	0.104	N.D.	#
4) MA	Heptachlor	4.286	0.000	120475	0	0.130	N.D.	#
6) B	beta-BHC	4.286f	0.000	120475	0	0.258	N.D.	#
7) B	delta-BHC	4.398f	0.000	70884	0	<MDL	N.D.	#
8) B	Heptachlo...	4.948	0.000	354203	0	0.386	N.D.	#
14) MA	Endrin	5.759	0.000	192370	0	0.231	N.D.	#
18) B	Endrin al...	6.204	0.000	169119	0	0.233	N.D.	#
20) A	Methoxychlor	6.701	0.000	134712	0	0.380	N.D.	#
21) B	Endrin ke...	6.983f	0.000	64947	0	<MDL	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100319\
Data File : PD055169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 10:02
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 07:28:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD092319CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 24 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

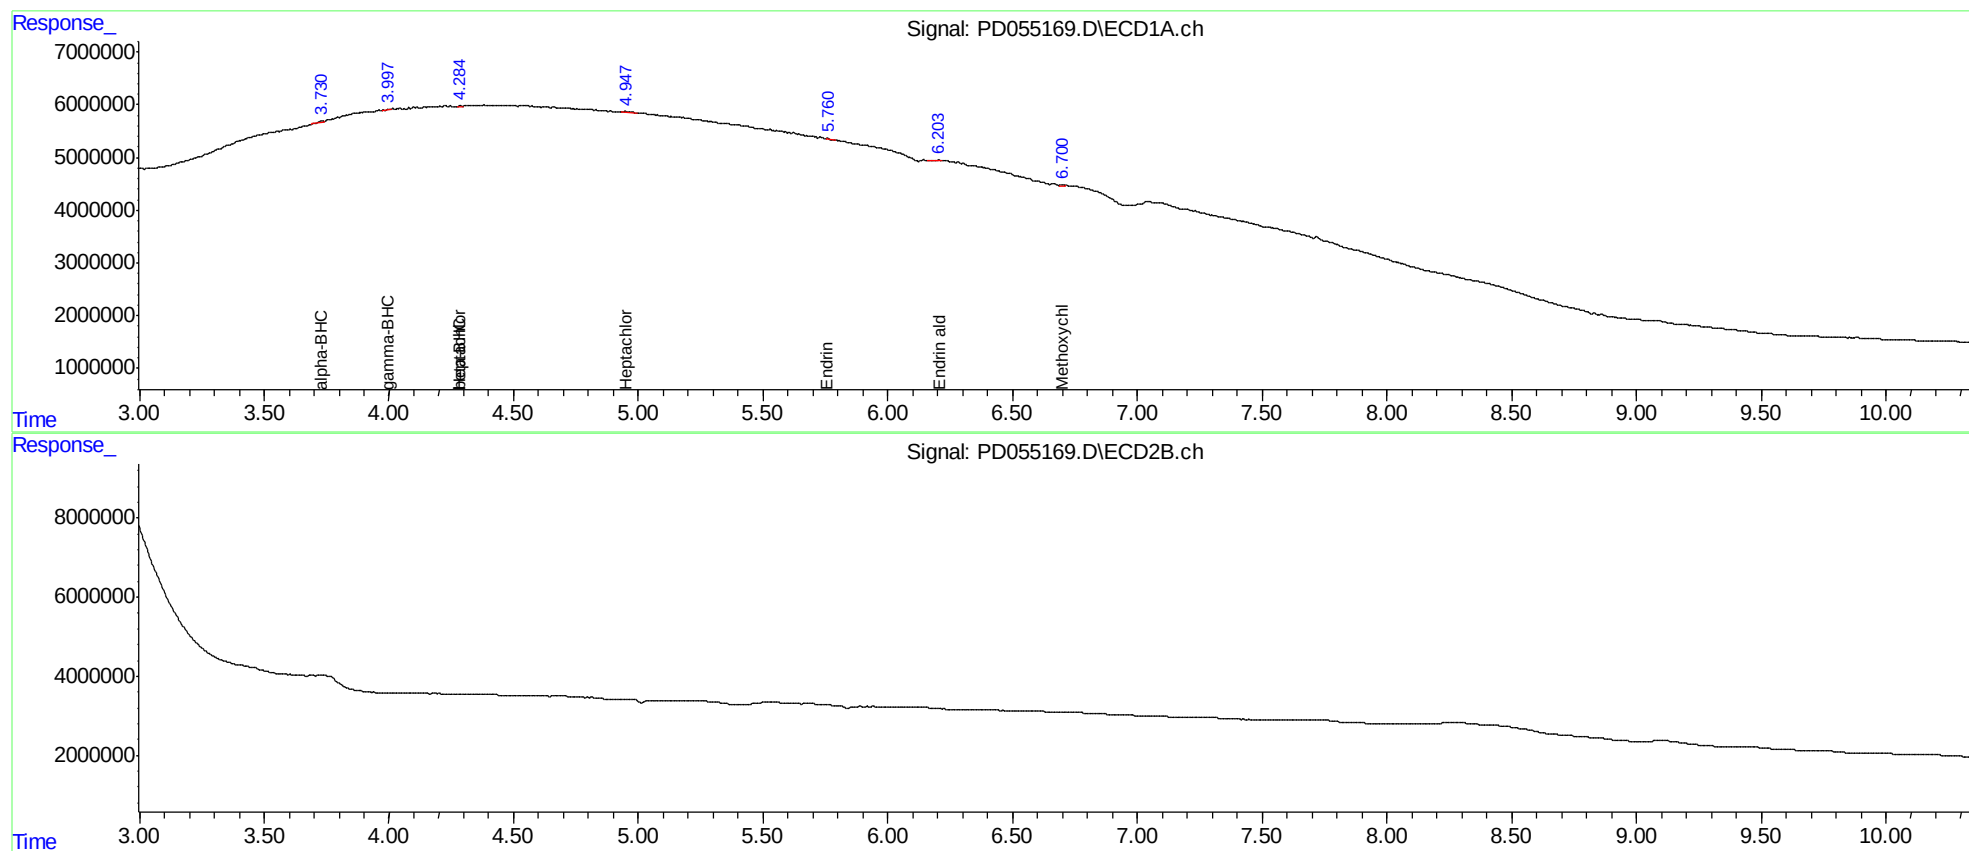


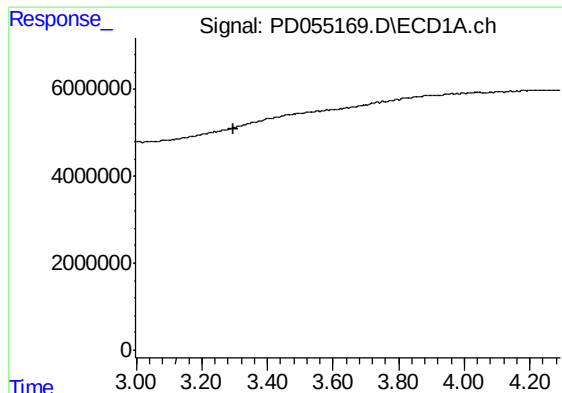

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

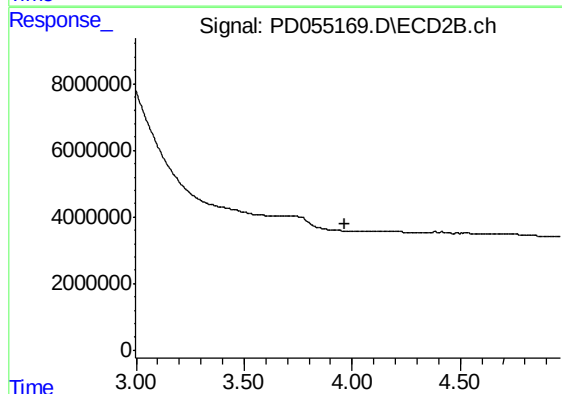


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

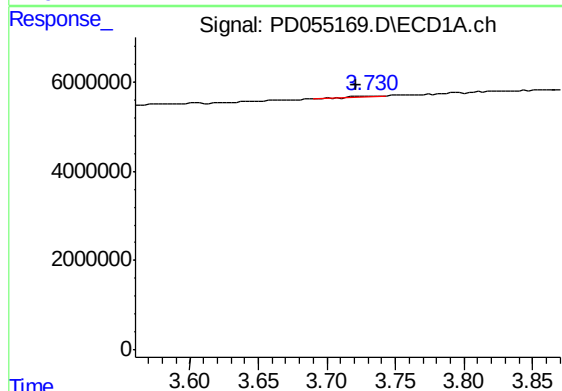


#2 alpha-BHC

R.T.: 3.733 min
Delta R.T.: 0.011 min
Response: 261942
Conc: 0.24 ng/ml

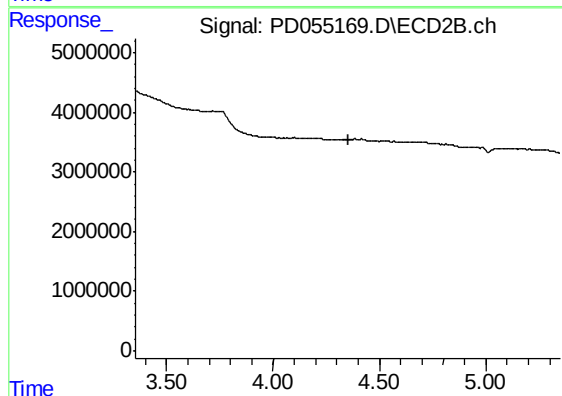

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.353 min
Response: 0
Conc: N.D.

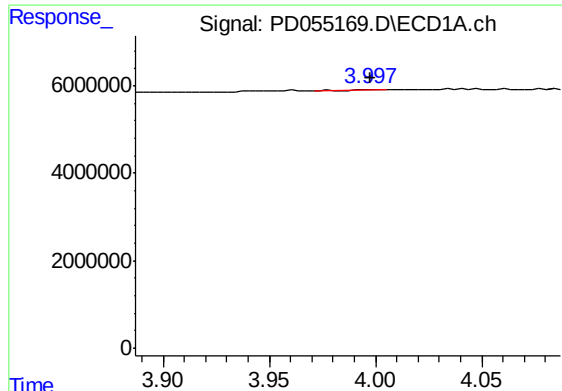

#3 gamma-BHC (Lindane)


R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 111398
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

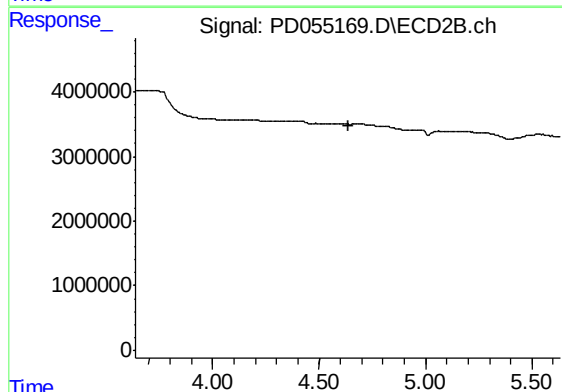


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.635 min
Response: 0
Conc: N.D.

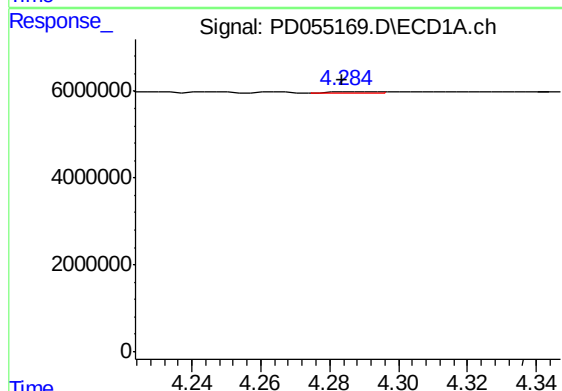


#4 Heptachlor

R.T.: 4.286 min
Delta R.T.: 0.002 min
Response: 120475
Conc: 0.13 ng/ml

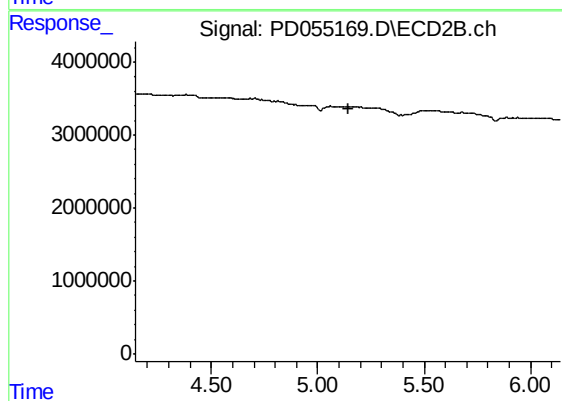

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.142 min
Response: 0
Conc: N.D.

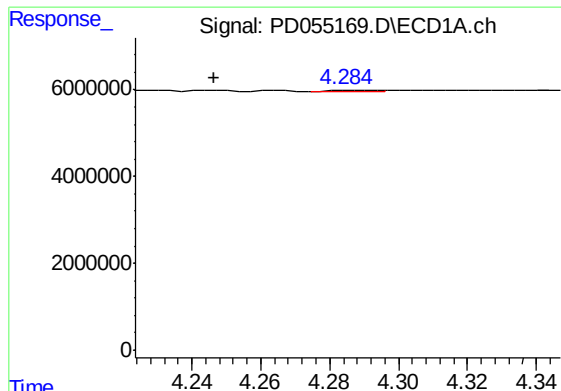

#6 beta-BHC


R.T.: 4.286 min
Delta R.T.: 0.039 min
Response: 120475
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

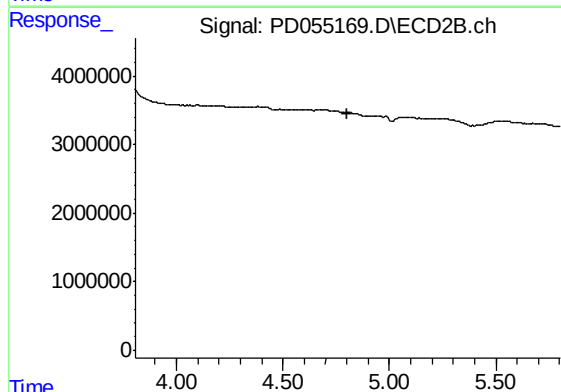


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

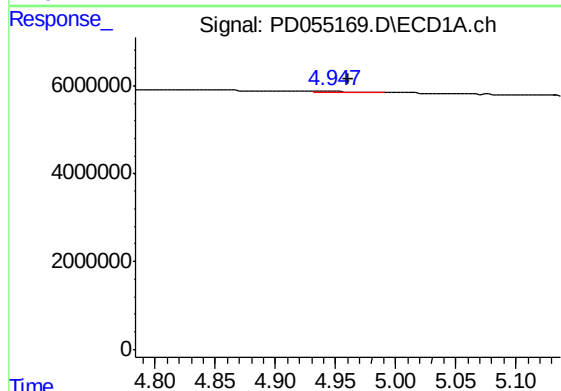


#8 Heptachlor epoxide

R.T.: 4.948 min
Delta R.T.: -0.013 min
Response: 354203
Conc: 0.39 ng/ml

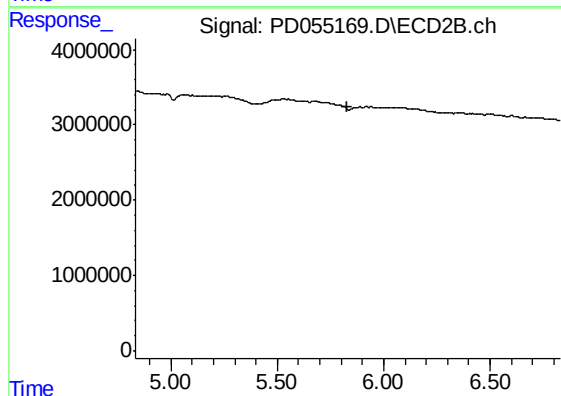

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

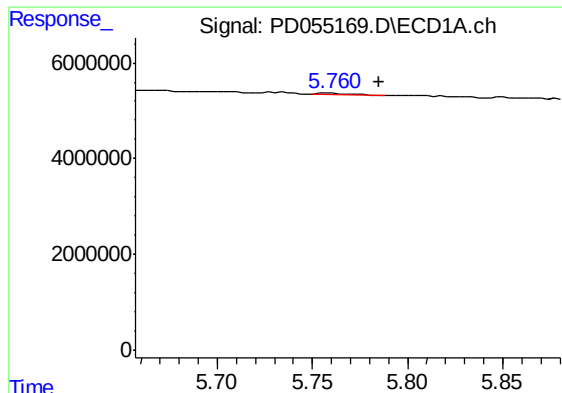

#14 Endrin


R.T.: 5.759 min
Delta R.T.: -0.027 min
Response: 192370
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

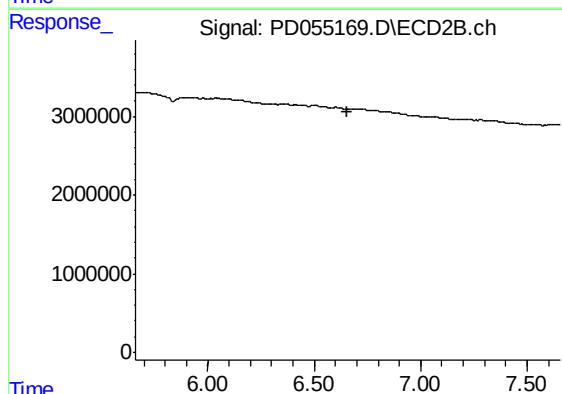


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.658 min
Response: 0
Conc: N.D.

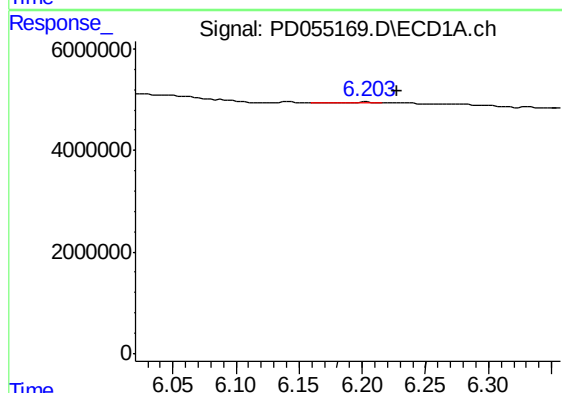


#18 Endrin aldehyde

R.T.: 6.204 min
Delta R.T.: -0.024 min
Response: 169119
Conc: 0.23 ng/ml

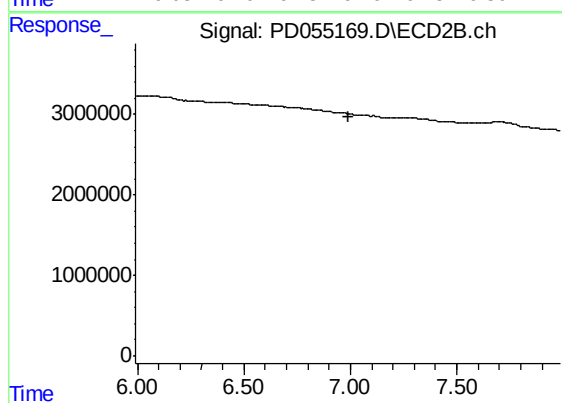

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

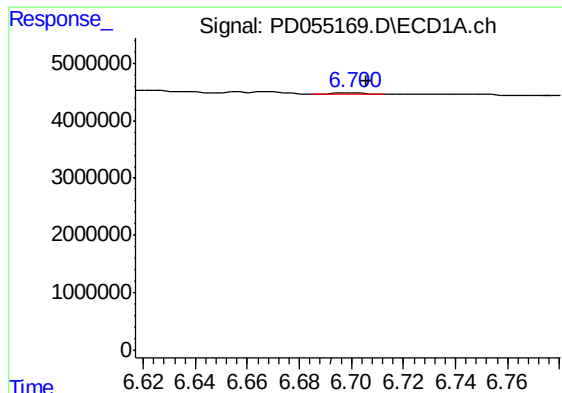

#20 Methoxychlor


R.T.: 6.701 min
Delta R.T.: -0.004 min
Response: 134712
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

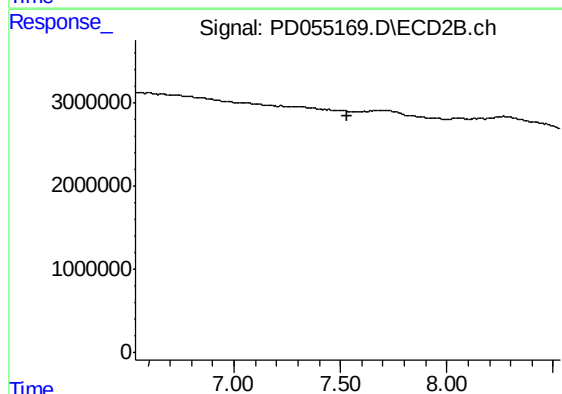


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.535 min
Response: 0
Conc: N.D.

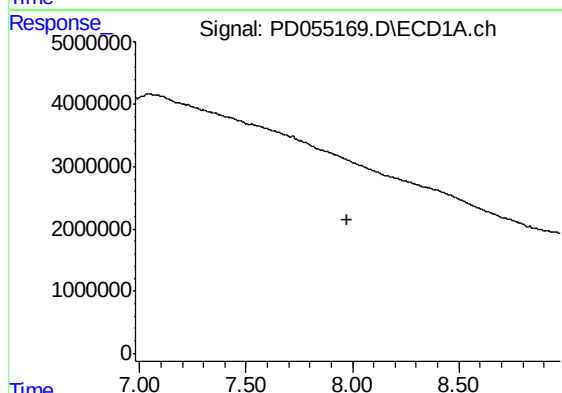

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.977 min
Response: 0
Conc: N.D.

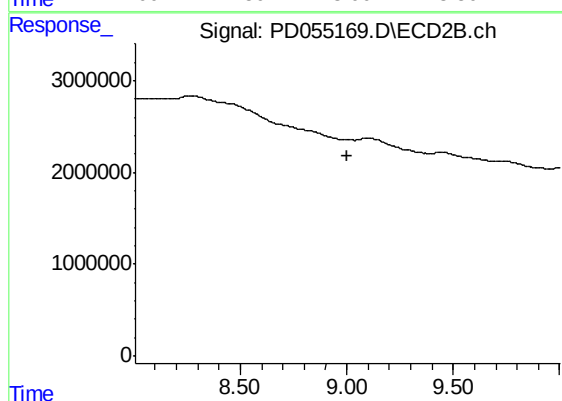

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.005 min
Response: 0
Conc: N.D.