

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 19:21
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 03:42:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 03:41:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	211.5E6	2192.0E6	72.169	70.069
28)	SA Decachlor...	7.988	9.084	168.3E6	606.7E6	70.190	69.530
Target Compounds							
23)	Chlordane-1	3.814	4.725	68030305	686.4E6	714.006	684.018
24)	Chlordane-2	4.396	5.258	69254921	481.7E6	700.757	686.041
25)	Chlordane-3	5.032	5.969	227.6E6	1522.1E6	724.768	697.937
26)	Chlordane-4	5.095	6.047	205.4E6	1770.6E6	709.127	696.876
27)	Chlordane-5	5.997	6.908	76808136	324.1E6	711.995	702.505



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 19:21
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 03:42:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 03:41:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

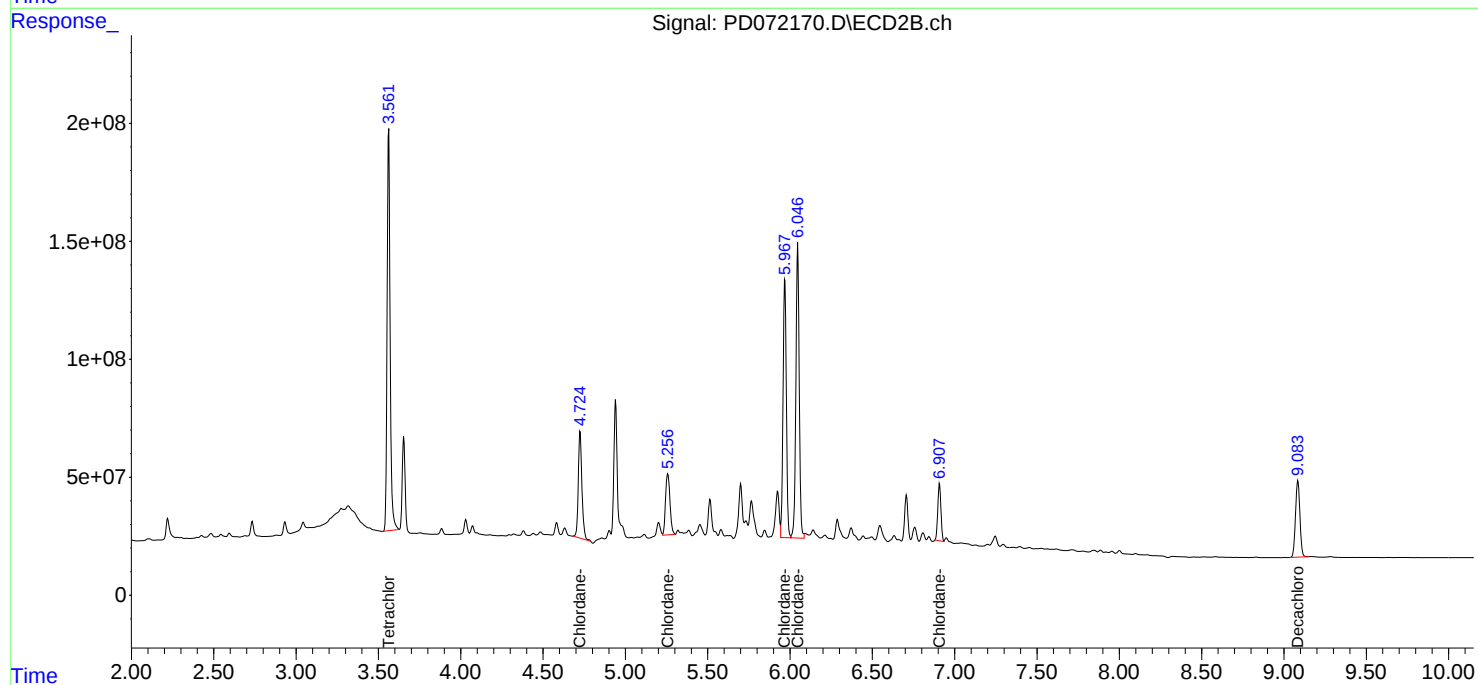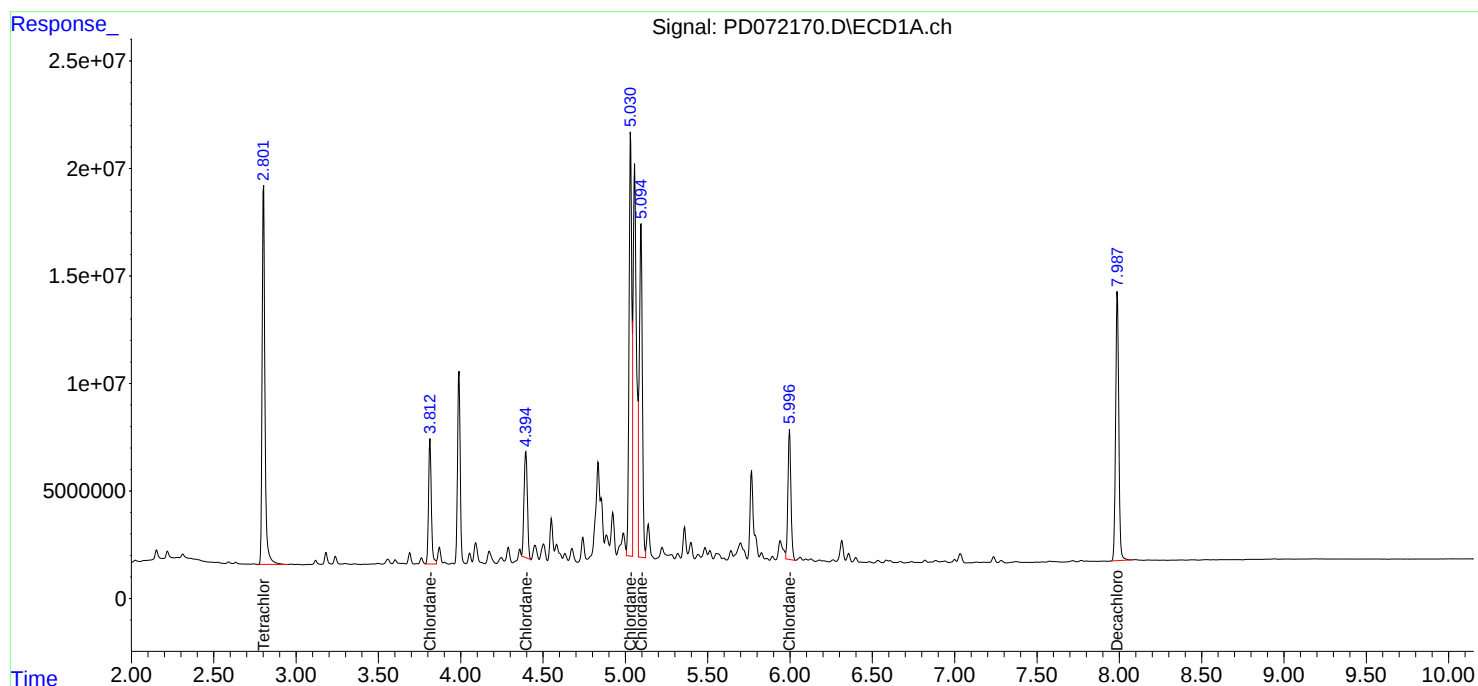


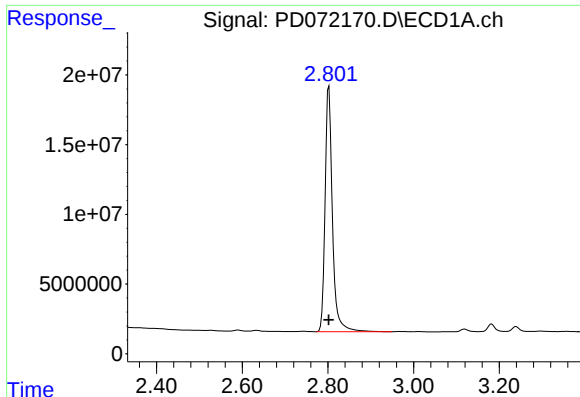

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 211467318
Conc: 72.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

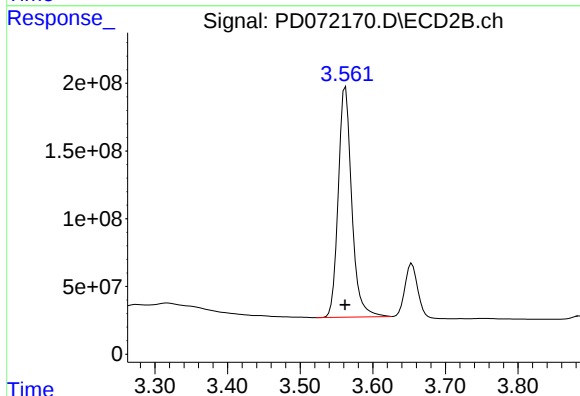


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 2192028745
Conc: 70.07 ng/ml

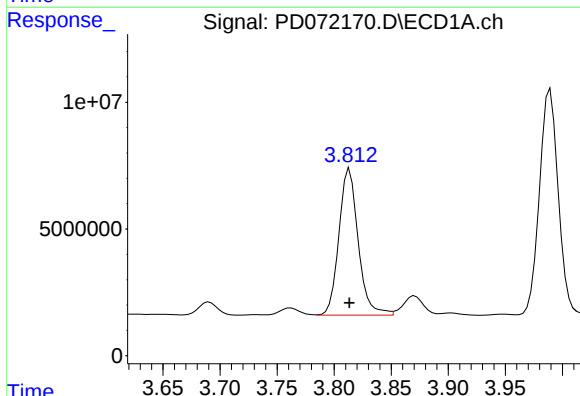


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 68030305
Conc: 714.01 ng/ml

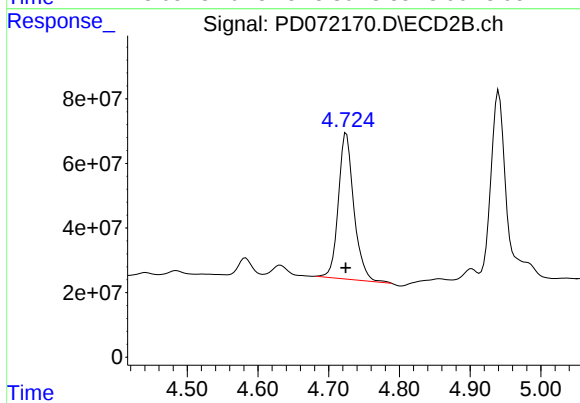

#23 Chlordane-1


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 686385993
Conc: 684.02 ng/ml

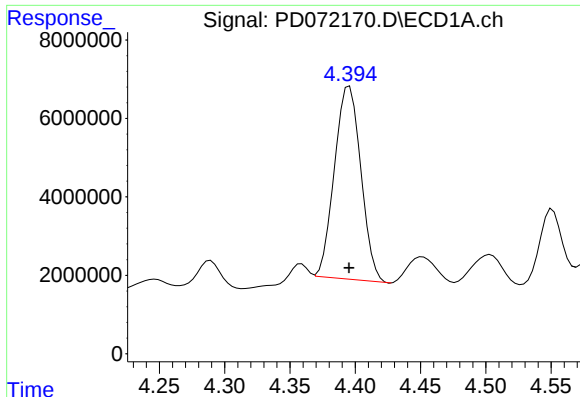

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 69254921
Conc: 700.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

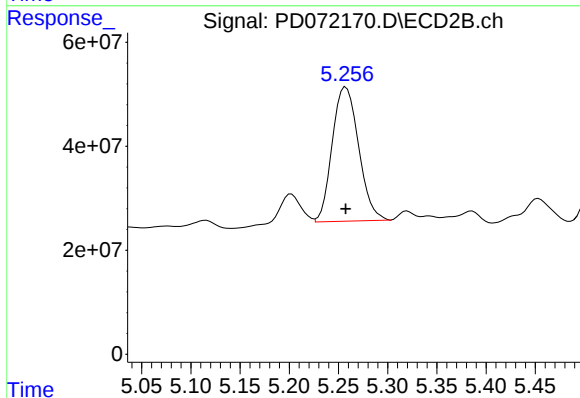


#24 Chlordane-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 481654066
Conc: 686.04 ng/ml

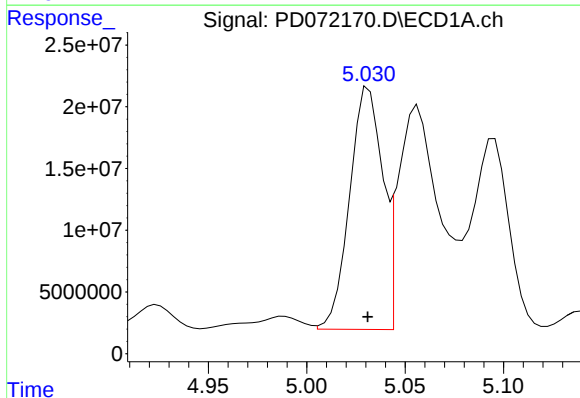


#25 Chlordane-3

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 227630302
Conc: 724.77 ng/ml

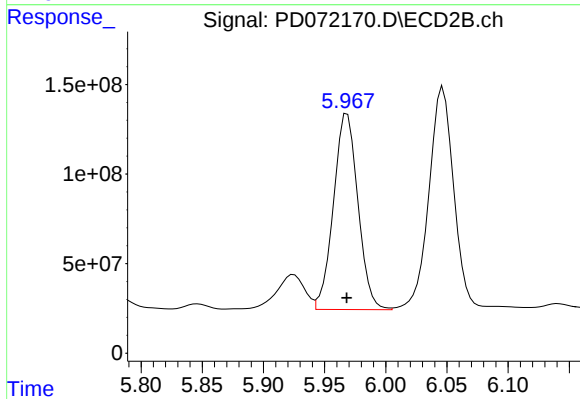

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 1522147003
Conc: 697.94 ng/ml

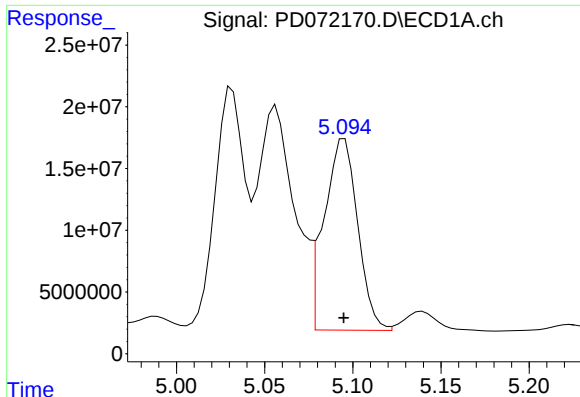

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 205405427
Conc: 709.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

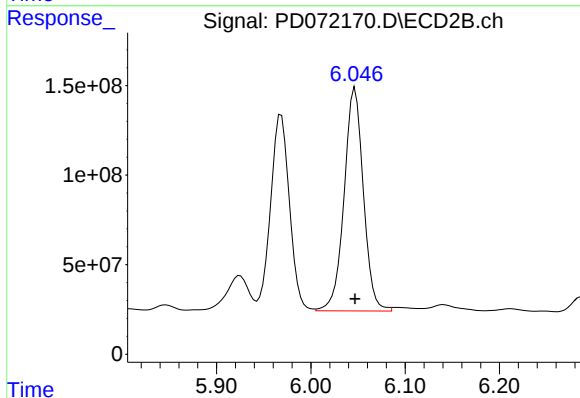


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 1770599654
Conc: 696.88 ng/ml

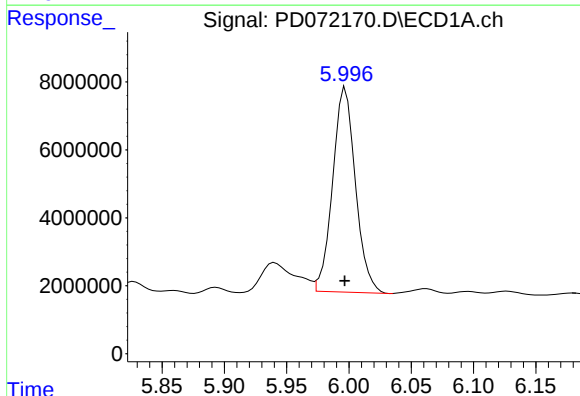


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 76808136
Conc: 711.99 ng/ml

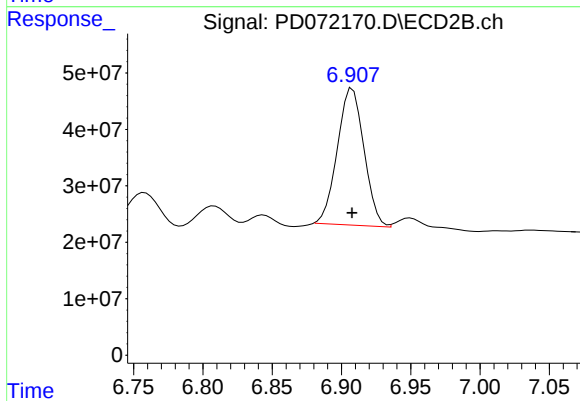

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 324125603
Conc: 702.50 ng/ml

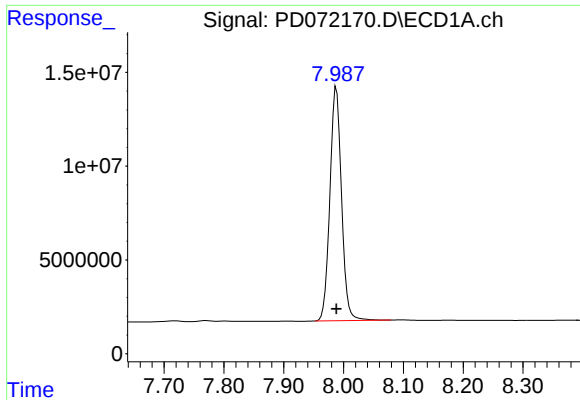

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 168261980
Conc: 70.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

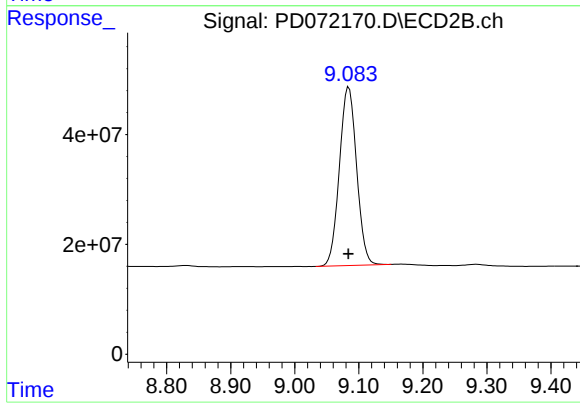

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 606746804
Conc: 69.53 ng/ml