

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 21:34
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD100322

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 04:08:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 04:06:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	148.8E6	1560.2E6	51.450	49.438
28)	SA Decachlor...	7.987	9.084	122.3E6	444.3E6	49.724	49.589
Target Compounds							
23)	Chlordane-1	3.813	4.724	48491517	488.3E6	507.355	494.097
24)	Chlordane-2	4.395	5.257	51099738	344.1E6	497.474	483.170
25)	Chlordane-3	5.031	5.969	160.6E6	1101.2E6	519.645	495.683
26)	Chlordane-4	5.095	6.046	147.8E6	1289.8E6	515.435	494.716
27)	Chlordane-5	5.997	6.908	55199334	235.8E6	511.661	510.173



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 21:34
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD100322

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 04:08:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 04:06:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

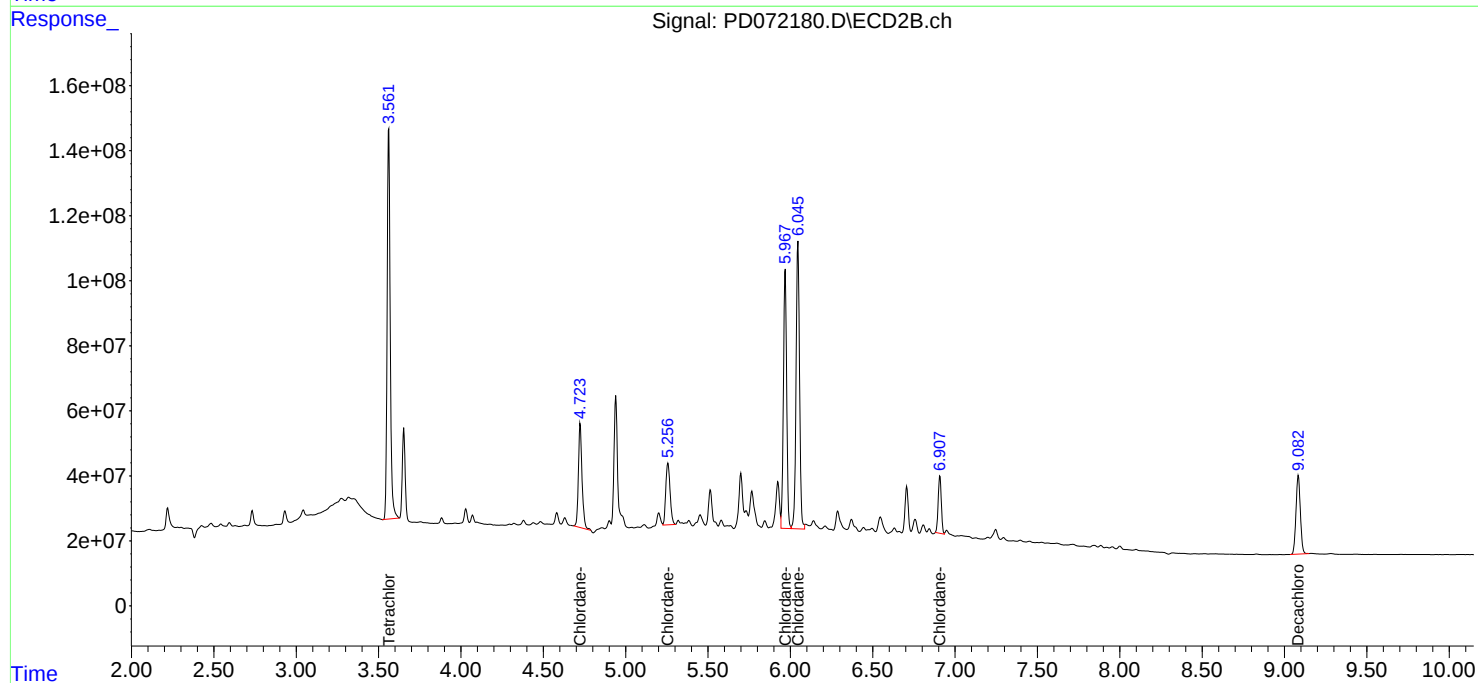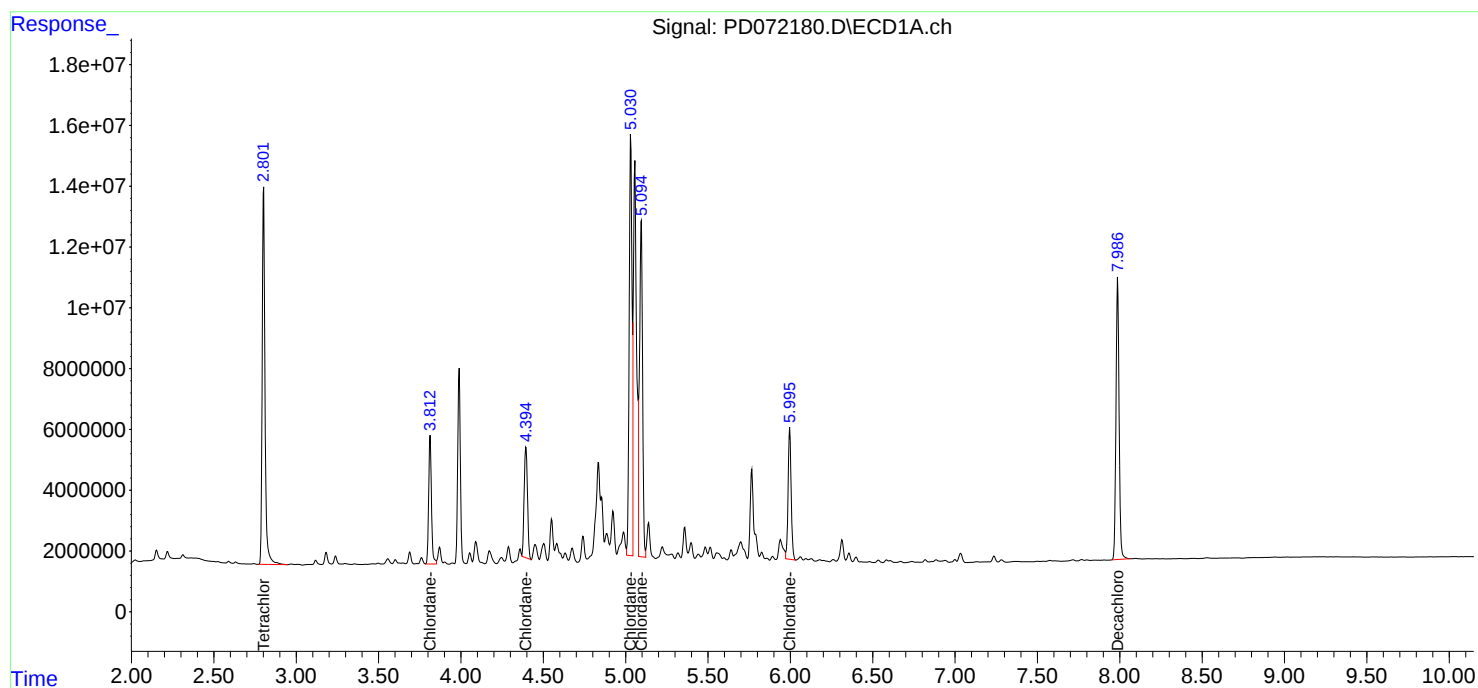


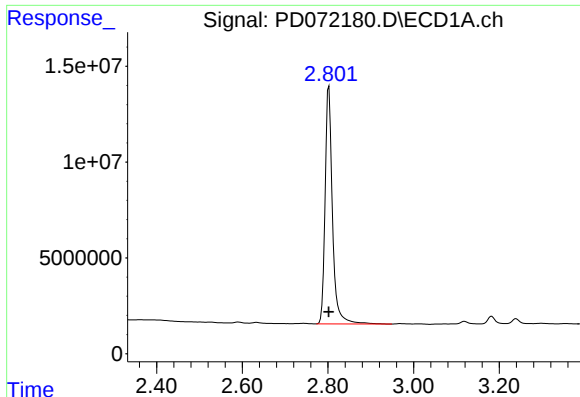

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 148772162
Conc: 51.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100322

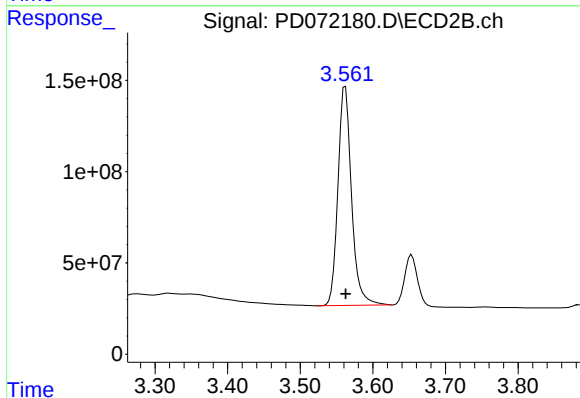


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 1560170442
Conc: 49.44 ng/ml

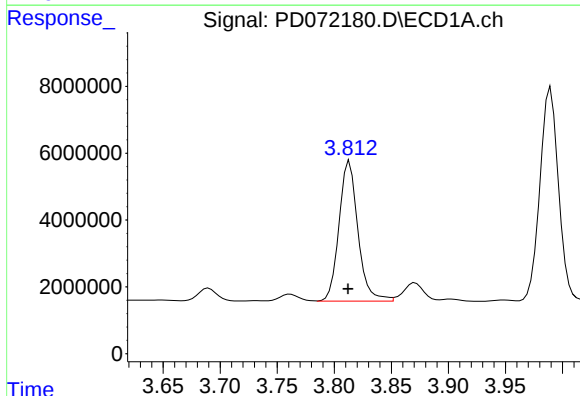


#23 Chlordane-1

R.T.: 3.813 min
Delta R.T.: 0.001 min
Response: 48491517
Conc: 507.35 ng/ml

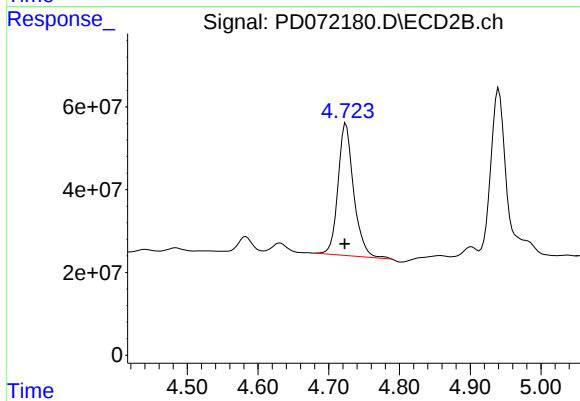

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.002 min
Response: 488272018
Conc: 494.10 ng/ml

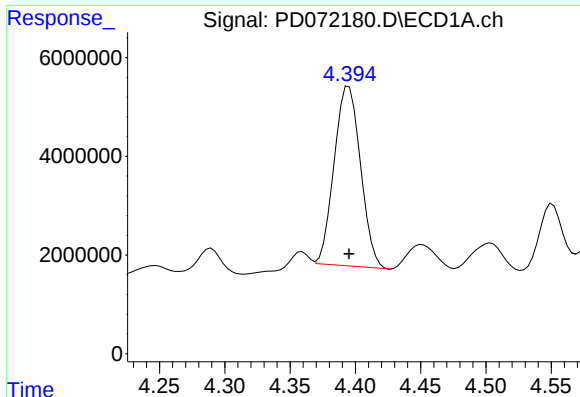

#24 Chlordane-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 51099738
Conc: 497.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100322

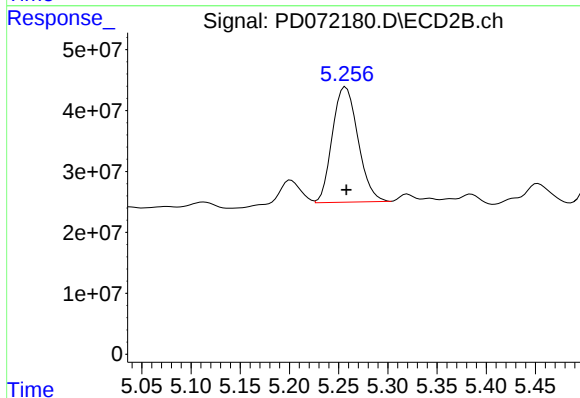


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 344061042
Conc: 483.17 ng/ml

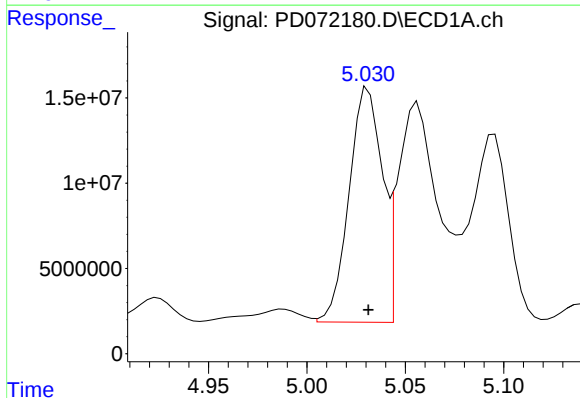


#25 Chlordane-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 160603982
Conc: 519.64 ng/ml

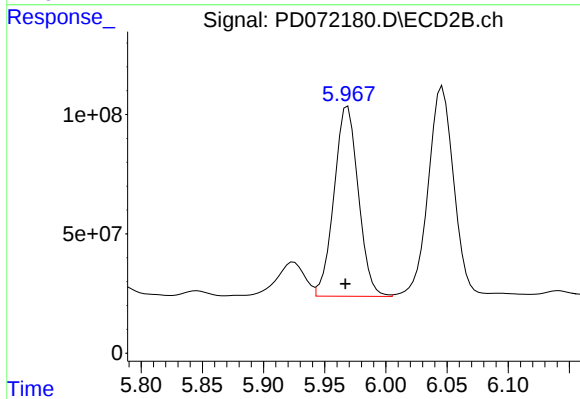

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.002 min
Response: 1101228119
Conc: 495.68 ng/ml

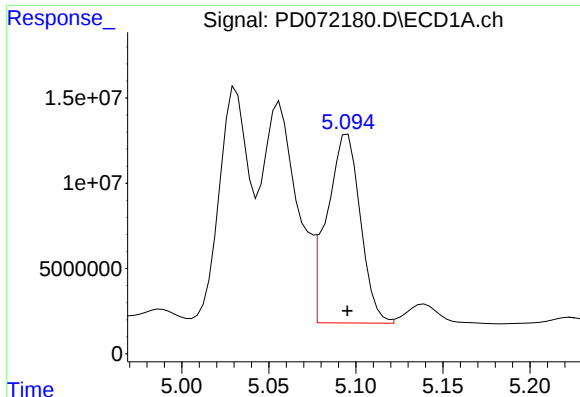

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 147775576
Conc: 515.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100322

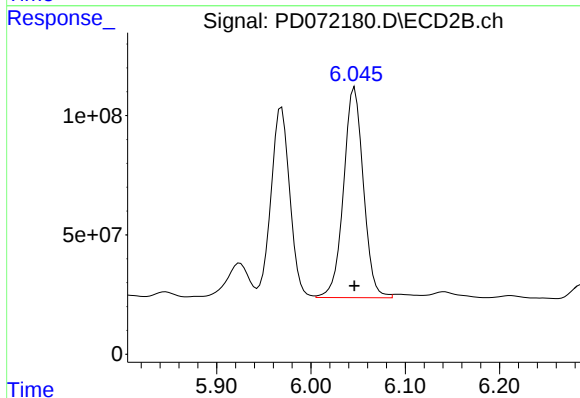


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1289836990
Conc: 494.72 ng/ml

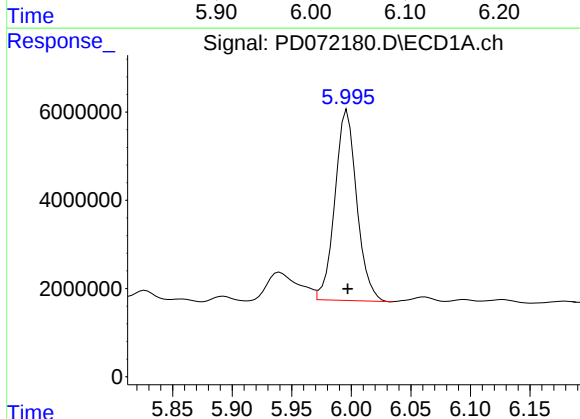


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 55199334
Conc: 511.66 ng/ml

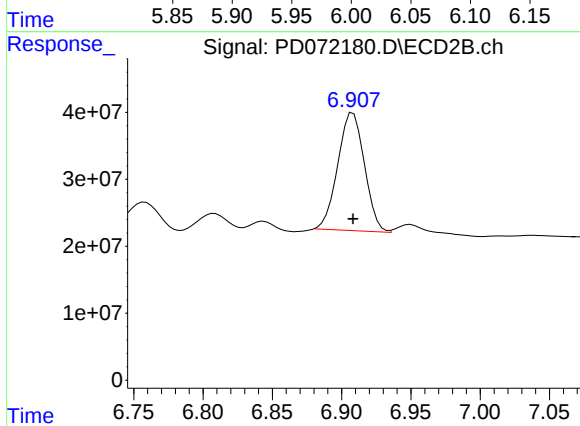

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 235783987
Conc: 510.17 ng/ml

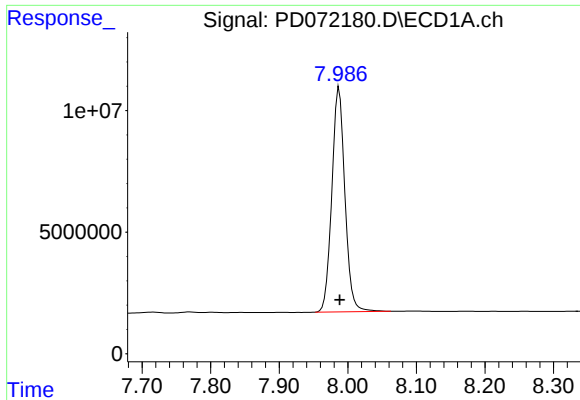

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: 0.000 min
Response: 122289470
Conc: 49.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD100322

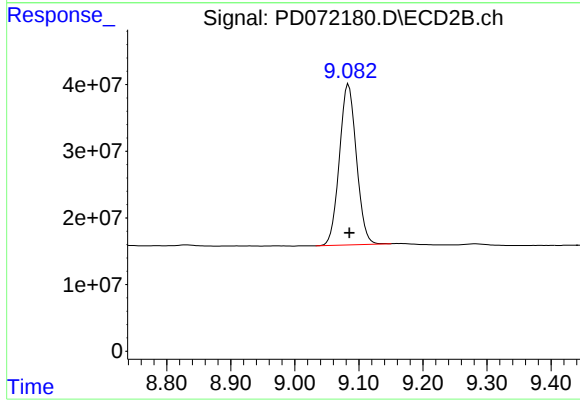

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 444346970
Conc: 49.59 ng/ml