

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 19:21
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 03:58:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 03:58:47 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	211.5E6	2192.0E6	73.839	73.741
28)	SA Decachlor...	7.988	9.084	168.3E6	606.7E6	73.560	73.648
Target Compounds							
23)	Chlordane-1	3.814	4.725	68030305	686.4E6	736.652	735.521
24)	Chlordane-2	4.396	5.258	69254921	481.7E6	739.311	737.657
25)	Chlordane-3	5.032	5.969	227.6E6	1522.1E6	740.348	735.327
26)	Chlordane-4	5.095	6.047	205.4E6	1770.6E6	731.127	730.961
27)	Chlordane-5	5.997	6.908	76808136	324.1E6	735.532	740.446



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 19:21
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 03:58:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 03:58:47 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

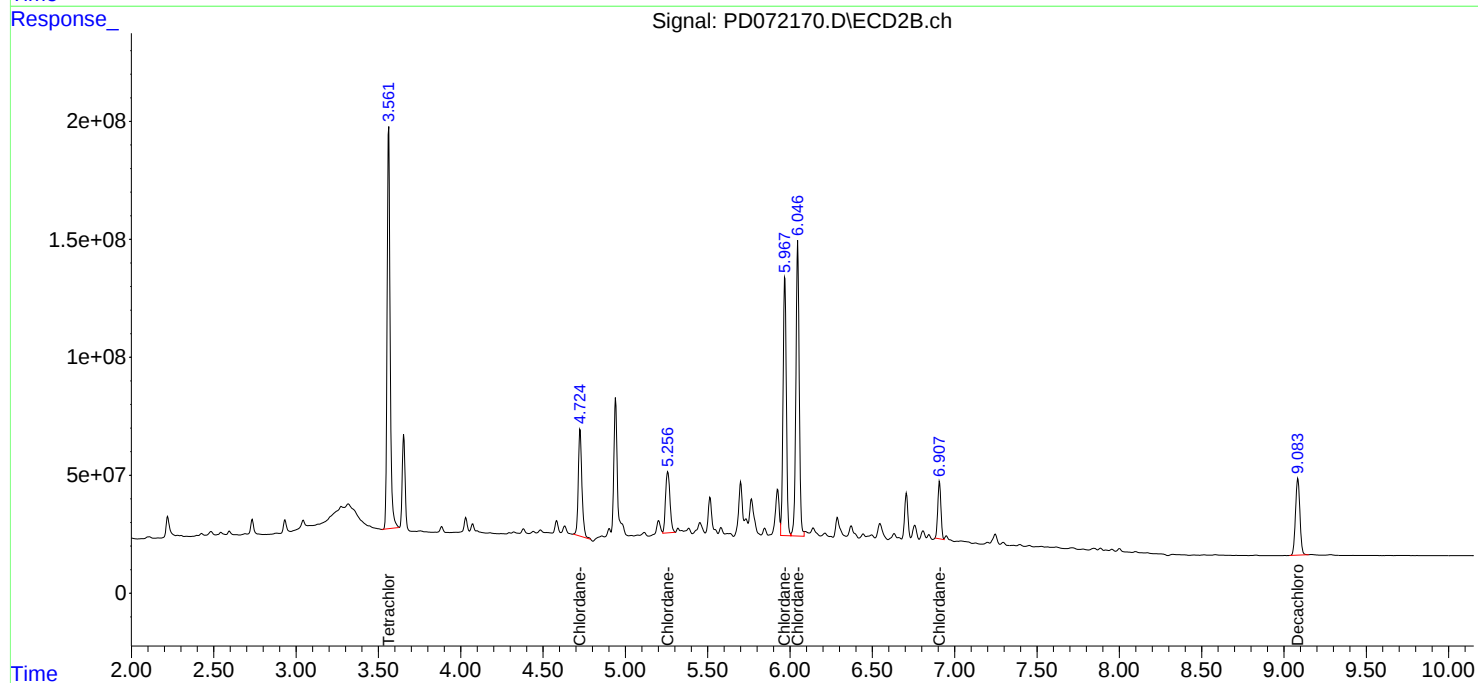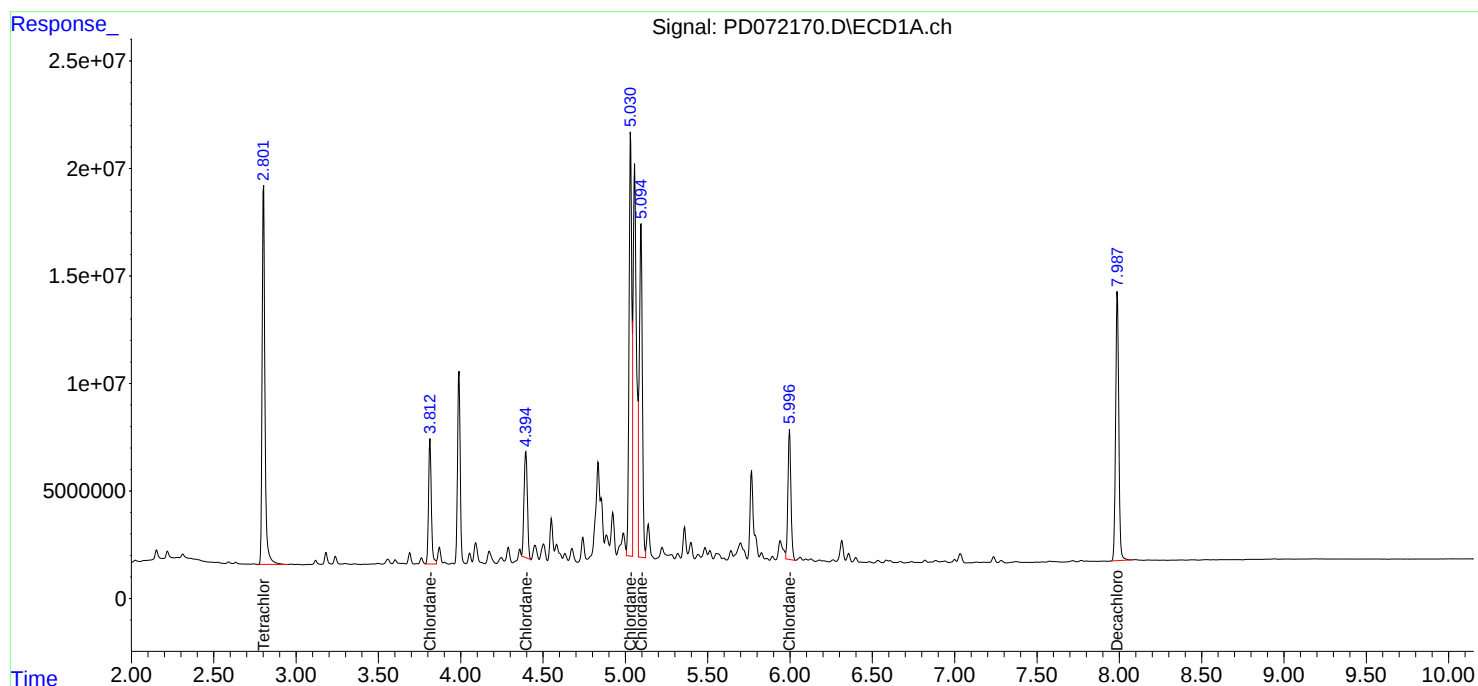


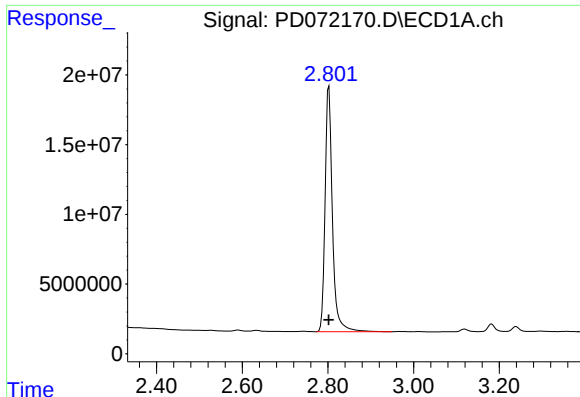

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 211467318
Conc: 73.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

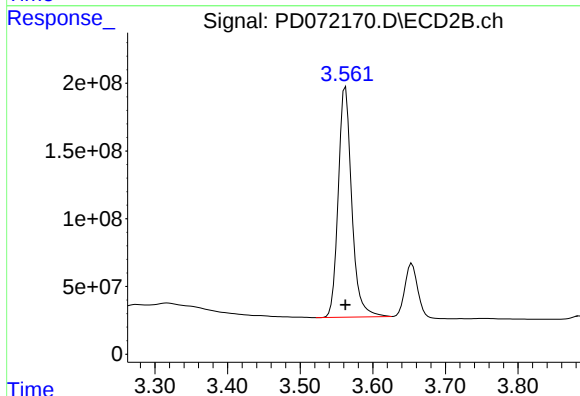


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 2192028745
Conc: 73.74 ng/ml

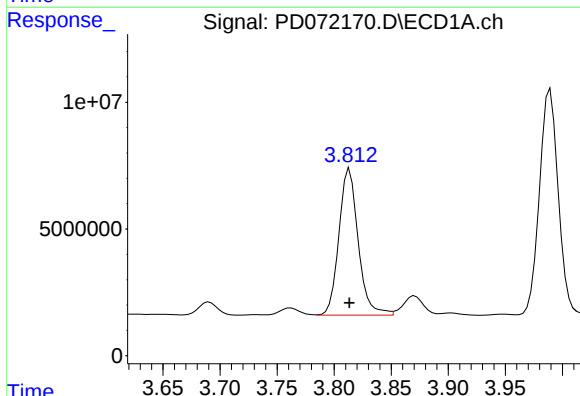


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 68030305
Conc: 736.65 ng/ml

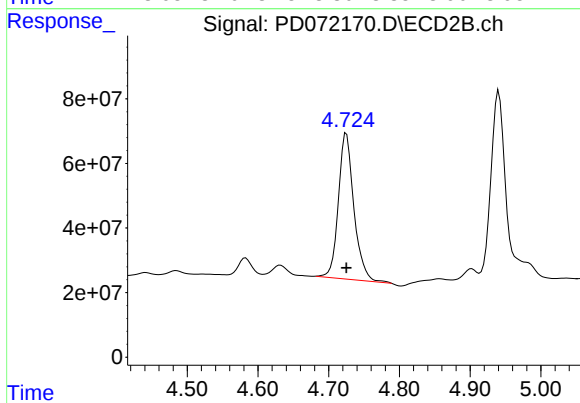

#23 Chlordane-1


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 686385993
Conc: 735.52 ng/ml

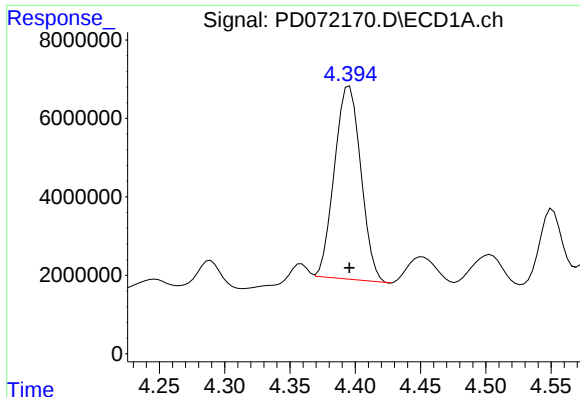

#24 Chlordane-2


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 69254921
Conc: 739.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

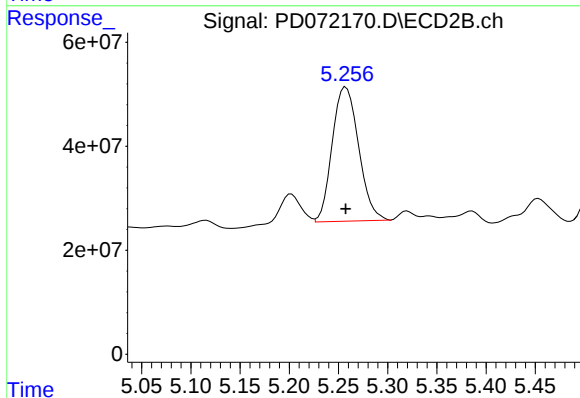


#24 Chlordane-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 481654066
Conc: 737.66 ng/ml

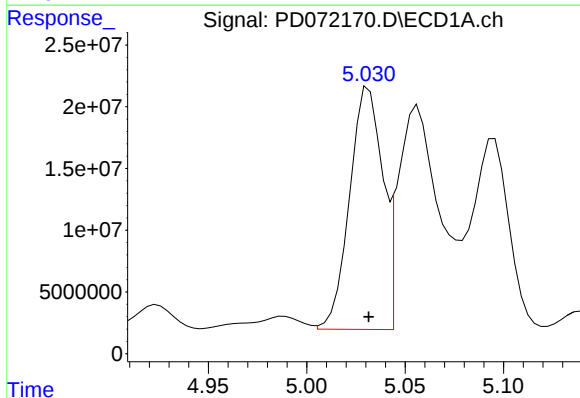


#25 Chlordane-3

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 227630302
Conc: 740.35 ng/ml

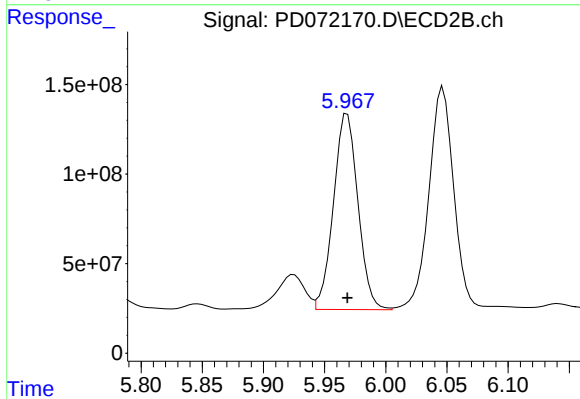

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 1522147003
Conc: 735.33 ng/ml

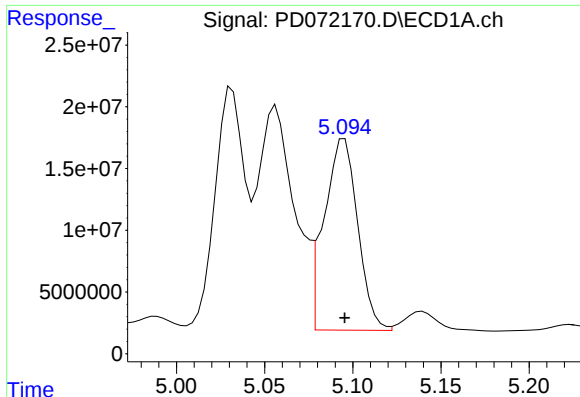

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 205405427
Conc: 731.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

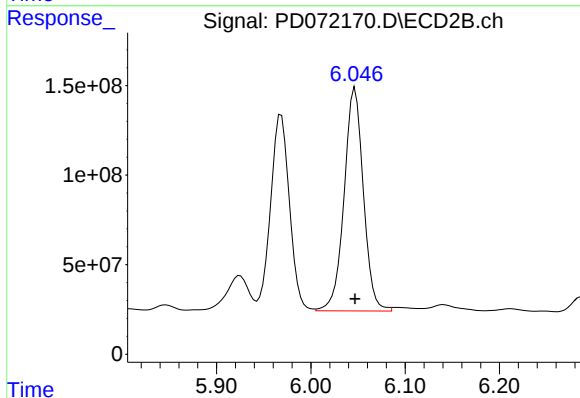


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 1770599654
Conc: 730.96 ng/ml

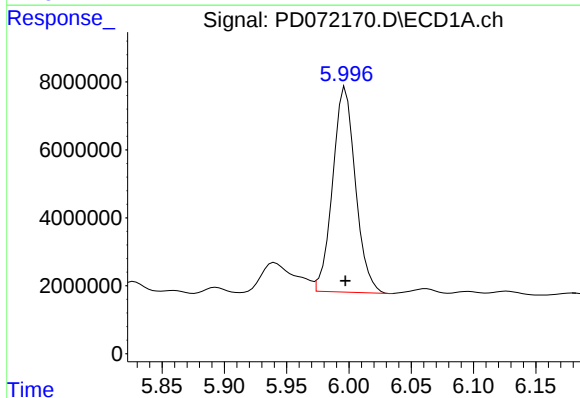


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 76808136
Conc: 735.53 ng/ml

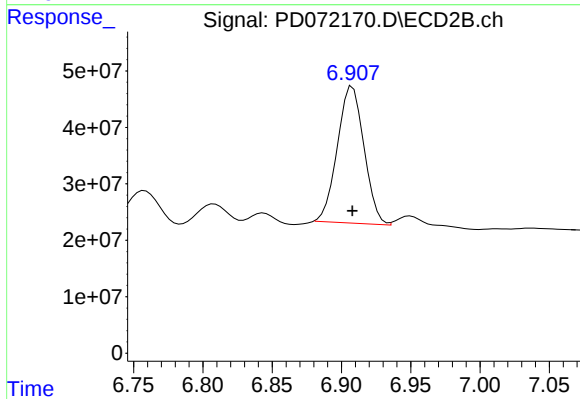

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 324125603
Conc: 740.45 ng/ml

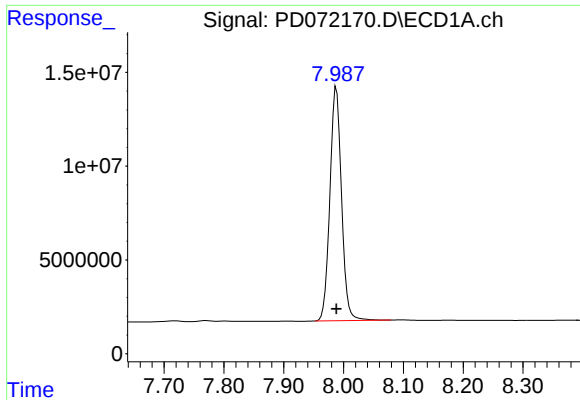

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 168261980
Conc: 73.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

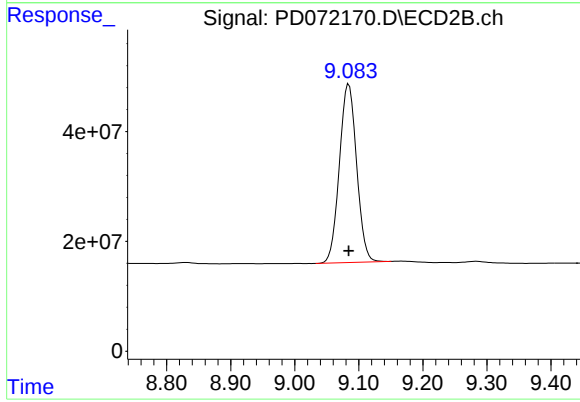

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 606746804
Conc: 73.65 ng/ml