

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 19:47
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 04:01:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 04:00:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	71765453	810.6E6	25.044	26.665
28)	SA Decachlor...	7.988	9.084	62048643	229.8E6	26.561	27.111
Target Compounds							
23)	Chlordane-1	3.813	4.724	23885117	263.9E6	256.421	273.775
24)	Chlordane-2	4.395	5.257	26248928	182.8E6	271.995	271.812
25)	Chlordane-3	5.031	5.969	75855426	568.0E6	247.527	267.861
26)	Chlordane-4	5.095	6.047	70403555	665.6E6	250.447	268.125
27)	Chlordane-5	5.997	6.908	26687222	119.5E6	254.149	266.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 19:47
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 04:01:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 04:00:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

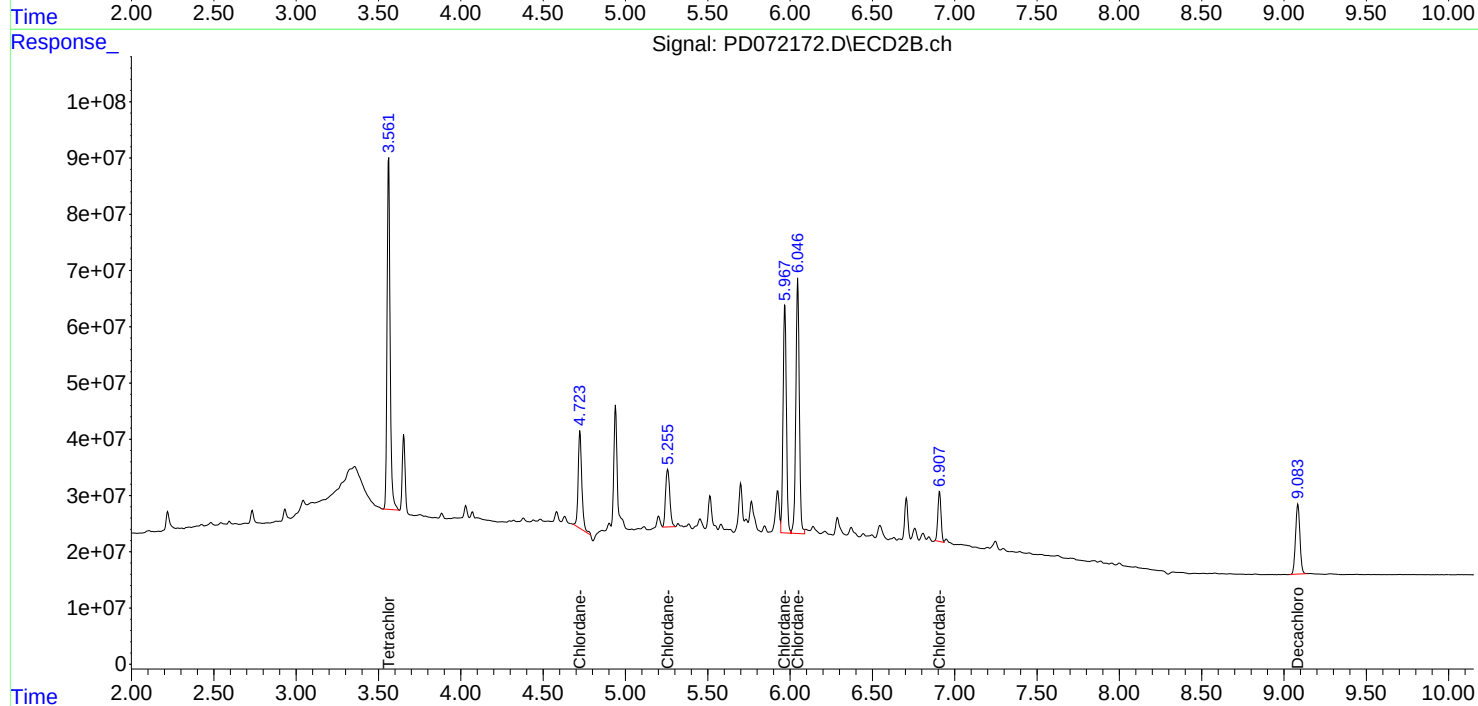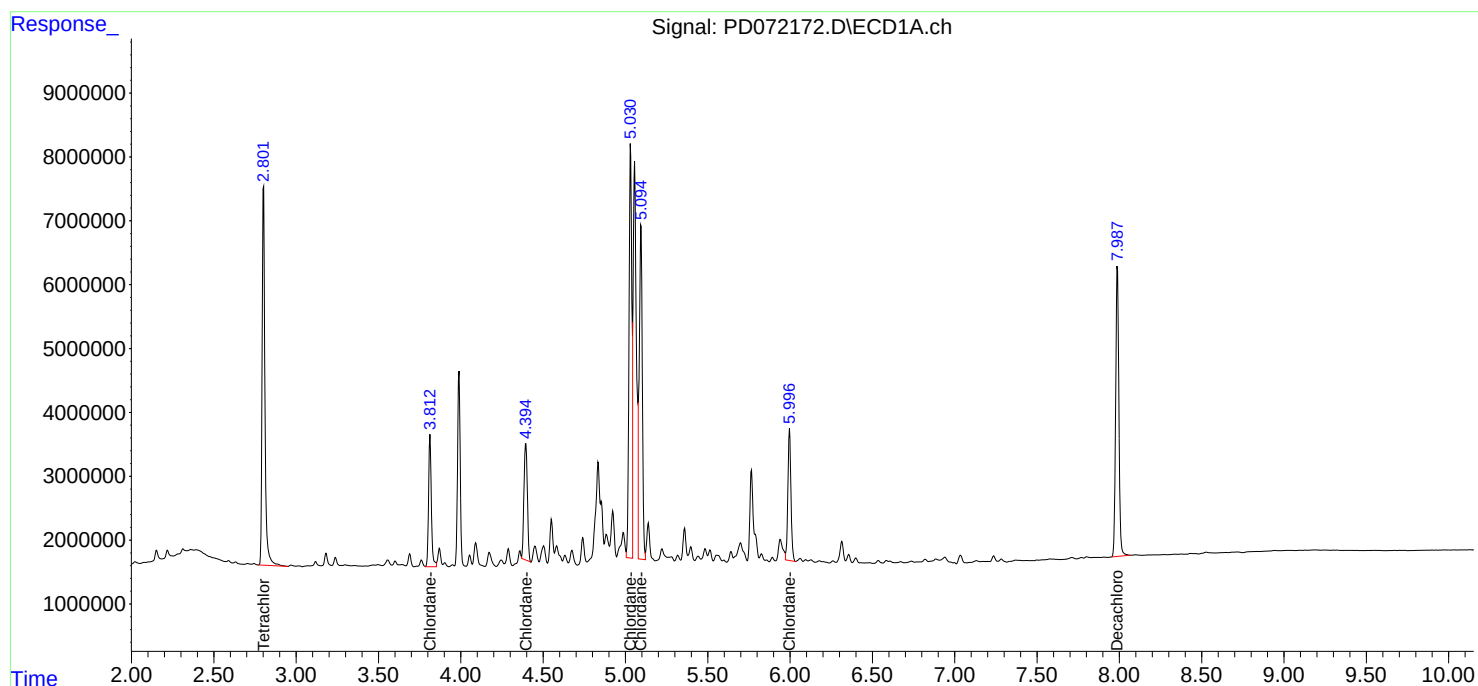


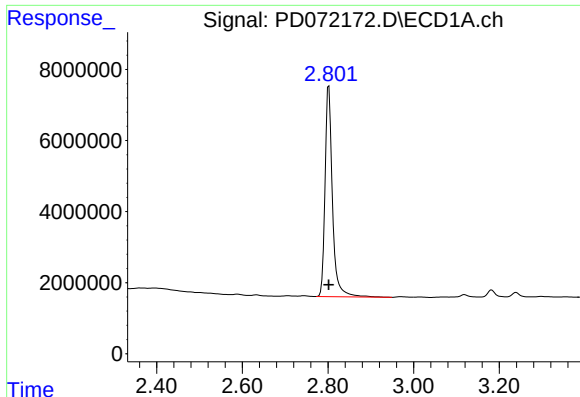

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 71765453
Conc: 25.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

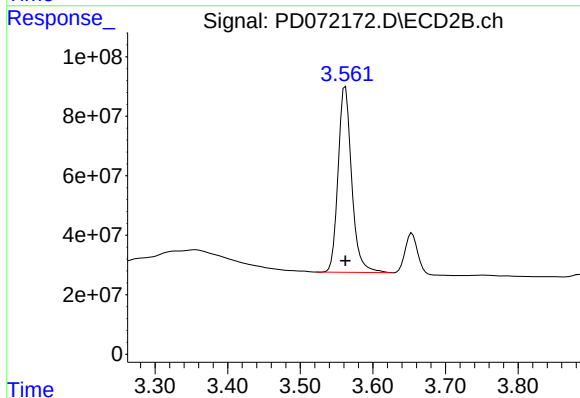


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 810647598
Conc: 26.67 ng/ml

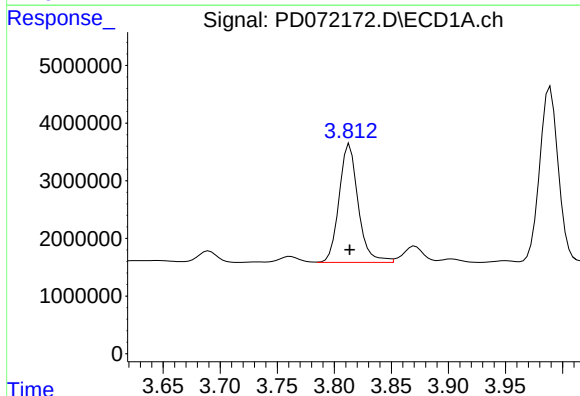


#23 Chlordane-1

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 23885117
Conc: 256.42 ng/ml

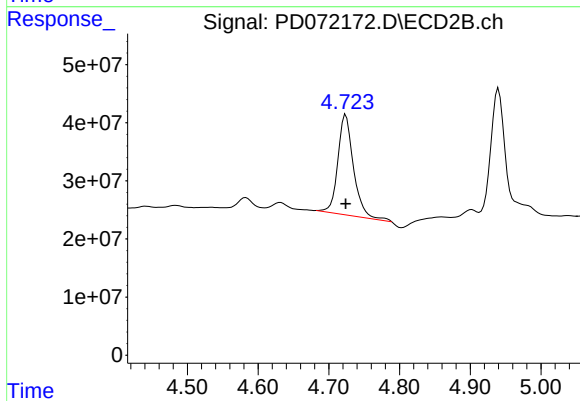

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 263850218
Conc: 273.78 ng/ml

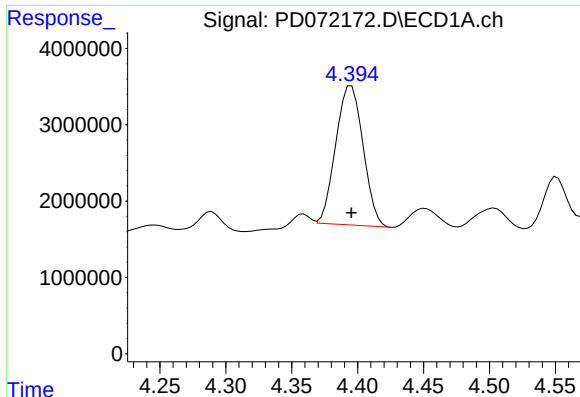

#24 Chlordane-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 26248928
Conc: 272.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

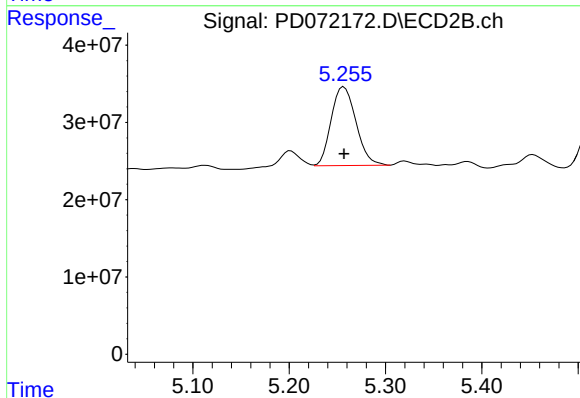


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 182795978
Conc: 271.81 ng/ml

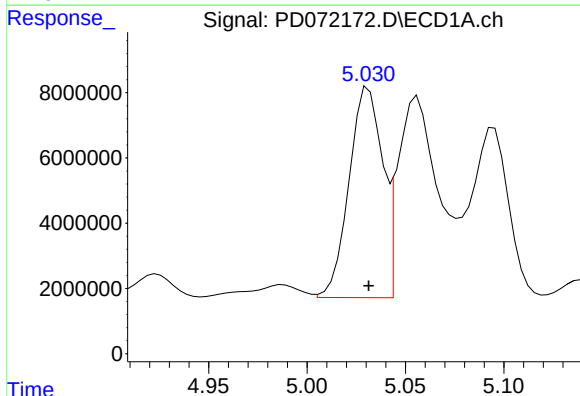


#25 Chlordane-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 75855426
Conc: 247.53 ng/ml

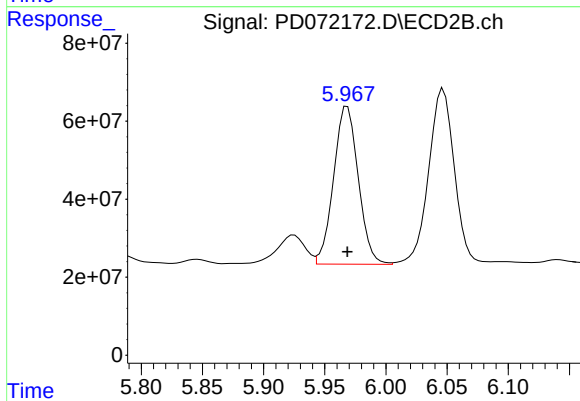

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 568007410
Conc: 267.86 ng/ml

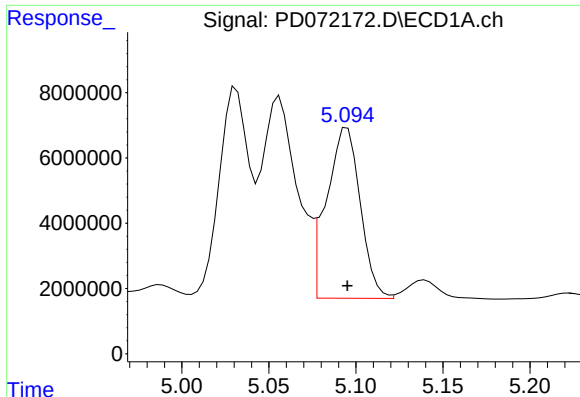

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 70403555
Conc: 250.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

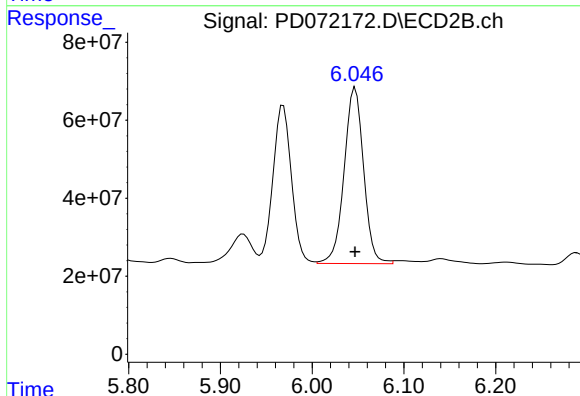


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 665562180
Conc: 268.13 ng/ml

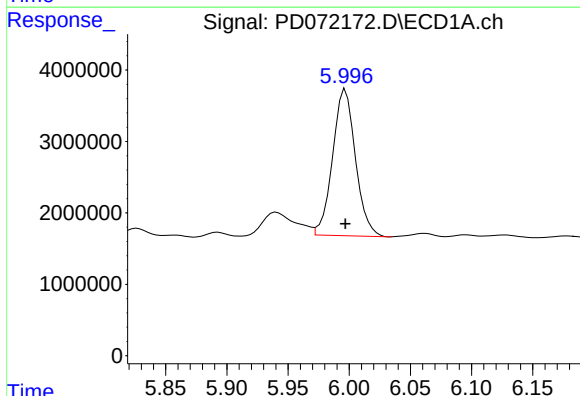


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 26687222
Conc: 254.15 ng/ml

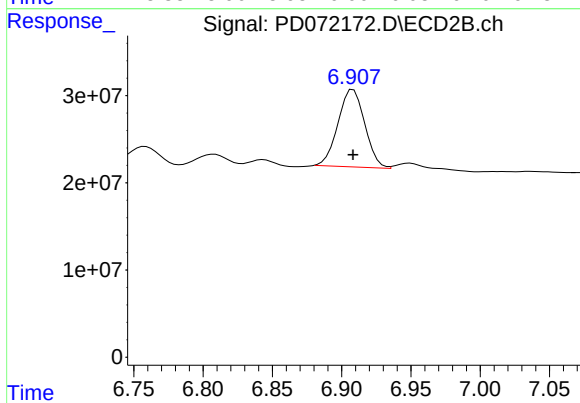

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 119486077
Conc: 266.83 ng/ml

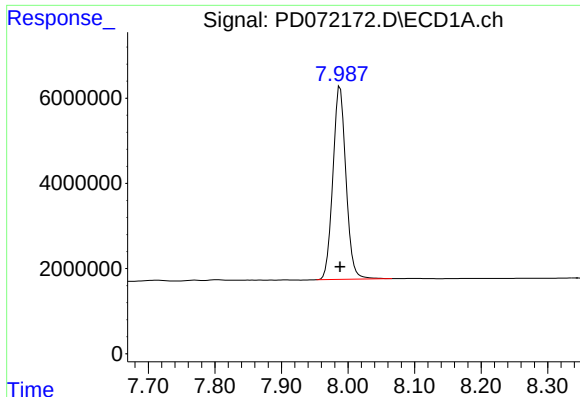

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 62048643
Conc: 26.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

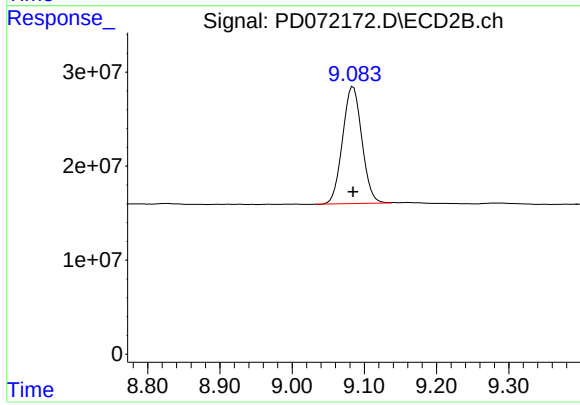

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 229817382
Conc: 27.11 ng/ml