

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 02:15
 Operator : AR\AJ
 Sample : PB147989BS
 Misc : CH BS
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB147989BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:00:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 04:48:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.802	3.562	52250477	604.3E6	21.618	19.170
28)	SA Decachlor...	7.988	9.084	48099273	176.6E6	20.234	20.000
Target Compounds							
23)	Chlordane-1	3.813	4.724	17821354	201.1E6	184.681	199.702
24)	Chlordane-2	4.395	5.257	20075265	147.8E6	195.440	207.553
25)	Chlordane-3	5.031	5.968	56379428	435.0E6	182.419	193.752
26)	Chlordane-4	5.095	6.047	52846197	506.9E6	184.325	192.696
27)	Chlordane-5	5.997	6.908	20124133	88373655	186.537	191.217



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 02:15
Operator : AR\AJ
Sample : PB147989BS
Misc : CH BS
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB147989BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:00:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 04:48:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

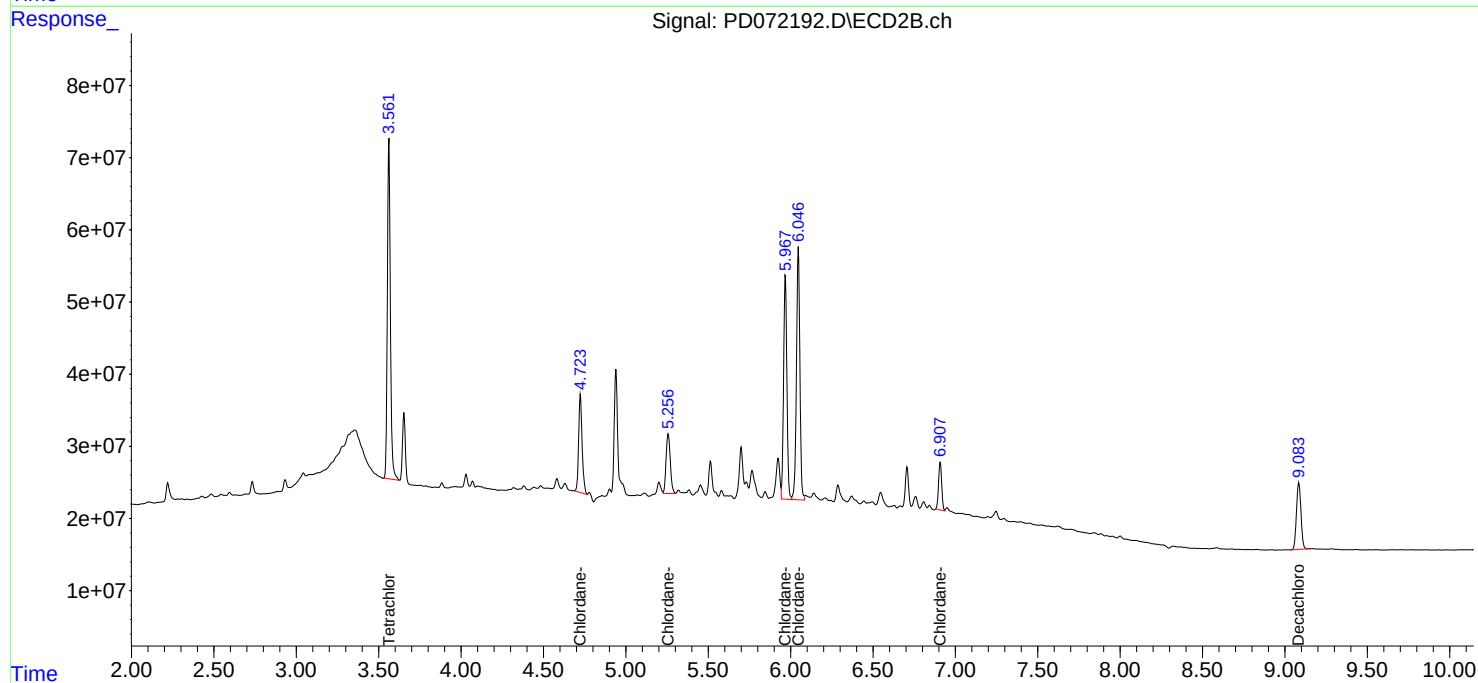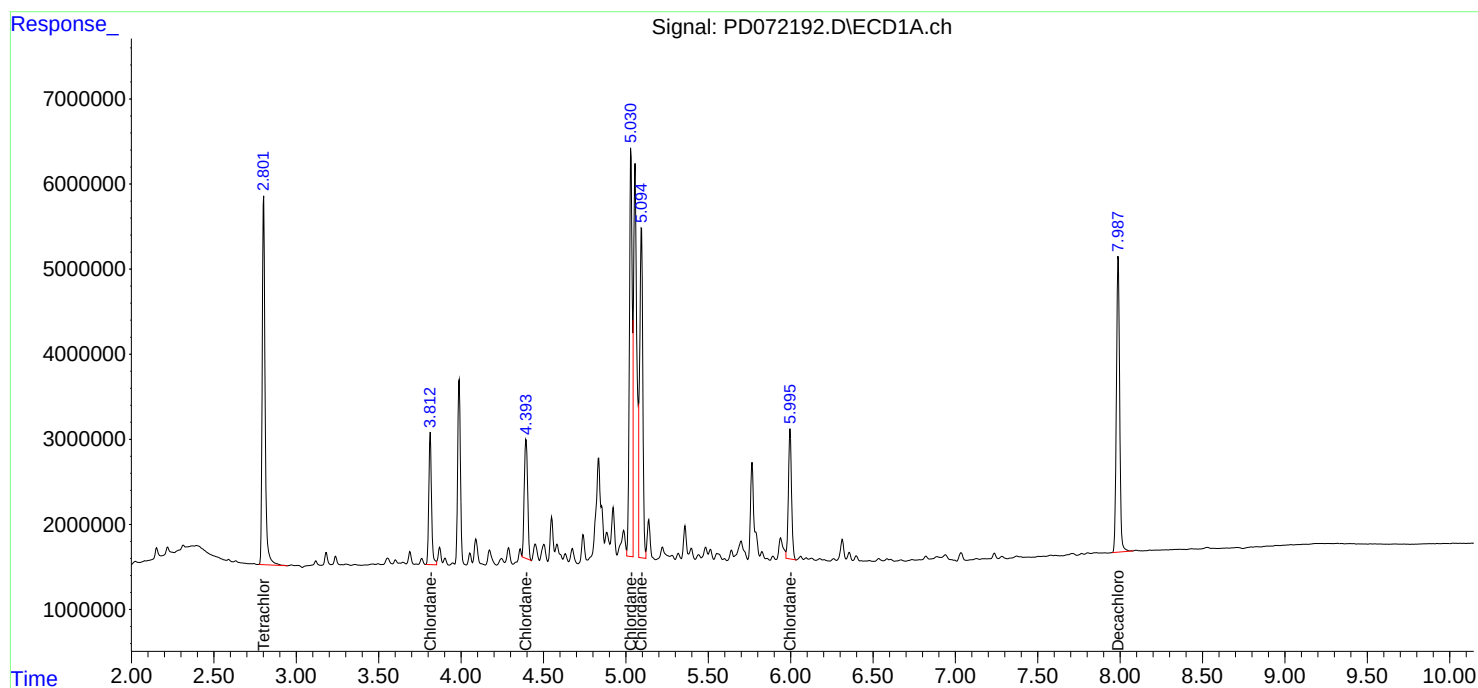


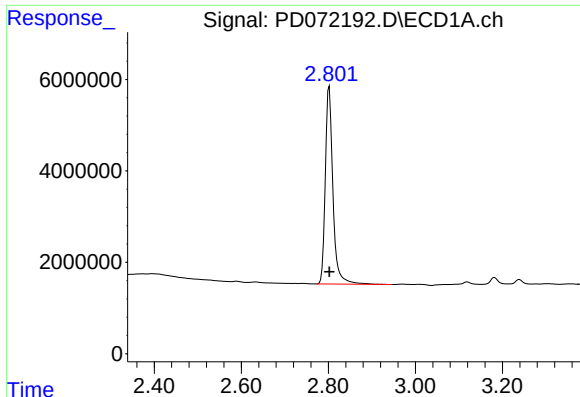

#1 Tetrachloro-m-xylene


R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 52250477
Conc: 21.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147989BS

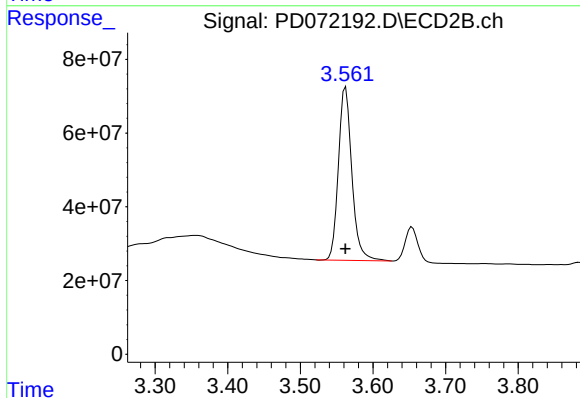


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 604270839
Conc: 19.17 ng/ml

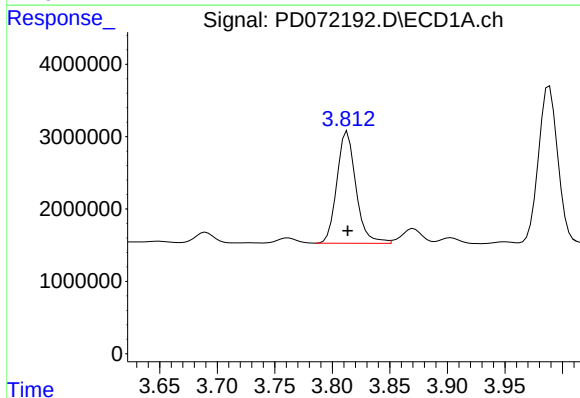


#23 Chlordane-1

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 17821354
Conc: 184.68 ng/ml

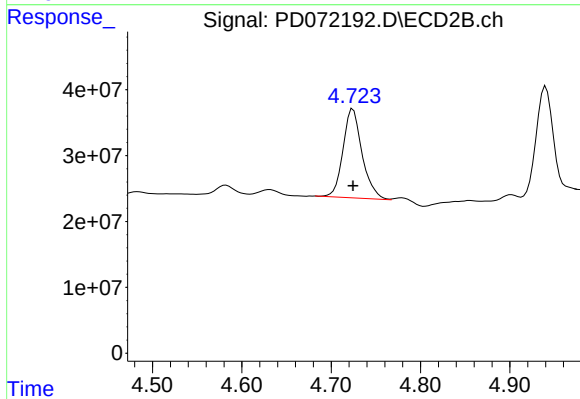

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 201113403
Conc: 199.70 ng/ml

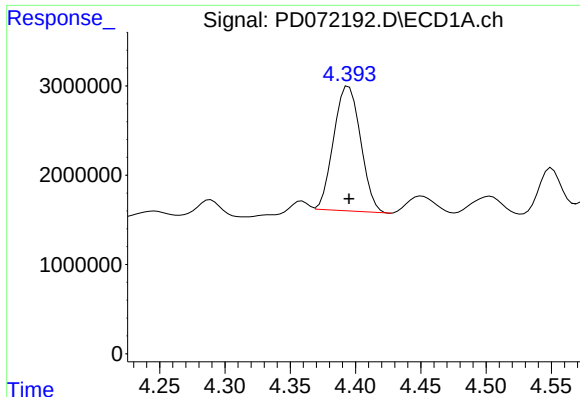

#24 Chlordane-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 20075265
Conc: 195.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147989BS

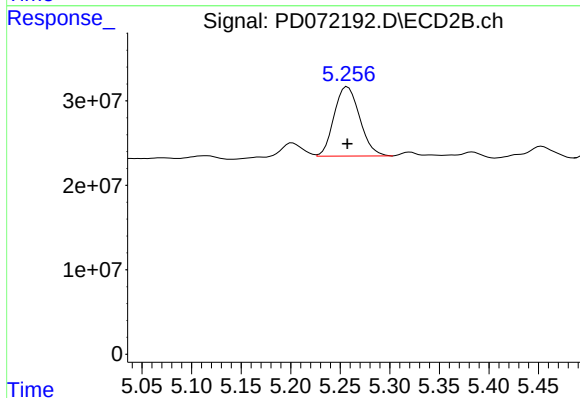


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 147796567
Conc: 207.55 ng/ml

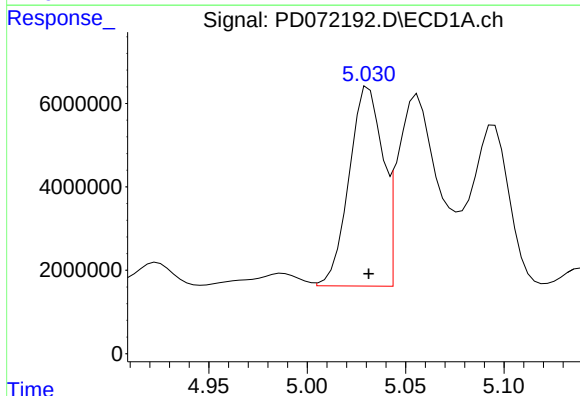


#25 Chlordane-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 56379428
Conc: 182.42 ng/ml

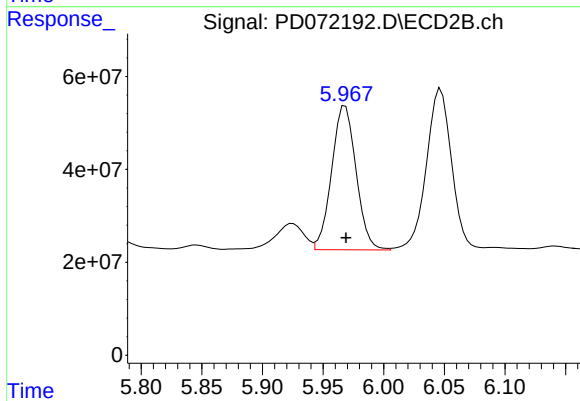

#25 Chlordane-3


R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 434992574
Conc: 193.75 ng/ml

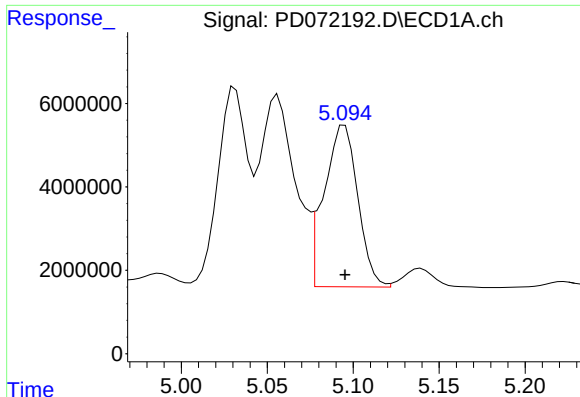

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 52846197
Conc: 184.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147989BS

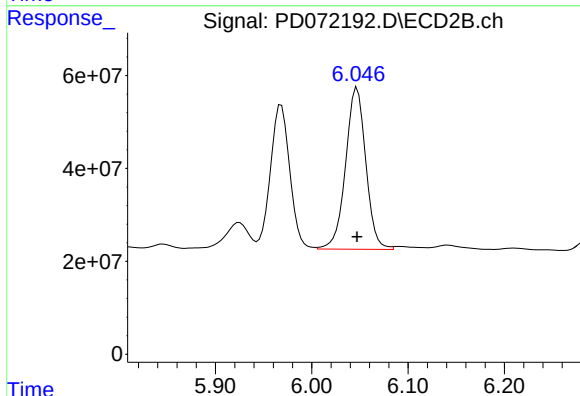


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 506940675
Conc: 192.70 ng/ml

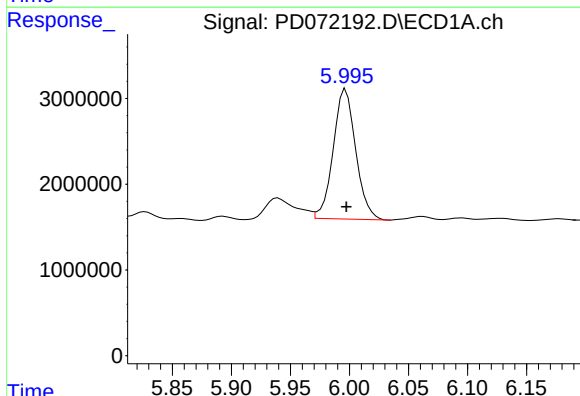


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 20124133
Conc: 186.54 ng/ml

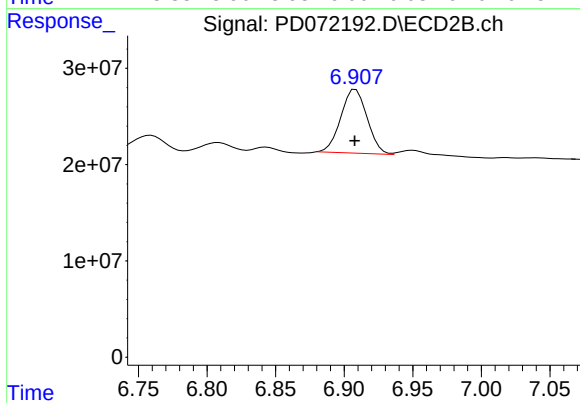

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 88373655
Conc: 191.22 ng/ml

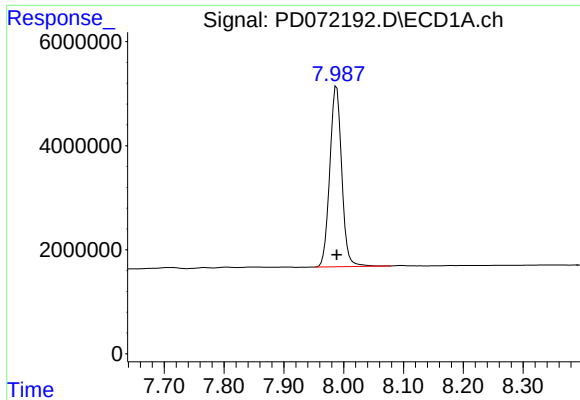

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 48099273
Conc: 20.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB147989BS

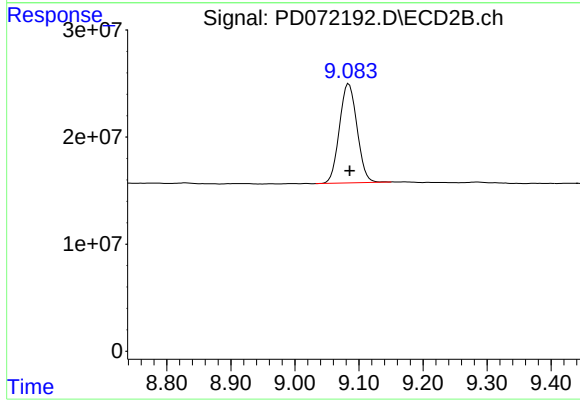

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 176563527
Conc: 20.00 ng/ml