

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 02:28
 Operator : AR\AJ
 Sample : N4785-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:01:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 04:48:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.801	3.562	127.6E6	681.9E6	52.790	21.634 #
28)	SA Decachlor...	7.988	9.085	59576812	200.6E6	25.062	22.722
Target Compounds							
23)	Chlordane-1	3.814	4.725	204.5E6	1860.9E6	2119.285	1847.832
24)	Chlordane-2	4.395	5.258	193.2E6	1244.8E6	1880.592	1748.064
25)	Chlordane-3	5.032	5.969	763.2E6	4251.9E6	2469.250	1893.873
26)	Chlordane-4	5.096	6.047	699.3E6	4809.4E6	2439.046	1828.133 #
27)	Chlordane-5	5.997	6.908	213.8E6	775.5E6	1981.792	1677.923



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 02:28
Operator : AR\AJ
Sample : N4785-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:01:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 04:48:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

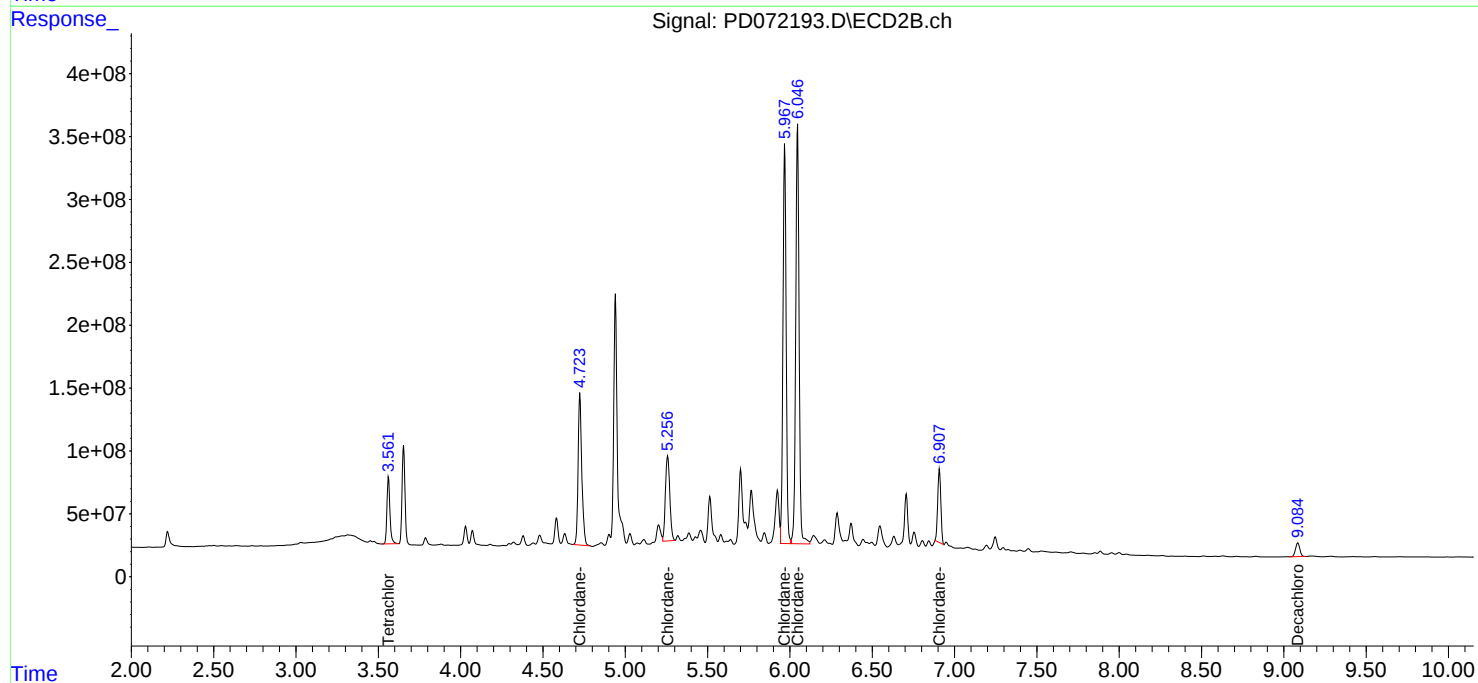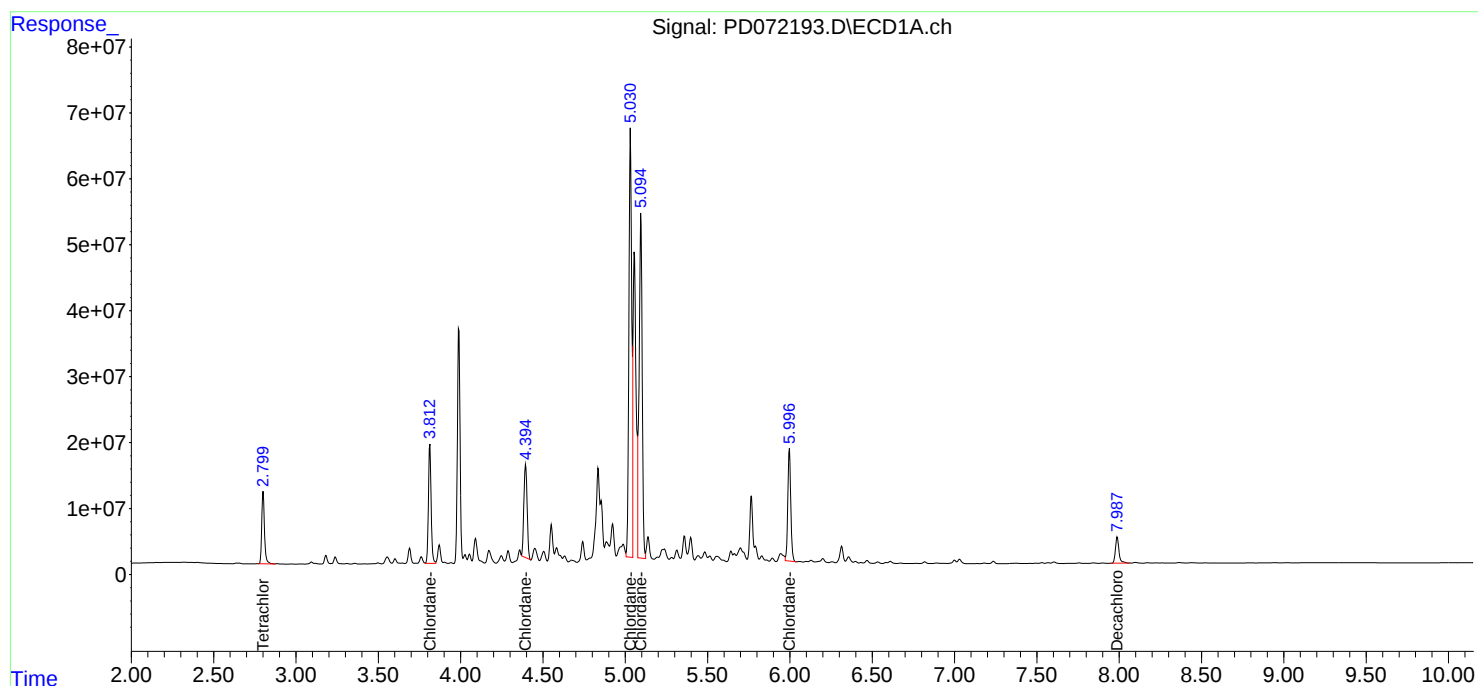


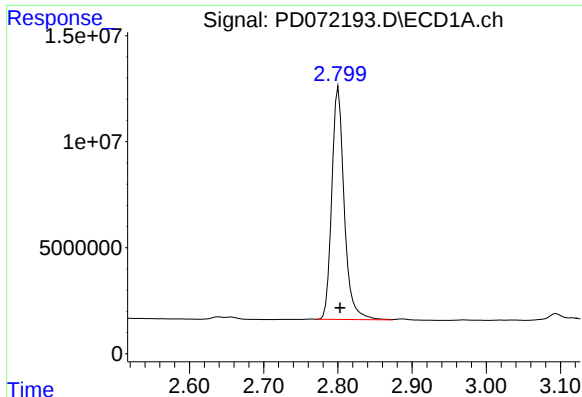

#1 Tetrachloro-m-xylene


R.T.: 2.801 min
Delta R.T.: -0.002 min
Response: 127594170
Conc: 52.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

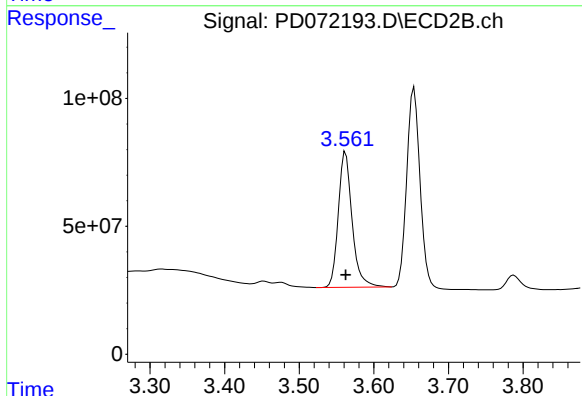


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 681927434
Conc: 21.63 ng/ml

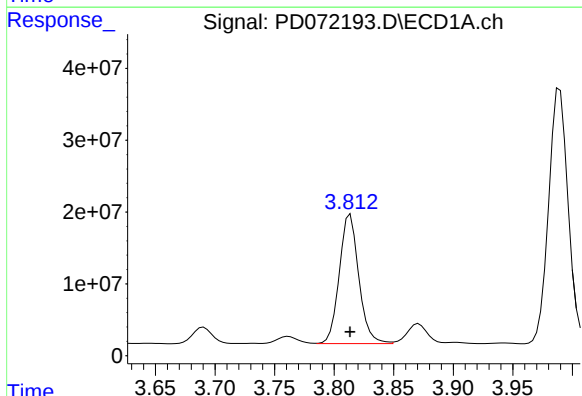


#23 Chlordane-1

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 204506992
Conc: 2119.28 ng/ml

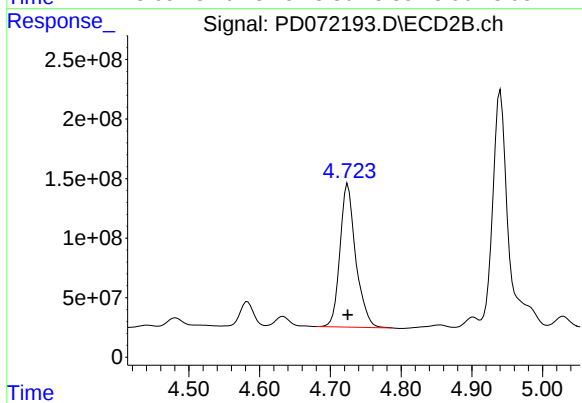

#23 Chlordane-1


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 1860888698
Conc: 1847.83 ng/ml

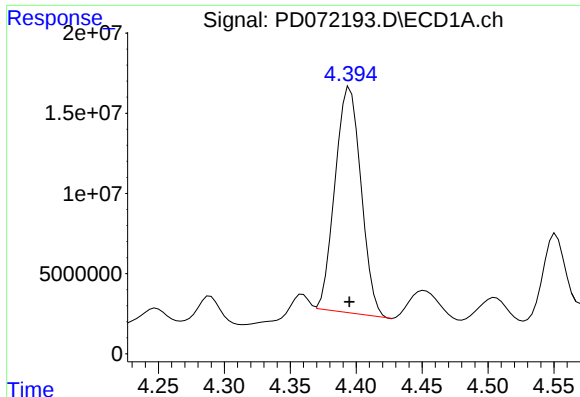

#24 Chlordane-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 193171403
Conc: 1880.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

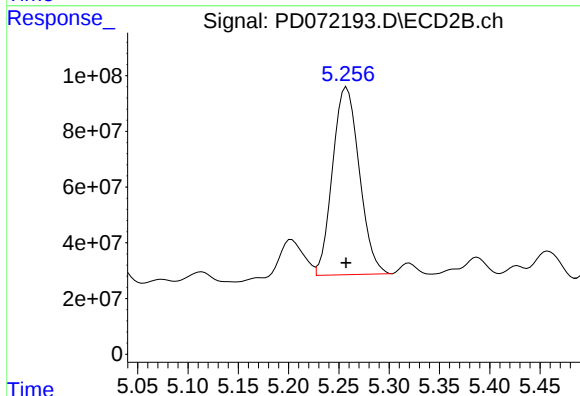


#24 Chlordane-2

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 1244780015
Conc: 1748.06 ng/ml

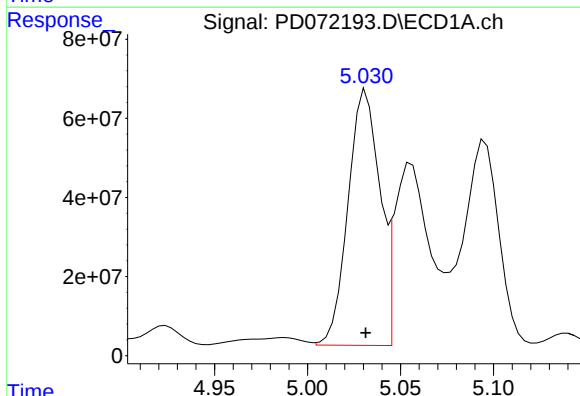


#25 Chlordane-3

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 763158990
Conc: 2469.25 ng/ml

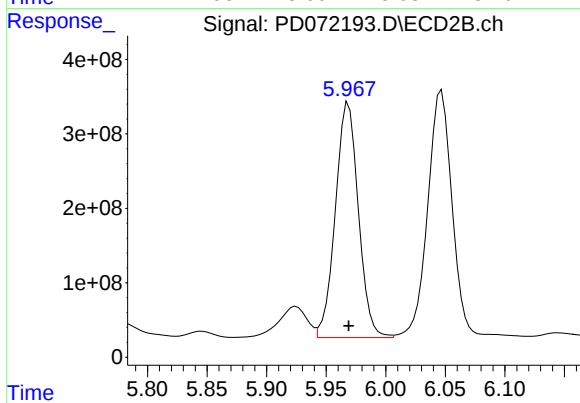

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 4251937103
Conc: 1893.87 ng/ml

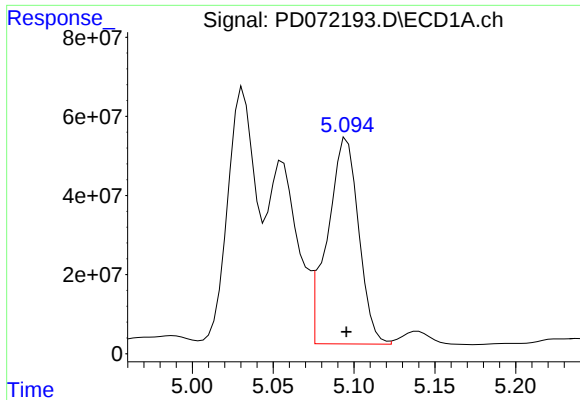

#26 Chlordane-4


R.T.: 5.096 min
Delta R.T.: 0.000 min
Response: 699276723
Conc: 2439.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

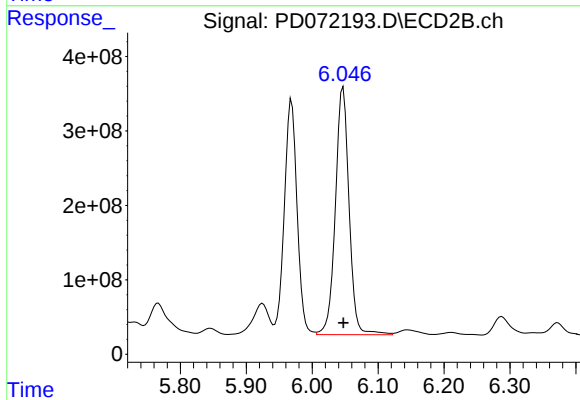


#26 Chlordane-4

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 4809412697
Conc: 1828.13 ng/ml

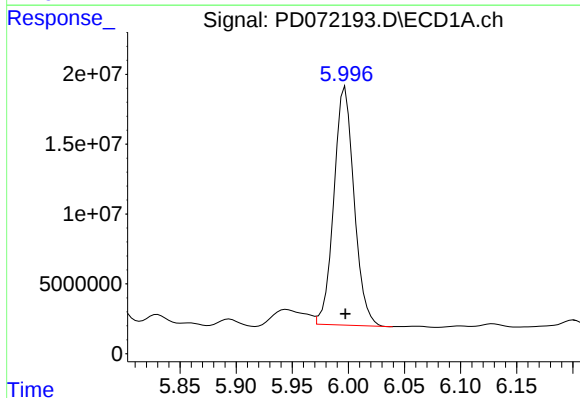


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 213801154
Conc: 1981.79 ng/ml

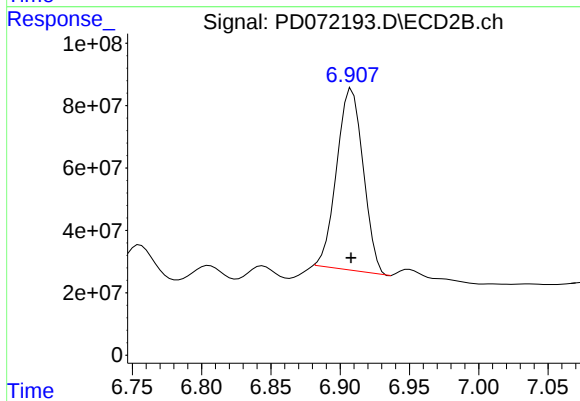

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 775477002
Conc: 1677.92 ng/ml

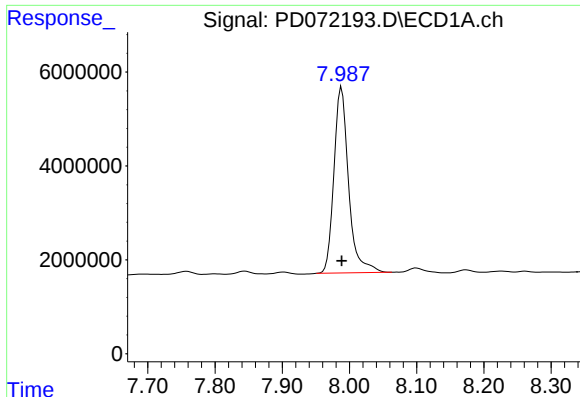

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 59576812
Conc: 25.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WP

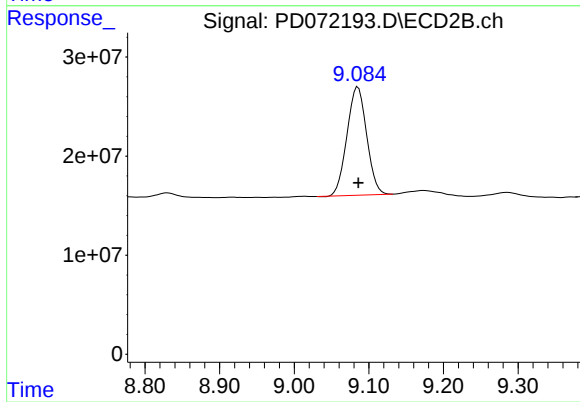

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 200590982
Conc: 22.72 ng/ml