

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
 Data File : PD072194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 02:42
 Operator : AR\AJ
 Sample : N4785-11DL 4X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:01:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 04:48:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.800	3.562	27396957	176.4E6	11.335	5.595 #
28)	SA Decachlor...	7.988	9.085	15592203	52877205	6.559	5.990
Target Compounds							
23)	Chlordane-1	3.813	4.724	45907262	507.7E6	475.732	504.146
24)	Chlordane-2	4.395	5.257	48904622	352.6E6	476.104	495.115
25)	Chlordane-3	5.031	5.968	167.7E6	1056.6E6	542.625	470.645
26)	Chlordane-4	5.095	6.046	151.0E6	1208.6E6	526.789	459.420
27)	Chlordane-5	5.997	6.908	47369800	196.5E6	439.086	425.232


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100322\
Data File : PD072194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 02:42
Operator : AR\AJ
Sample : N4785-11DL 4X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:01:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100322.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 04:48:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

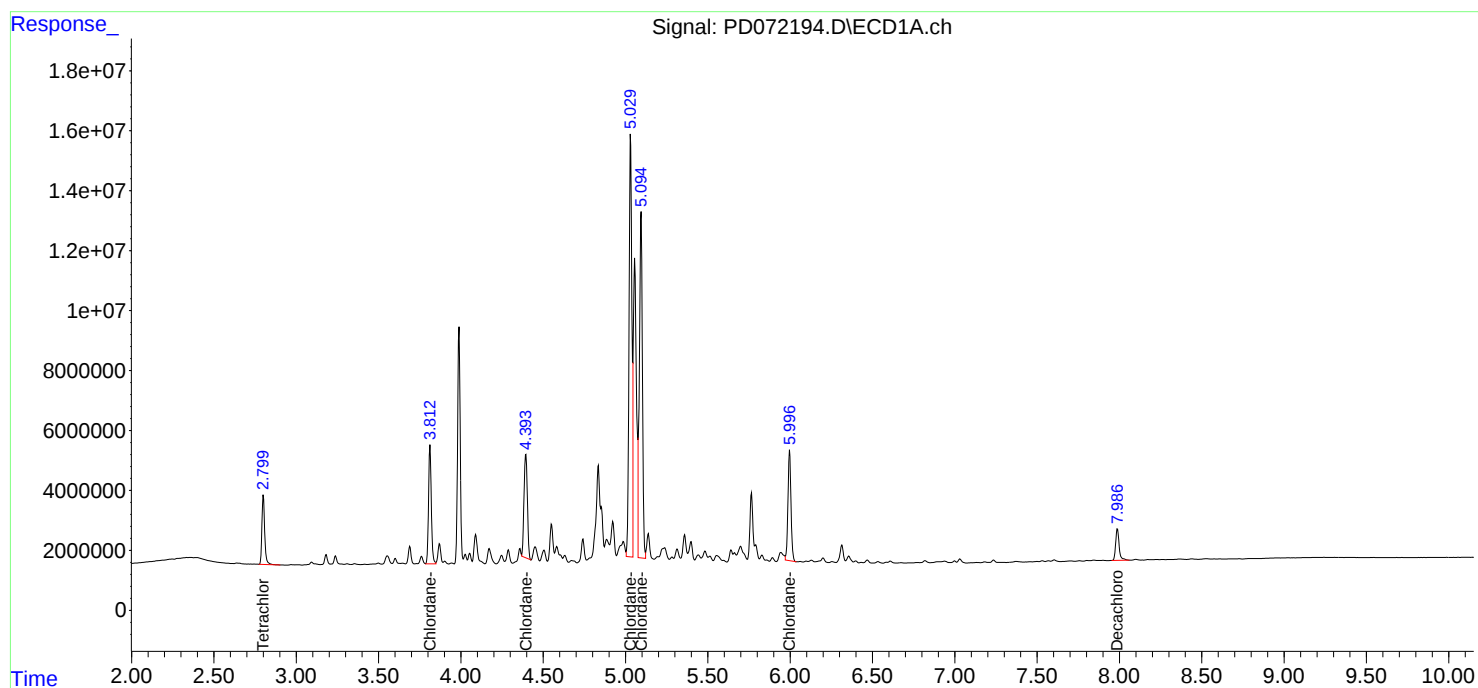


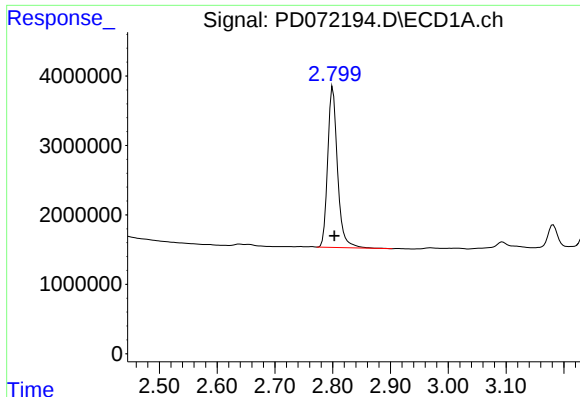

#1 Tetrachloro-m-xylene


R.T.: 2.800 min
Delta R.T.: -0.003 min
Response: 27396957
Conc: 11.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

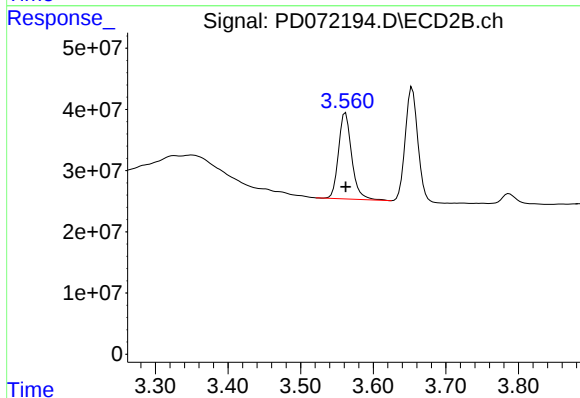


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 176368650
Conc: 5.60 ng/ml

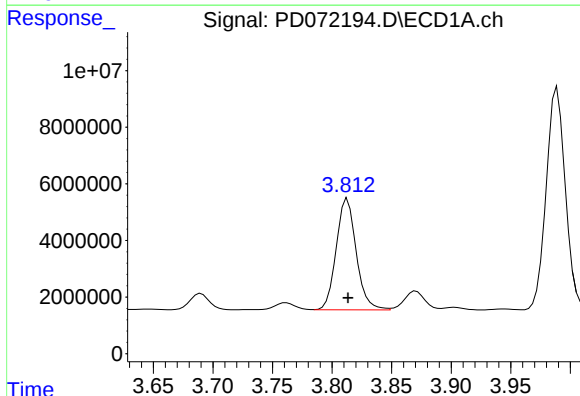


#23 Chlordane-1

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 45907262
Conc: 475.73 ng/ml

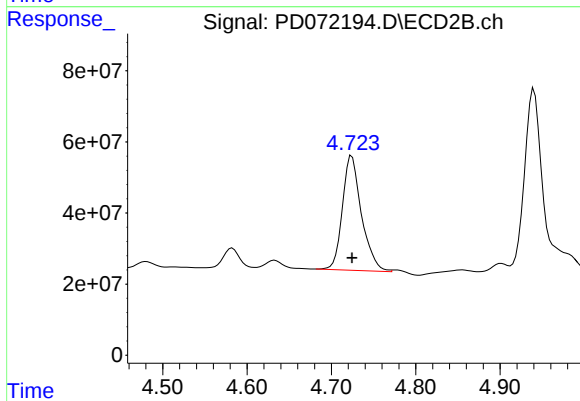

#23 Chlordane-1


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 507708063
Conc: 504.15 ng/ml

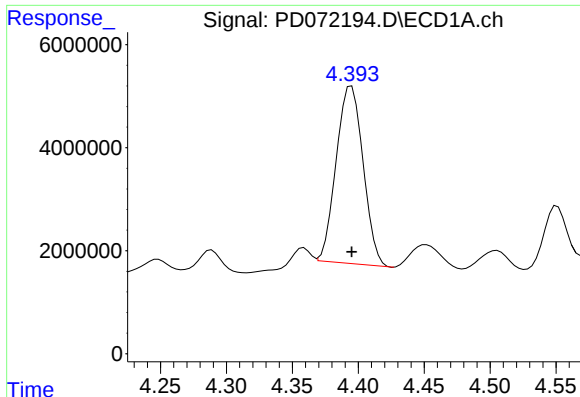

#24 Chlordane-2


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 48904622
Conc: 476.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

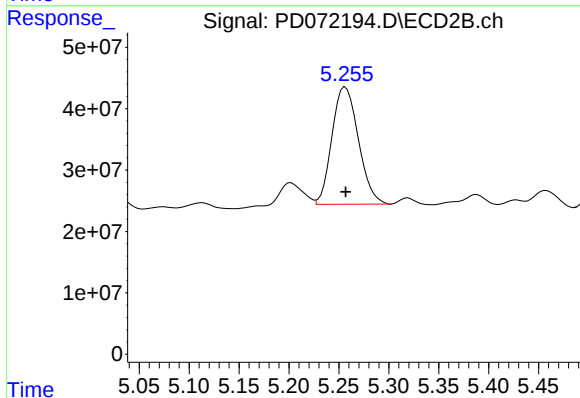


#24 Chlordane-2

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 352567070
Conc: 495.12 ng/ml

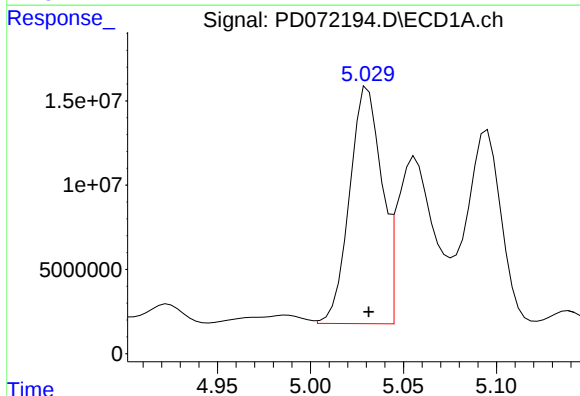


#25 Chlordane-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 167706567
Conc: 542.63 ng/ml

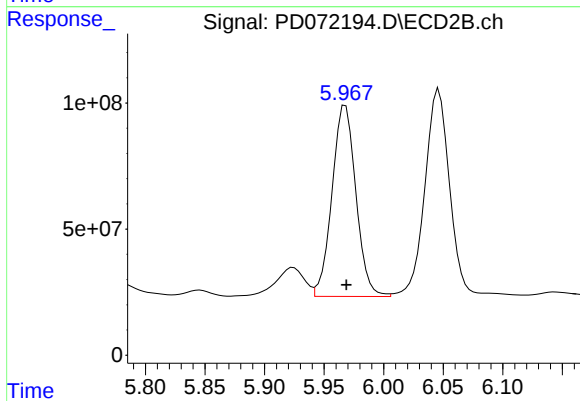

#25 Chlordane-3


R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 1056644806
Conc: 470.64 ng/ml

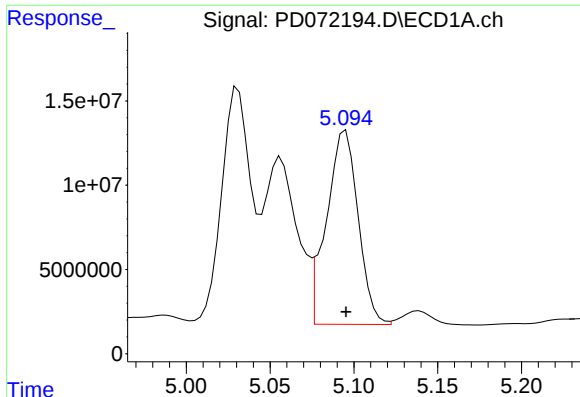

#26 Chlordane-4


R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 151030816
Conc: 526.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

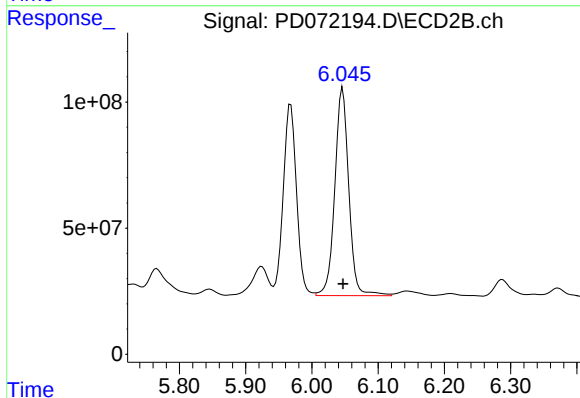


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 1208632116
Conc: 459.42 ng/ml

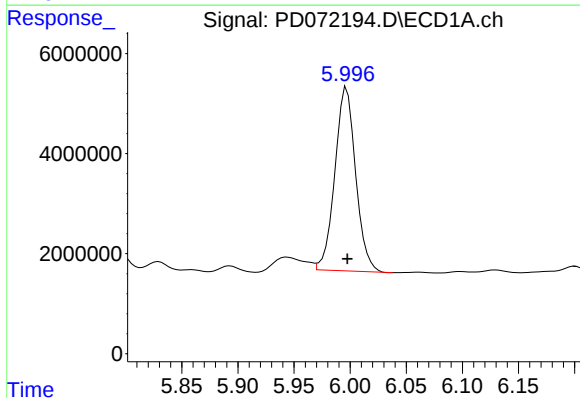


#27 Chlordane-5

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 47369800
Conc: 439.09 ng/ml

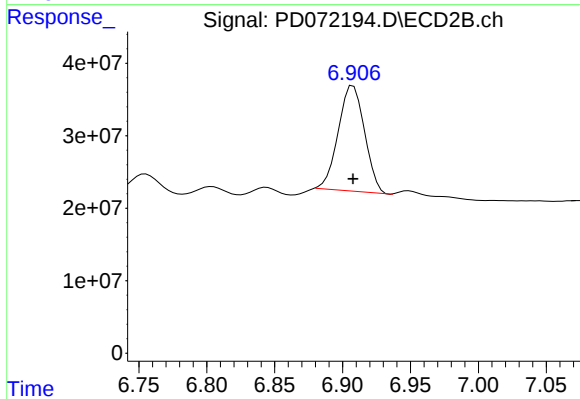

#27 Chlordane-5


R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 196527099
Conc: 425.23 ng/ml

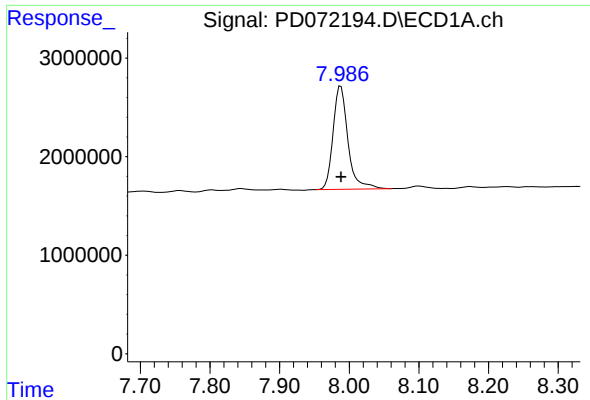

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 15592203
Conc: 6.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

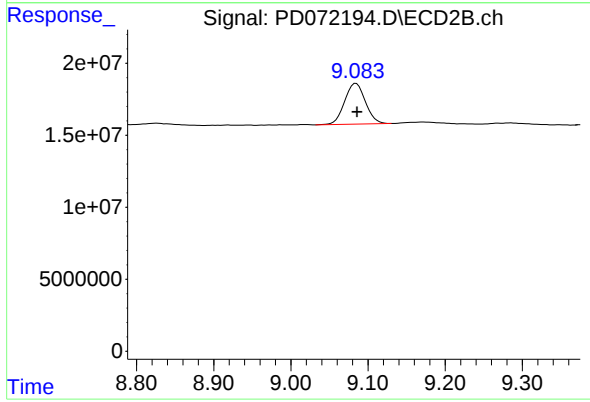

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.001 min
Response: 52877205
Conc: 5.99 ng/ml