

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 18:54
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 00:51:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 00:50:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.757	195.5E6	166.7E6	74.558	75.937
28)	SA Decachlor...	9.078	7.893	247.6E6	157.2E6	72.909	74.850
Target Compounds							
23)	Chlordane-1	4.704	3.753	98379217	54769168	753.670	759.303
24)	Chlordane-2	5.236	4.329	102.2E6	57617952	733.430	759.436
25)	Chlordane-3	5.947	4.959	446.2E6	199.2E6	761.050	777.198
26)	Chlordane-4	6.030	5.022	532.2E6	190.3E6	755.640	762.642
27)	Chlordane-5	6.882	5.918	84937572	67467004	761.144	767.765



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 18:54
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 00:51:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 00:50:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

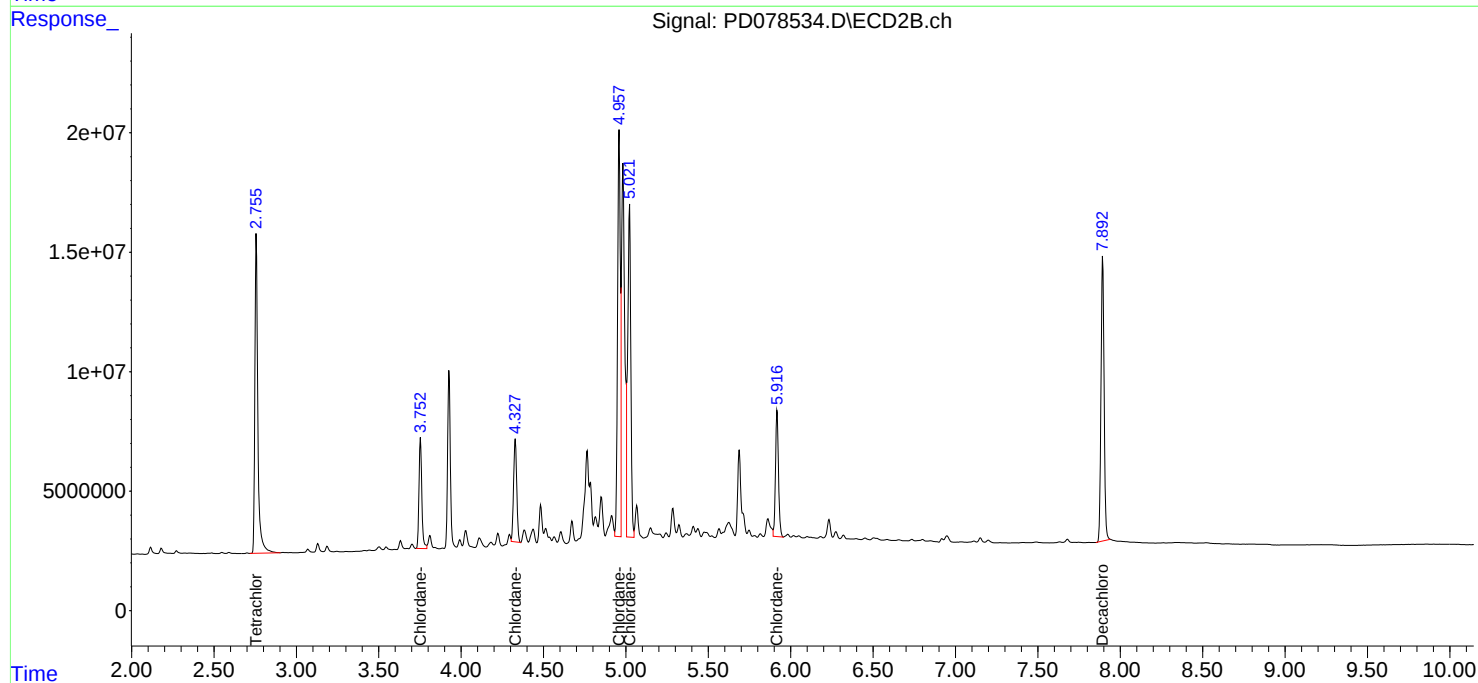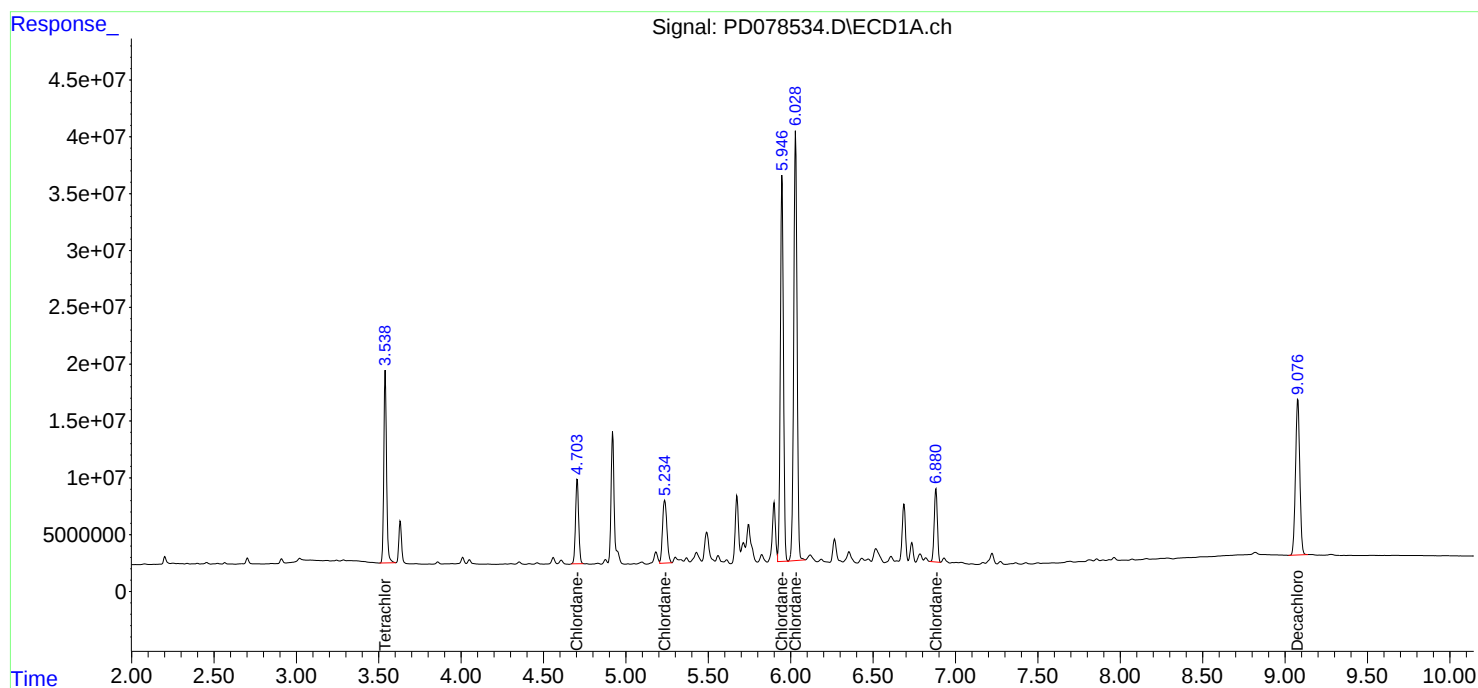


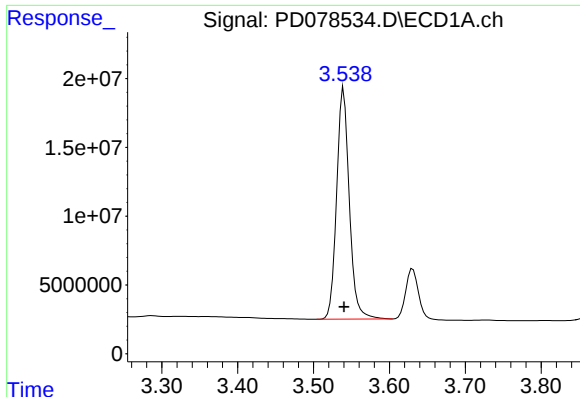

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 195498500
Conc: 74.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

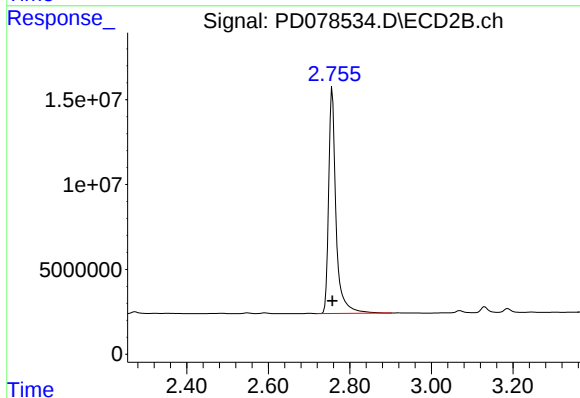


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 166714538
Conc: 75.94 ng/ml

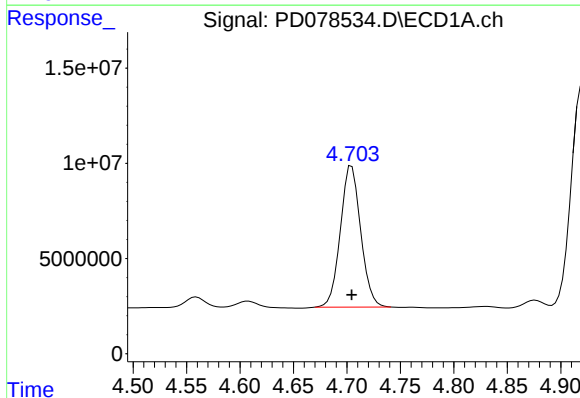


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 98379217
Conc: 753.67 ng/ml

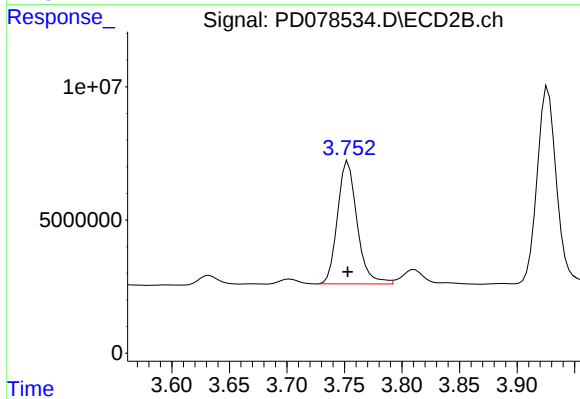

#23 Chlordane-1


R.T.: 3.753 min
Delta R.T.: 0.000 min
Response: 54769168
Conc: 759.30 ng/ml

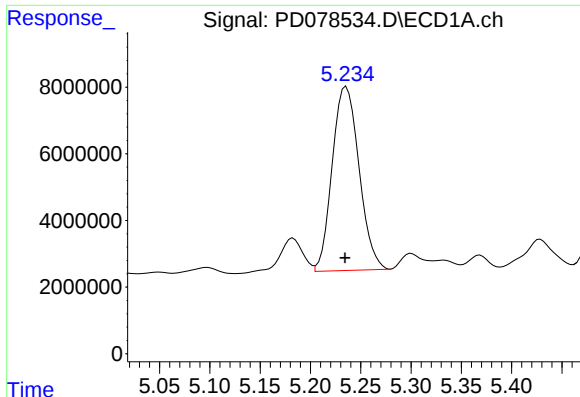

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 102216324
Conc: 733.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

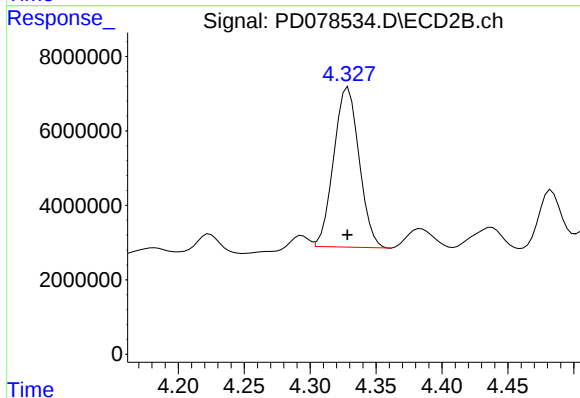


#24 Chlordane-2

R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 57617952
Conc: 759.44 ng/ml

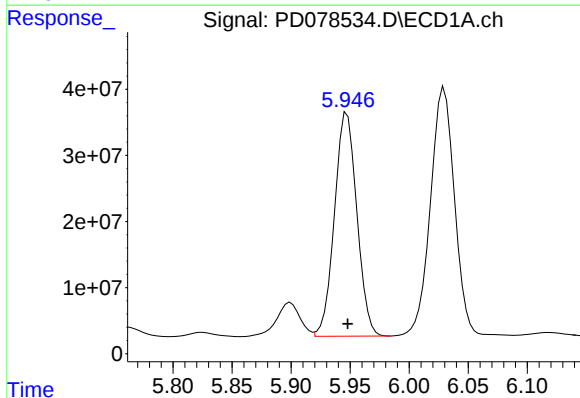


#25 Chlordane-3

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 446196995
Conc: 761.05 ng/ml

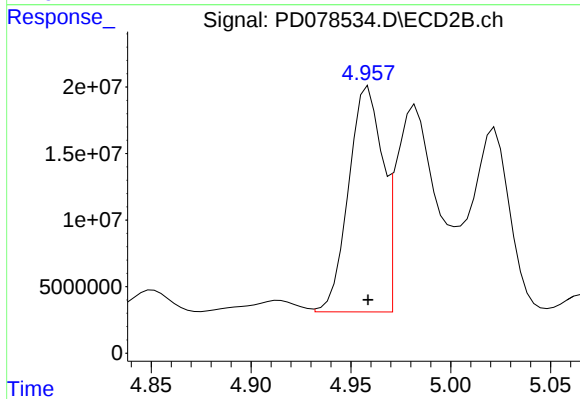

#25 Chlordane-3


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 199170796
Conc: 777.20 ng/ml

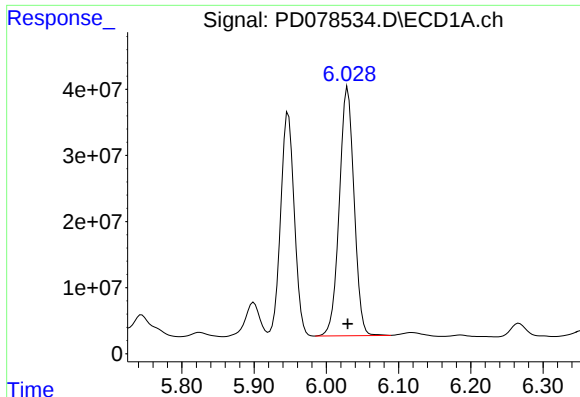

#26 Chlordane-4


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 532155497
Conc: 755.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

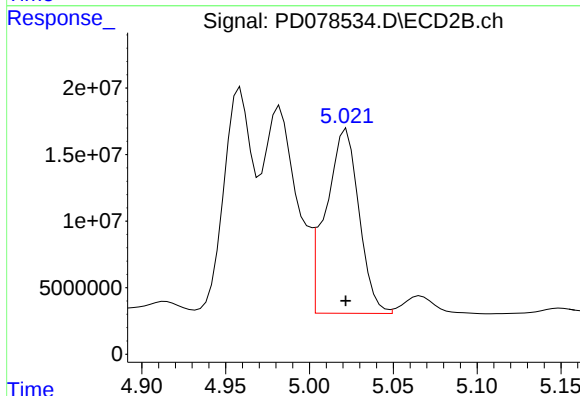


#26 Chlordane-4

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 190271325
Conc: 762.64 ng/ml

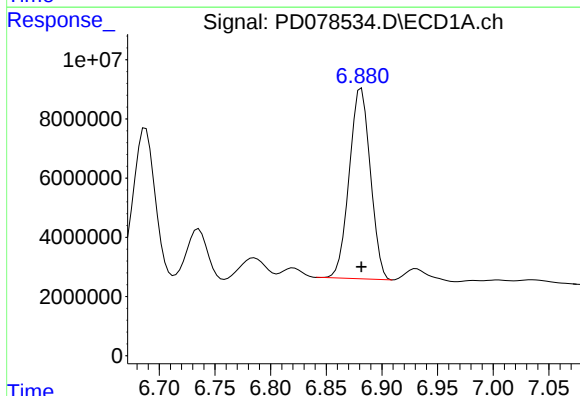


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 84937572
Conc: 761.14 ng/ml

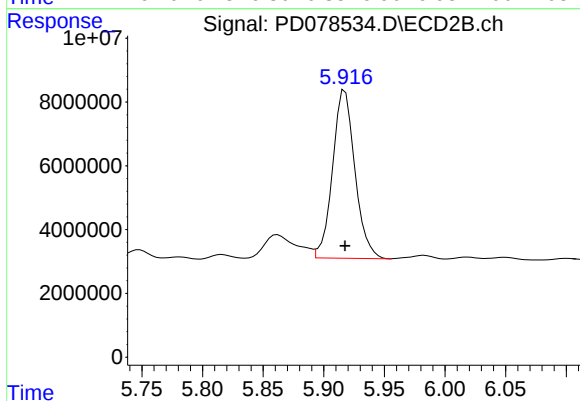

#27 Chlordane-5


R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 67467004
Conc: 767.76 ng/ml

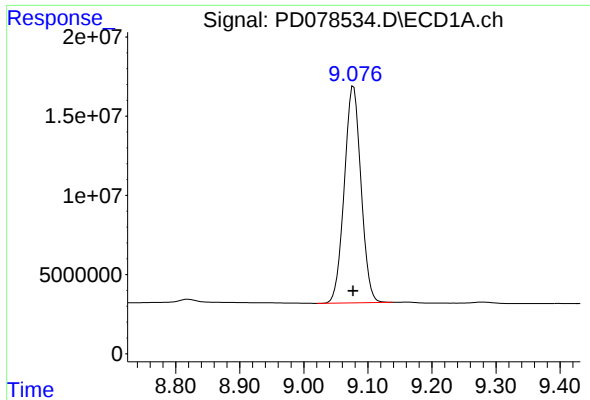

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.000 min
Response: 247568789
Conc: 72.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

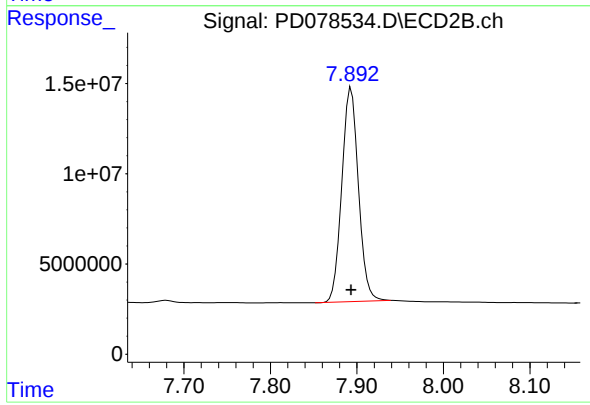

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 157231189
Conc: 74.85 ng/ml