

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 19:08
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 00:51:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 00:50:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.757	131.1E6	109.8E6	50.000	50.000
28)	SA Decachlor...	9.077	7.893	169.8E6	105.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.704	3.753	65266778	36065426	500.000	500.000
24)	Chlordane-2	5.235	4.328	69683774	37934694	500.000	500.000
25)	Chlordane-3	5.948	4.959	293.1E6	128.1E6	500.000	500.000
26)	Chlordane-4	6.030	5.022	352.1E6	124.7E6	500.000	500.000
27)	Chlordane-5	6.882	5.917	55796012	43937287	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 19:08
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 00:51:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 00:50:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

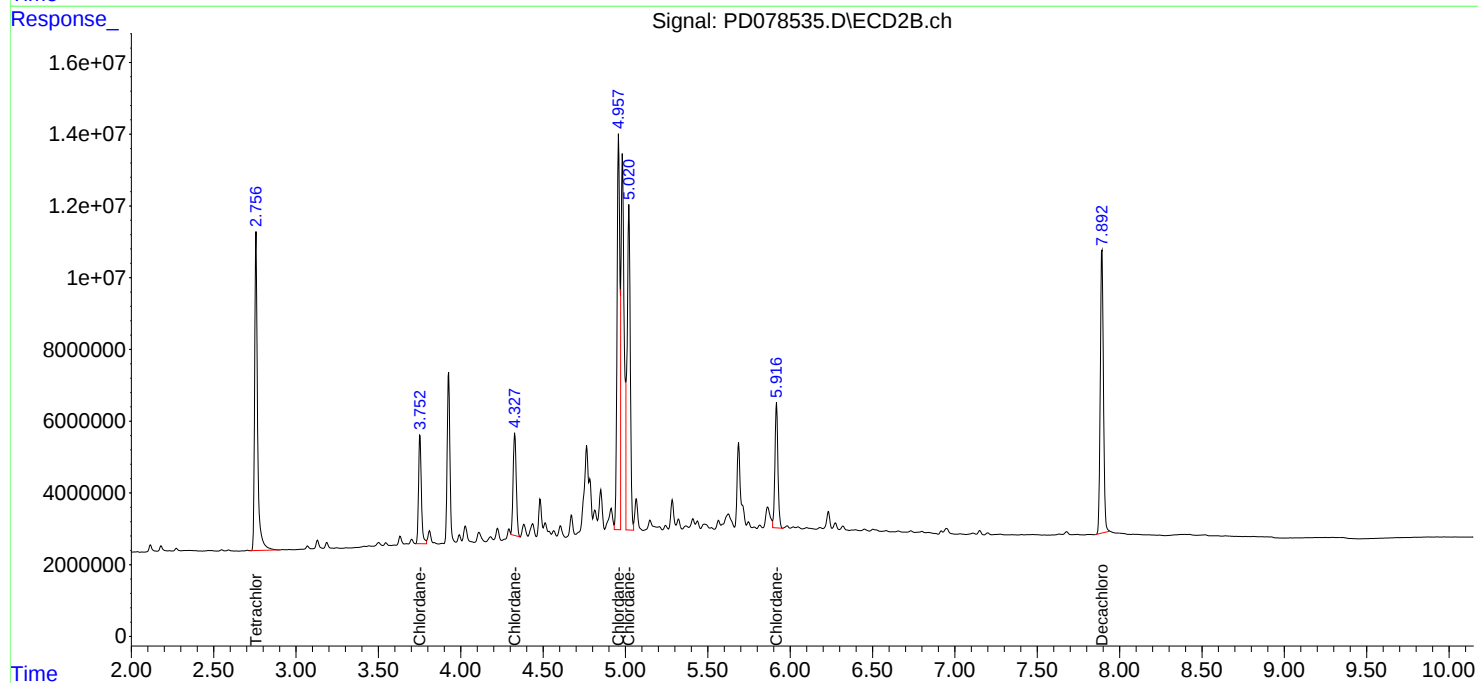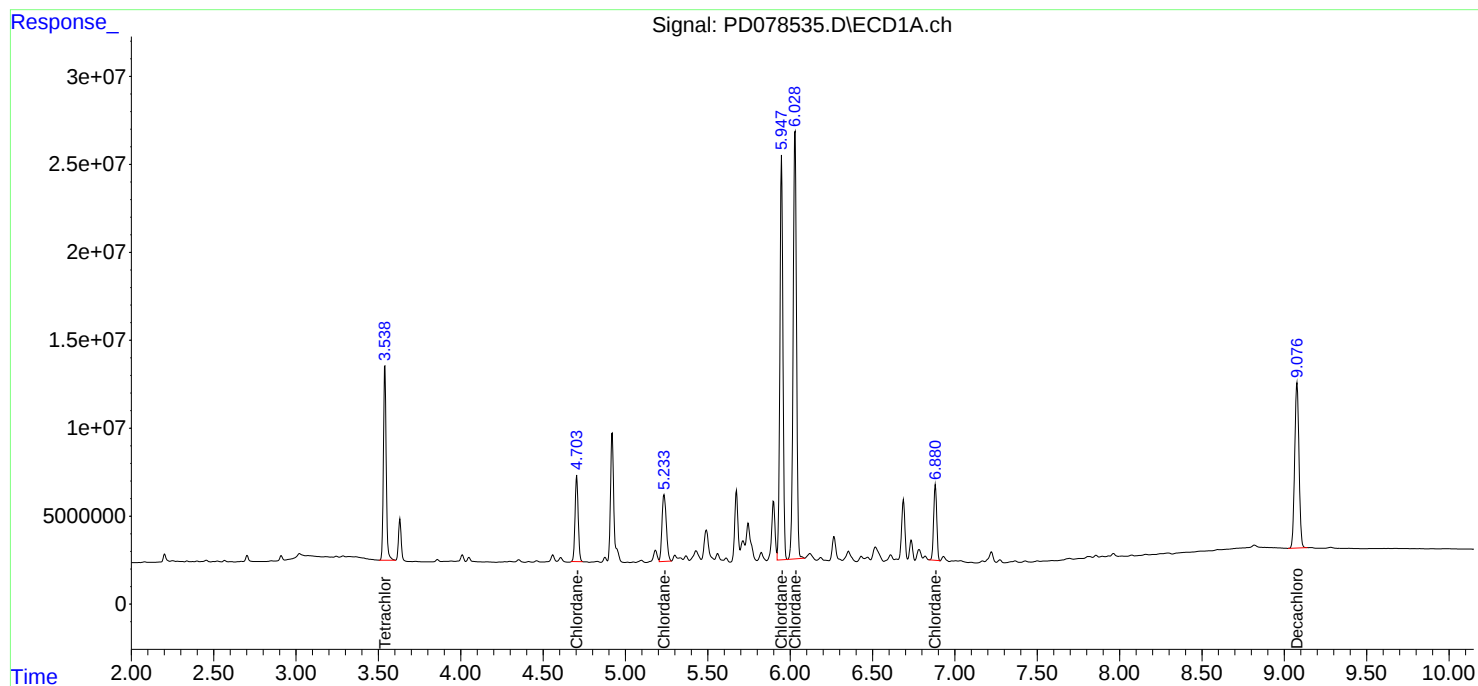


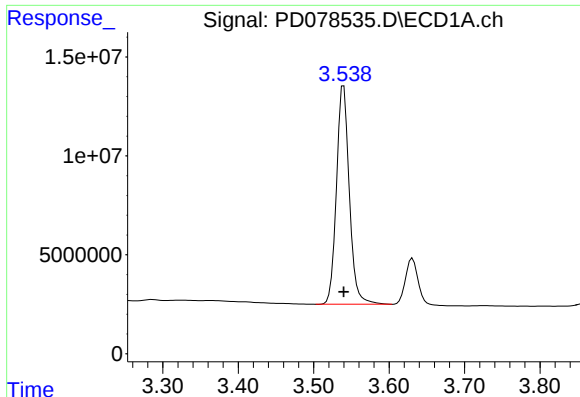

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 131105256
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

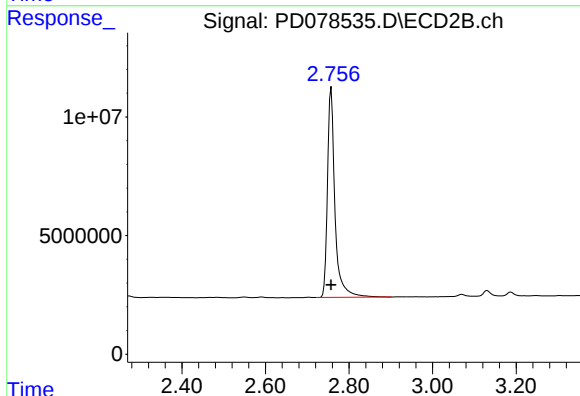


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 109770996
Conc: 50.00 ng/ml

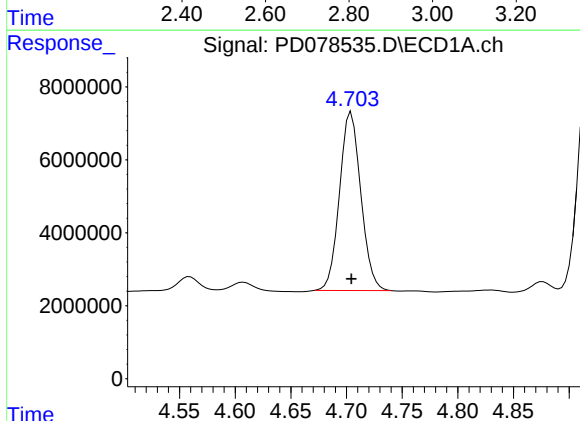


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 65266778
Conc: 500.00 ng/ml

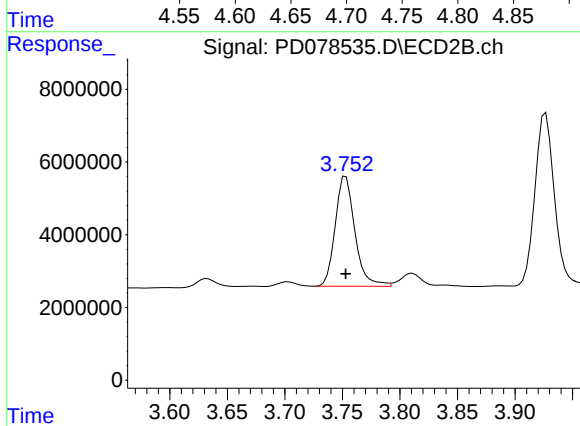

#23 Chlordane-1


R.T.: 3.753 min
Delta R.T.: 0.000 min
Response: 36065426
Conc: 500.00 ng/ml

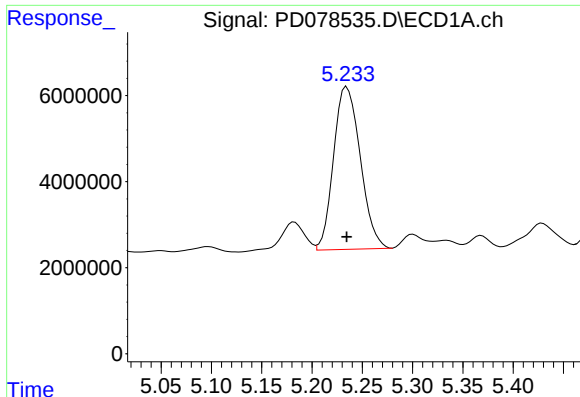

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 69683774
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

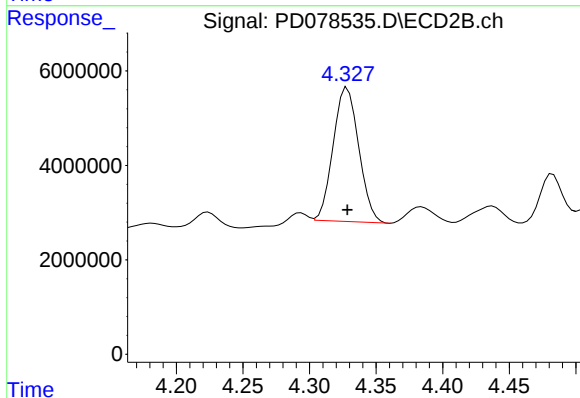


#24 Chlordane-2

R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 37934694
Conc: 500.00 ng/ml

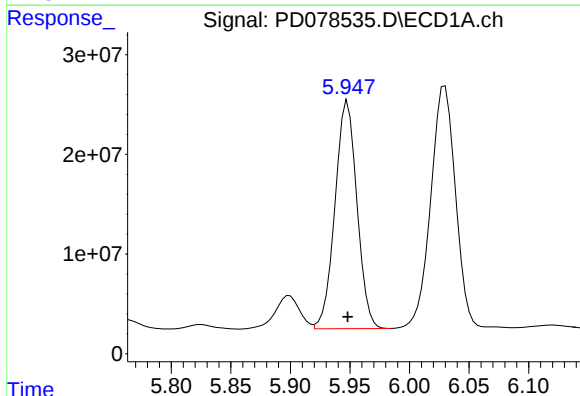


#25 Chlordane-3

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 293145508
Conc: 500.00 ng/ml

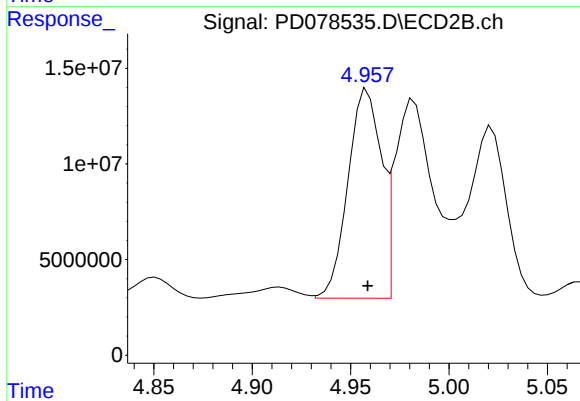

#25 Chlordane-3


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 128133871
Conc: 500.00 ng/ml

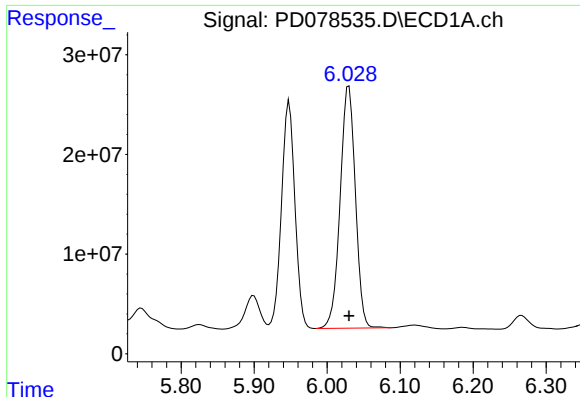

#26 Chlordane-4


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 352122285
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

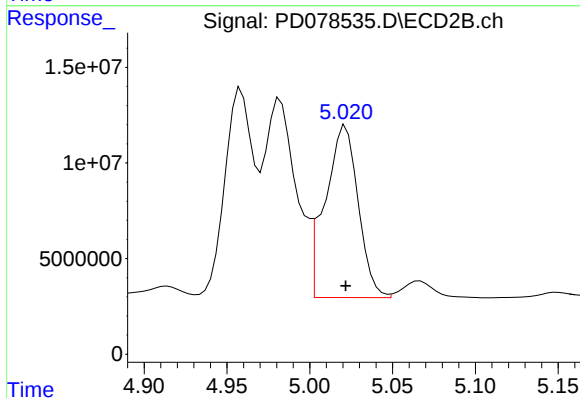


#26 Chlordane-4

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 124744834
Conc: 500.00 ng/ml

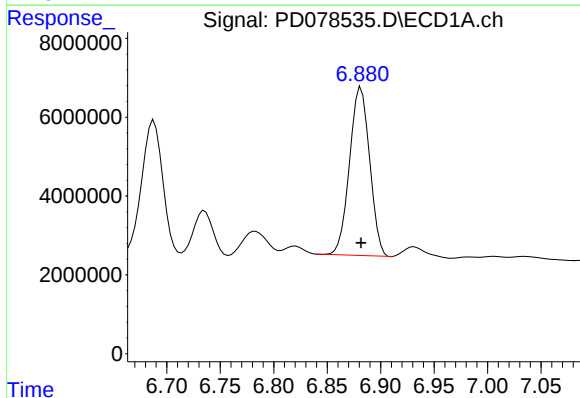


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 55796012
Conc: 500.00 ng/ml

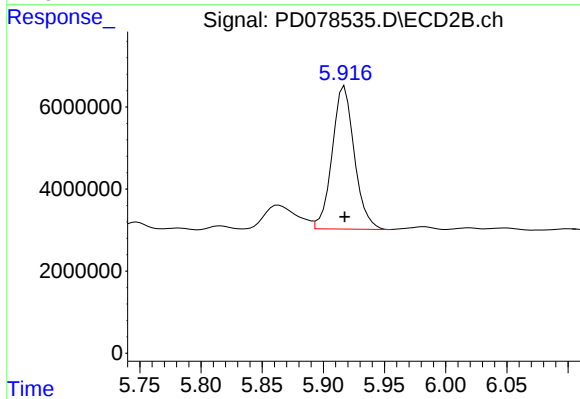

#27 Chlordane-5


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 43937287
Conc: 500.00 ng/ml

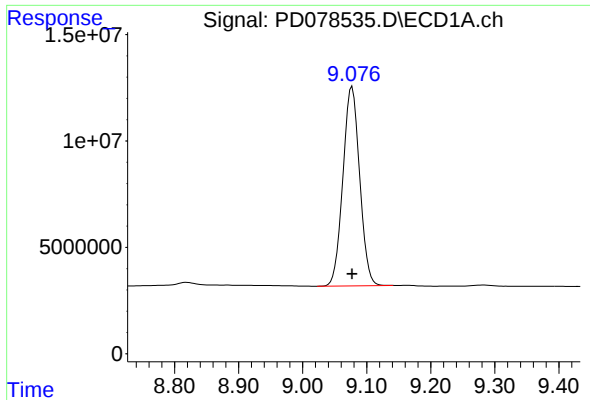

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 169778554
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

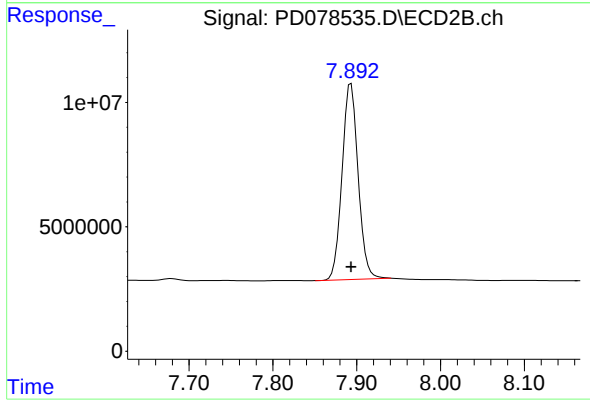

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 105030193
Conc: 50.00 ng/ml