

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
 Data File : PD078536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2023 19:21
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 00:51:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 00:50:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.757	64254624	52499736	24.505	23.913
28)	SA Decachlor...	9.077	7.893	85546371	51938034	25.194	24.725
Target Compounds							
23)	Chlordane-1	4.704	3.752	31690289	17507369	242.775	242.717
24)	Chlordane-2	5.235	4.328	35187284	19176161	252.478	252.752
25)	Chlordane-3	5.947	4.958	138.9E6	61656363	236.839	240.594
26)	Chlordane-4	6.030	5.021	168.8E6	60227966	239.752	241.405
27)	Chlordane-5	6.881	5.917	26732023	20804804	239.551	236.756



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100323\
Data File : PD078536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2023 19:21
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 00:51:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 00:50:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

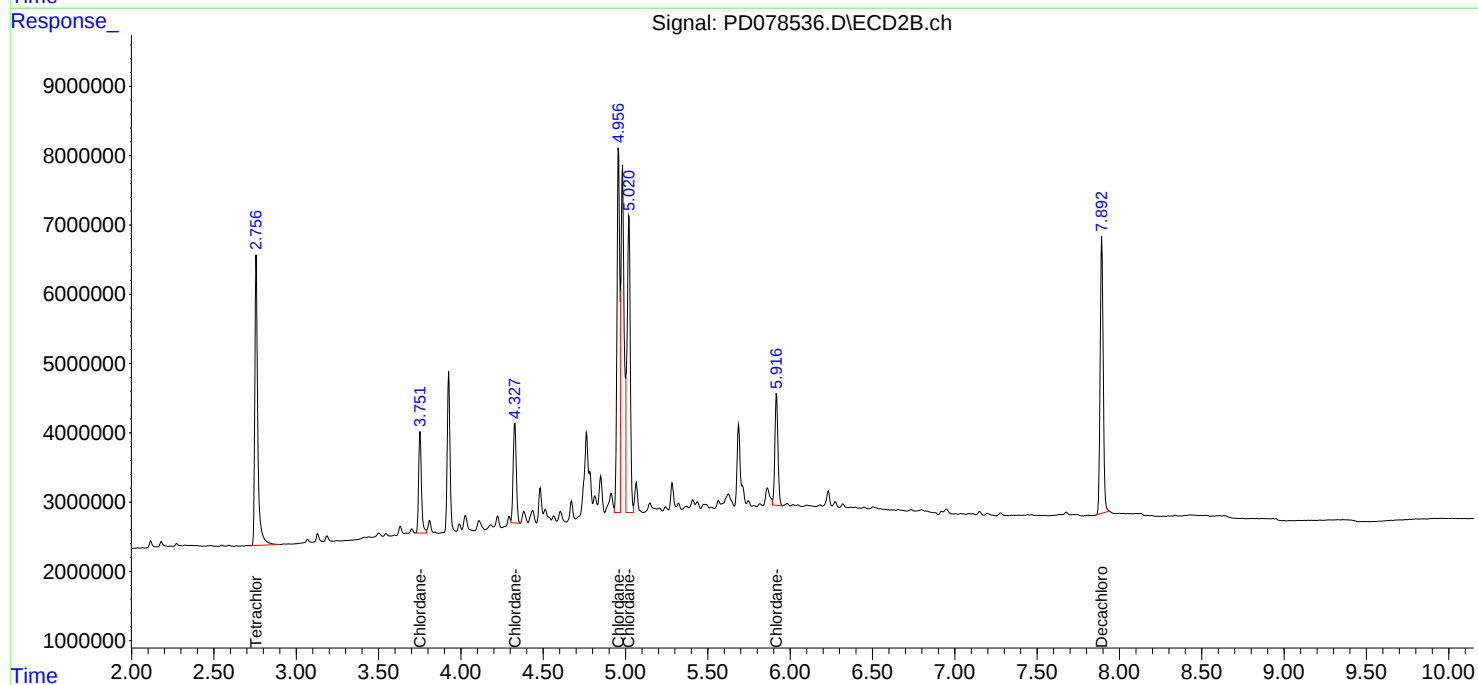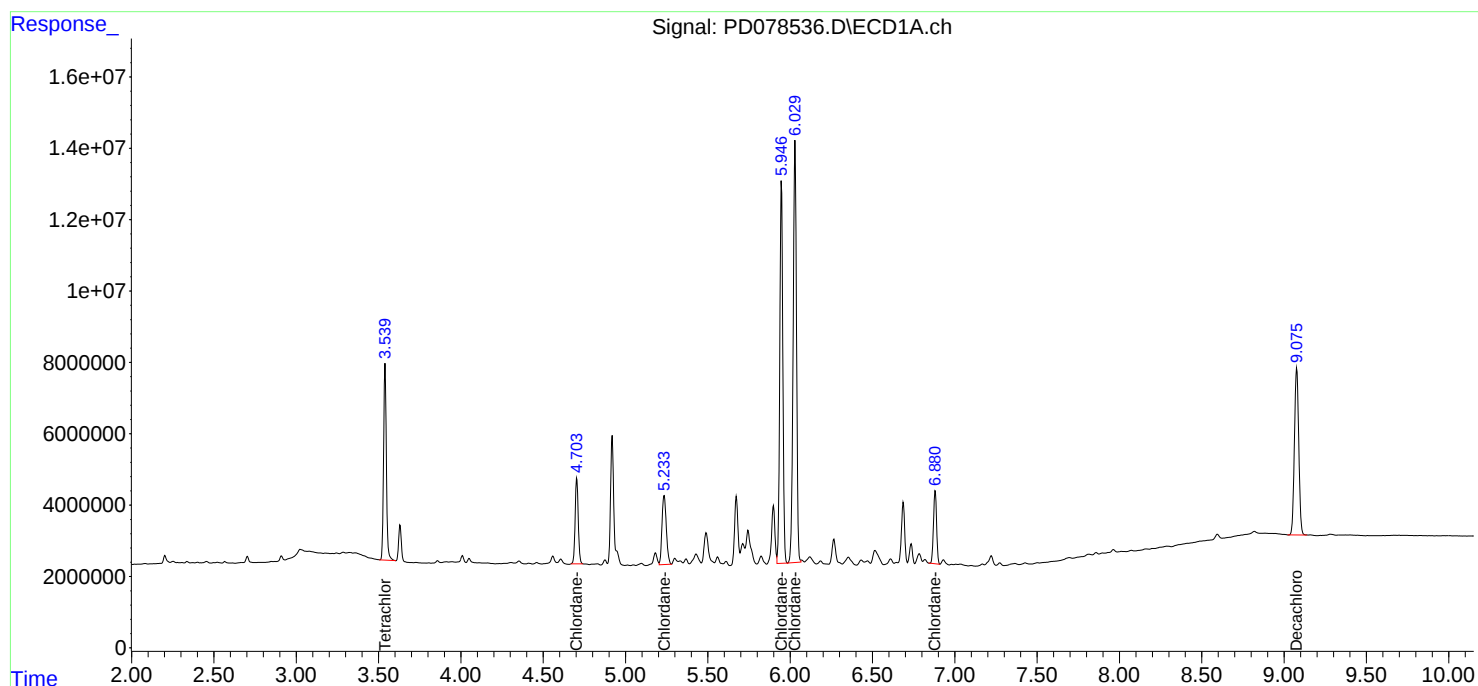


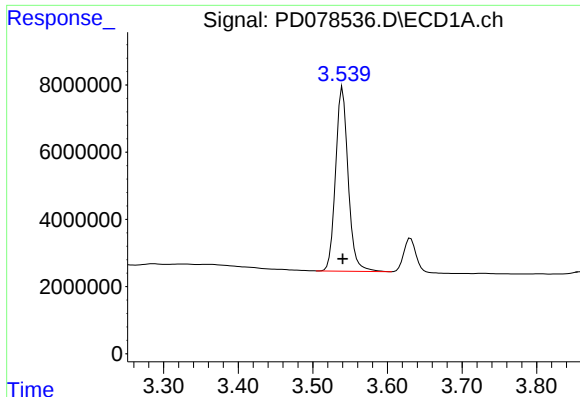

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 64254624
Conc: 24.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

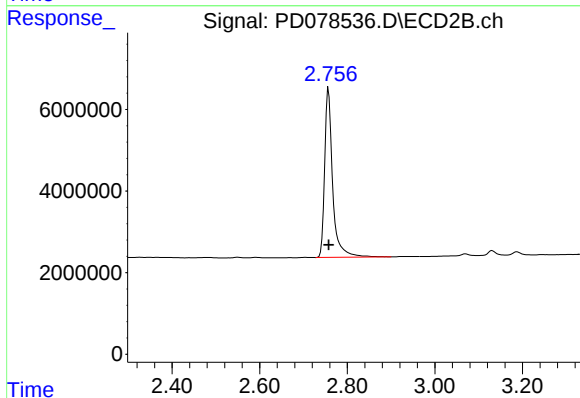


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: 0.000 min
Response: 52499736
Conc: 23.91 ng/ml

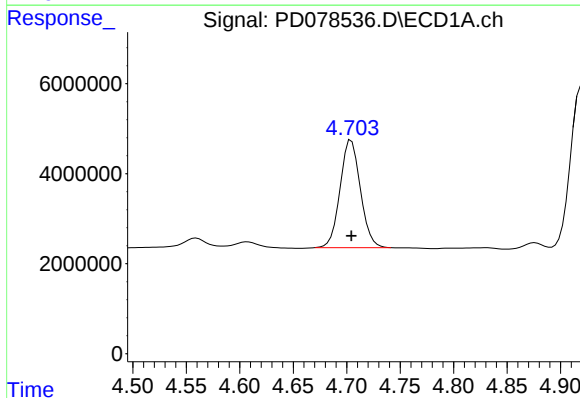


#23 Chlordane-1

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 31690289
Conc: 242.78 ng/ml

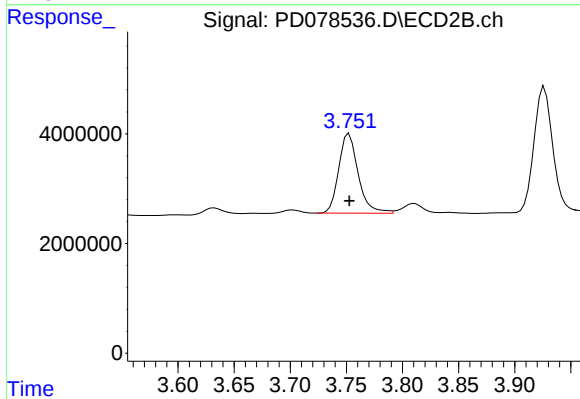

#23 Chlordane-1


R.T.: 3.752 min
Delta R.T.: 0.000 min
Response: 17507369
Conc: 242.72 ng/ml

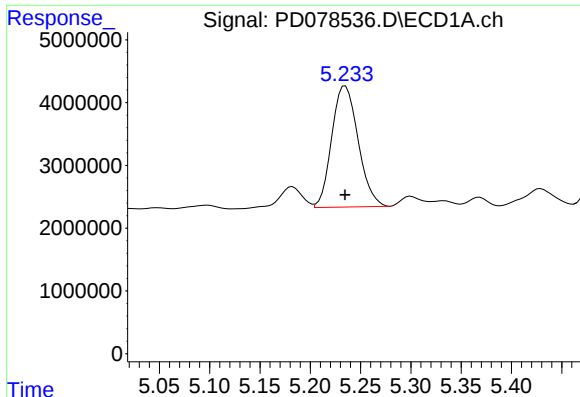

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 35187284
Conc: 252.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

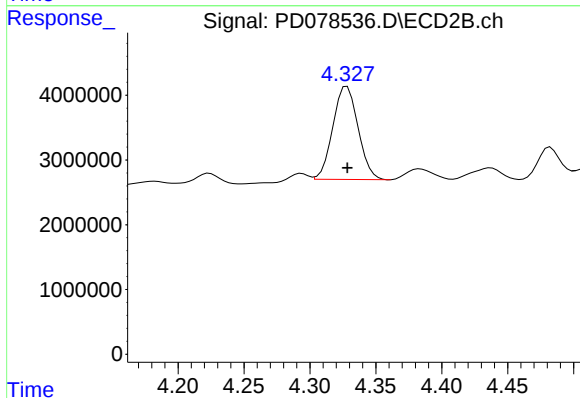


#24 Chlordane-2

R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 19176161
Conc: 252.75 ng/ml

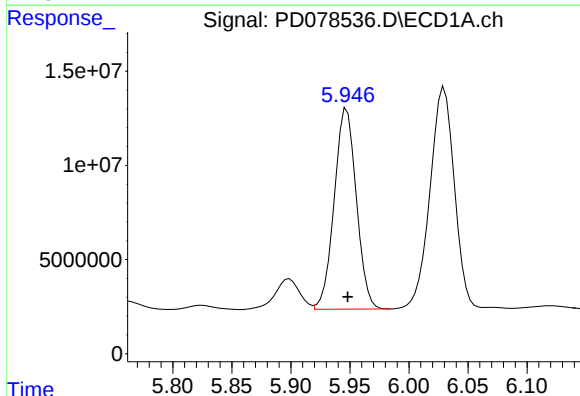


#25 Chlordane-3

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 138856861
Conc: 236.84 ng/ml

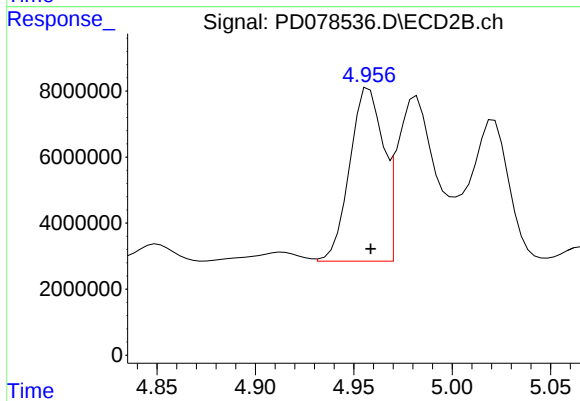

#25 Chlordane-3


R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 61656363
Conc: 240.59 ng/ml

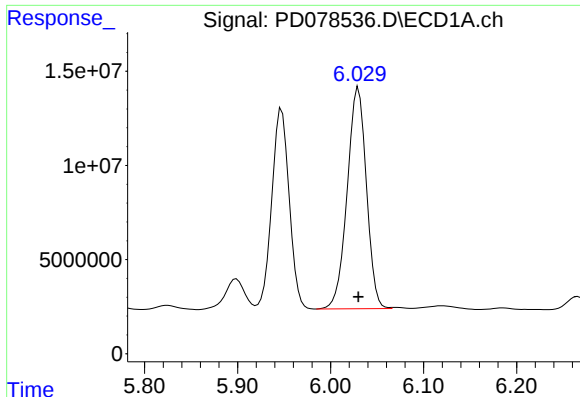

#26 Chlordane-4


R.T.: 6.030 min
Delta R.T.: 0.000 min
Response: 168844030
Conc: 239.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

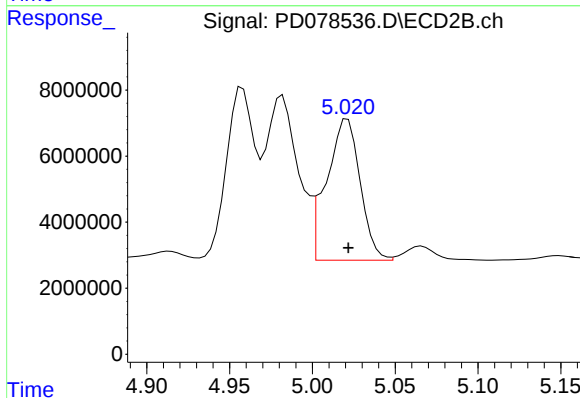


#26 Chlordane-4

R.T.: 5.021 min
Delta R.T.: 0.000 min
Response: 60227966
Conc: 241.40 ng/ml

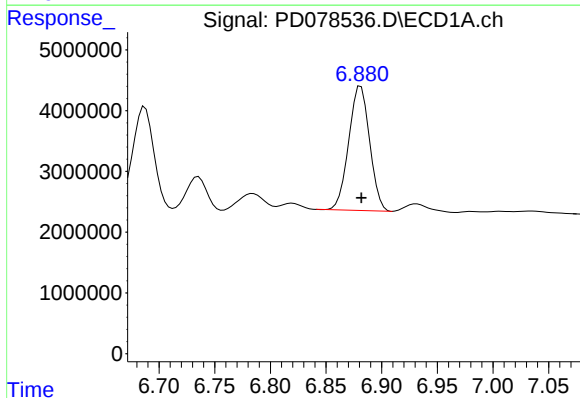


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 26732023
Conc: 239.55 ng/ml

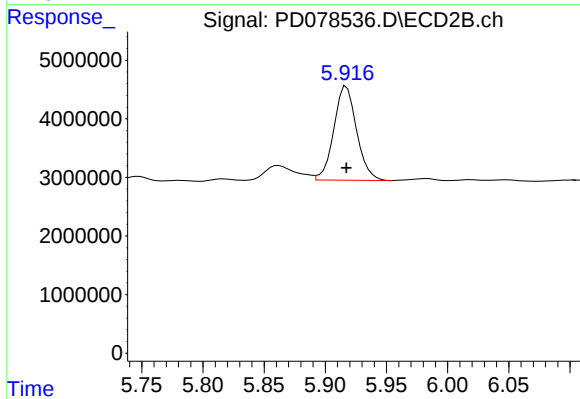

#27 Chlordane-5


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 20804804
Conc: 236.76 ng/ml

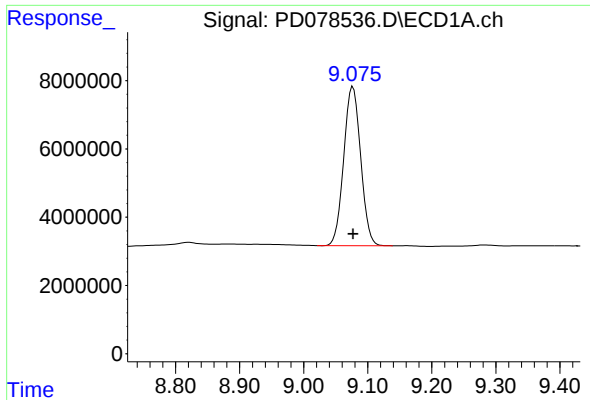

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 85546371
Conc: 25.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

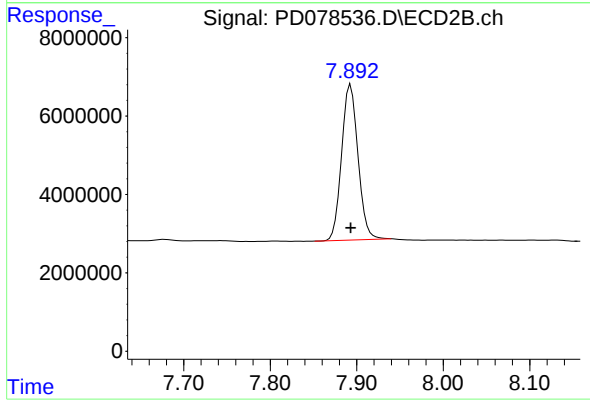

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 51938034
Conc: 24.73 ng/ml